


Data Path : Z:\HPCHEM1\BNA_F\Data\BF092617\
 Data File : BF098826.D
 Acq On : 26 Sep 2017 12:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

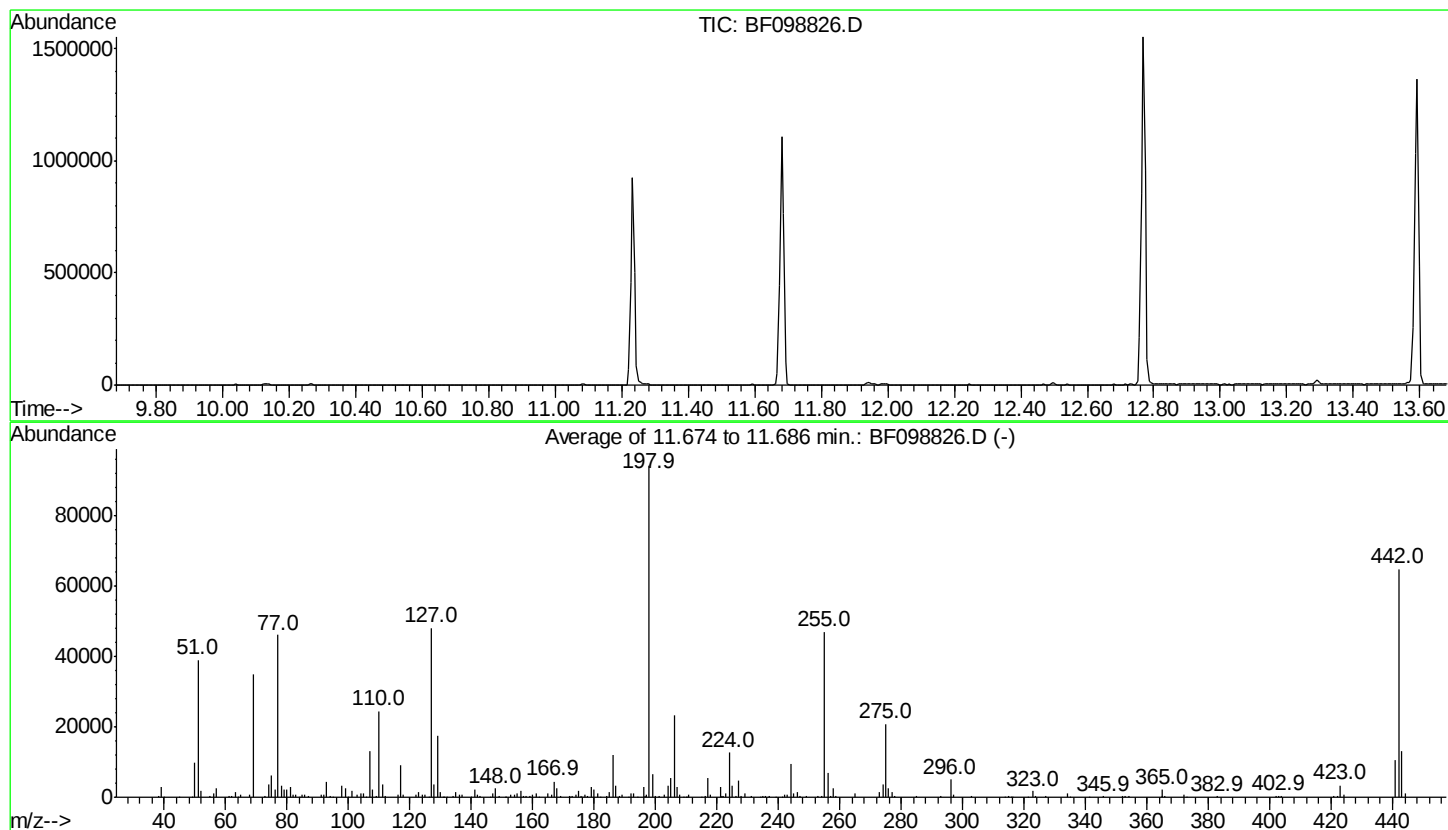

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	39008	PASS
68	69	0.00	2	1.7	605	PASS
69	198	0.00	100	37.1	34930	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.1	48114	PASS
197	198	0.00	2	0.7	681	PASS
198	198	100	100	100.0	94130	PASS
199	198	5	9	6.8	6443	PASS
275	198	10	60	22.2	20905	PASS
365	198	1	100	2.2	2058	PASS
441	442	0.01	24	16.3	10585	PASS
442	198	50	100	68.9	64870	PASS
443	442	15	24	20.2	13103	PASS