
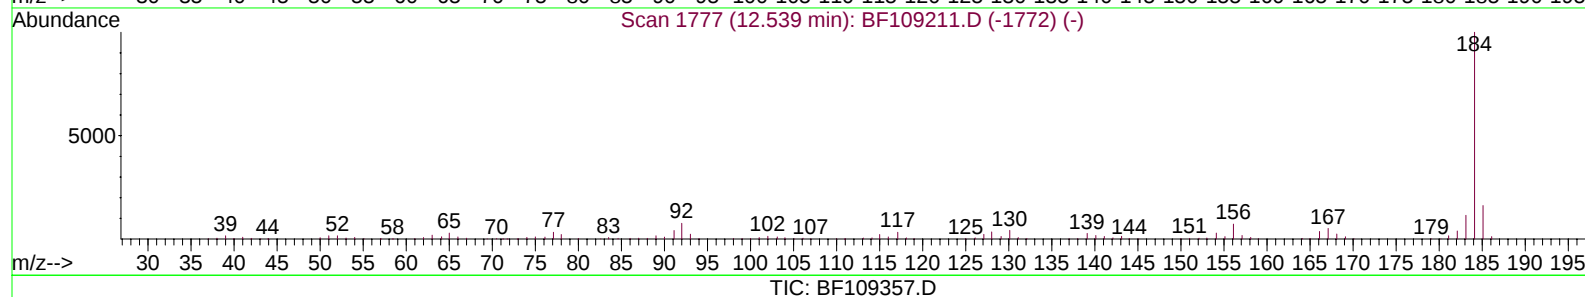
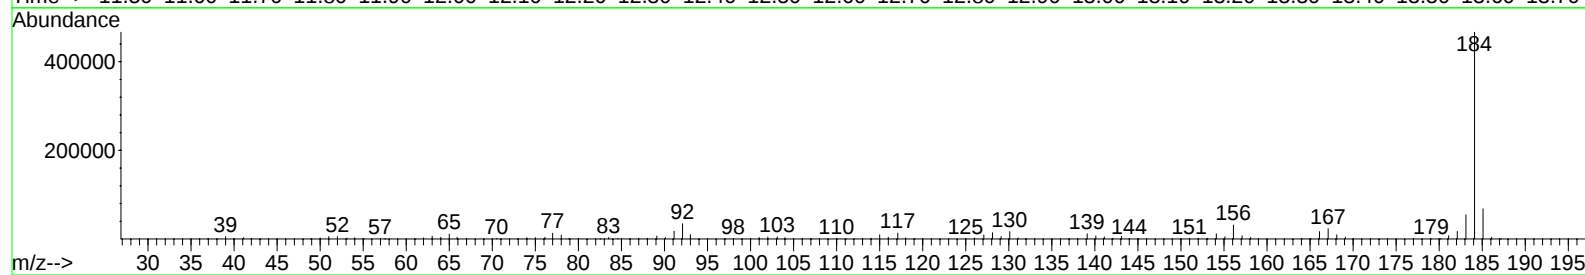


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092618\  
Data File : BF109357.D  
Acq On : 27 Sep 2018 00:45  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 13:43:14 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Sep 22 13:32:18 2018  
Response via : Initial Calibration

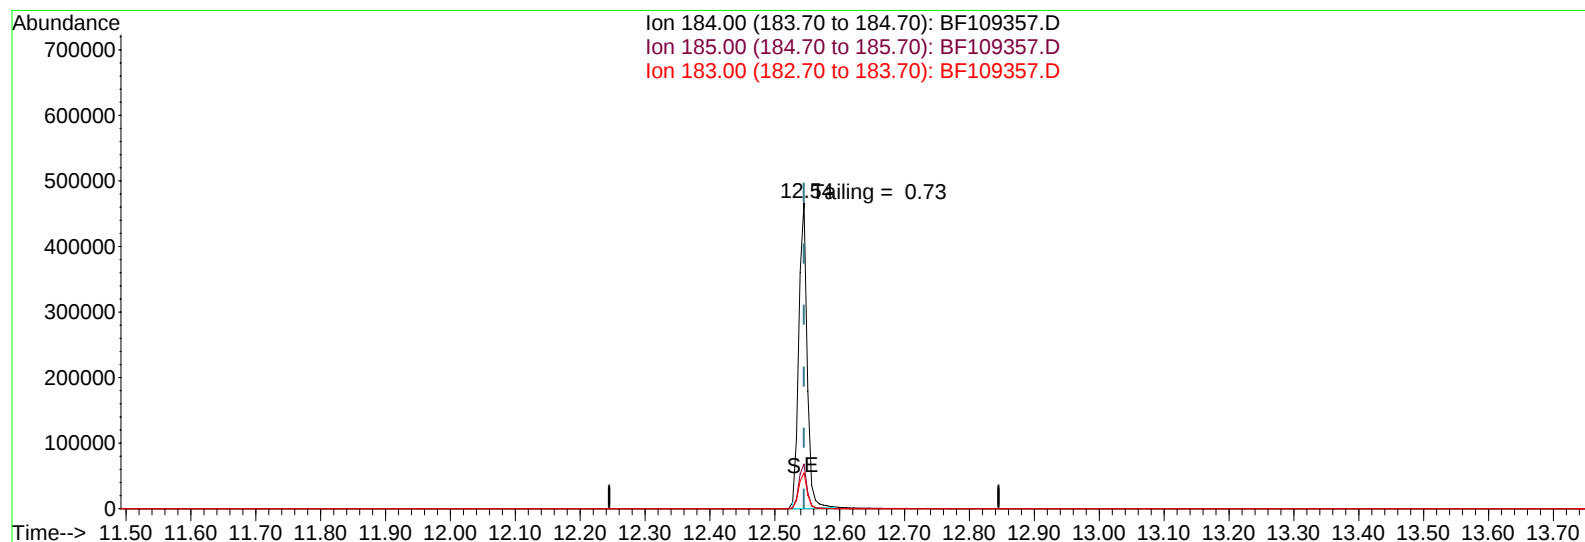

(76) Benzidine




12.545min (-0.000) 0.00ng

response 429054

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.63 |
| 183.00 | 11.60 | 11.72 |
| 0.00   | 0.00  | 0.00  |

```
Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092618\  
Data File : BF109357.D  
Acq On    : 27 Sep 2018  00:45  
Operator  : JU/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Sep 27 13:43:14 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Sep 22 13:32:18 2018  
Response via : Initial Calibration

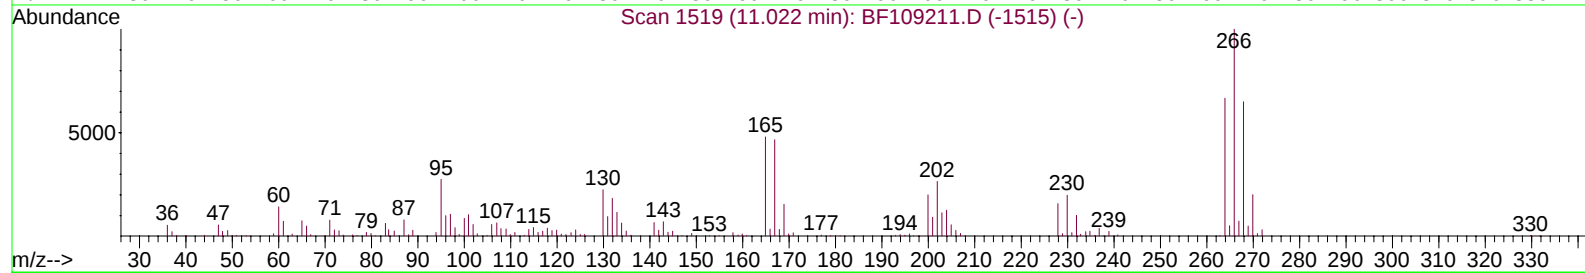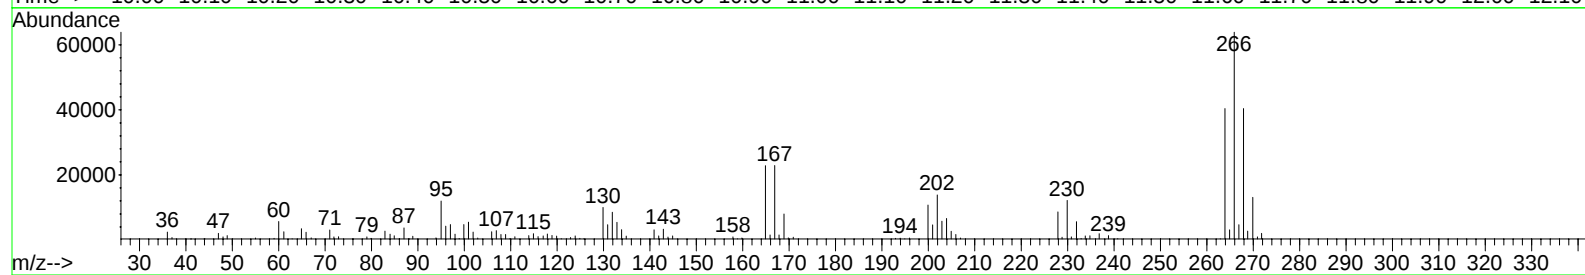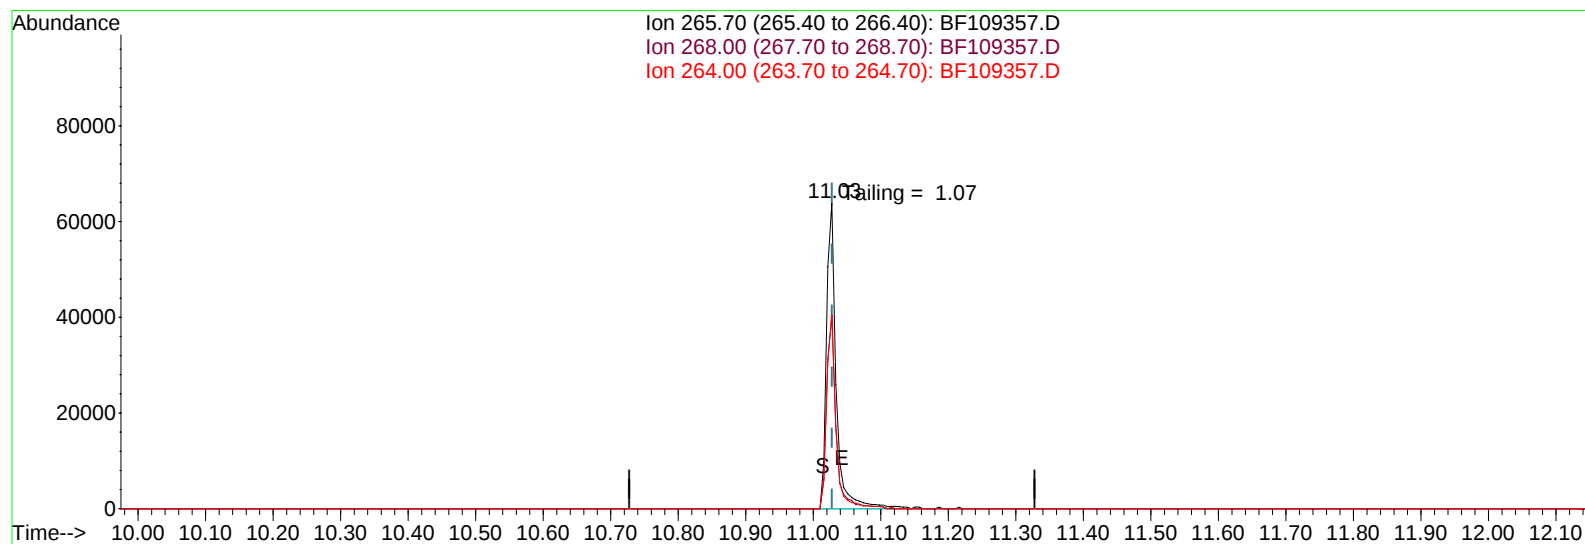

TIC: BF109357.D

(69) Pentachlorophenol (C)

11.027min (-0.000) 0.00ng m

response 63066

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 63.28 |
| 264.00 | 61.90 | 63.29 |
| 0.00   | 0.00  | 0.00  |