

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092618\
 Data File : BF109354.D
 Acq On : 26 Sep 2018 22:59
 Operator : JU/SJ
 Sample : J5069-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SLUDGE-B

Quant Time: Sep 27 06:43:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	85467	20.00	ng	0.00
21) Naphthalene-d8	7.99	136	292023	20.00	ng	0.00
38) Acenaphthene-d10	9.74	164	120500	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	252947	20.00	ng	0.00
75) Chrysene-d12	13.84	240	281664	20.00	ng	0.00
86) Perylene-d12	15.24	264	223532	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	269593	51.95	ng	0.00
7) Phenol-d6	6.34	99	323534	48.86	ng	-0.02
23) Nitrobenzene-d5	7.26	82	288964	58.41	ng	-0.02
41) 2,4,6-Tribromophenol	10.52	330	73084	61.52	ng	-0.01
44) 2-Fluorobiphenyl	9.06	172	444130	55.59	ng	-0.01
78) Terphenyl-d14	12.79	244	527444	45.96	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.46	163	101700	11.604	ng	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092618\
Data File : BF109354.D
Acq On : 26 Sep 2018 22:59
Operator : JU/SJ
Sample : J5069-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLUDGE-B

Quant Time: Sep 27 06:43:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

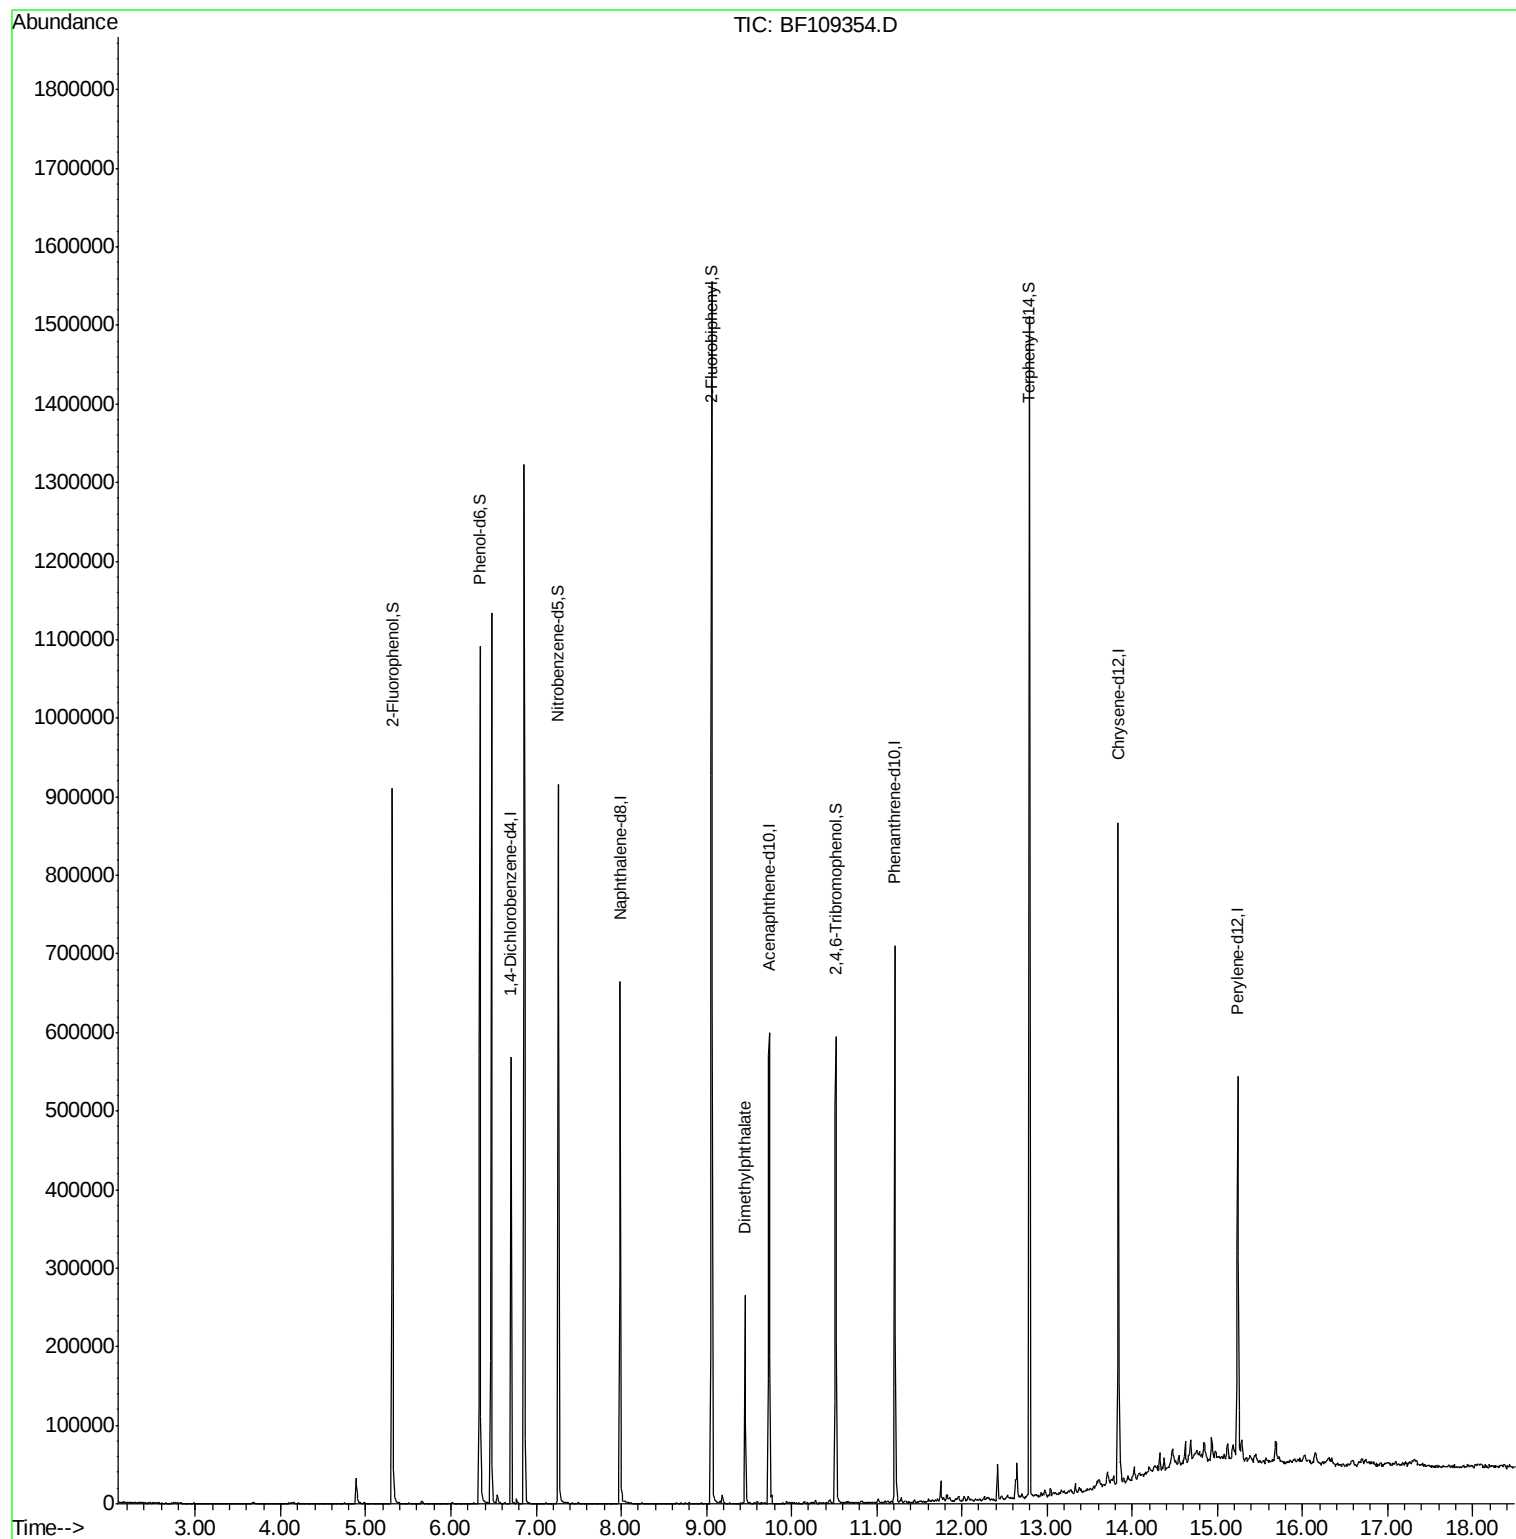




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.70 min Scan# 785
 Delta R.T. -0.01 min
 Lab File: BF109354.D
 Acq: 26 Sep 2018 22:59

Instrument :
 BNA_F
 ClientSampleId :
 SLUDGE-B

Tot Ion:152 Resp: 85467
 Ion Ratio Lower Upper
 152 100
 150 159.1 124.6 186.8
 115 62.5 50.1 75.1

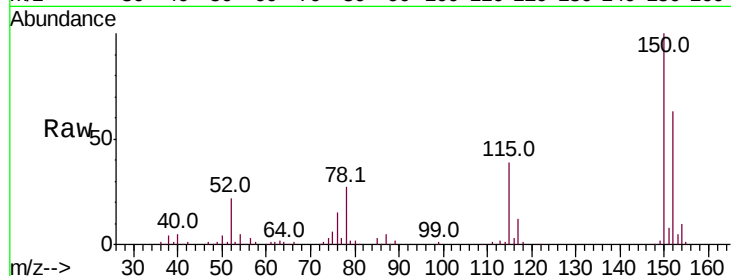


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

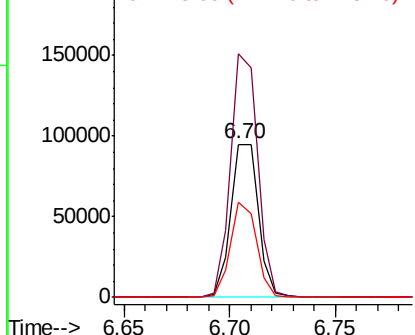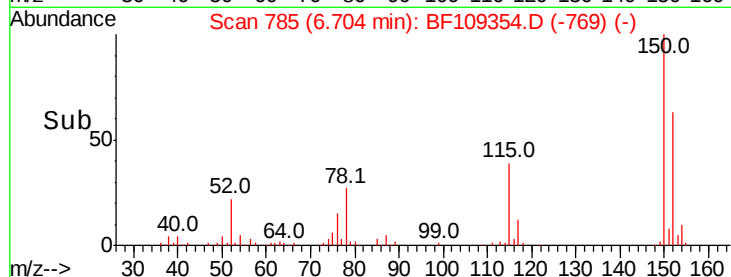



#5


2-Fluorophenol
 Concen: 51.955 ng
 RT: 5.32 min Scan# 549
 Delta R.T. 0.00 min
 Lab File: BF109354.D
 Acq: 26 Sep 2018 22:59

Tgt Ion:112 Resp: 269593
 Ion Ratio Lower Upper
 112 100
 64 54.1 47.9 71.9
 63 27.3 23.7 35.5

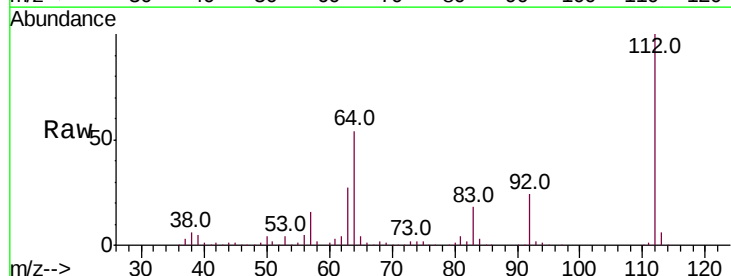

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

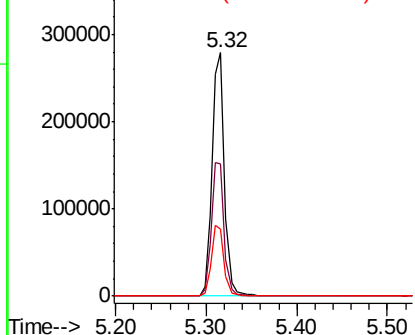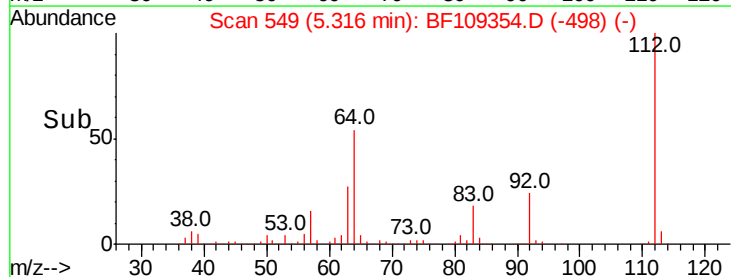

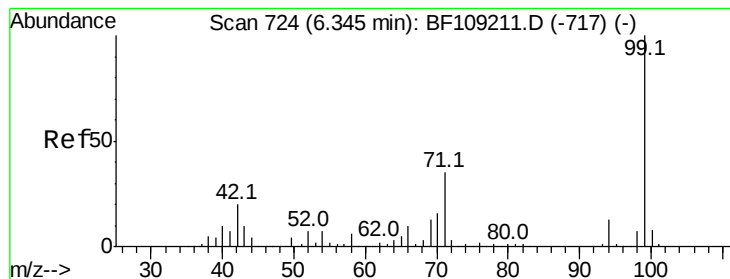

#7

Phenol-d6

Concen: 48.862 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.02 min

Lab File: BF109354.D

Acq: 26 Sep 2018 22:59

Instrument :

BNA_F

ClientSampled :

SLUDGE-B


Tot Ion: 99 Resp: 323534

Ion Ratio Lower Upper




99 100

42 18.7 14.5 21.7

71 34.6 25.4 38.0

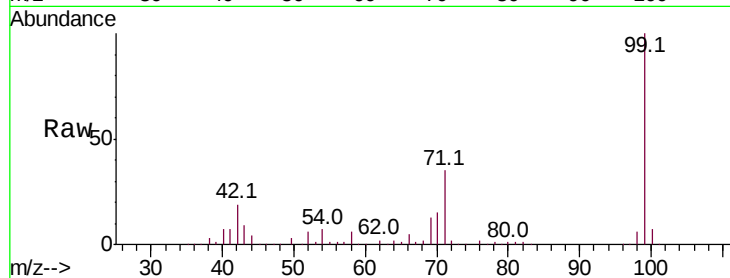

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

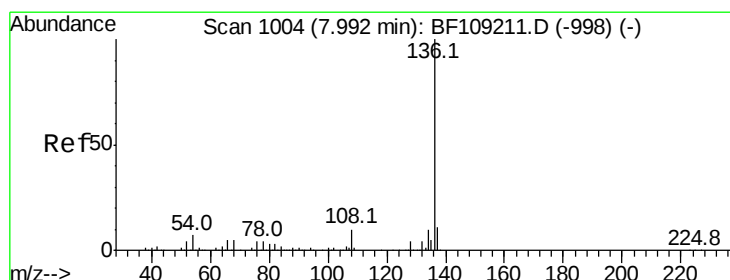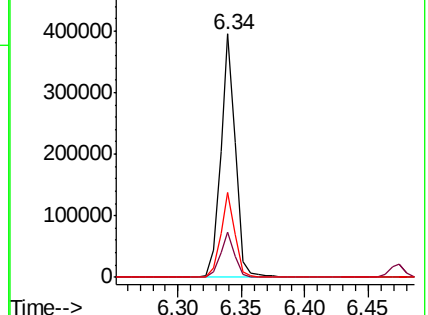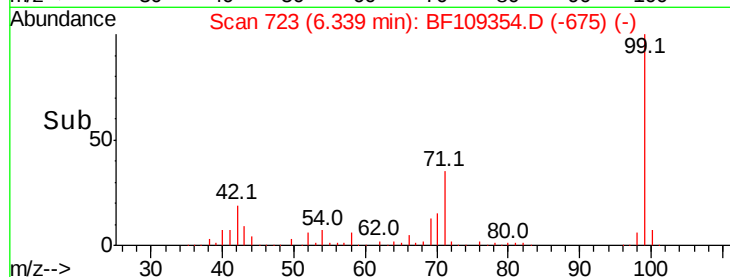

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.99 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF109354.D

Acq: 26 Sep 2018 22:59

Tgt Ion: 136 Resp: 292023


Ion Ratio Lower Upper

136 100



137 10.7 8.9 13.3

54 7.2 6.6 9.8

68 6.1 5.0 7.4

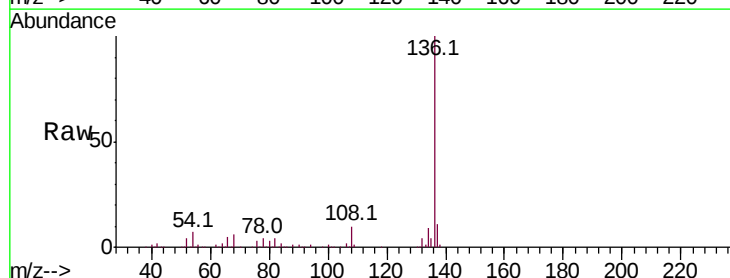

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

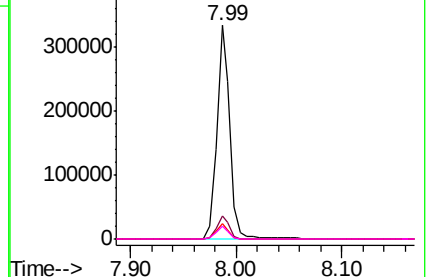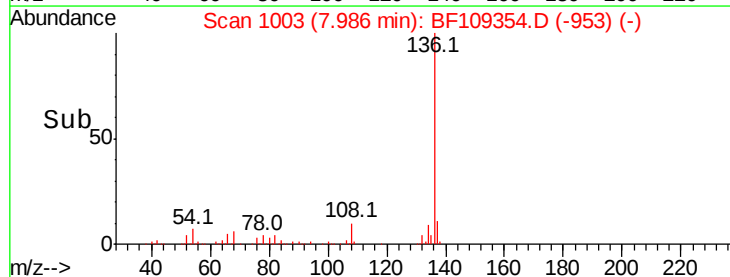







#23
 Nitrobenzene-d5
 Concen: 58.413 ng
 RT: 7.26 min Scan# 880
 Delta R.T. -0.02 min
 Lab File: BF109354.D
 Acq: 26 Sep 2018 22:59

Instrument :
 BNA_F
 ClientSampleId :
 SLUDGE-B

Tot Ion: 82 Resp: 288964
 Ion Ratio Lower Upper
 82 100
 128 42.6 36.1 54.1
 54 47.4 41.4 62.2

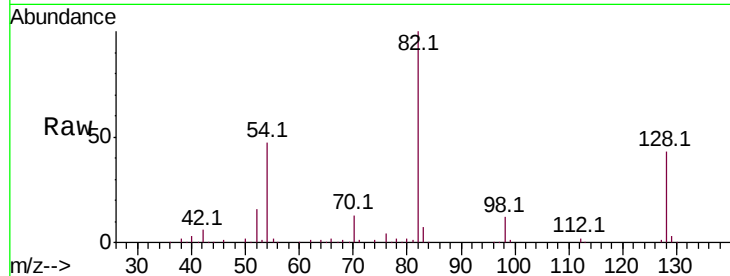


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

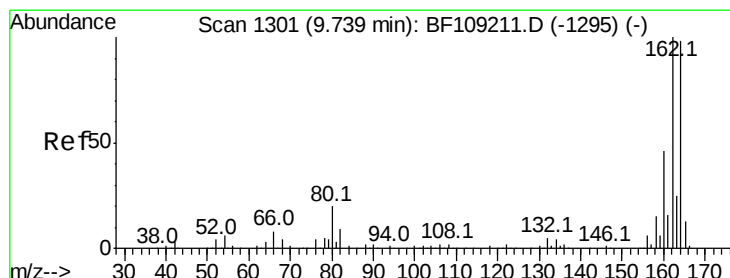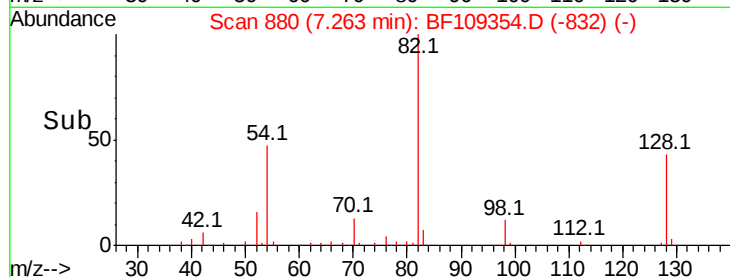
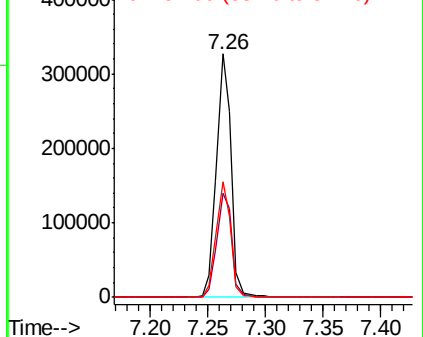



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.74 min Scan# 1301
 Delta R.T. 0.00 min
 Lab File: BF109354.D
 Acq: 26 Sep 2018 22:59

Tgt Ion: 164 Resp: 120500
 Ion Ratio Lower Upper
 164 100
 162 104.7 86.1 129.1
 160 48.3 38.3 57.5

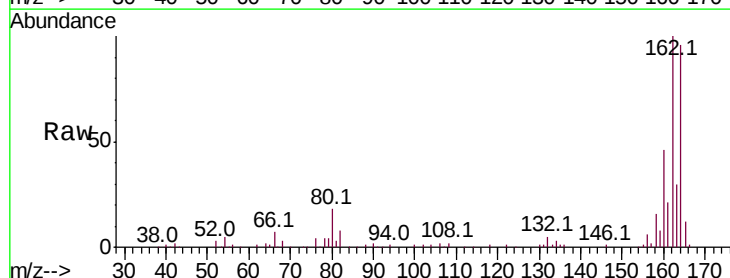

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

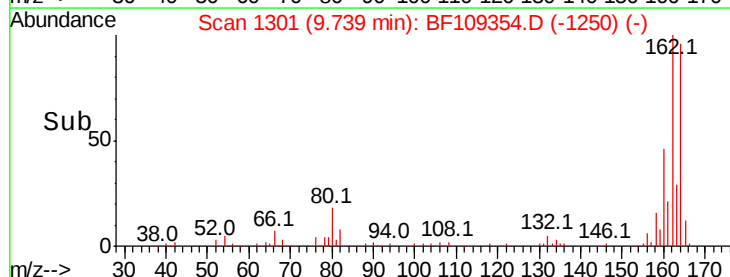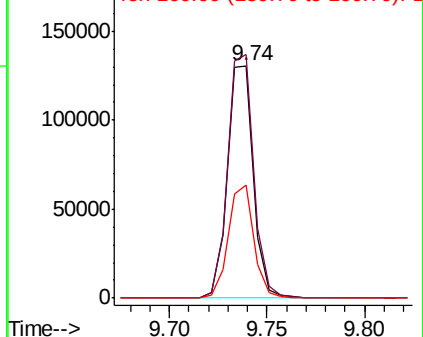


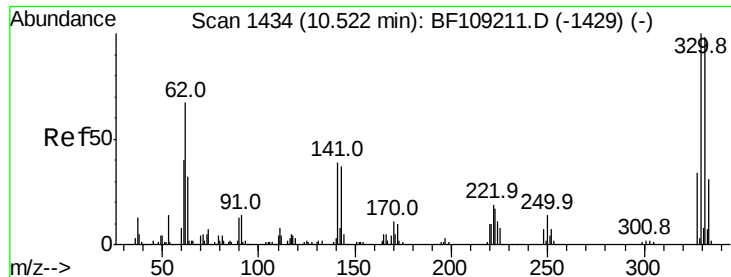




#41
 2,4,6-Tribromophenol
 Concen: 61.525 ng
 RT: 10.52 min Scan# 1434
 Delta R.T. -0.01 min
 Lab File: BF109354.D
 Acq: 26 Sep 2018 22:59

Instrument :
 BNA_F
 ClientSampleId :
 SLUDGE-B

Tot Ion:330 Resp: 73084
 Ion Ratio Lower Upper
 330 100
 332 94.1 77.0 115.6
 141 31.4 29.9 44.9

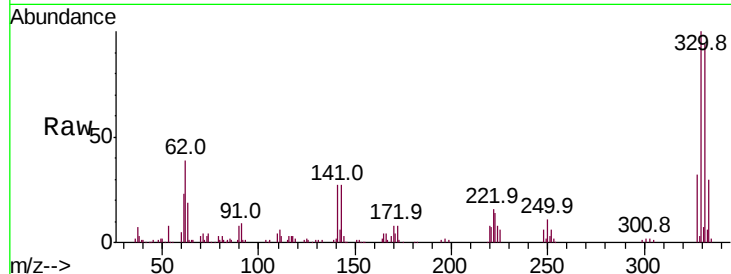


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

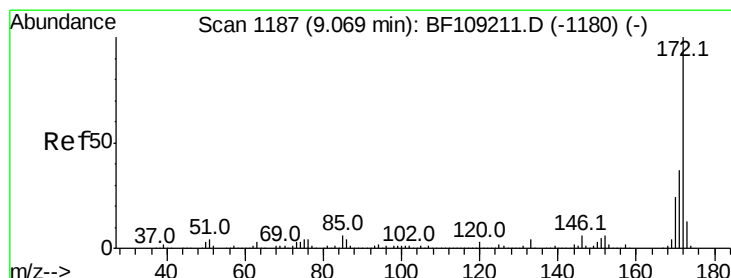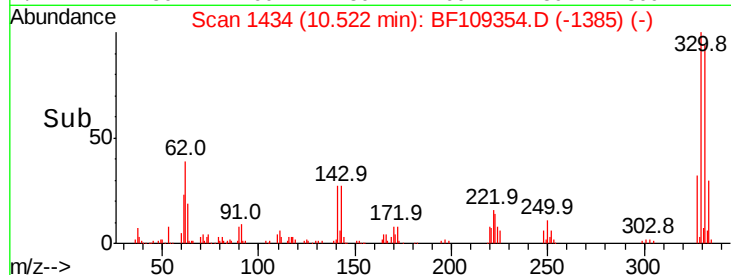
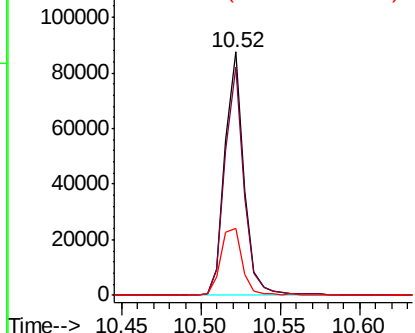



#44
 2-Fluorobiphenyl
 Concen: 55.588 ng
 RT: 9.06 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF109354.D
 Acq: 26 Sep 2018 22:59

Tgt Ion:172 Resp: 444130
 Ion Ratio Lower Upper
 172 100
 171 35.0 29.7 44.5
 170 23.1 19.6 29.4

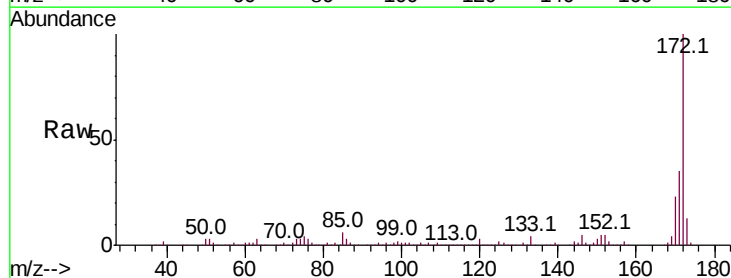

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

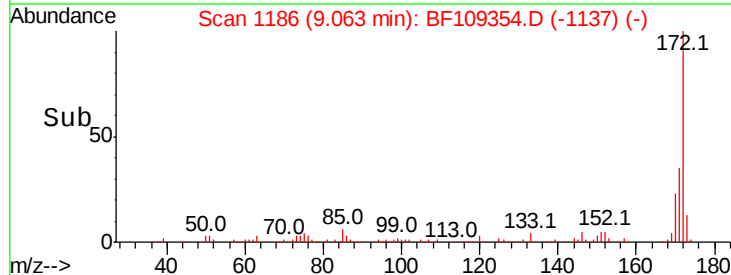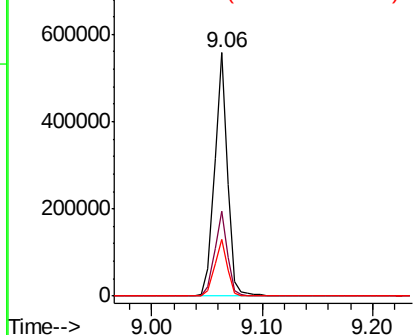


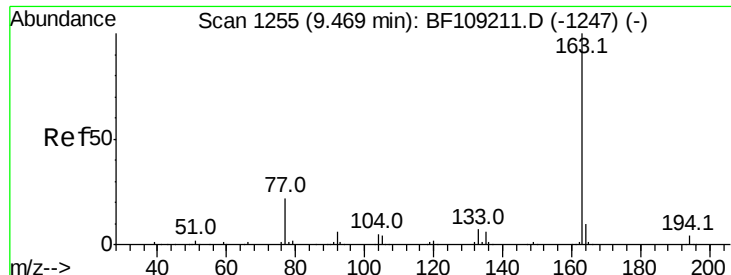




#49
 Dimethylphthalate
 Concen: 11.604 ng
 RT: 9.46 min Scan# 1253
 Delta R.T. -0.02 min
 Lab File: BF109354.D
 Acq: 26 Sep 2018 22:59

Instrument :
 BNA_F
 ClientSampleId :
 SLUDGE-B

Tot Ion:163 Resp: 101700
 Ion Ratio Lower Upper
 163 100
 194 3.8 2.7 4.1
 164 10.5 8.2 12.2

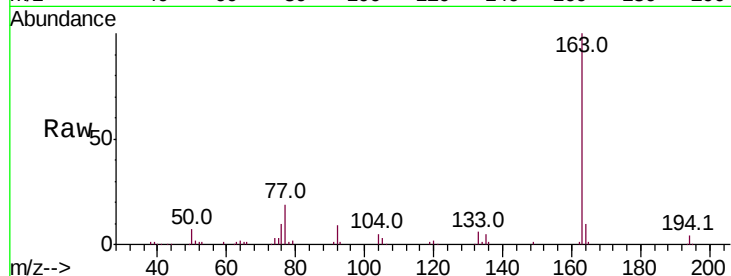


Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

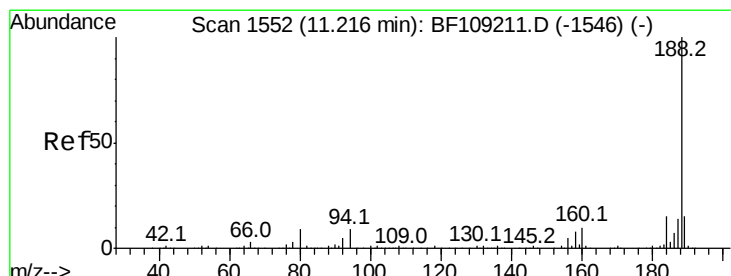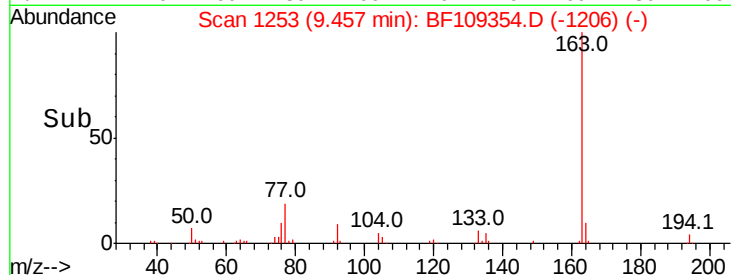
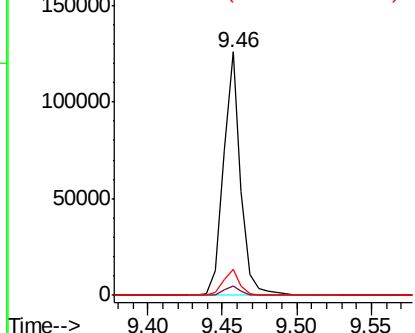



#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.22 min Scan# 1552
 Delta R.T. 0.00 min
 Lab File: BF109354.D
 Acq: 26 Sep 2018 22:59

Tgt Ion:188 Resp: 252947
 Ion Ratio Lower Upper
 188 100
 94 8.4 8.5 12.7#
 80 8.7 9.2 13.8#

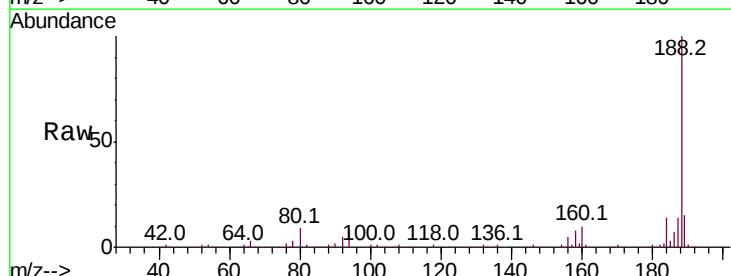

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF1
 Ion 80.00 (79.70 to 80.70): BF1

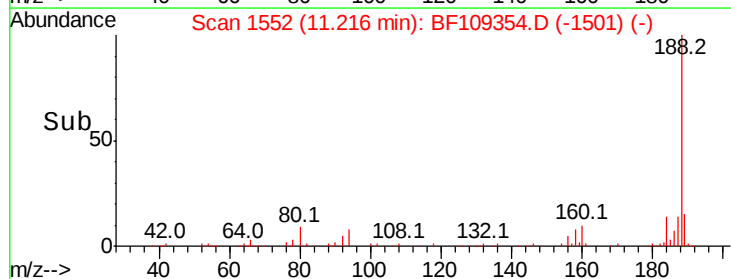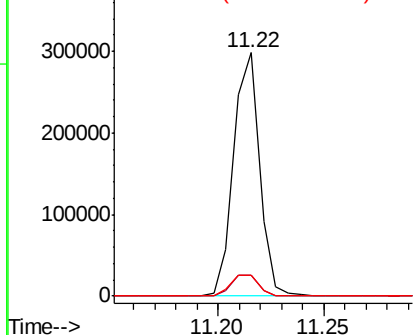

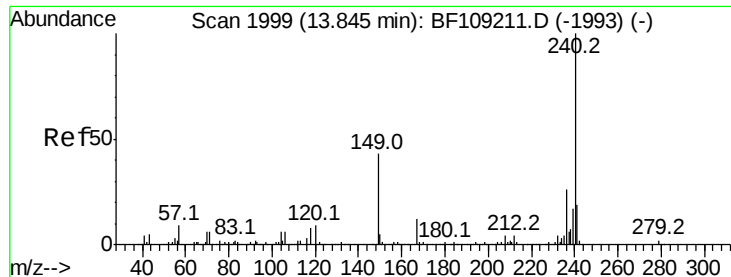

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.84 min Scan# 1998

Delta R.T. -0.01 min

Lab File: BF109354.D

Acq: 26 Sep 2018 22:59

Instrument :

BNA_F

ClientSampleId :

SLUDGE-B


Tot Ion:240 Resp: 281664

Ion Ratio Lower Upper

240 100

120 11.4 9.5 14.3




236 24.8 20.7 31.1

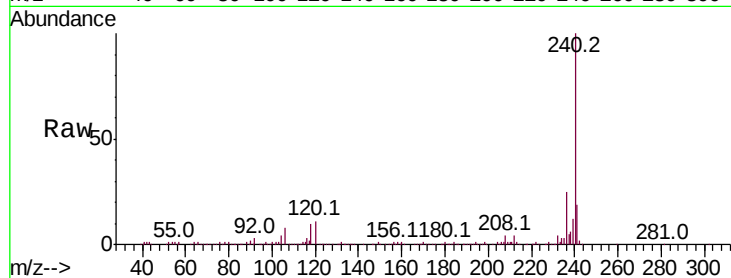

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

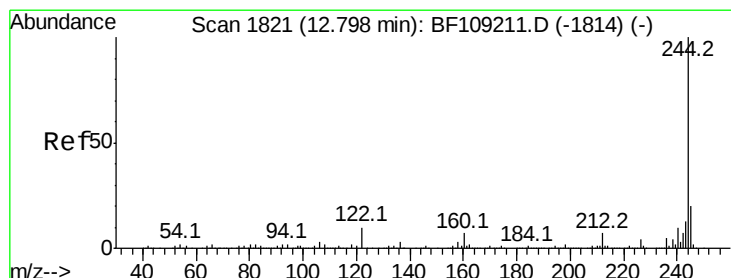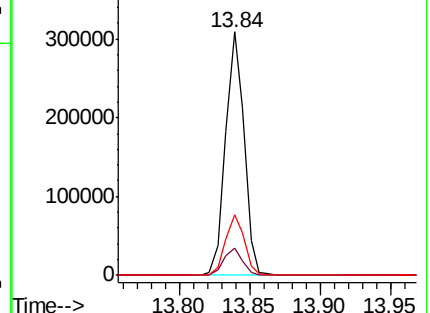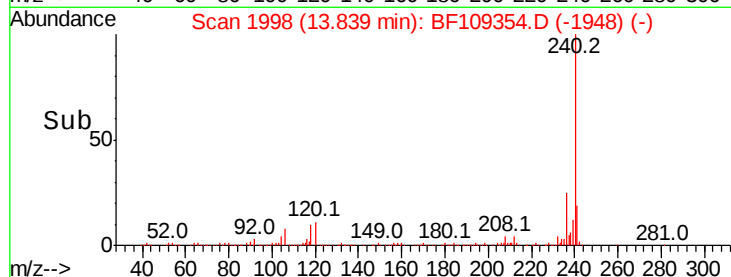

#78

Terphenyl-d14

Concen: 45.957 ng

RT: 12.79 min Scan# 1820

Delta R.T. -0.01 min

Lab File: BF109354.D

Acq: 26 Sep 2018 22:59


Tgt Ion:244 Resp: 527444

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0



122 12.5 11.0 16.4

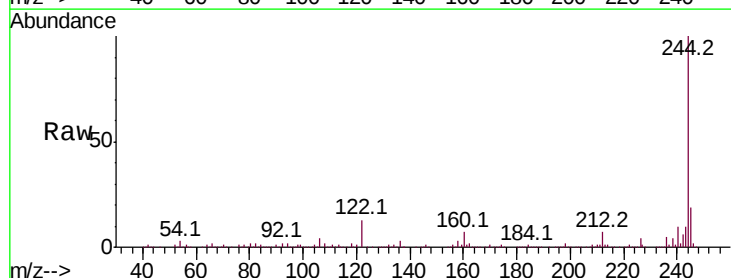


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

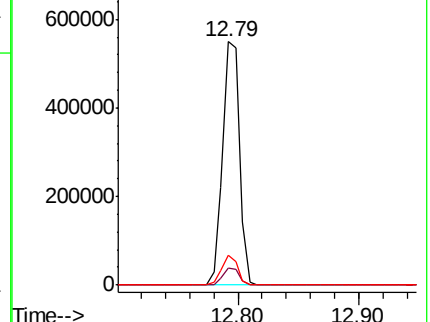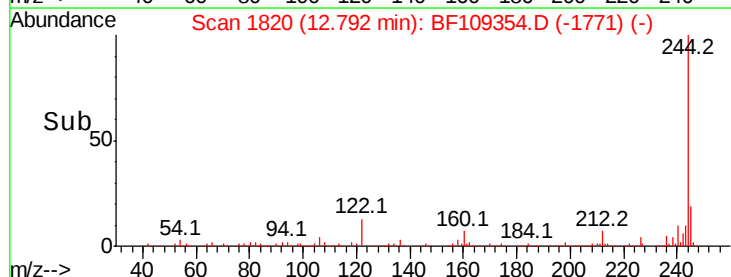


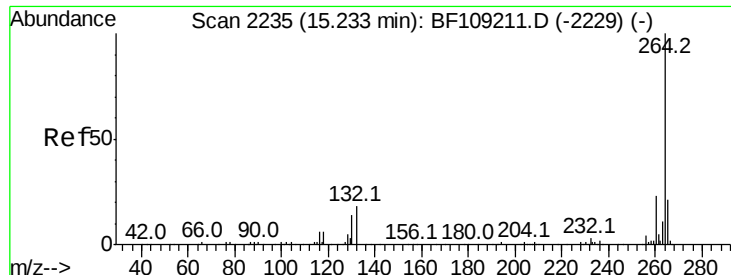

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.24 min Scan# 2237
 Delta R.T. 0.01 min
 Lab File: BF109354.D
 Acq: 26 Sep 2018 22:59

Instrument :
 BNA_F
 ClientSampleId :
 SLUDGE-B

Tot Ion:	264	Resp:	223532
Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.2	28.8
265	21.3	17.5	26.3

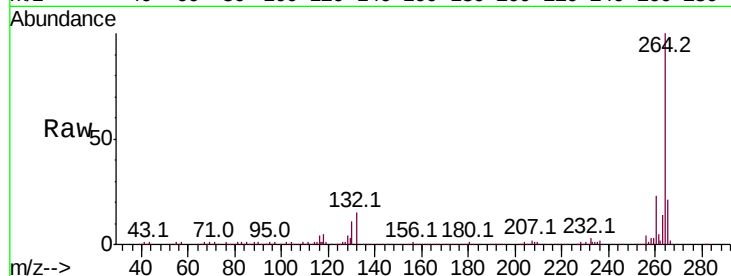

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

