

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092618\
 Data File : BF109354.D
 Acq On : 26 Sep 2018 22:59
 Operator : JU/SJ
 Sample : J5069-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SLUDGE-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.887	473	476	483	rBV	31822	34226	2.44%	0.284%
2	5.316	545	549	560	rBV	909346	897819	63.91%	7.444%
3	6.339	719	723	738	rBV	1091610	912432	64.95%	7.565%
4	6.475	742	746	749	rBV	1133421	920172	65.50%	7.630%
5	6.704	782	785	789	rBV	568644	494008	35.17%	4.096%
6	6.863	808	812	815	rBV	1322660	1055872	75.16%	8.755%
7	7.263	876	880	888	rBV	915886	805895	57.37%	6.682%
8	7.986	999	1003	1009	rBV	664323	561887	40.00%	4.659%
9	9.063	1182	1186	1189	rBV	1555673	1215502	86.53%	10.078%
10	9.457	1249	1253	1260	rBV	265550	213414	15.19%	1.770%
11	9.739	1297	1301	1304	rBV	599074	551296	39.24%	4.571%
12	10.522	1430	1434	1446	rBV	592947	535904	38.15%	4.443%
13	11.216	1548	1552	1555	rBV	708400	613011	43.64%	5.083%
14	11.751	1639	1643	1647	rBV3	26120	27090	1.93%	0.225%
15	12.421	1753	1757	1760	rBV	46577	42643	3.04%	0.354%
16	12.645	1790	1795	1799	rBV	46035	55130	3.92%	0.457%
17	12.792	1816	1820	1824	rBV	1500282	1404781	100.00%	11.648%
18	13.710	1972	1976	1981	rBV3	15828	25612	1.82%	0.212%
19	13.839	1994	1998	2001	rBV	839161	791501	56.34%	6.563%
20	13.863	2001	2002	2007	rVB	25694	19654	1.40%	0.163%
21	14.027	2027	2030	2034	rVB4	15359	16448	1.17%	0.136%
22	14.327	2078	2081	2083	rBV2	22063	21645	1.54%	0.179%
23	14.621	2128	2131	2135	rBV	27508	27041	1.92%	0.224%
24	14.686	2140	2142	2145	rVB	24994	22215	1.58%	0.184%
25	14.845	2167	2169	2176	rVB	24715	38506	2.74%	0.319%
26	14.933	2181	2184	2188	rBV2	30044	34058	2.42%	0.282%
27	15.121	2213	2216	2219	rVB4	18849	22311	1.59%	0.185%
28	15.180	2224	2226	2232	rVV3	19037	35344	2.52%	0.293%
29	15.245	2232	2237	2241	rVV	489733	599678	42.69%	4.972%
30	15.286	2242	2244	2249	rVB3	28054	35669	2.54%	0.296%
31	15.686	2309	2312	2317	rBV4	23750	29743	2.12%	0.247%


Sum of corrected areas: 12060507

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092618\
Data File : BF109354.D
Acq On : 26 Sep 2018 22:59
Operator : JU/SJ
Sample : J5069-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLUDGE-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

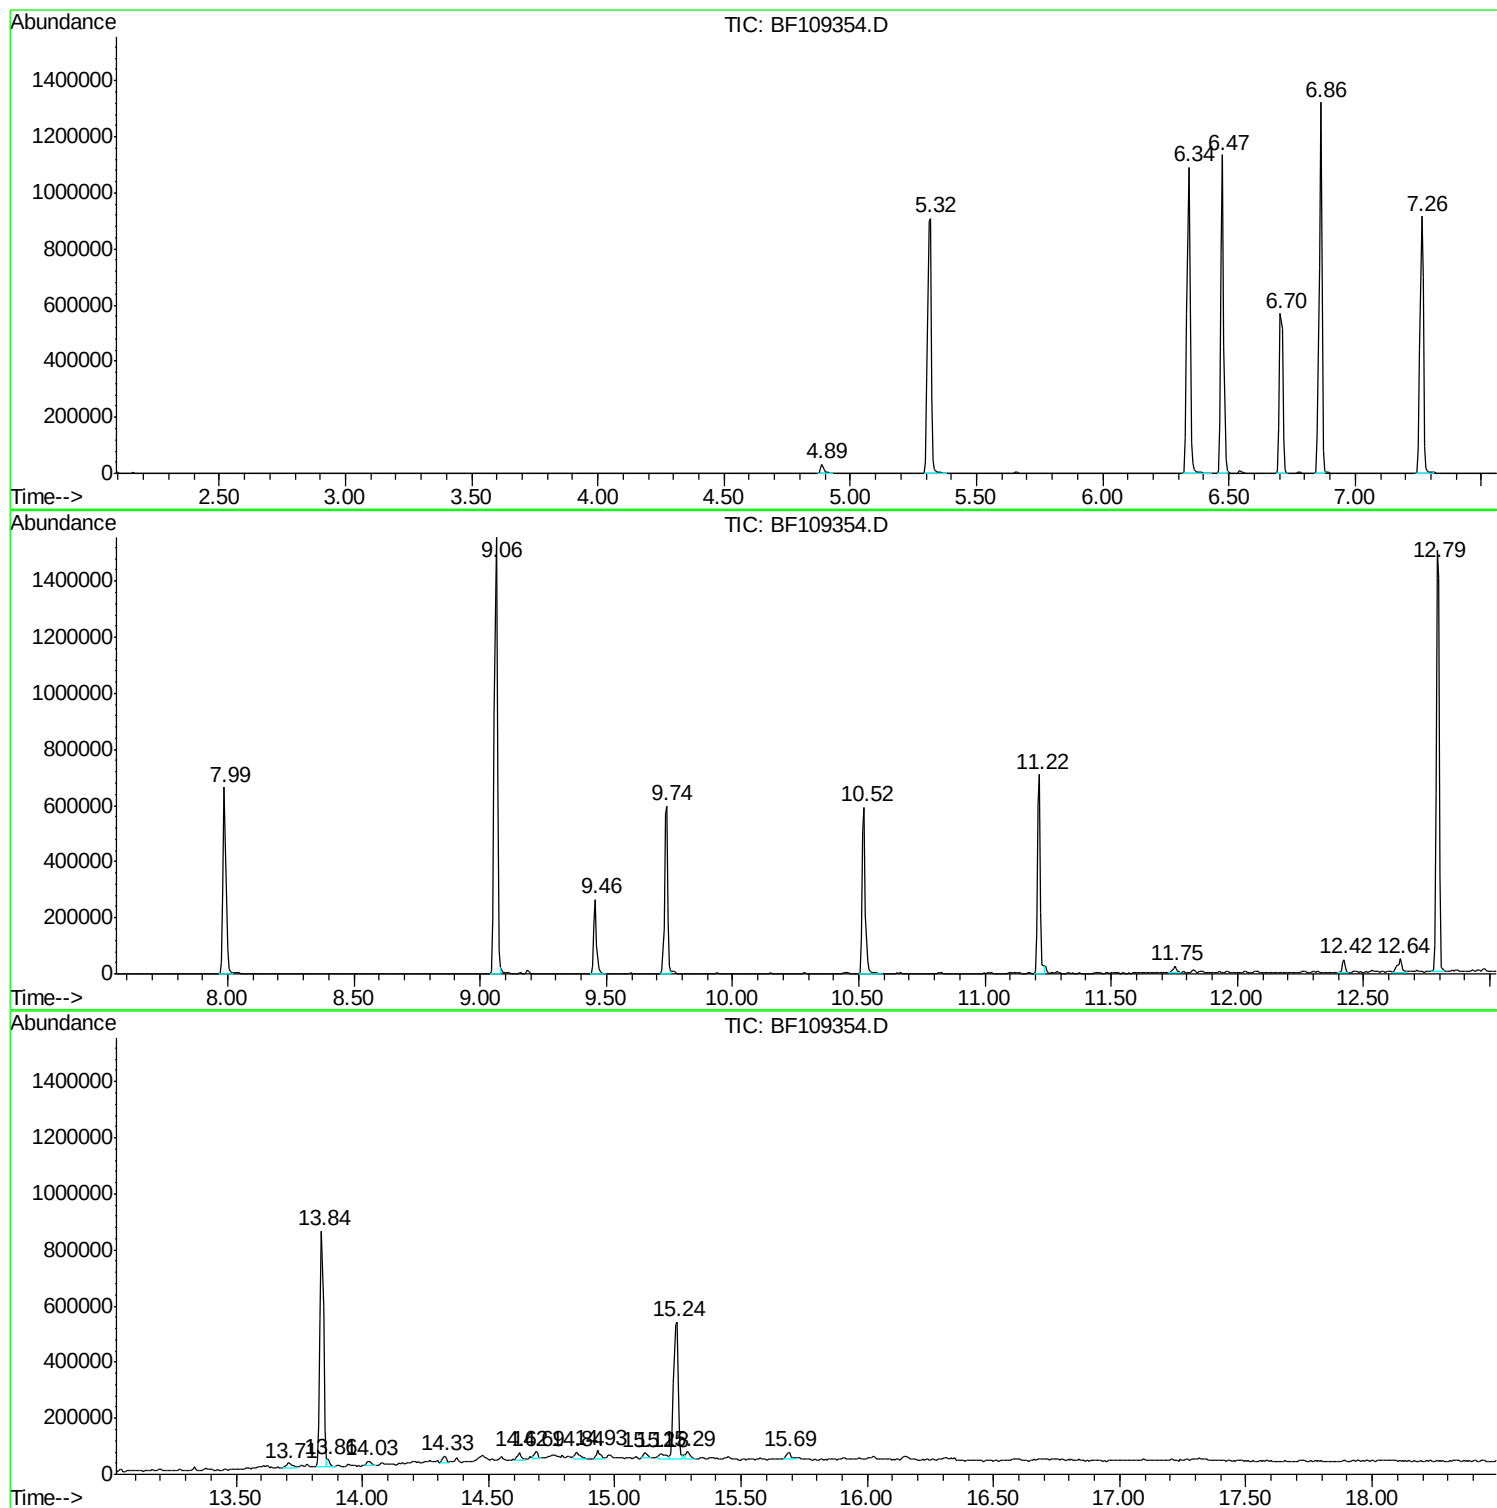

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092618\
Data File : BF109354.D
Acq On : 26 Sep 2018 22:59
Operator : JU/SJ
Sample : J5069-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLUDGE-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.47 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.47	37.25 ng	920172	1,4-Dichlorobenzene-d4	6.70

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	16
2	Bicyclo[4.2.0]octa-1,3,5-triene,...			132	C10H12	028749-81-7	9
3	(E)-3-Chloro-2-methyl-2-pentenal			132	C6H9ClO	031357-76-3	9
4	4-Chloro-6-fluoro-pyrimidine			132	C4H2ClFN2	051422-01-6	9
5	Imidazole, 4,5-dicyano-1-methyl-			132	C6H4N4	019485-35-9	9

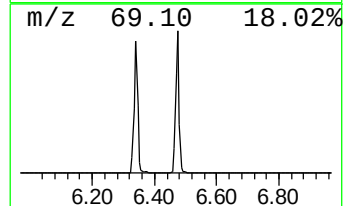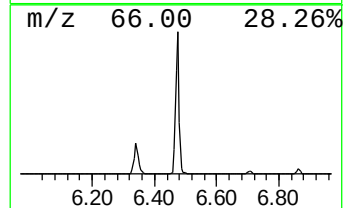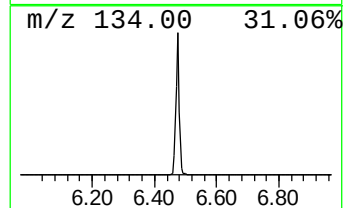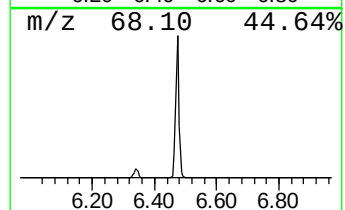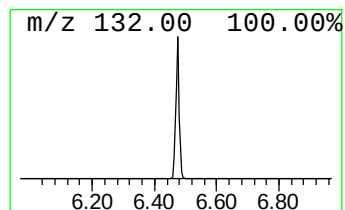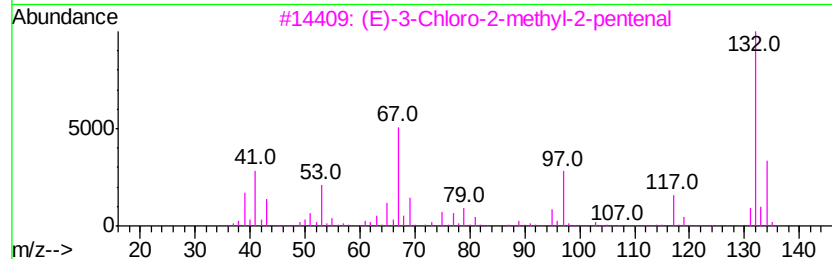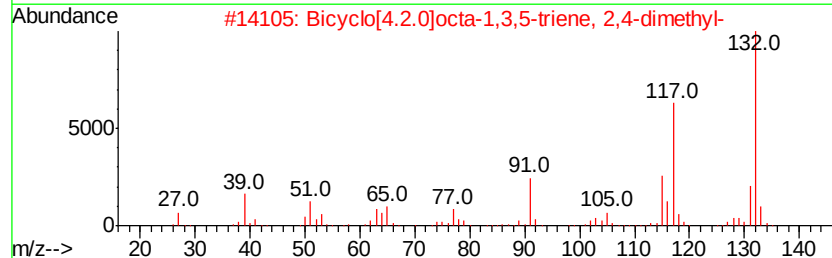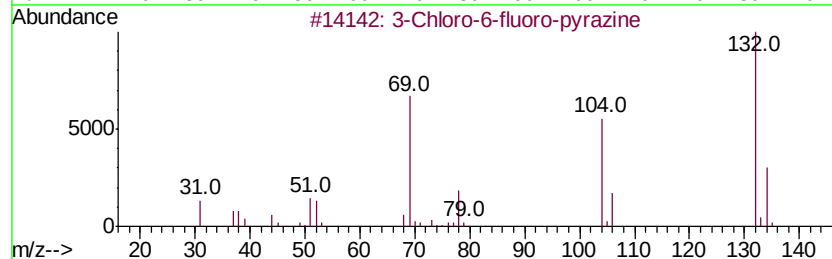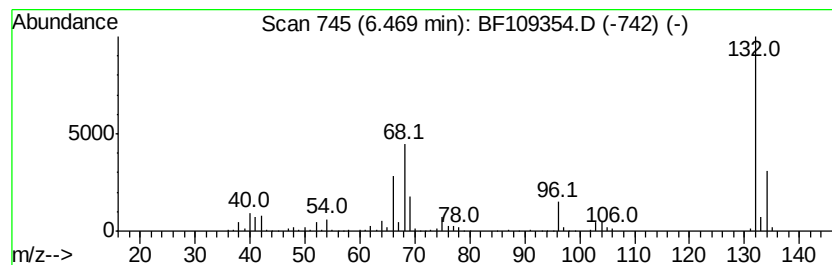

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092618\
Data File : BF109354.D
Acq On : 26 Sep 2018 22:59
Operator : JU/SJ
Sample : J5069-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SLUDGE-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.47	6.47	37.3	ng	920172	1	6.70	494008	20.0