


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092716\
 Data File : BF090248.D
 Acq On : 27 Sep 2016 13:11
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 26 15:58:38 2016

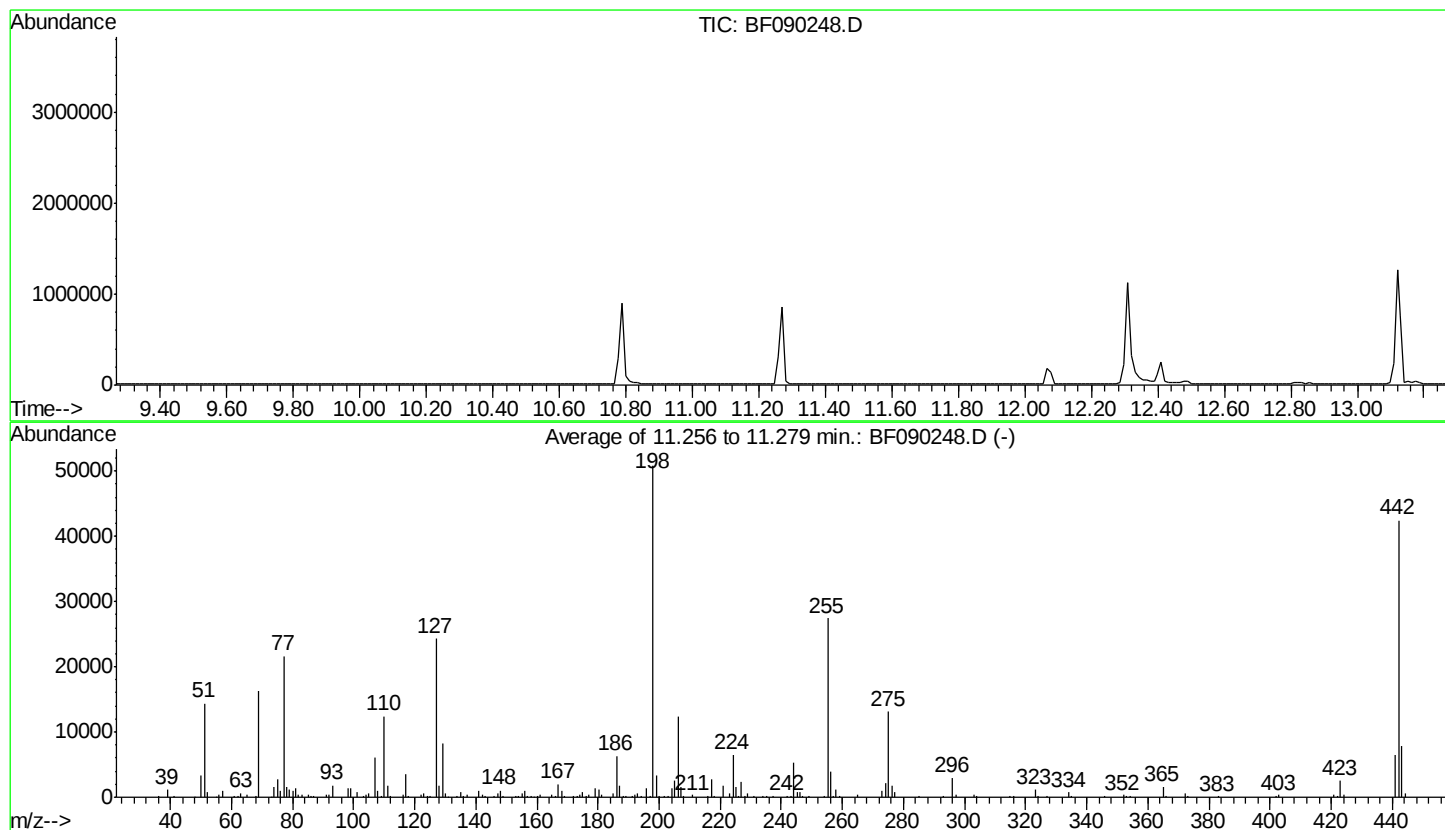

AutoFind: Scans 846, 847, 848; Background Corrected with Scan 842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	14373	PASS
68	69	0.00	2	1.5	251	PASS
69	198	0.00	100	31.9	16224	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.8	24274	PASS
197	198	0.00	2	0.5	230	PASS
198	198	100	100	100.0	50830	PASS
199	198	5	9	6.5	3329	PASS
275	198	10	60	25.7	13074	PASS
365	198	1	100	3.2	1615	PASS
441	442	0.01	24	15.4	6551	PASS
442	198	50	100	83.5	42466	PASS
443	442	15	24	18.5	7869	PASS