
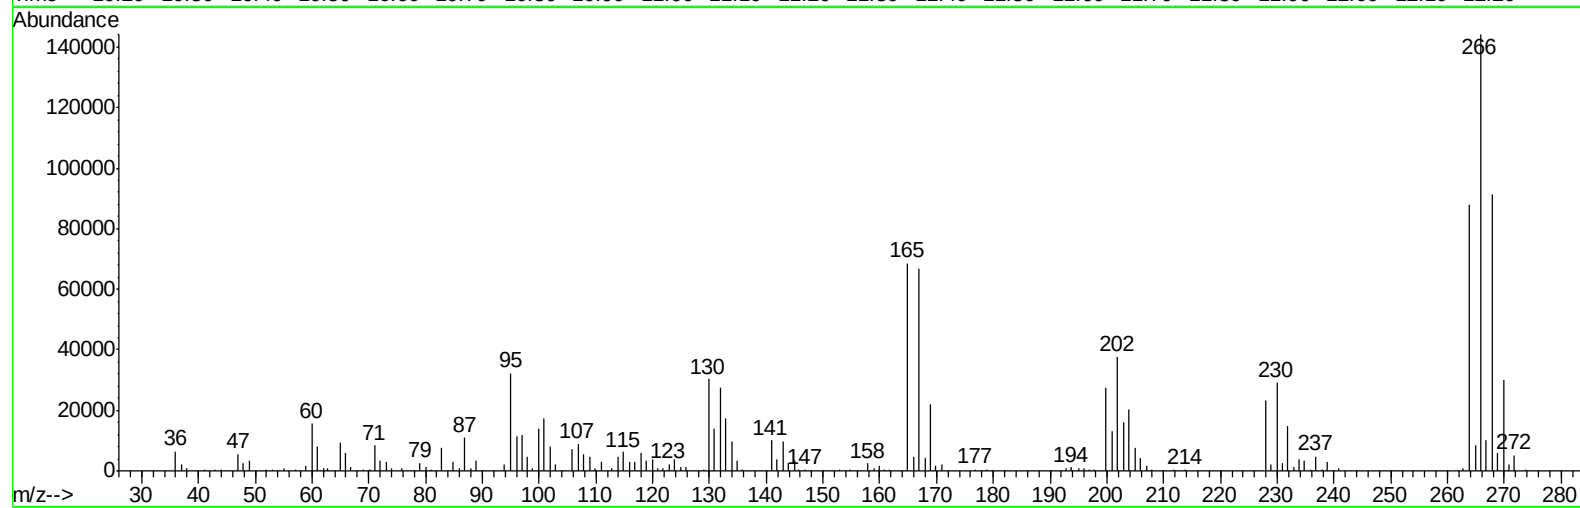


Data Path : Z:\HPCHEM1\BNA F\DATA\BF092717\
Data File : BF098865.D
Acq On : 27 Sep 2017 16:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 09:07:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

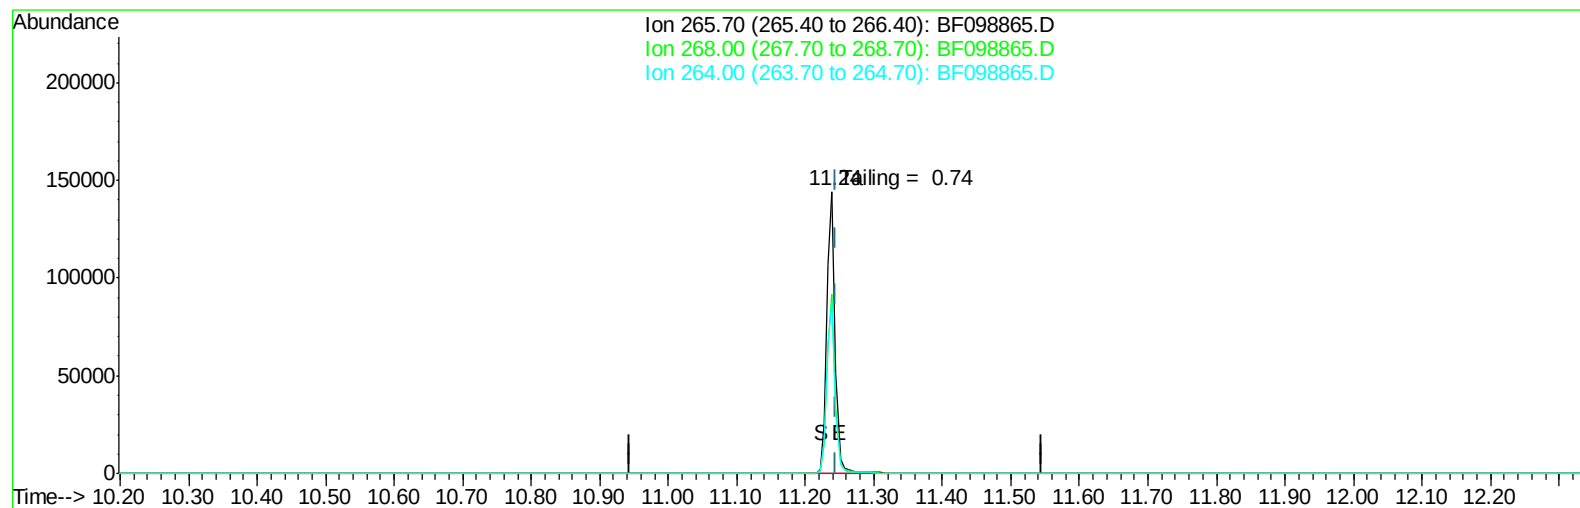

TIC: BF098865.D

(69) Pentachlorophenol (C)



11.239min (-0.006) 50085.06ng

response 122854

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.44
264.00	61.90	61.04
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF092717\
Data File : BF098865.D
Acq On : 27 Sep 2017 16:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 09:07:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

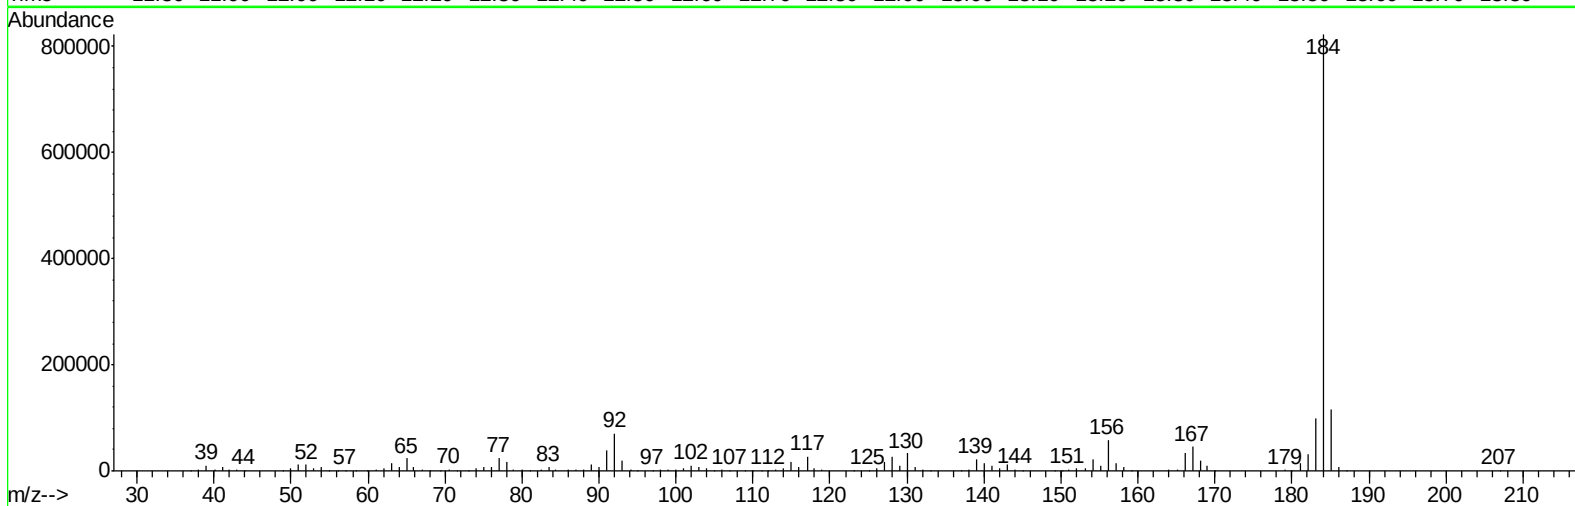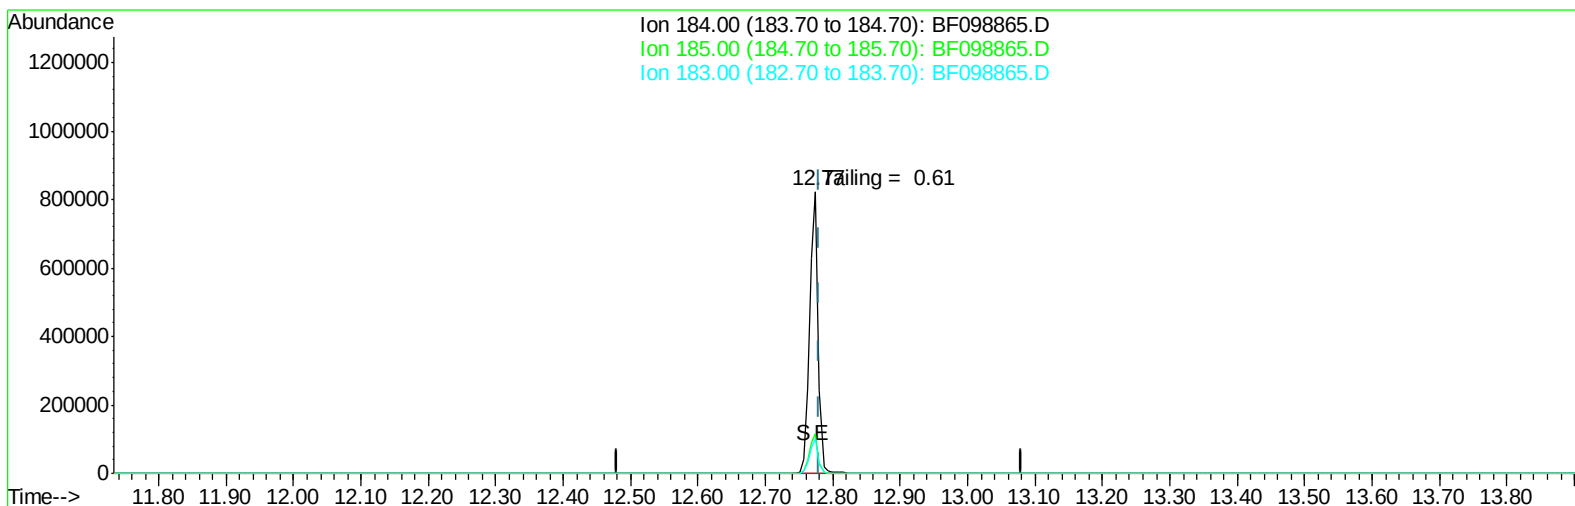

TIC: BF098865.D

(76) Benzidine

12.774min (-0.006) 0.00ng

response 718529

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.09
183.00	11.60	12.07
0.00	0.00	0.00