

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092717\
 Data File : BF098854.D
 Acq On : 27 Sep 2017 11:00
 Operator : SJ/JU
 Sample : I5363-09 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SP-3-E-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.187	14	17	24	rVB3	13854	21616	1.58%	0.167%
2	5.128	513	517	524	rBV	71833	77417	5.67%	0.598%
3	5.398	559	563	568	rBV	22624	21066	1.54%	0.163%
4	5.522	580	584	587	rBV	579377	476168	34.87%	3.679%
5	6.528	751	755	762	rBV	561058	495898	36.32%	3.832%
6	6.675	777	780	784	rBV	642685	521265	38.18%	4.028%
7	6.916	817	821	824	rVB	997425	900030	65.92%	6.955%
8	7.069	843	847	850	rBV	472149	393269	28.80%	3.039%
9	7.469	911	915	918	rBV	382295	297641	21.80%	2.300%
10	8.198	1034	1039	1045	rVB	1394069	1340565	98.18%	10.359%
11	8.904	1156	1159	1163	rVB	40631	31395	2.30%	0.243%
12	9.004	1173	1176	1179	rBV	22664	18456	1.35%	0.143%
13	9.263	1217	1220	1224	rBV	720783	618456	45.30%	4.779%
14	9.533	1261	1266	1269	rBV3	12767	16943	1.24%	0.131%
15	9.657	1285	1287	1291	rVB	62839	50735	3.72%	0.392%
16	9.810	1311	1313	1316	rBV	22193	20454	1.50%	0.158%
17	9.951	1331	1337	1341	rBV	1637107	1365390	100.00%	10.551%
18	9.980	1341	1342	1346	rVB	31009	22456	1.64%	0.174%
19	10.151	1368	1371	1375	rVB2	33185	28997	2.12%	0.224%
20	10.498	1426	1430	1433	rBV	25797	24512	1.80%	0.189%
21	10.733	1467	1470	1474	rBV	382321	314415	23.03%	2.430%
22	10.857	1486	1491	1494	rBV3	34328	46855	3.43%	0.362%
23	11.086	1528	1530	1534	rVB5	13681	16292	1.19%	0.126%
24	11.204	1547	1550	1553	rVB3	15154	17961	1.32%	0.139%
25	11.239	1553	1556	1559	rBV	18338	16597	1.22%	0.128%
26	11.292	1559	1565	1567	rBV3	41169	37658	2.76%	0.291%
27	11.333	1567	1572	1574	rVV2	11996	17047	1.25%	0.132%
28	11.439	1586	1590	1592	rBV	1550522	1309713	95.92%	10.120%
29	11.457	1592	1593	1597	rVV	186754	150717	11.04%	1.165%
30	11.510	1600	1602	1605	rVV	53795	39651	2.90%	0.306%
31	11.639	1622	1624	1627	rBV4	15748	21182	1.55%	0.164%
32	11.663	1627	1628	1632	rVB	25609	19604	1.44%	0.151%
33	11.816	1651	1654	1656	rBV	26410	20850	1.53%	0.161%
34	11.963	1672	1679	1682	rBV4	42693	104137	7.63%	0.805%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092717\
Data File : BF098854.D
Acq On : 27 Sep 2017 11:00
Operator : SJ/JU
Sample : I5363-09 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-3-E-COMPRES

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.051	1690	1694	1695	rBV2	32275	35166	2.58%	0.272%
36	12.233	1722	1725	1727	rBV	60121	48099	3.52%	0.372%
37	12.380	1747	1750	1752	rBV	57855	40098	2.94%	0.310%
38	12.486	1766	1768	1770	rVB	22323	18192	1.33%	0.141%
39	12.568	1780	1782	1787	rVB3	17368	18764	1.37%	0.145%
40	12.651	1793	1796	1799	rVB	262716	222512	16.30%	1.719%
41	12.692	1800	1803	1805	rBV4	17656	18528	1.36%	0.143%
42	12.833	1824	1827	1829	rVB	27445	23811	1.74%	0.184%
43	12.857	1829	1831	1832	rBV	42495	32870	2.41%	0.254%
44	12.880	1832	1835	1841	rVB	213805	212879	15.59%	1.645%
45	13.015	1855	1858	1865	rVB	632819	559821	41.00%	4.326%
46	13.157	1879	1882	1884	rBV	40449	36050	2.64%	0.279%
47	13.204	1888	1890	1894	rVB	41192	38641	2.83%	0.299%
48	13.268	1899	1901	1904	rBV2	23321	25710	1.88%	0.199%
49	13.880	2002	2005	2006	rBV	34064	37809	2.77%	0.292%
50	14.074	2034	2038	2041	rBV	953696	911761	66.78%	7.045%
51	14.098	2041	2042	2047	rVB	103131	90430	6.62%	0.699%
52	14.210	2058	2061	2062	rBV2	39134	39483	2.89%	0.305%
53	14.245	2065	2067	2070	rVB	48619	46240	3.39%	0.357%
54	15.127	2213	2217	2224	rVB	99247	184254	13.49%	1.424%
55	15.433	2267	2269	2275	rVB	65026	81489	5.97%	0.630%
56	15.498	2278	2280	2287	rVV	68662	100914	7.39%	0.780%
57	15.568	2287	2292	2304	rVB	658258	890301	65.20%	6.879%
58	17.121	2551	2556	2572	rVB4	135479	352170	25.79%	2.721%


Sum of corrected areas: 12941400

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092717\
Data File : BF098854.D
Acq On : 27 Sep 2017 11:00
Operator : SJ/JU
Sample : I5363-09 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SP-3-E-COMPRE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

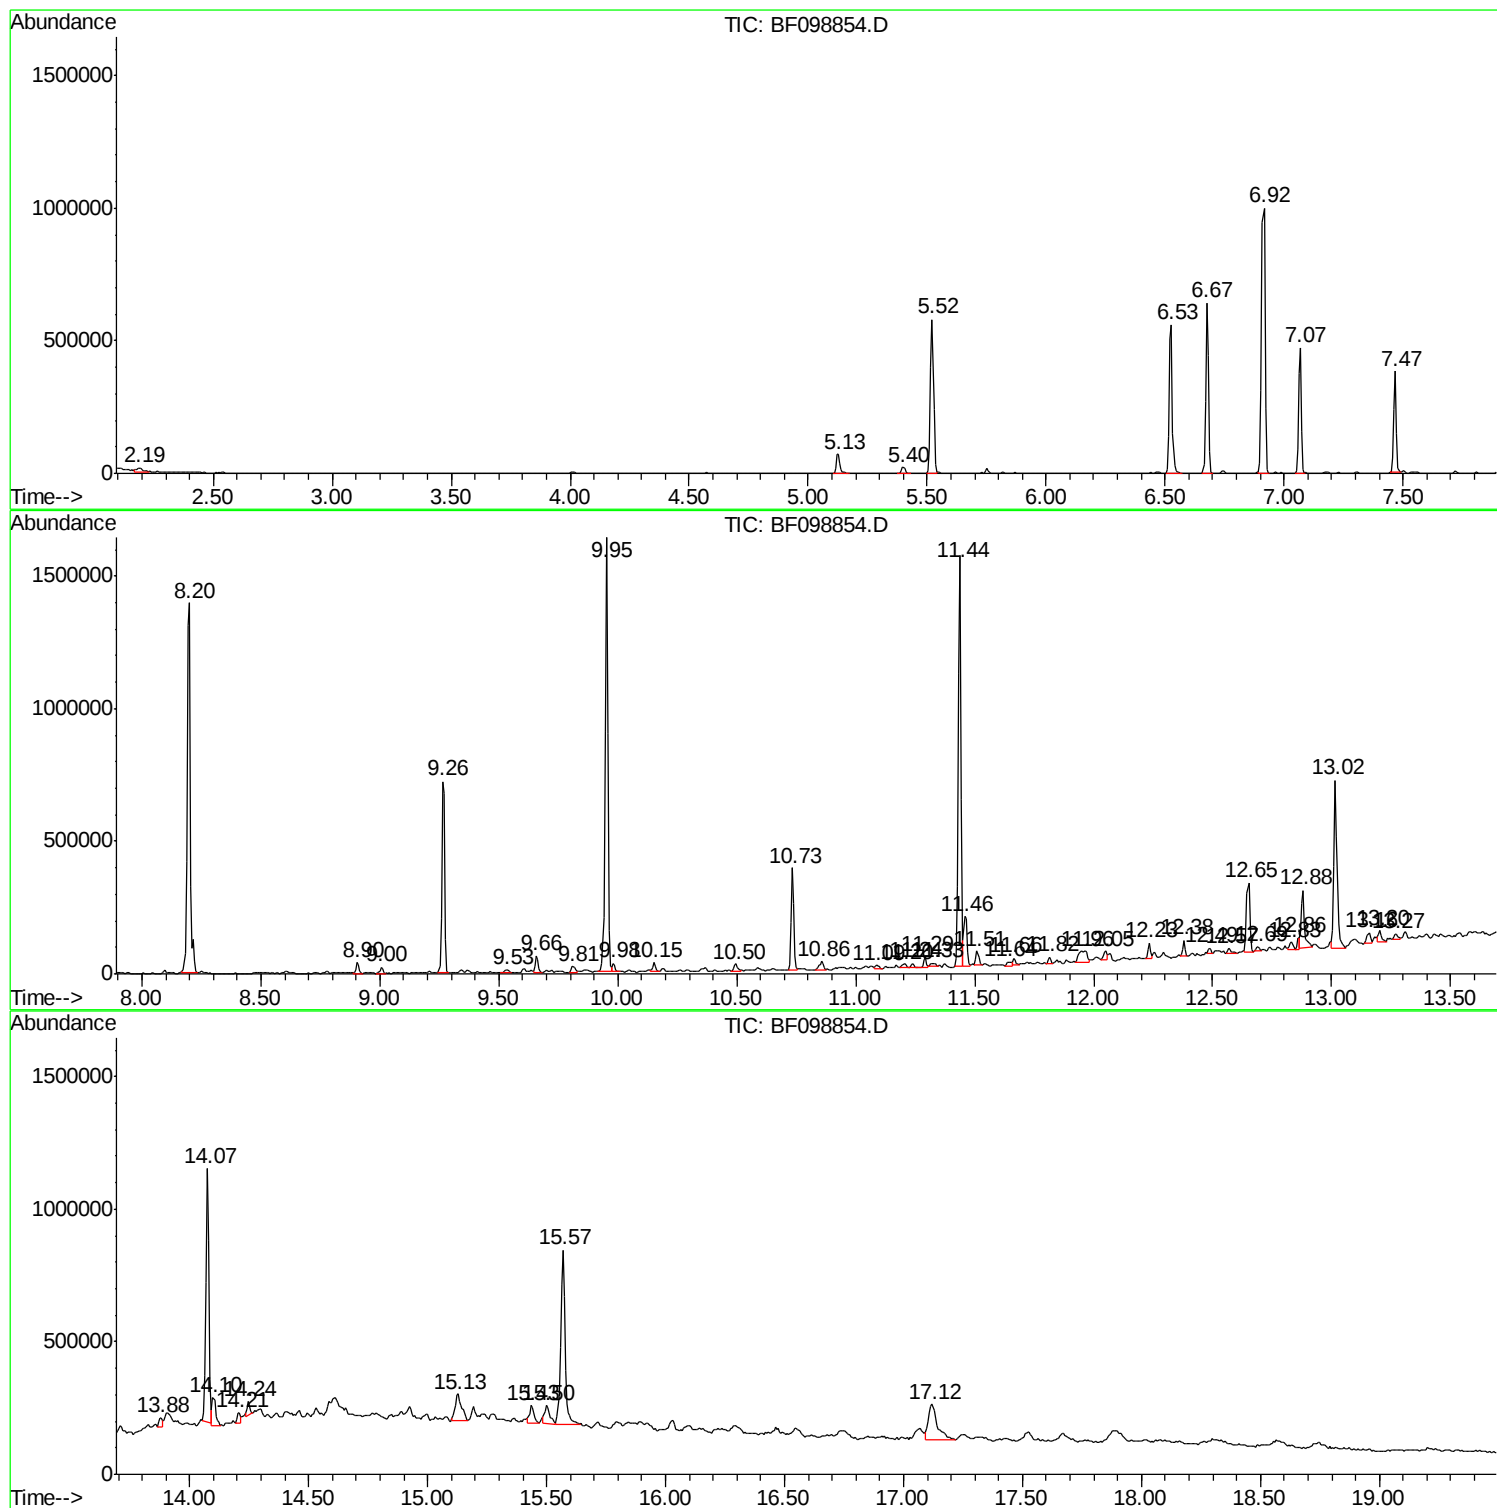

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF092717\
Data_File : BF098854.D
Acq_On : 27-Sep-2017 11:000
Operator : SJ/JUU
Sample : I5363-09-10XX
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SP-3-E-COMPRES

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
