


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092717\
 Data File : BF098865.D
 Acq On : 27 Sep 2017 16:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

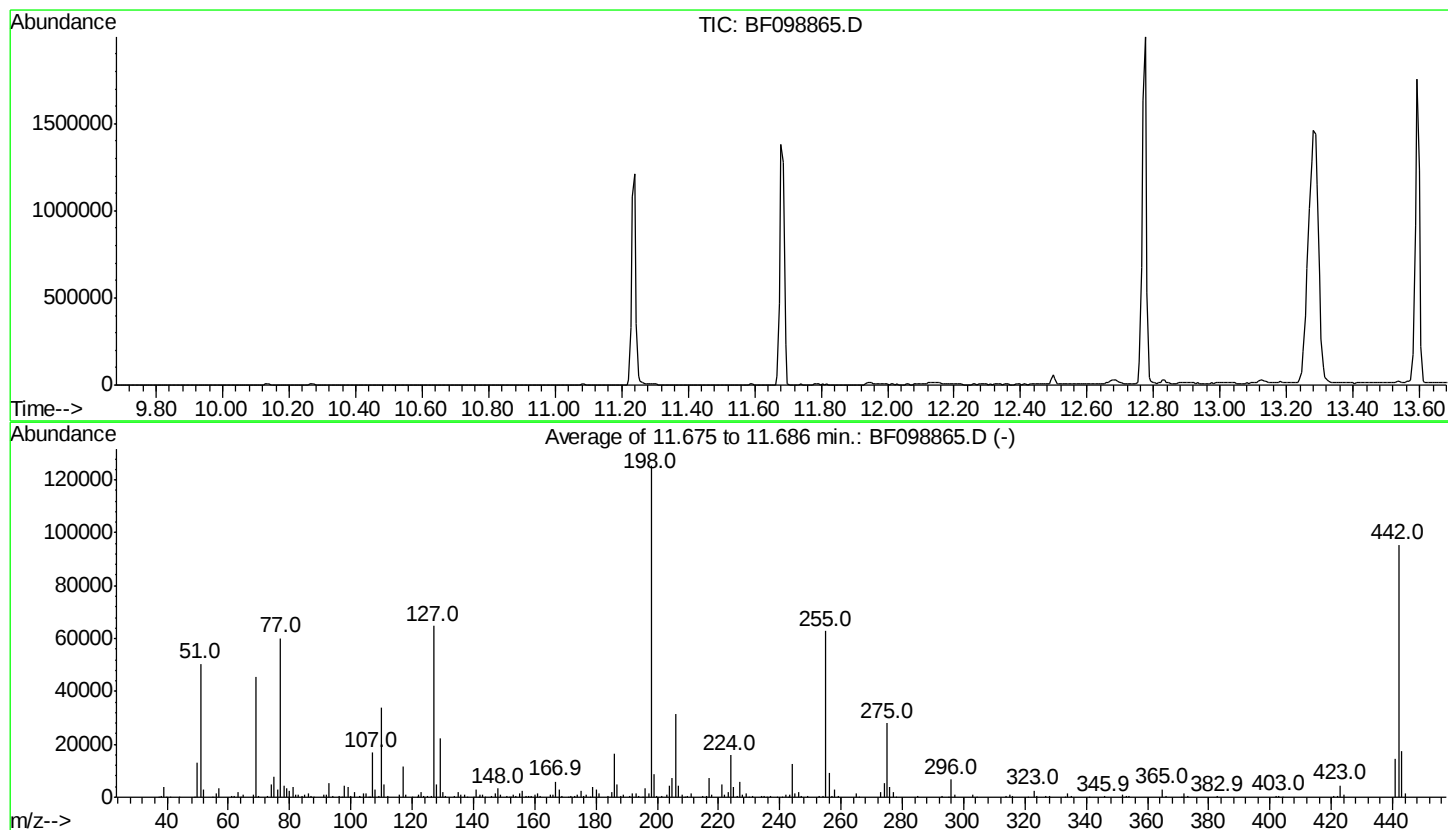

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	50546	PASS
68	69	0.00	2	1.7	784	PASS
69	198	0.00	100	36.2	45323	PASS
70	69	0.00	2	0.6	274	PASS
127	198	10	80	51.7	64784	PASS
197	198	0.00	2	1.1	1347	PASS
198	198	100	100	100.0	125357	PASS
199	198	5	9	6.8	8522	PASS
275	198	10	60	22.4	28045	PASS
365	198	1	100	2.4	3042	PASS
441	442	0.01	24	15.2	14470	PASS
442	198	50	100	76.1	95426	PASS
443	442	15	24	18.4	17541	PASS