
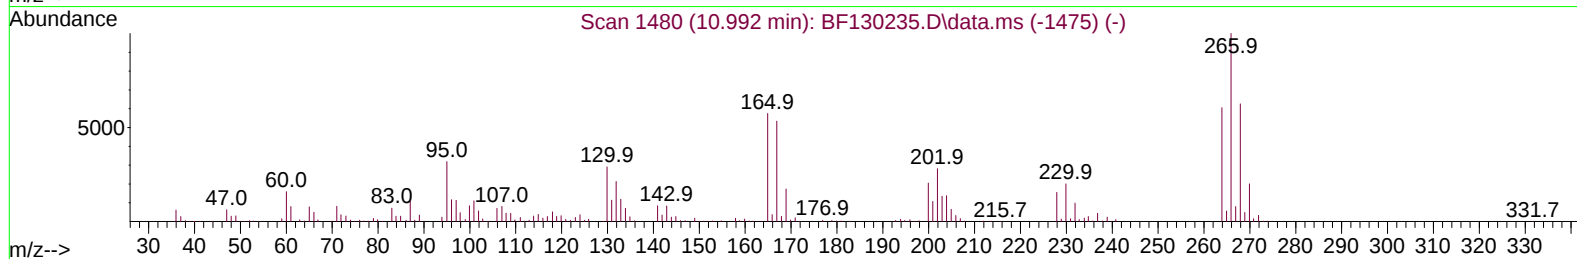
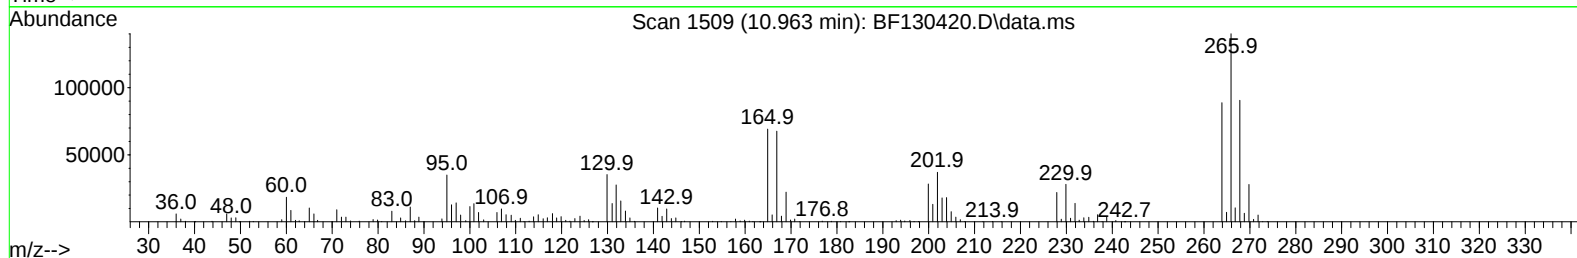


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092722\
Data File : BF130420.D
Acq On : 27 Sep 2022 11:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 19:04:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 27 01:00:47 2022
Response via : Initial Calibration

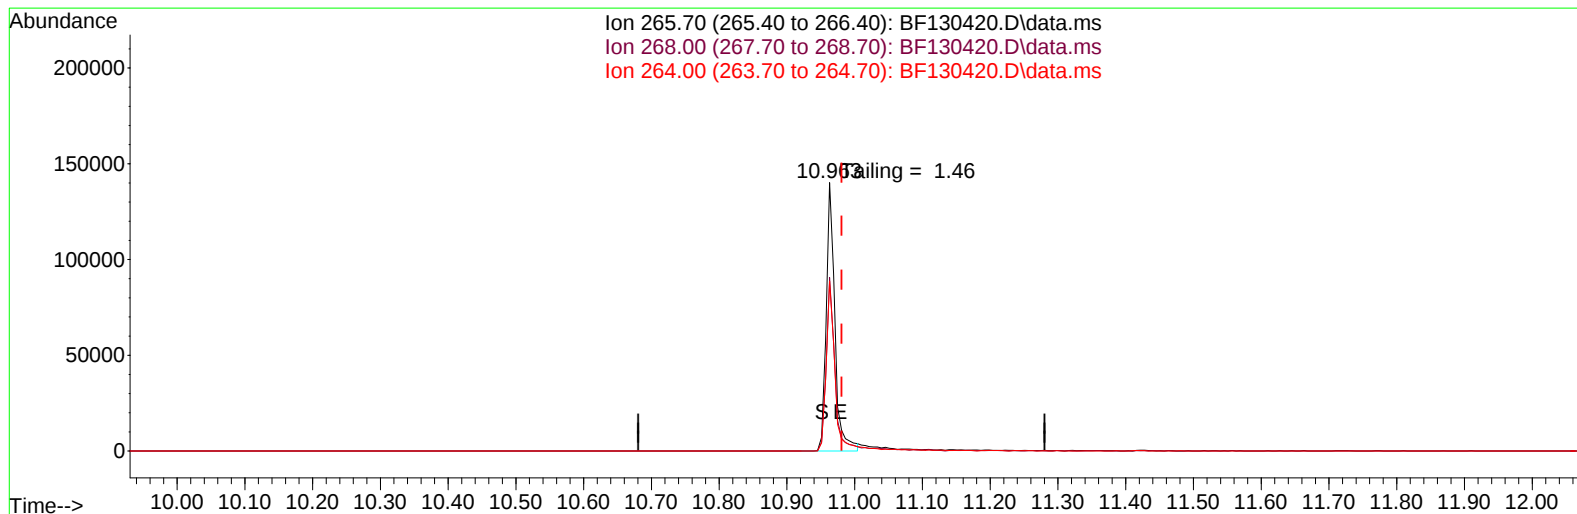

TIC: BF130420.D\data.ms

(70) Pentachlorophenol (C)




10.963min (-0.018) 24230.41 ng

response 131233

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.63
264.00	63.10	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092722\
Data File : BF130420.D
Acq On : 27 Sep 2022 11:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 27 19:04:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 27 01:00:47 2022
Response via : Initial Calibration

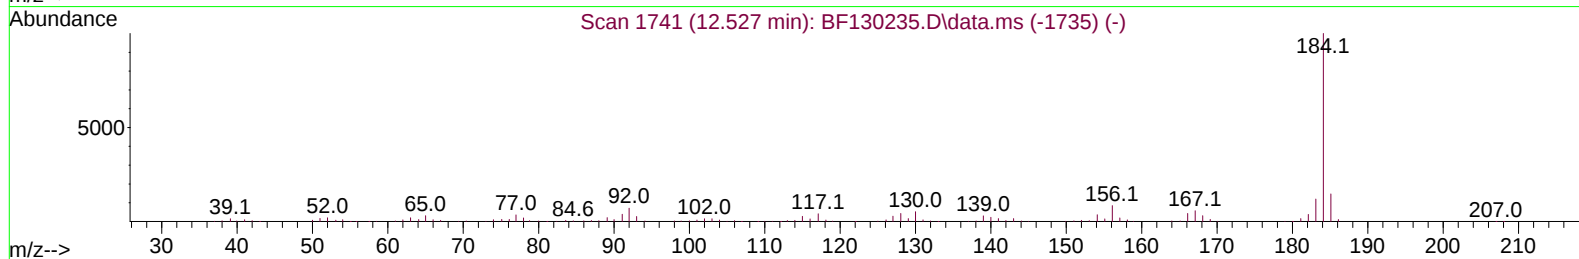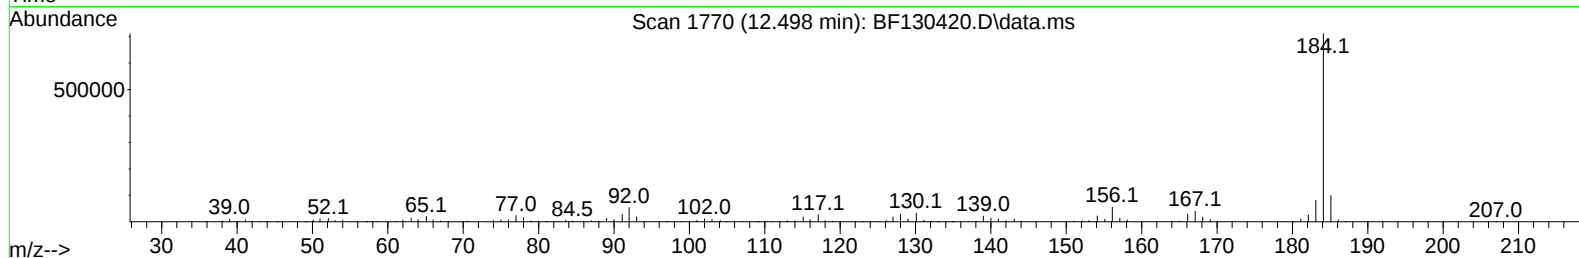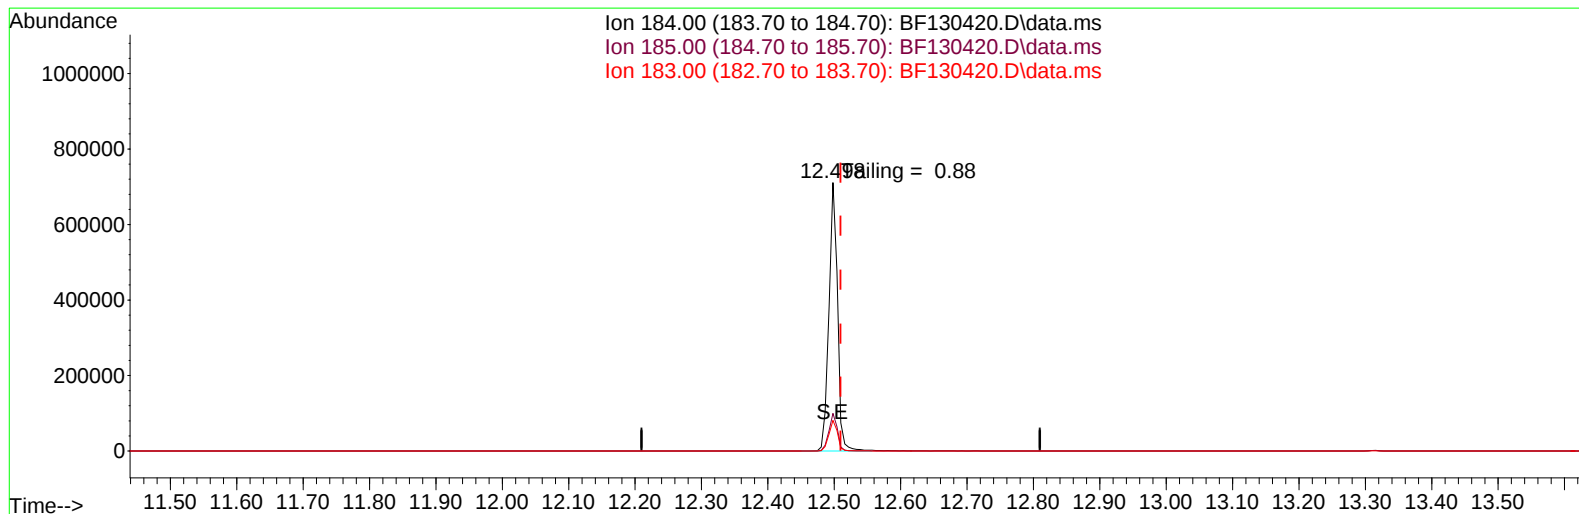

TIC: BF130420.D\data.ms

(77) Benzidine

12.498min (-0.012) 0.00 ng

response 642494

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.00
183.00	11.40	11.43
0.00	0.00	0.00