

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092722\
 Data File : BF130422.D
 Acq On : 27 Sep 2022 13:19
 Operator : CG\JU
 Sample : PB147890BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147890BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.851	466	470	481	rBV	36140	52958	1.39%	0.238%
2	5.257	533	539	542	rBV	2752143	2894792	76.17%	13.034%
3	6.287	708	714	717	rBV	2718184	2831022	74.49%	12.747%
4	6.640	771	774	778	rBV	707640	595255	15.66%	2.680%
5	7.210	865	871	874	rBV	1926010	1904967	50.12%	8.577%
6	7.922	987	992	996	rBV	843394	809385	21.30%	3.644%
7	9.004	1169	1176	1179	rBV	4235609	3800454	100.00%	17.112%
8	9.675	1285	1290	1293	rBV	1149060	928930	24.44%	4.183%
9	10.463	1418	1424	1427	rBV	2805284	2421260	63.71%	10.902%
10	11.157	1537	1542	1545	rBV	966697	908474	23.90%	4.091%
11	12.745	1807	1812	1815	rBV	4246875	3722554	97.95%	16.762%
12	13.786	1984	1989	1992	rBV	645247	623921	16.42%	2.809%
13	13.886	2000	2006	2014	rBV	46468	54287	1.43%	0.244%
14	15.168	2219	2224	2228	rBV	426168	481213	12.66%	2.167%
15	15.598	2292	2297	2305	rVB2	30466	44437	1.17%	0.200%
16	16.051	2369	2374	2380	rVB3	27845	46894	1.23%	0.211%
17	16.580	2458	2464	2471	rVB3	22552	47670	1.25%	0.215%
18	17.198	2564	2569	2577	rVB5	16993	40482	1.07%	0.182%




Sum of corrected areas: 22208955

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092722\
Data File : BF130422.D
Acq On : 27 Sep 2022 13:19
Operator : CG\JU
Sample : PB147890BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147890BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

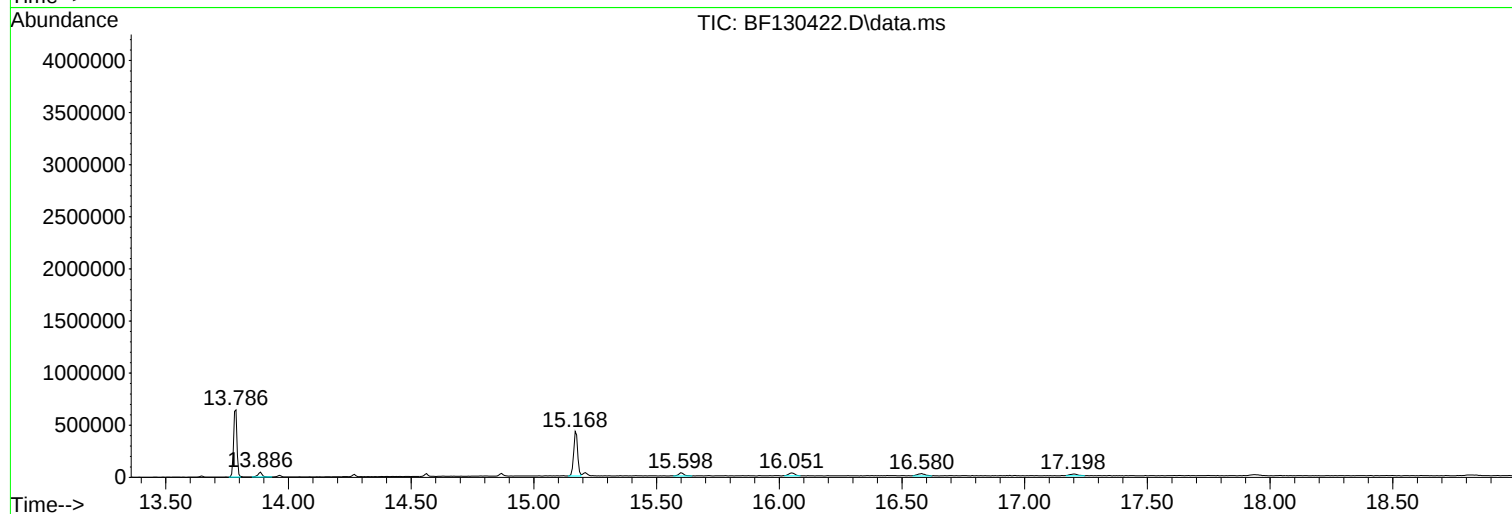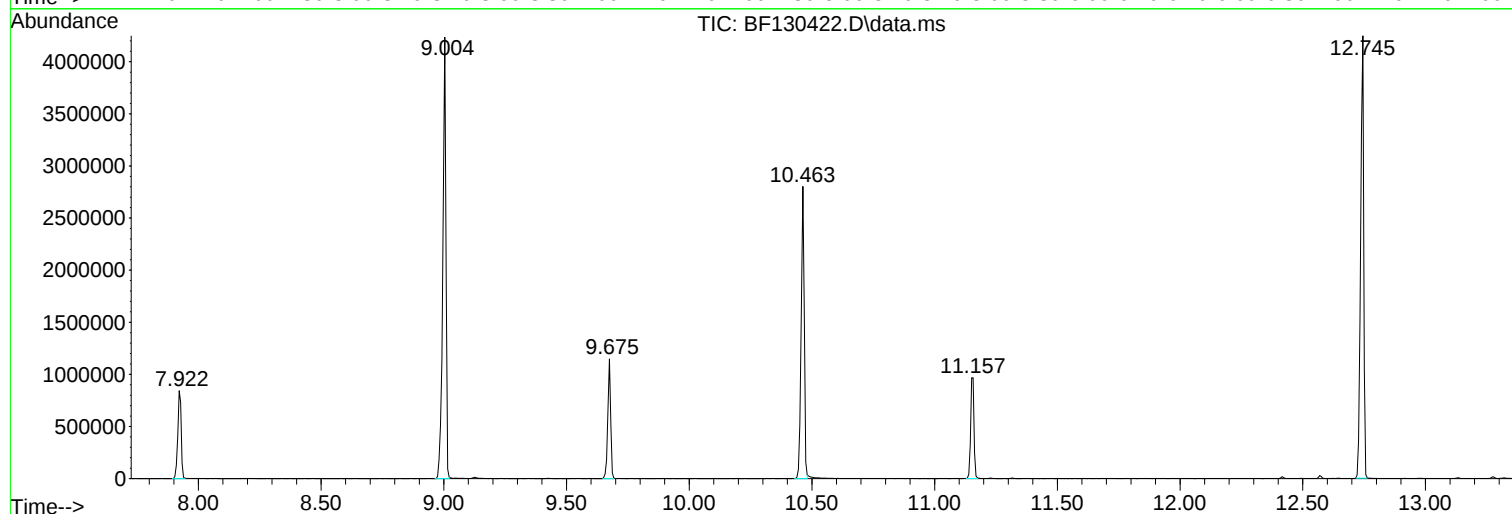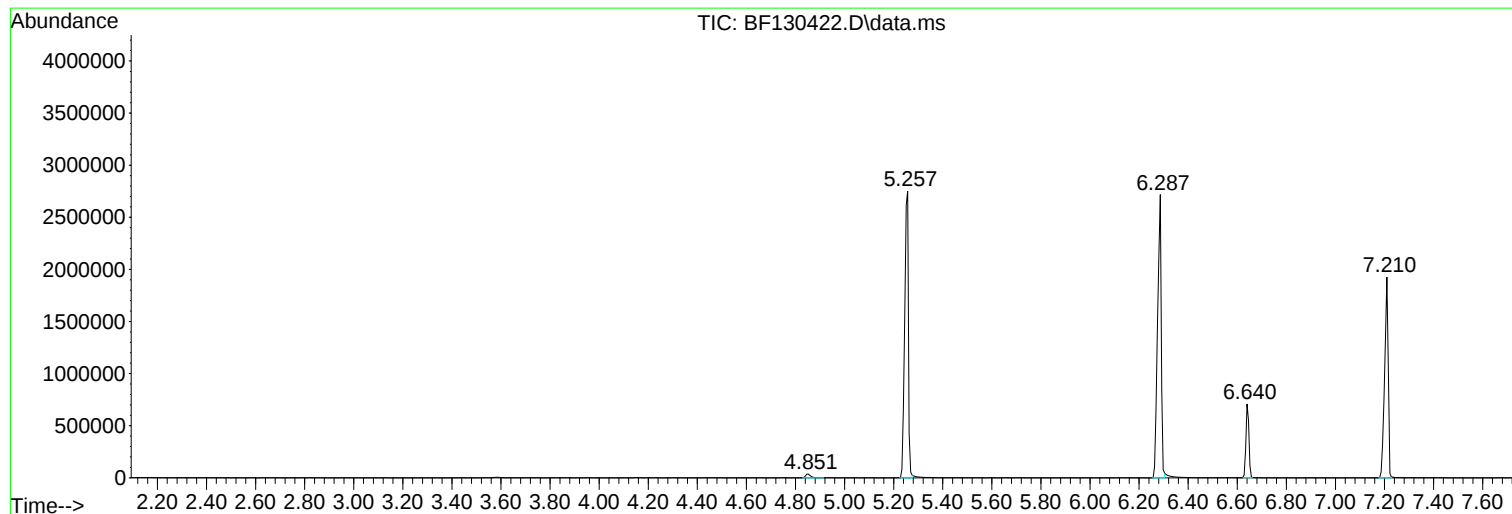

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092722\
Data File : BF130422.D
Acq On : 27 Sep 2022 13:19
Operator : CG\JU
Sample : PB147890BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147890BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092722\
Data File : BF130422.D
Acq On : 27 Sep 2022 13:19
Operator : CG\JU
Sample : PB147890BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147890BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------