


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092722\
 Data File : BF130420.D
 Acq On : 27 Sep 2022 11:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 02:59:31 2022

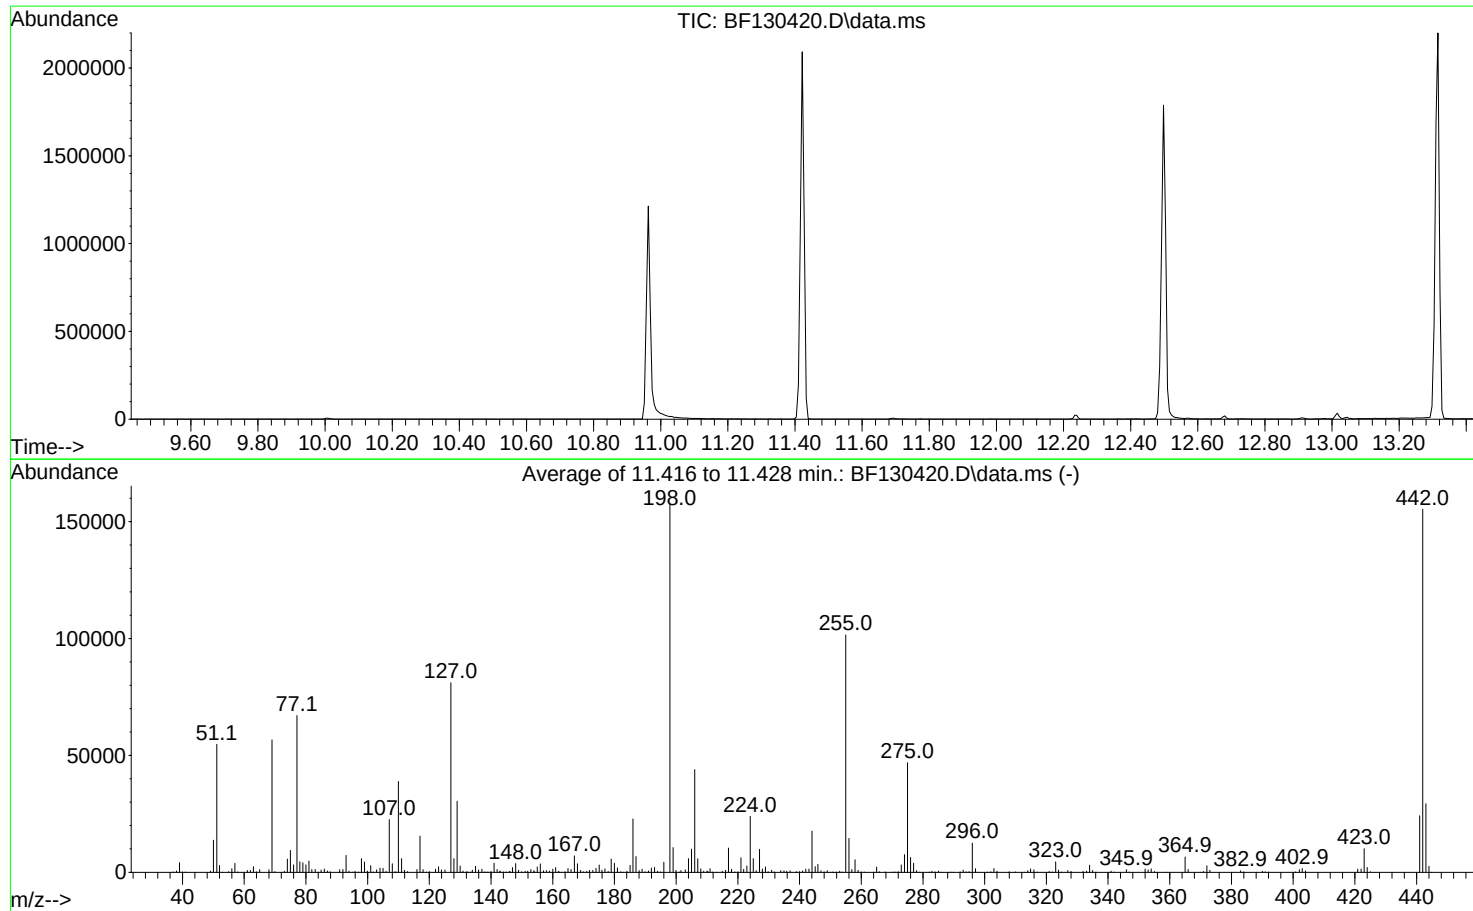




AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	54723	PASS
68	69	0.00	2	1.9	1068	PASS
69	198	0.00	100	36.0	56669	PASS
70	69	0.00	2	0.5	291	PASS
127	198	10	80	51.5	81077	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	157379	PASS
199	198	5	9	6.7	10567	PASS
275	198	10	60	29.8	46835	PASS
365	198	1	100	4.1	6528	PASS
441	198	0.01	100	15.4	24186	PASS
442	442	50	100	100.0	155328	PASS
443	442	15	24	18.9	29334	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092722\
 Data File : BF130420.D
 Acq On : 27 Sep 2022 11:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 27 19:04:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 27 01:00:47 2022
 Response via : Initial Calibration

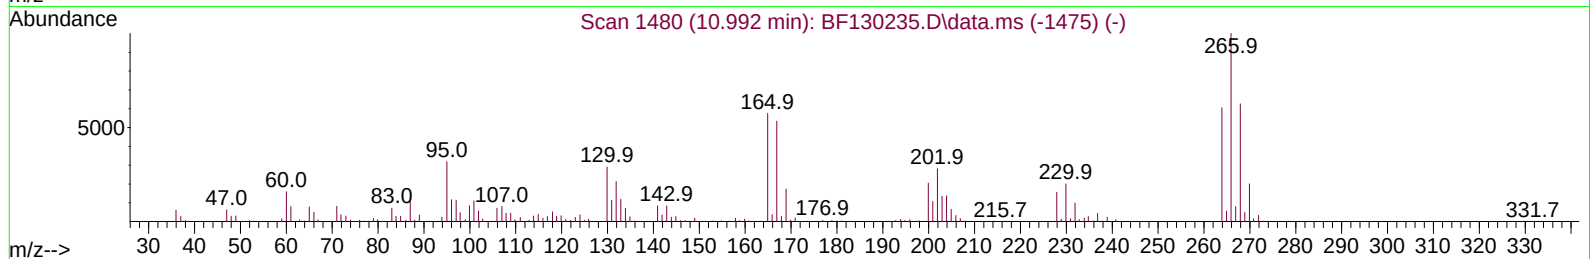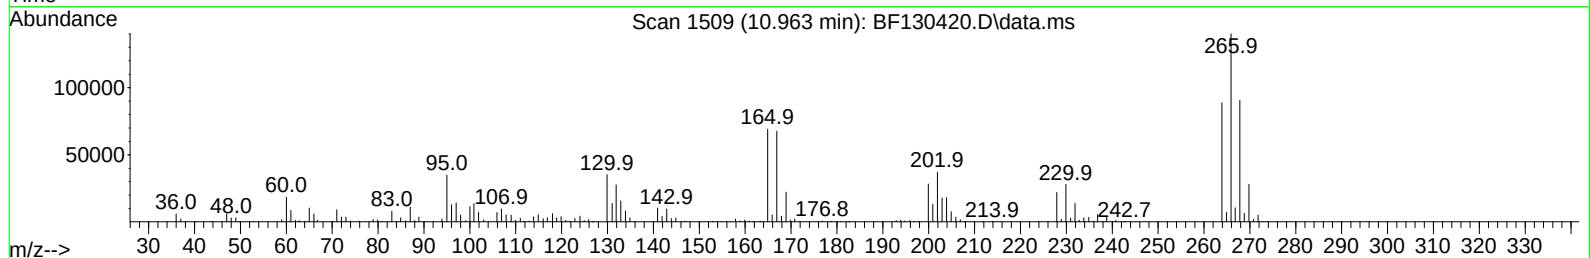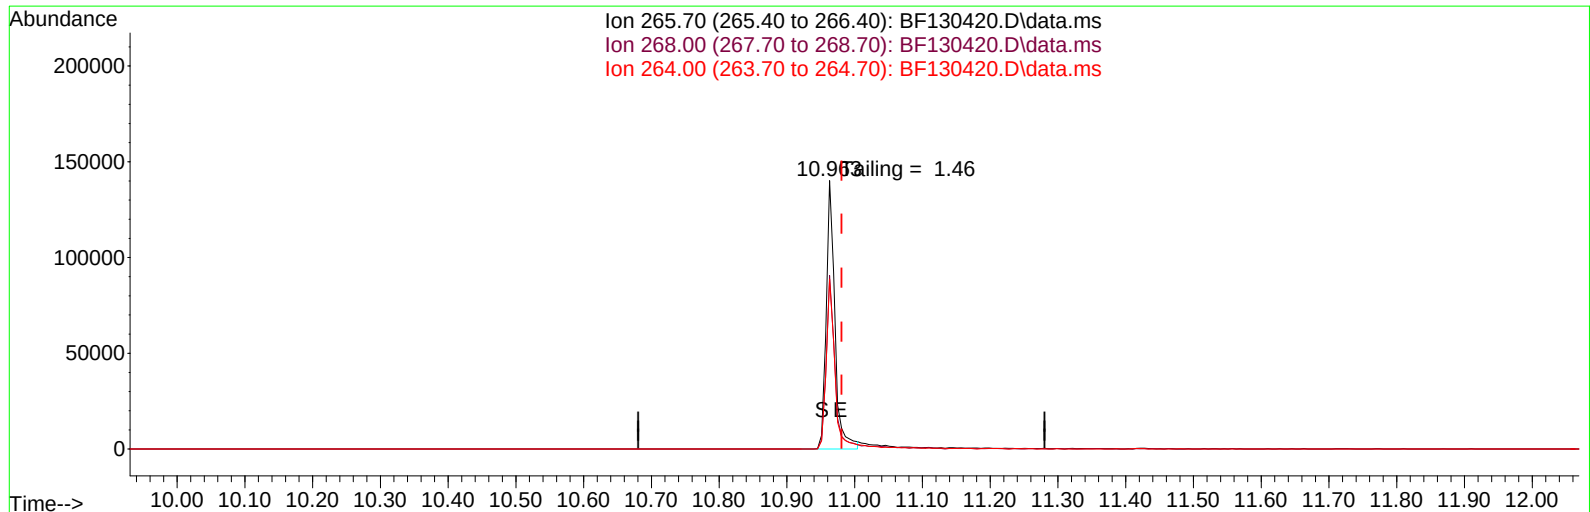

TIC: BF130420.D\data.ms

(70) Pentachlorophenol (C)

10.963min (-0.018) 24230.41 ng




response 131233

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.63
264.00	63.10	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092722\
Data File : BF130420.D
Acq On : 27 Sep 2022 11:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 27 19:04:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 27 01:00:47 2022
Response via : Initial Calibration

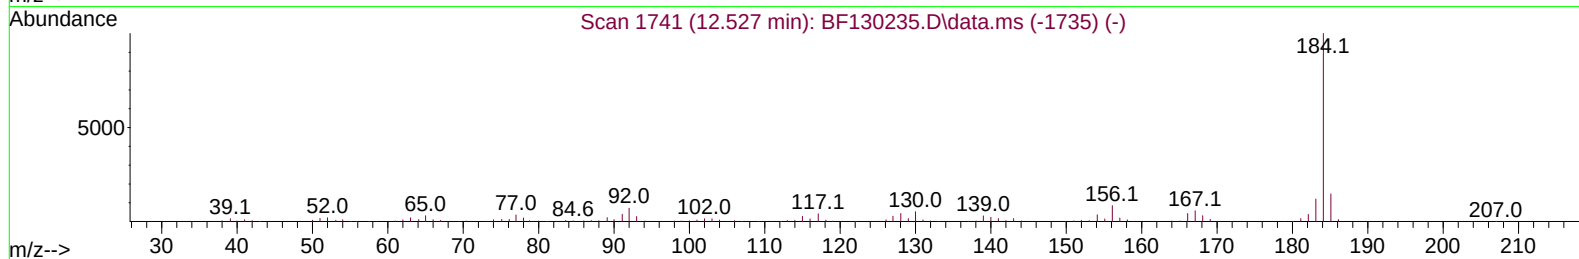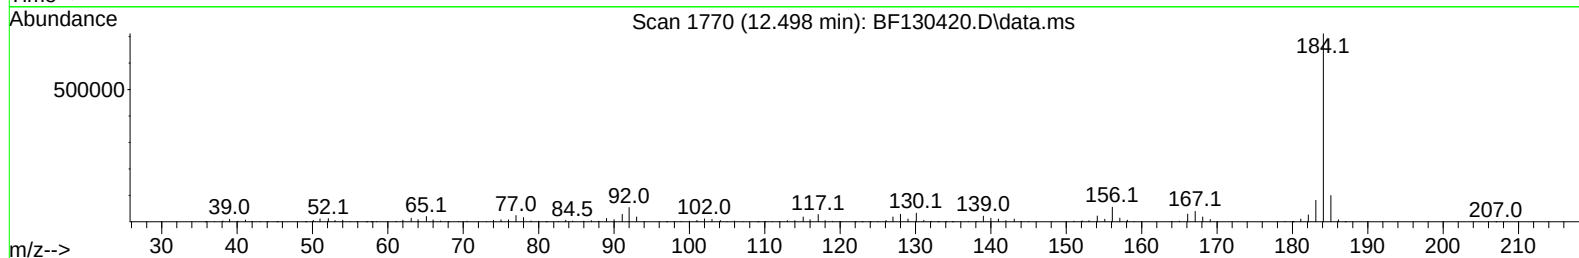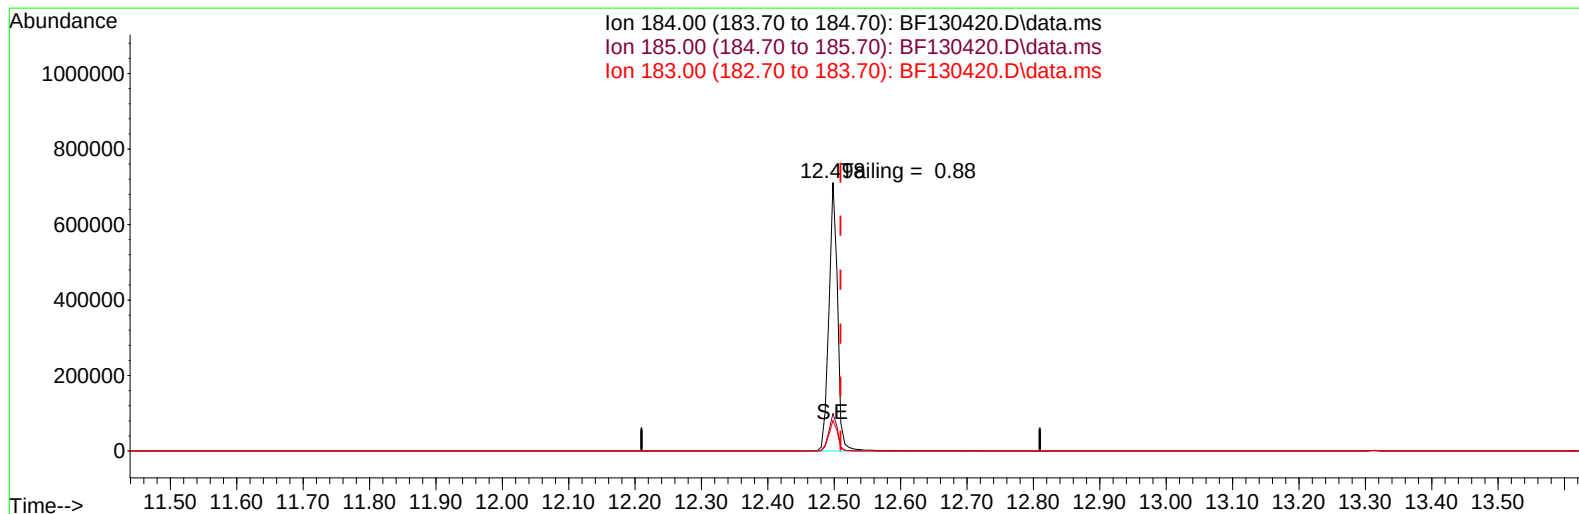

TIC: BF130420.D\data.ms

(77) Benzidine

12.498min (-0.012) 0.00 ng

response 642494

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.00
183.00	11.40	11.43
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/27/2022	BNA_F	<u>BF130420.D</u>
Compound Name	Response	Retention Time
DDT	352742	13.31
DDD	5565	13.01
DDE	1977	12.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7542	360284	2.09

Instrument :
BNA_F
ClientSampleId :
DFTPP