

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092815\
 Data File : BF081858.D
 Acq On : 28 Sep 2015 22:48
 Operator : UM/IZ
 Sample : G3704-16
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK-9-15-15

Quant Time: Sep 29 02:22:08 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 18:10:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	143615	20.00	ng	0.00
21) Naphthalene-d8	8.22	136	578319	20.00	ng	0.00
38) Acenaphthene-d10	9.98	164	276021	20.00	ng	0.00
63) Phenanthrene-d10	11.46	188	517093	20.00	ng	0.00
75) Chrysene-d12	14.10	240	451010	20.00	ng	-0.01
86) Perylene-d12	15.58	264	371150	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.52	112	469525	59.35	ng	0.00
7) Phenol-d6	6.55	99	394172	39.60	ng	-0.01
23) Nitrobenzene-d5	7.50	82	857609	98.85	ng	0.00
41) 2,4,6-Tribromophenol	10.77	330	381203	136.37	ng	0.00
44) 2-Fluorobiphenyl	9.30	172	1697577	108.73	ng	0.00
78) Terphenyl-d14	13.05	244	1633822	142.76	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
9) Benzaldehyde	6.70	77	20064	3.08	ng	# 63
19) n-Nitroso-di-n-propylamine	7.50	70	113141	18.70	ng	# 60
25) Isophorone	7.50	82	793667	46.16	ng	# 58
50) 2,6-Dinitrotoluene	9.98	165	35054	8.47	ng	# 39
56) 2,4-Dinitrotoluene	9.98	165	35425	6.72	ng	# 33
57) Fluorene	10.77	166	14409	Below Cal		# 85
66) 4-Bromophenyl-phenylether	10.77	248	23440	4.50	ng	# 1
70) Phenanthrene	11.49	178	247	Below Cal		# 62
73) Di-n-butylphthalate	12.02	149	2252	Below Cal		# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092815\
Data File : BF081858.D
Acq On : 28 Sep 2015 22:48
Operator : UM/IZ
Sample : G3704-16
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FIELDBLANK-9-15-15

Quant Time: Sep 29 02:22:08 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration

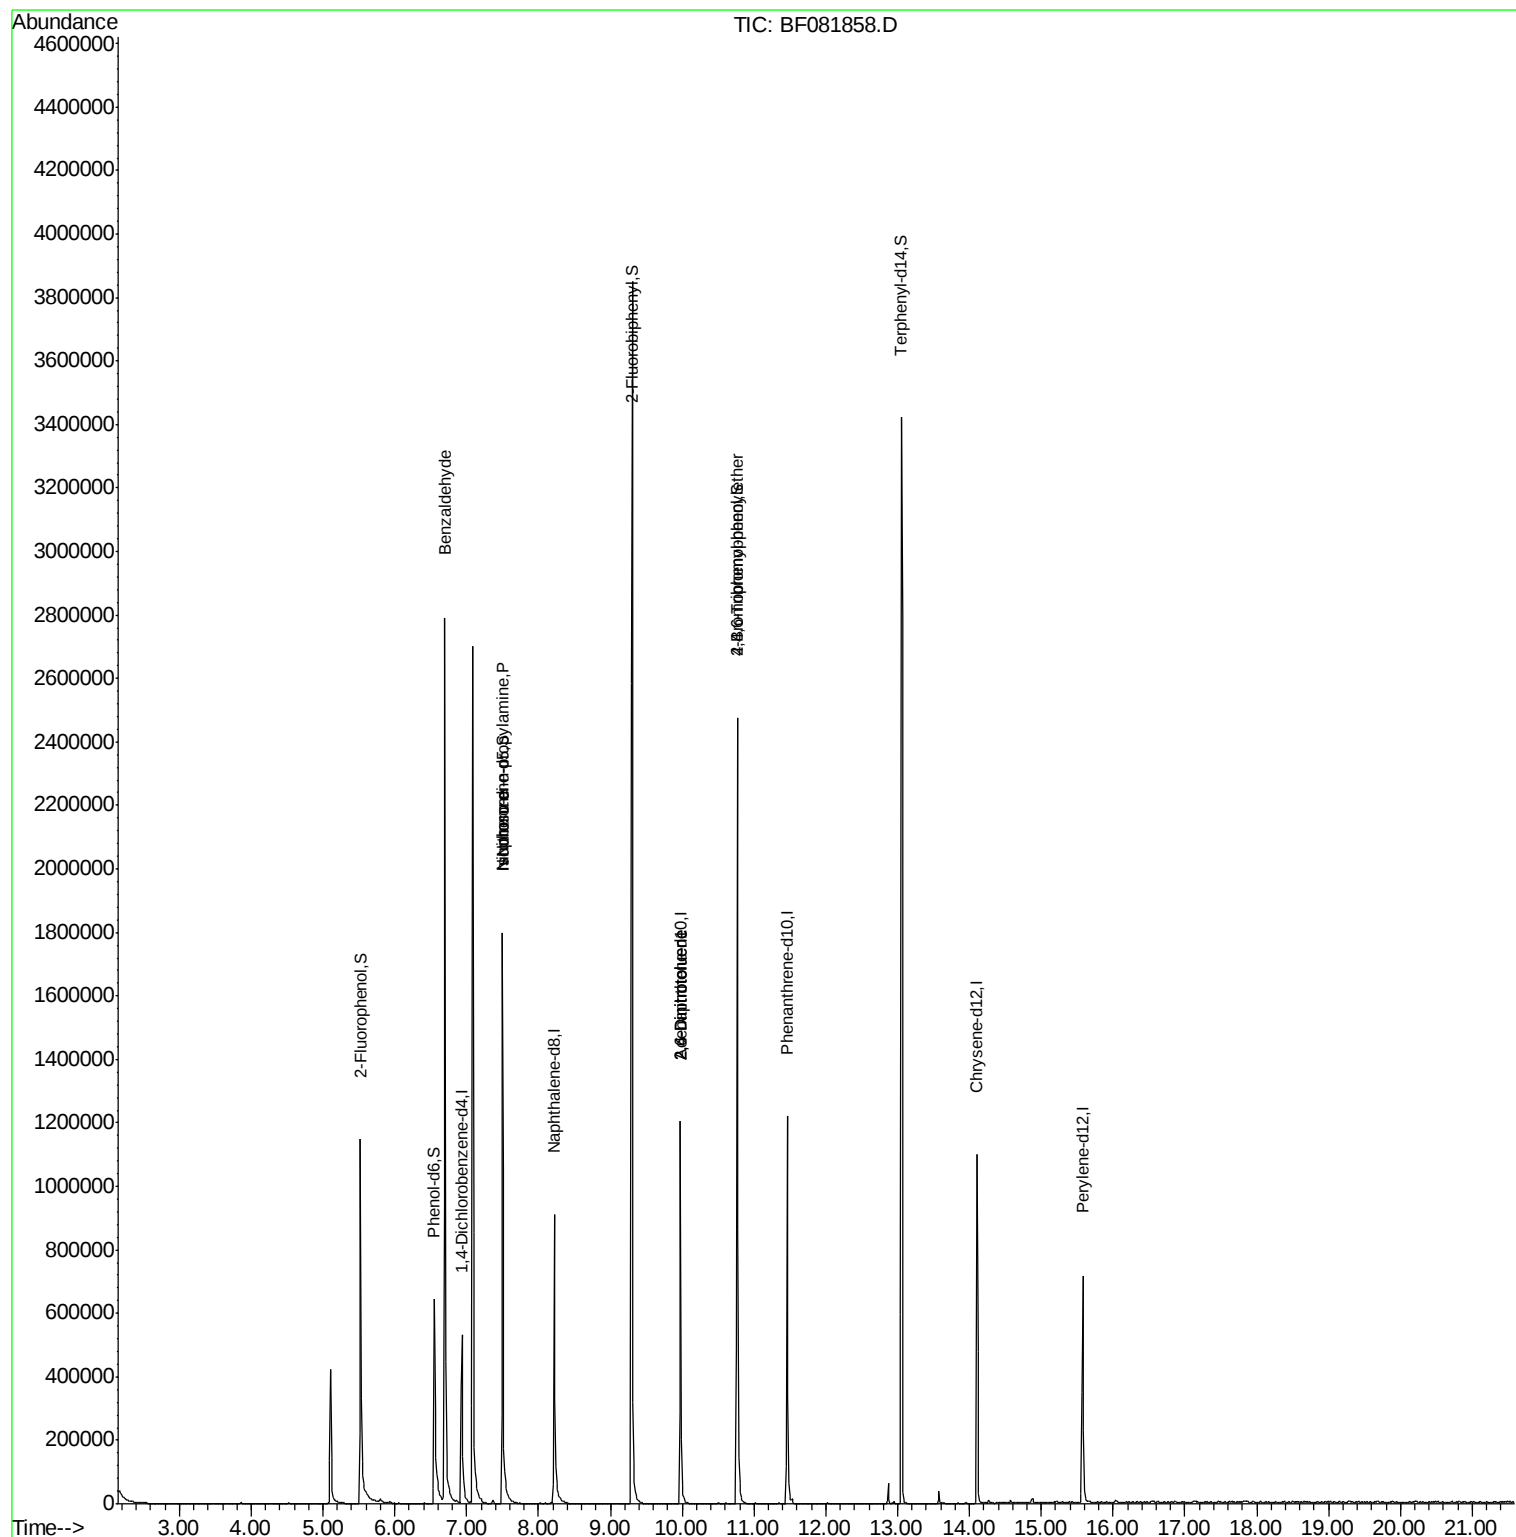

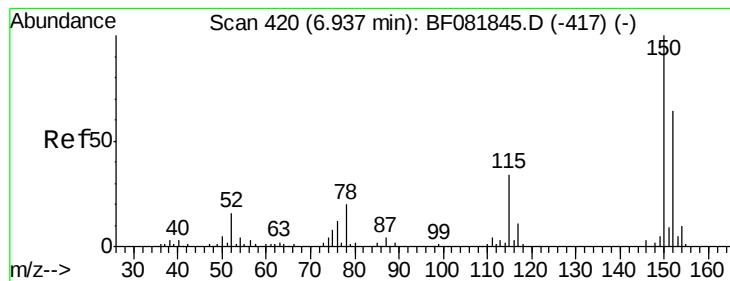

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.94 min Scan# 420

Delta R.T. 0.00 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK-9-15-15


Tgt Ion:152 Resp: 143615

Ion Ratio Lower Upper

152 100

150 154.9 124.7 187.1




115 54.1 39.0 58.4

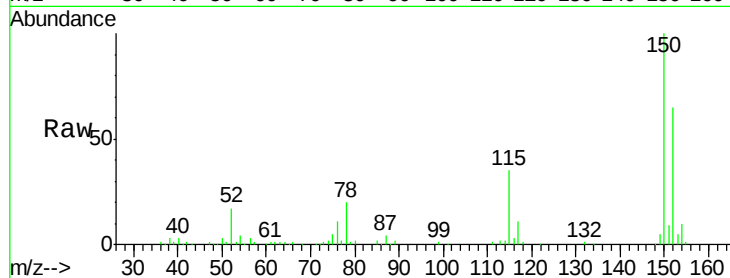

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

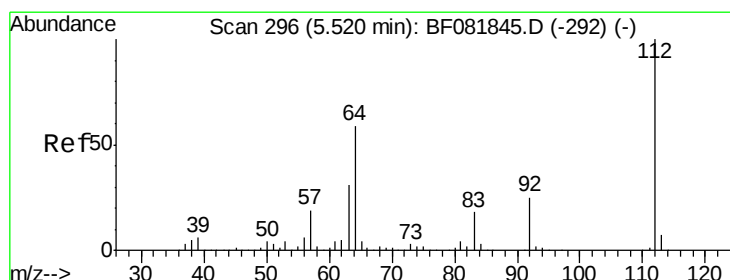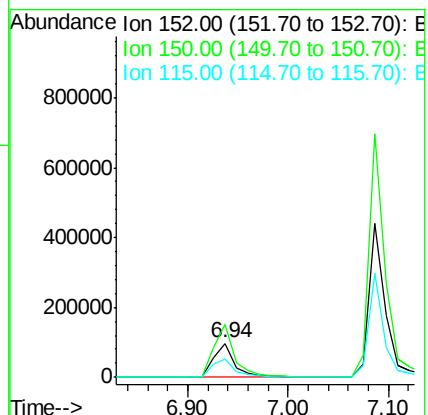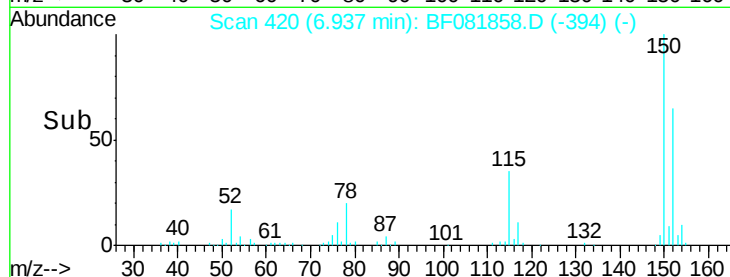

#5

2-Fluorophenol

Concen: 59.35 ng

RT: 5.52 min Scan# 296

Delta R.T. 0.00 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48


Tgt Ion:112 Resp: 469525

Ion Ratio Lower Upper

112 100

64 59.9 39.7 59.5#



63 31.9 17.4 26.0#

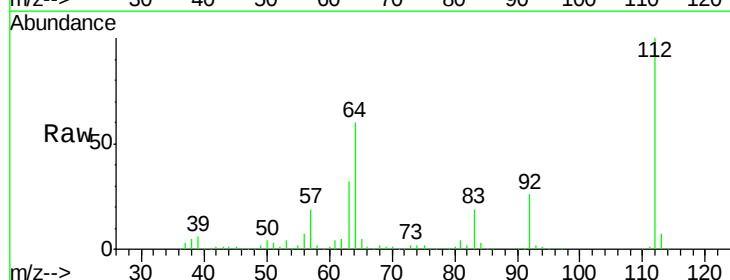


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

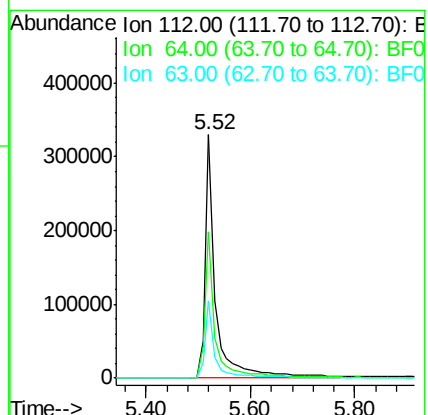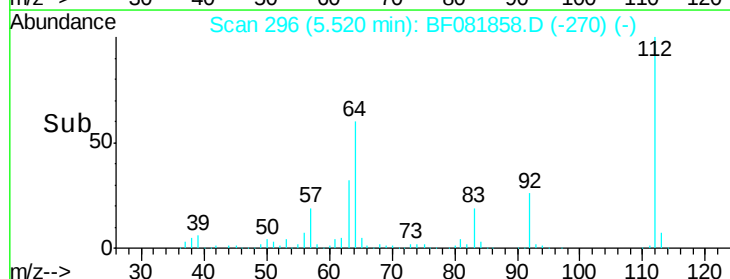

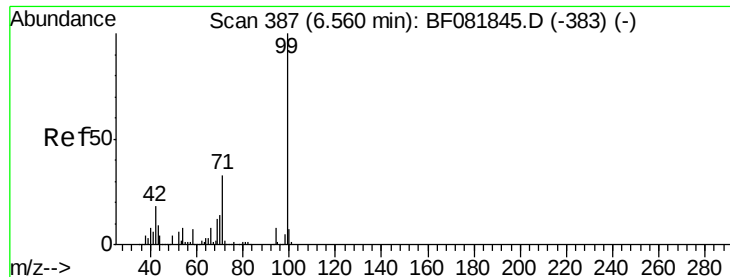

#7

Phenol-d6

Concen: 39.60 ng

RT: 6.55 min Scan# 386

Delta R.T. -0.01 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK-9-15-15


Tgt Ion: 99 Resp: 394172

Ion Ratio Lower Upper

99 100

42 17.9 13.7 20.5




71 32.5 14.2 21.2#

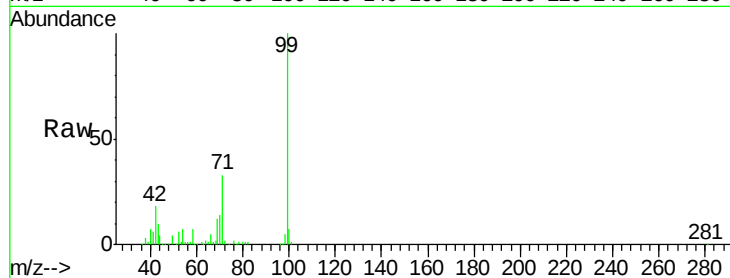

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

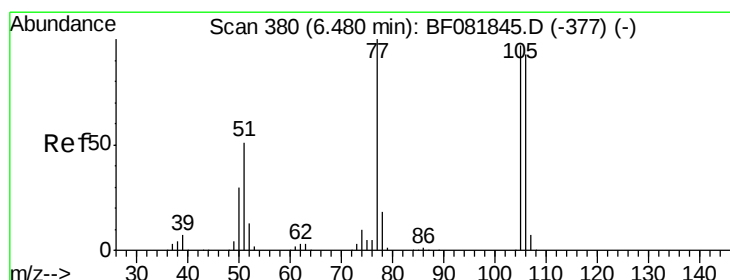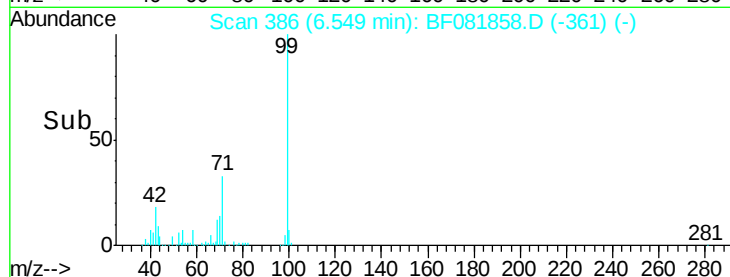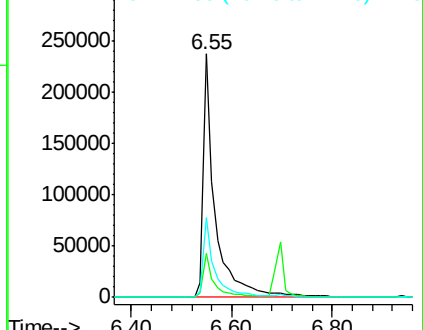

#9

Benzaldehyde

Concen: 3.08 ng

RT: 6.70 min Scan# 399

Delta R.T. 0.22 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48


Tgt Ion: 77 Resp: 20064

Ion Ratio Lower Upper

77 100

105 80.2 91.6 131.6#



106 72.6 102.6 142.6#

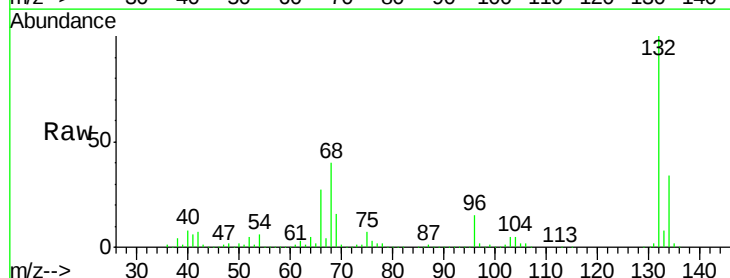


Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): E

Ion 106.00 (105.70 to 106.70): E



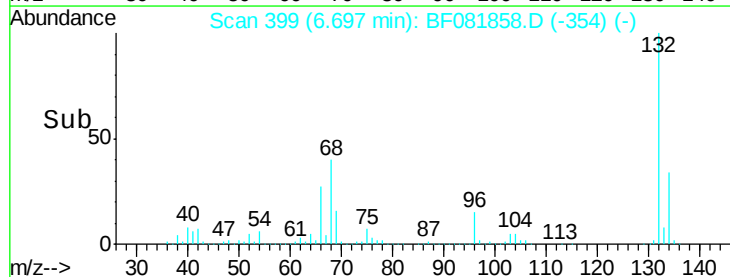
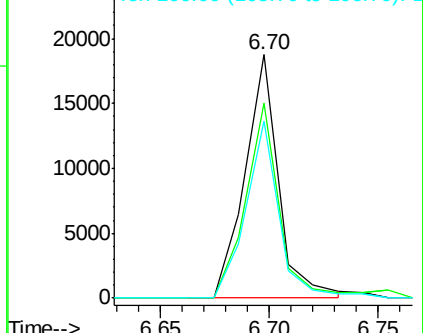




#19
n-Nitroso-di-n-propylamine
Concen: 18.70 ng
RT: 7.50 min Scan# 469
Delta R.T. 0.15 min
Lab File: BF081858.D
Acq: 28 Sep 2015 22:48




Instrument :
BNA_F
ClientSampleId :
FIELDBLANK-9-15-15


Tgt Ion:	70	Resp:	113141
Ion	Ratio	Lower	Upper
70	100		
42	48.6	63.8	95.6#
101	0.0	9.2	13.8#
130	1.9	27.3	40.9#

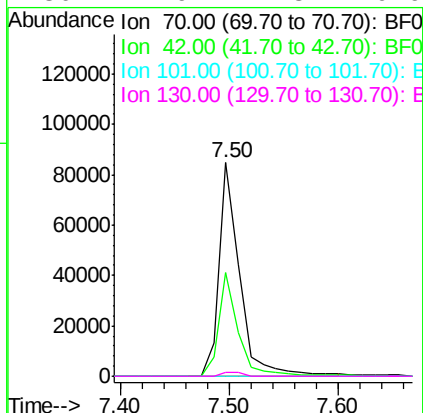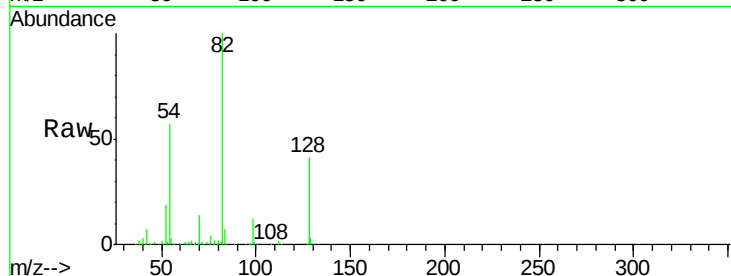

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.22 min Scan# 532
Delta R.T. 0.00 min
Lab File: BF081858.D
Acq: 28 Sep 2015 22:48

Tgt Ion:	136	Resp:	578319
Ion	Ratio	Lower	Upper
136	100		
137	11.3	9.0	13.6
54	8.6	8.2	12.2
68	5.9	5.8	8.6

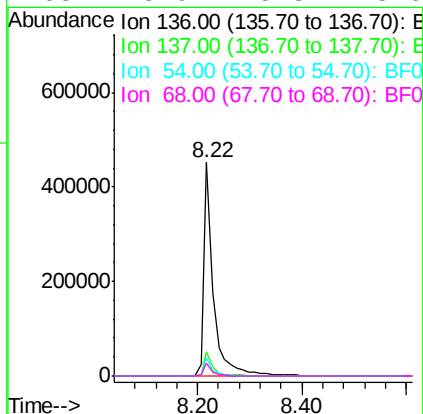

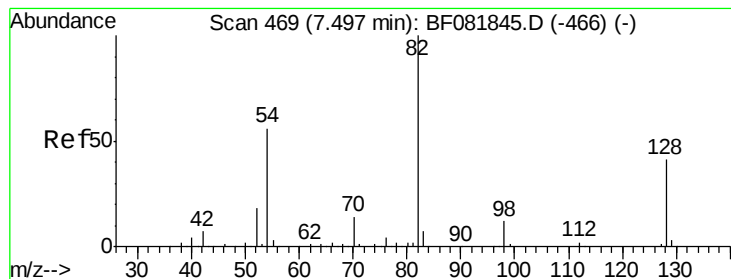

#23

Nitrobenzene-d5

Concen: 98.85 ng

RT: 7.50 min Scan# 469

Delta R.T. 0.00 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK-9-15-15


Tgt Ion: 82 Resp: 857609

Ion Ratio Lower Upper

82 100

128 41.4 51.0 76.6#




54 57.2 47.5 71.3



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): BF0

Ion 54.00 (53.70 to 54.70): BF0

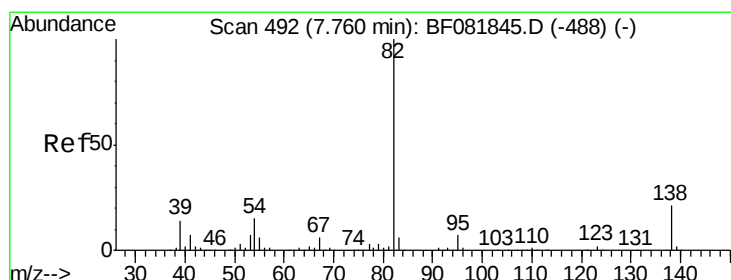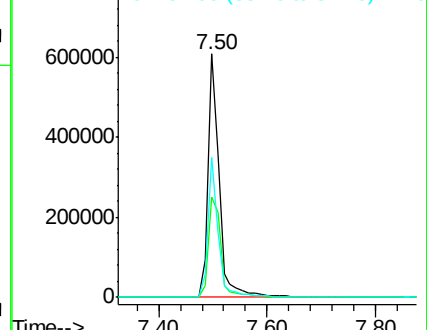

#25

Isophorone

Concen: 46.16 ng

RT: 7.50 min Scan# 469

Delta R.T. -0.26 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48


Tgt Ion: 82 Resp: 793667

Ion Ratio Lower Upper

82 100

95 0.0 4.0 6.0#



138 0.0 18.3 27.5#




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): BF0

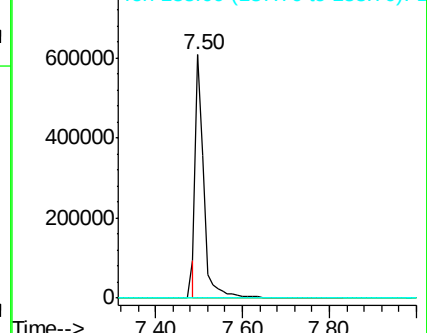

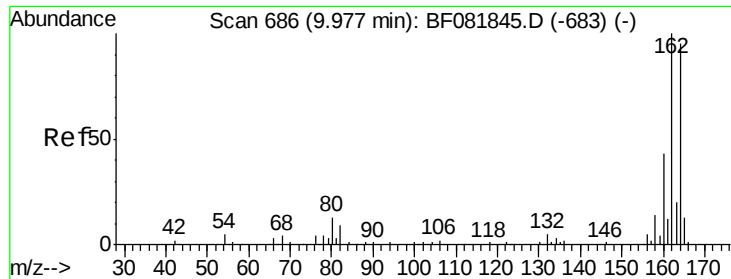

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.98 min Scan# 686

Delta R.T. 0.00 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK-9-15-15


Tgt Ion:164 Resp: 276021

Ion Ratio Lower Upper

164 100

162 105.2 75.2 112.8




160 46.4 31.5 47.3



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

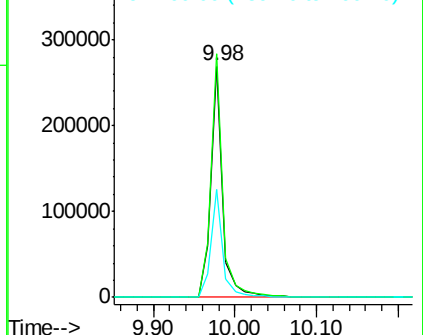

#41

2,4,6-Tribromophenol

Concen: 136.37 ng

RT: 10.77 min Scan# 755

Delta R.T. 0.00 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48


Tgt Ion:330 Resp: 381203

Ion Ratio Lower Upper

330 100

332 95.3 76.6 114.8



141 32.3 29.7 44.5




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

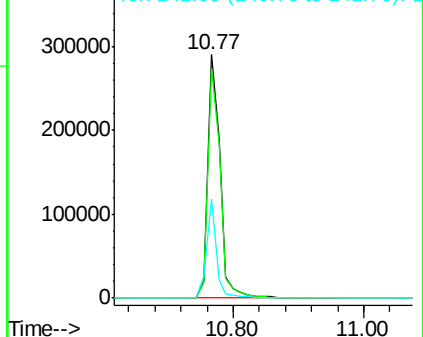







#44
 2-Fluorobiphenyl
 Concen: 108.73 ng
 RT: 9.30 min Scan# 627
 Delta R.T. 0.00 min
 Lab File: BF081858.D
 Acq: 28 Sep 2015 22:48

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK-9-15-15

Tgt Ion:172 Resp: 1697577
 Ion Ratio Lower Upper
 172 100
 171 37.4 26.1 39.1
 170 25.7 17.4 26.2

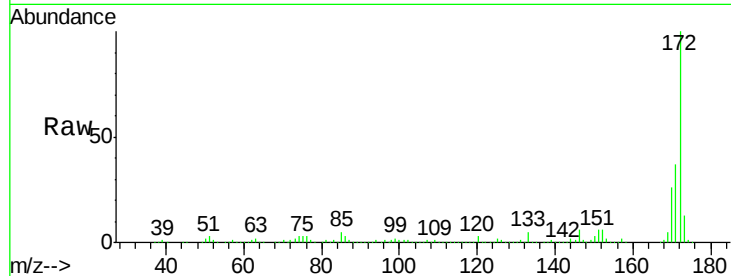


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


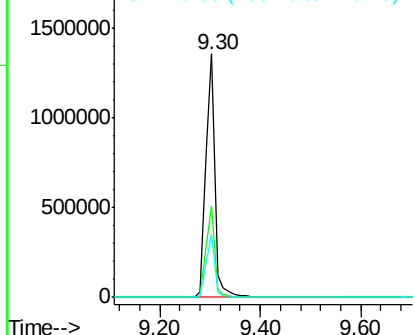



#50
 2,6-Dinitrotoluene
 Concen: 8.47 ng
 RT: 9.98 min Scan# 686
 Delta R.T. 0.22 min
 Lab File: BF081858.D
 Acq: 28 Sep 2015 22:48

Tgt Ion:165 Resp: 35054
 Ion Ratio Lower Upper
 165 100
 63 1.2 32.3 48.5#
 89 1.5 28.6 43.0#



Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0



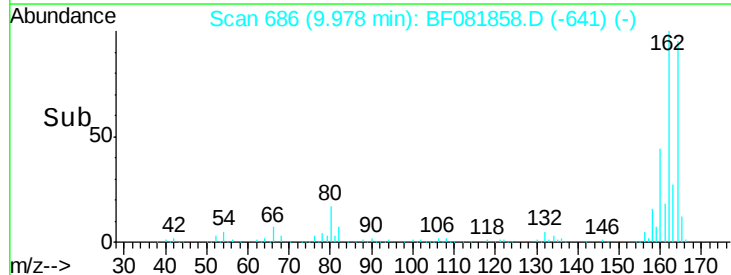
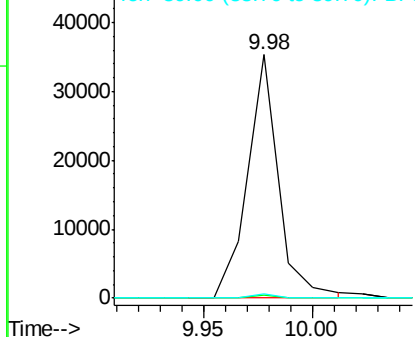


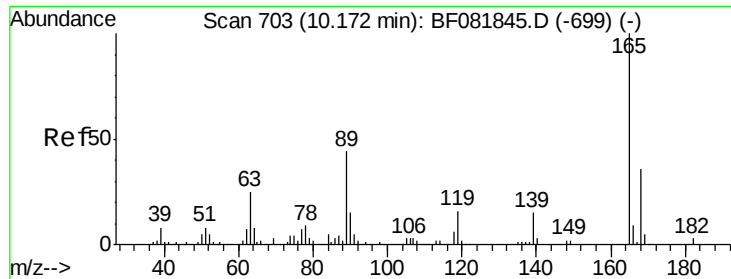

#56
 2,4-Dinitrotoluene
 Concen: 6.72 ng
 RT: 9.98 min Scan# 686
 Delta R.T. -0.19 min
 Lab File: BF081858.D
 Acq: 28 Sep 2015 22:48




Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK-9-15-15


Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.2	29.8	44.6#
89	1.5	44.5	66.7#
182	0.0	3.0	4.4#

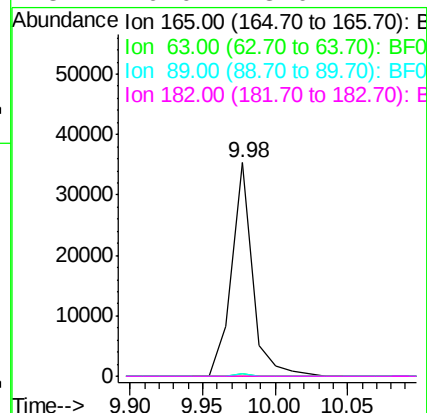

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.46 min Scan# 816
 Delta R.T. 0.00 min
 Lab File: BF081858.D
 Acq: 28 Sep 2015 22:48

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.3	11.1	16.7#
80	10.1	11.0	16.4#

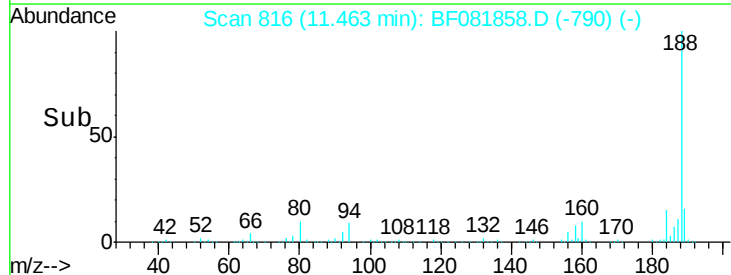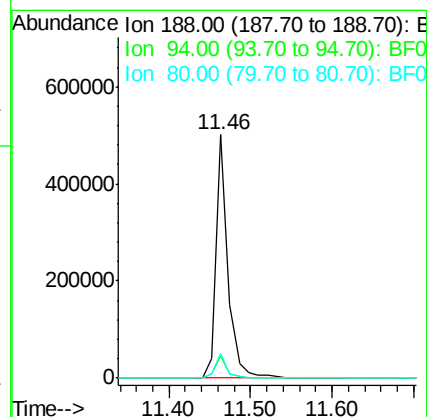

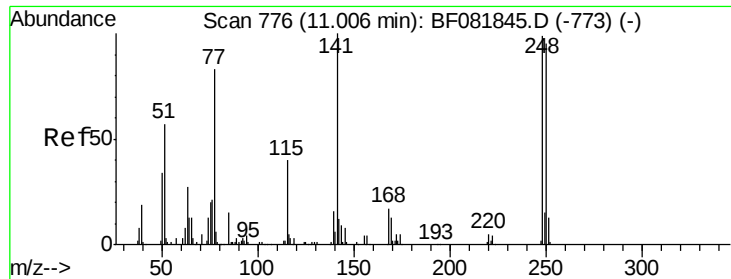

#66

4-Bromophenyl-phenylether

Concen: 4.50 ng

RT: 10.77 min Scan# 755

Delta R.T. -0.24 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK-9-15-15


Tgt Ion:248 Resp: 23440

Ion Ratio Lower Upper

248 100

250 201.4 78.5 117.7#




141 550.7 59.0 88.6#

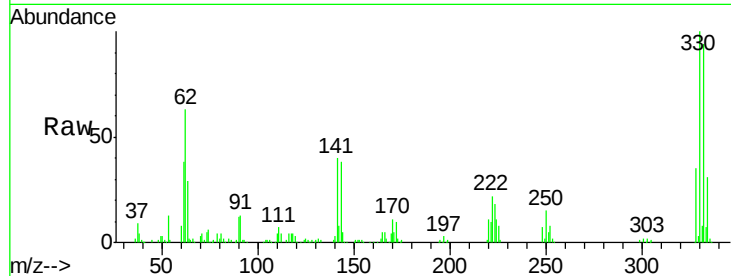

Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

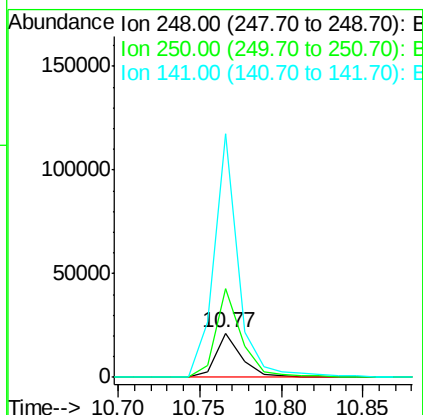

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.10 min Scan# 1047

Delta R.T. -0.01 min

Lab File: BF081858.D

Acq: 28 Sep 2015 22:48


Tgt Ion:240 Resp: 451010

Ion Ratio Lower Upper

240 100

120 13.0 16.2 24.2#



236 26.2 18.4 27.6




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



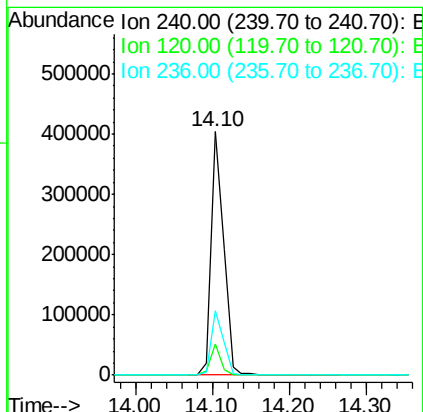



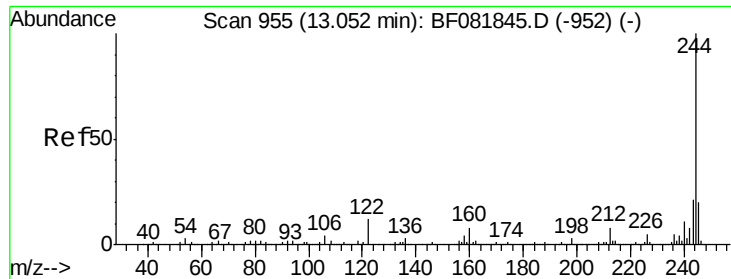

#78
 Terphenyl-d14
 Concen: 142.76 ng
 RT: 13.05 min Scan# 955
 Delta R.T. 0.00 min
 Lab File: BF081858.D
 Acq: 28 Sep 2015 22:48

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK-9-15-15

Tgt Ion:244 Resp: 1633822
 Ion Ratio Lower Upper
 244 100
 212 8.1 4.3 6.5#
 122 12.5 17.4 26.2#

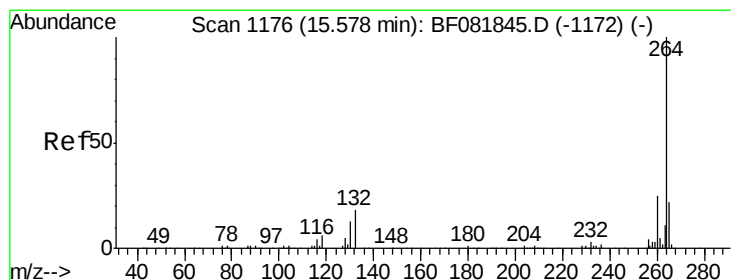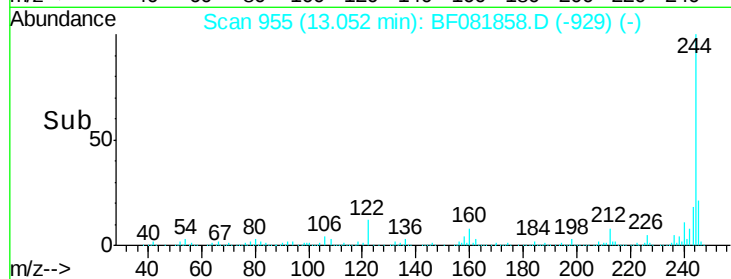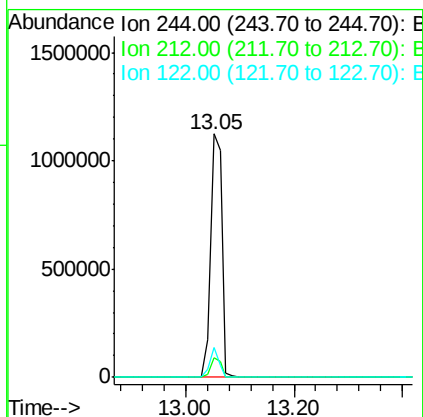

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.58 min Scan# 1176
 Delta R.T. 0.00 min
 Lab File: BF081858.D
 Acq: 28 Sep 2015 22:48

Tgt Ion:264 Resp: 371150
 Ion Ratio Lower Upper
 264 100
 260 24.0 16.7 25.1
 265 21.6 17.2 25.8

