

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092815\
 Data File : BF081866.D
 Acq On : 29 Sep 2015 5:02
 Operator : UM/IZ
 Sample : G3717-05
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LIP-12-9-16-15

Quant Time: Sep 29 05:36:34 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 18:10:42 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	119057	20.00	ng	0.00
21) Naphthalene-d8	8.22	136	482119	20.00	ng	0.00
38) Acenaphthene-d10	9.98	164	231633	20.00	ng	0.00
63) Phenanthrene-d10	11.46	188	432445	20.00	ng	0.00
75) Chrysene-d12	14.10	240	370874	20.00	ng	-0.01
86) Perylene-d12	15.58	264	290536	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	421951	64.34	ng	0.00
7) Phenol-d6	6.55	99	366911	44.46	ng	-0.01
23) Nitrobenzene-d5	7.50	82	767402	106.10	ng	0.00
41) 2,4,6-Tribromophenol	10.77	330	346718	147.80	ng	0.00
44) 2-Fluorobiphenyl	9.30	172	1520349	118.86	ng	0.00
78) Terphenyl-d14	13.05	244	1269376	127.71	ng	0.00
Target Compounds						
9) Benzaldehyde	6.70	77	18873	3.49	ng	# 59
15) Benzyl Alcohol	7.09	79	12264	2.06	ng	# 31
19) n-Nitroso-di-n-propylamine	7.50	70	98217	19.58	ng	# 59
25) Isophorone	7.50	82	705069	49.18	ng	# 58
50) 2,6-Dinitrotoluene	9.98	165	28310	8.16	ng	# 39
56) 2,4-Dinitrotoluene	9.98	165	29485	6.66	ng	# 34
57) Fluorene	10.77	166	12952	Below Cal		# 82
66) 4-Bromophenyl-phenylether	10.77	248	21653	4.97	ng	# 1
70) Phenanthrene	11.49	178	238	Below Cal		# 62
73) Di-n-butylphthalate	12.02	149	3036	Below Cal		# 83

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092815\
Data File : BF081866.D
Acq On : 29 Sep 2015 5:02
Operator : UM/IZ
Sample : G3717-05
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LIP-12-9-16-15

Quant Time: Sep 29 05:36:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration

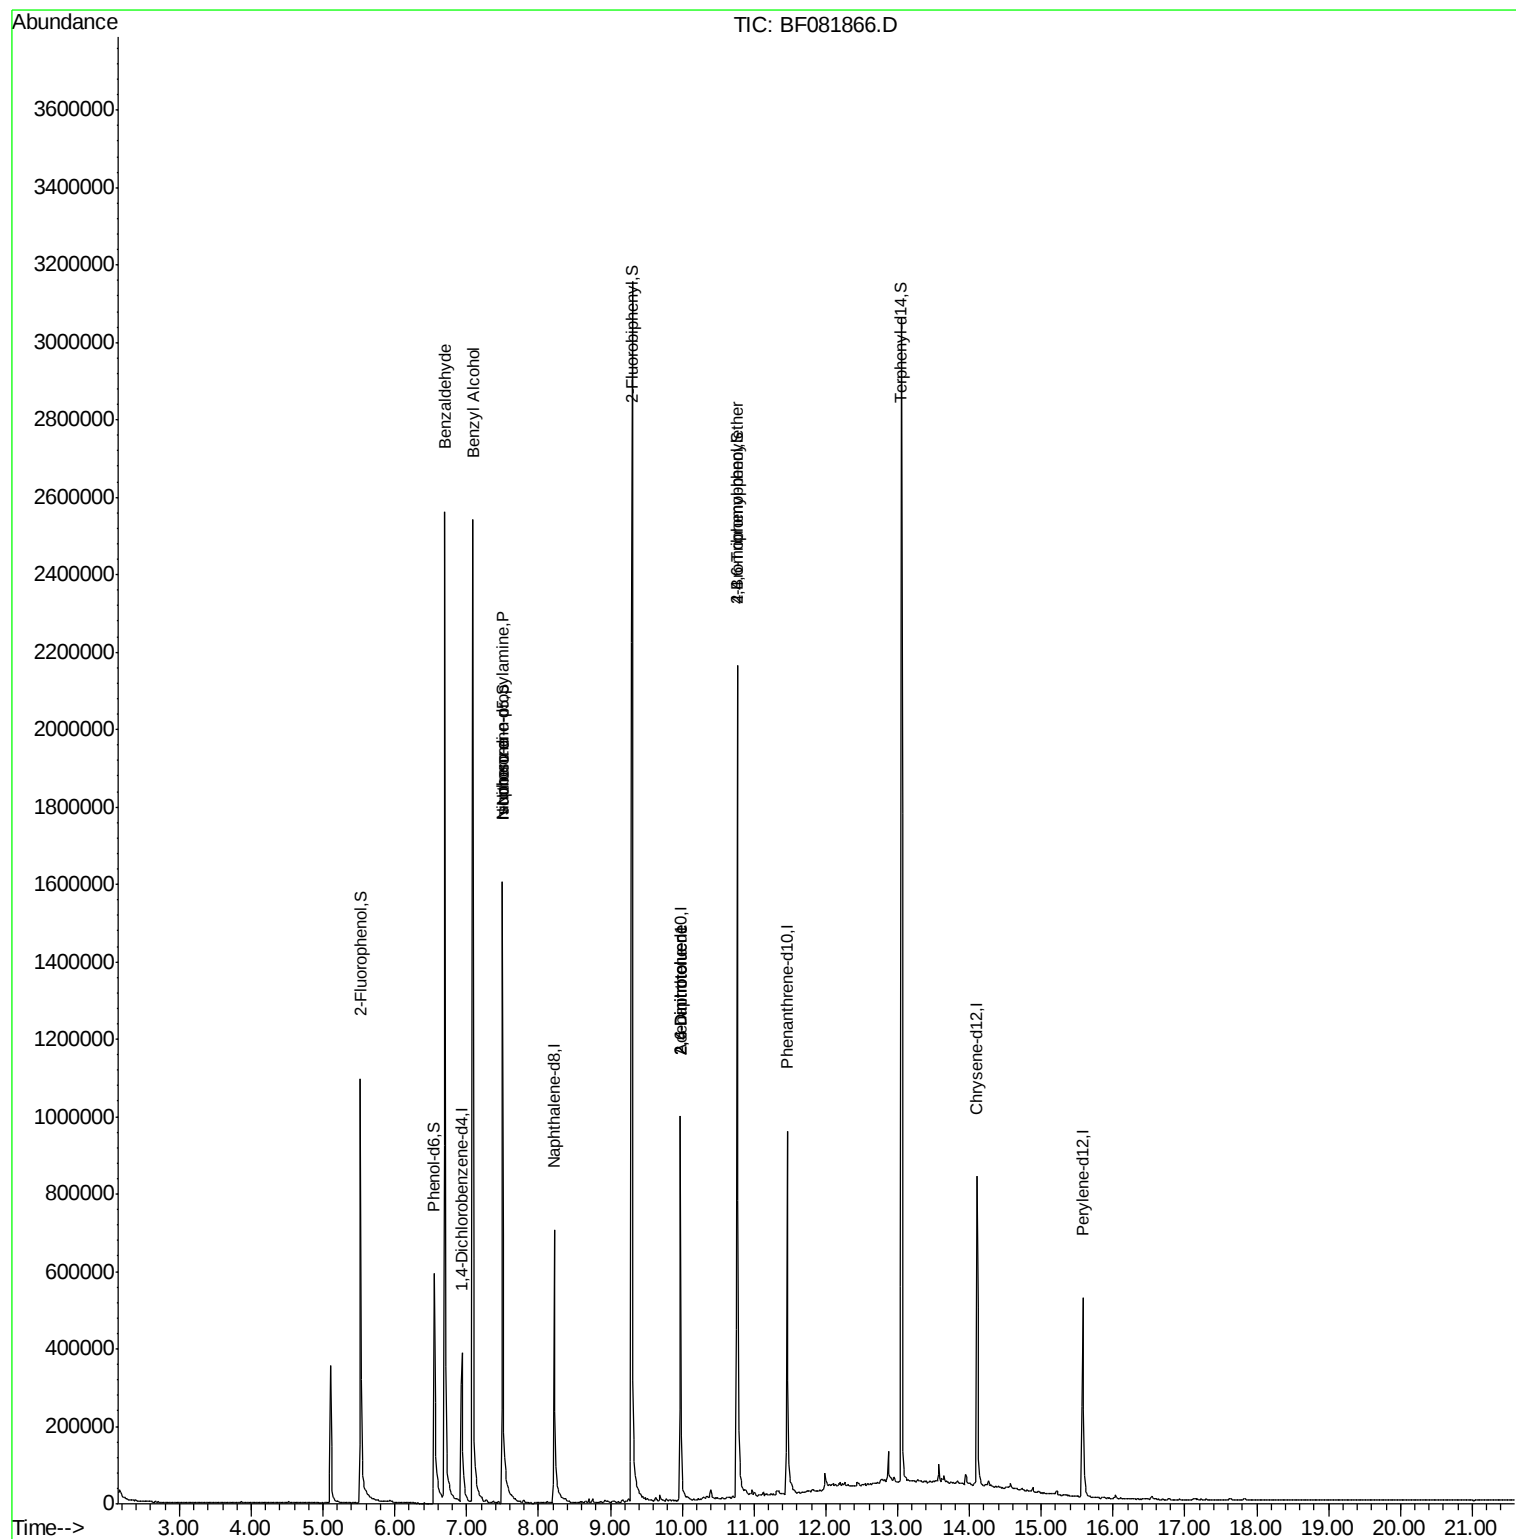



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.94 min Scan# 420

Delta R.T. 0.00 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02

Instrument :

BNA_F

ClientSampleId :

LIP-12-9-16-15





Tgt Ion:152 Resp: 119057

Ion Ratio Lower Upper

152 100

150 156.7 124.7 187.1

115 52.2 39.0 58.4

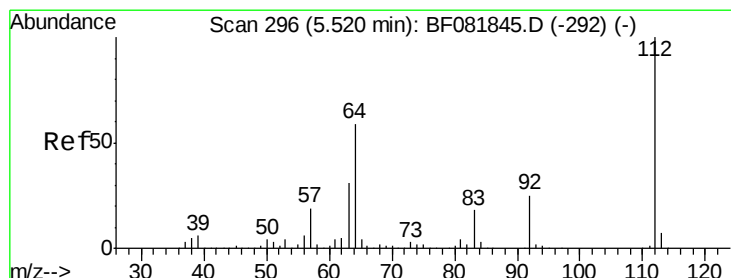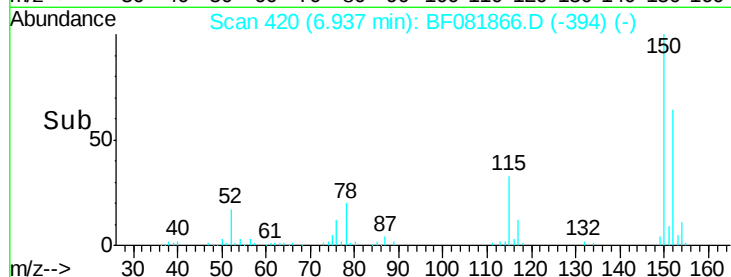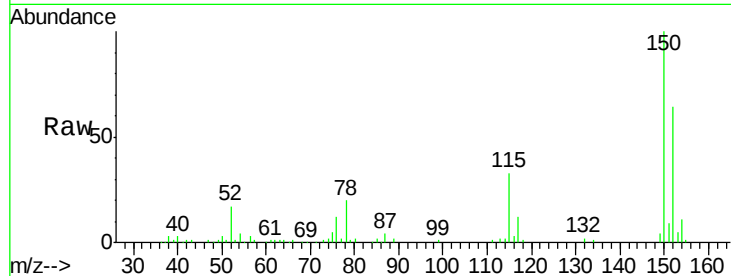

#5

2-Fluorophenol

Concen: 64.34 ng

RT: 5.52 min Scan# 296

Delta R.T. 0.00 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02




Tgt Ion:112 Resp: 421951


Ion Ratio Lower Upper

112 100

64 62.3 39.7 59.5#

63 33.1 17.4 26.0#

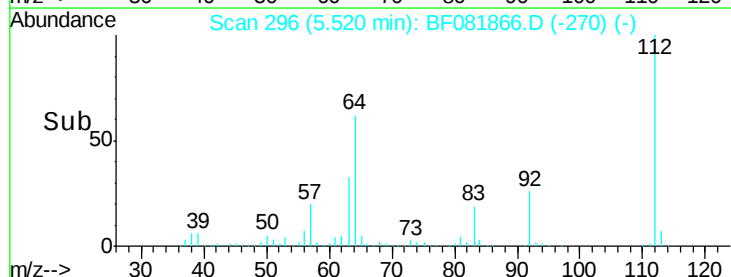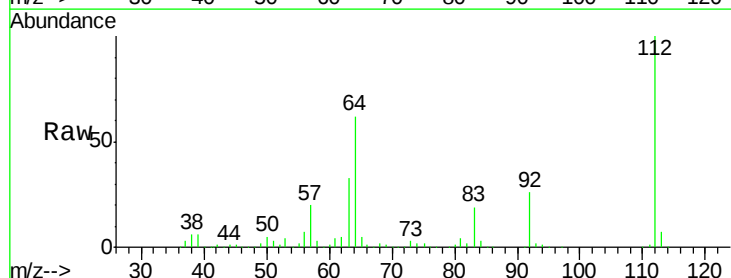

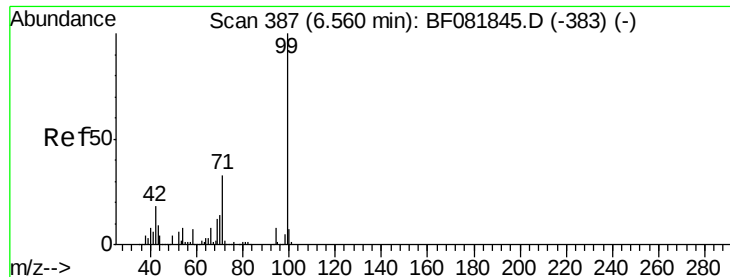

#7

Phenol-d6

Concen: 44.46 ng

RT: 6.55 min Scan# 386

Delta R.T. -0.01 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02

Instrument :

BNA_F

ClientSampleId :

LIP-12-9-16-15





Tgt Ion: 99 Resp: 366911

Ion Ratio Lower Upper

99 100

42 18.3 13.7 20.5

71 32.8 14.2 21.2#

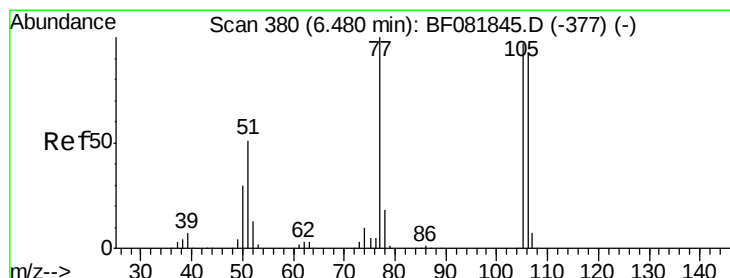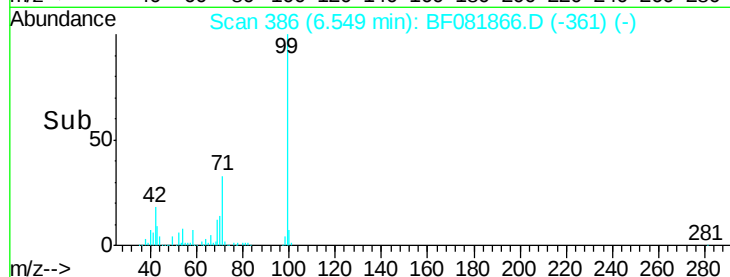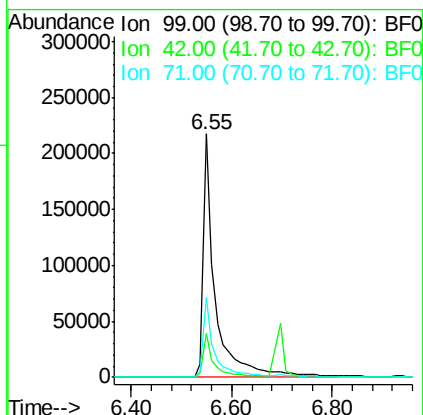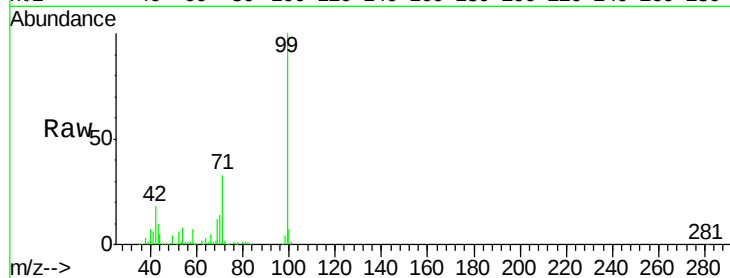

#9

Benzaldehyde

Concen: 3.49 ng

RT: 6.70 min Scan# 399

Delta R.T. 0.22 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02




Tgt Ion: 77 Resp: 18873


Ion Ratio Lower Upper

77 100

105 78.0 91.6 131.6#

106 67.0 102.6 142.6#

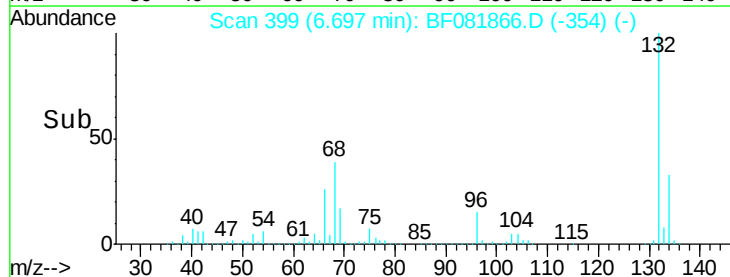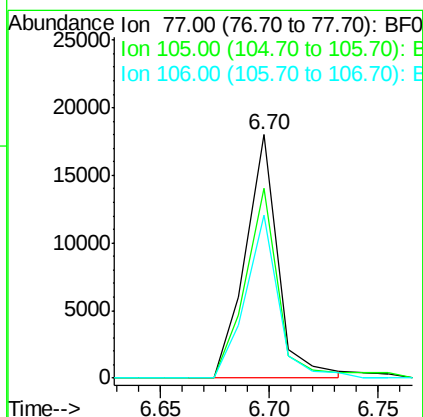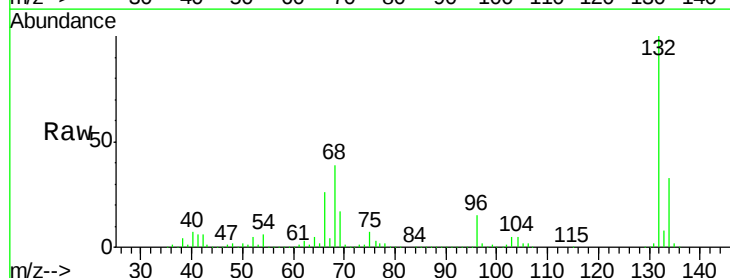

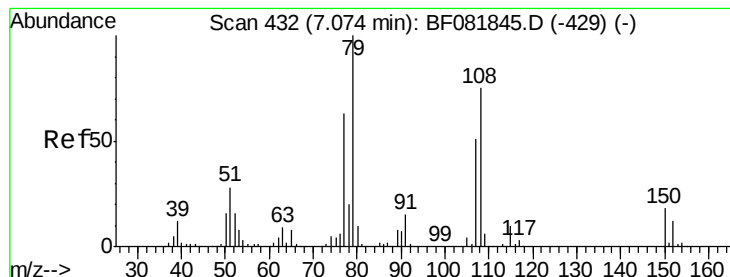

#15

Benzyl Alcohol

Concen: 2.06 ng

RT: 7.09 min Scan# 433

Delta R.T. 0.01 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02

Instrument :

BNA_F

ClientSampleId :

LIP-12-9-16-15





Tgt Ion: 79 Resp: 12264

Ion Ratio Lower Upper

79 100

108 25.8 88.6 132.8#

77 94.1 47.0 70.4#

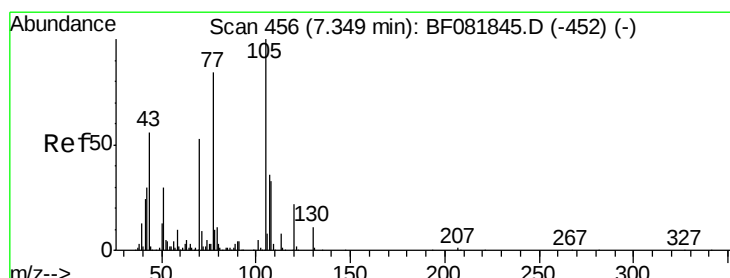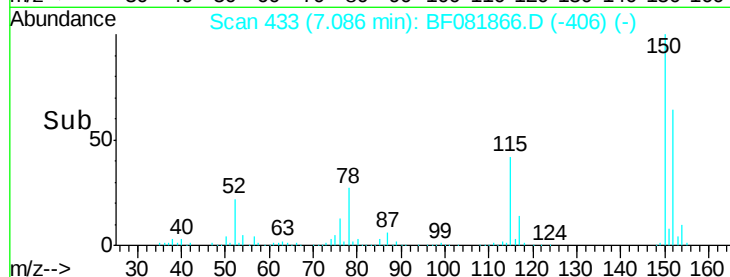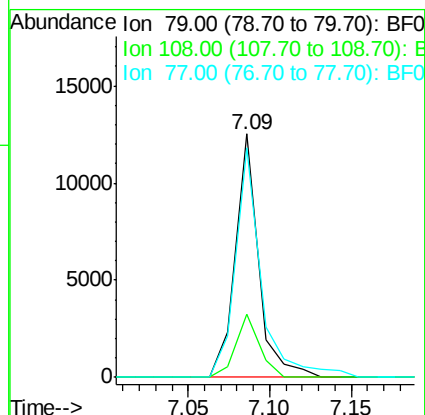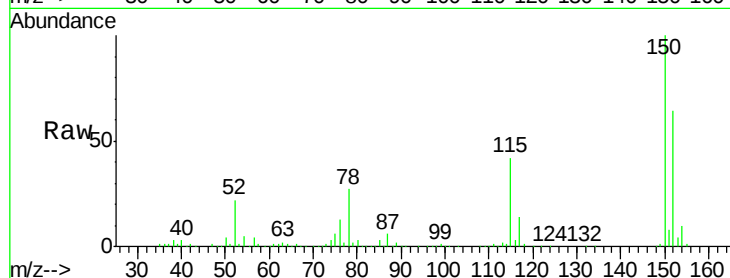

#19

n-Nitroso-di-n-propylamine

Concen: 19.58 ng

RT: 7.50 min Scan# 469

Delta R.T. 0.15 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02

Tgt Ion: 70 Resp: 98217




Ion Ratio Lower Upper


70 100

42 47.9 63.8 95.6#

101 0.0 9.2 13.8#

130 2.2 27.3 40.9#


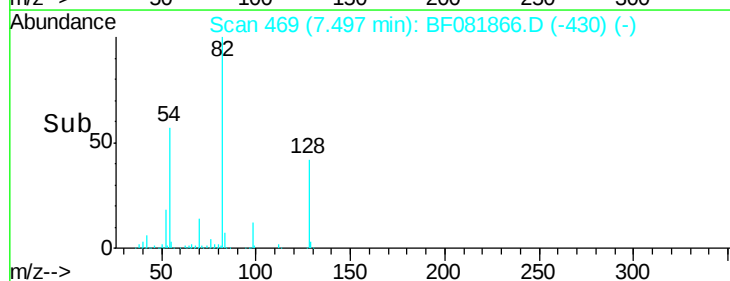
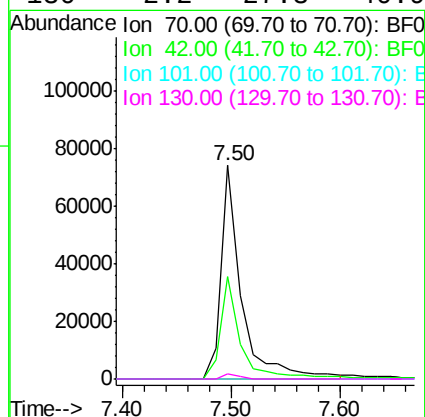
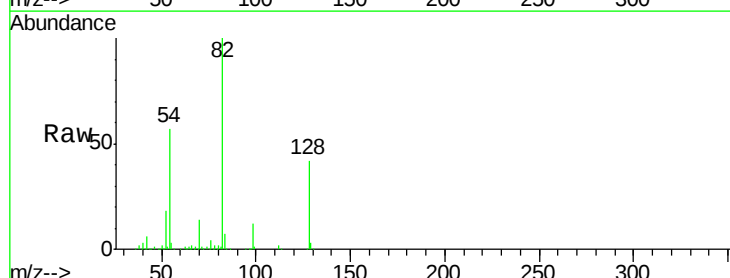


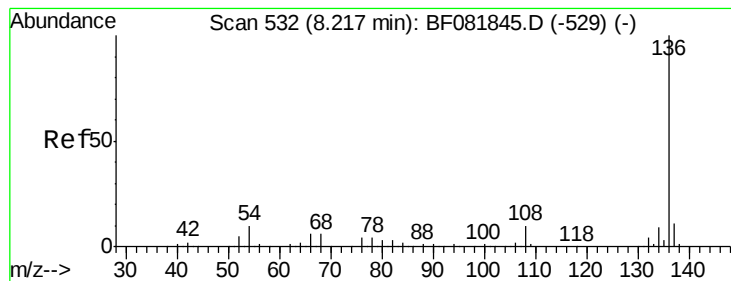

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.22 min Scan# 532
Delta R.T. 0.00 min
Lab File: BF081866.D
Acq: 29 Sep 2015 5:02




Instrument :
BNA_F
ClientSampleId :
LIP-12-9-16-15


Tgt Ion:	136	Resp:	482119
Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.0	13.6
54	8.2	8.2	12.2
68	5.6	5.8	8.6#

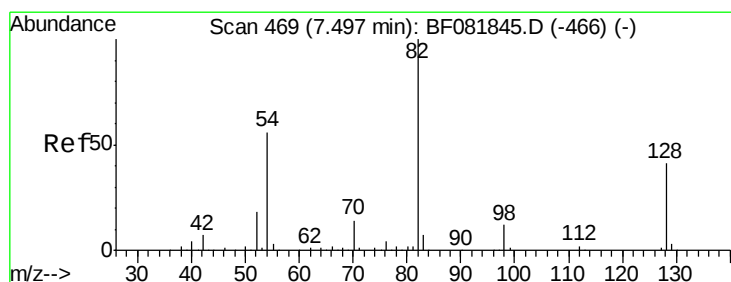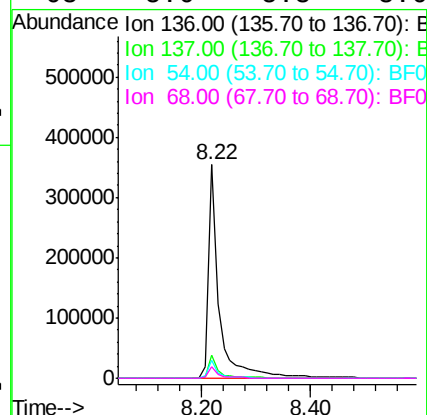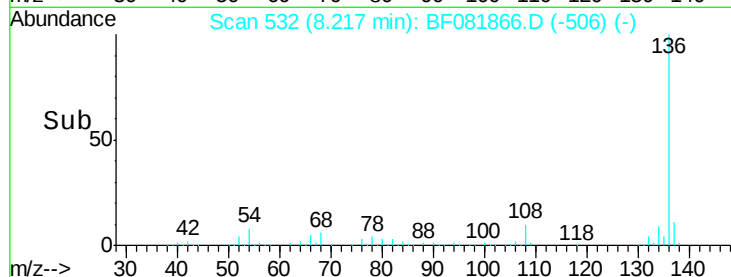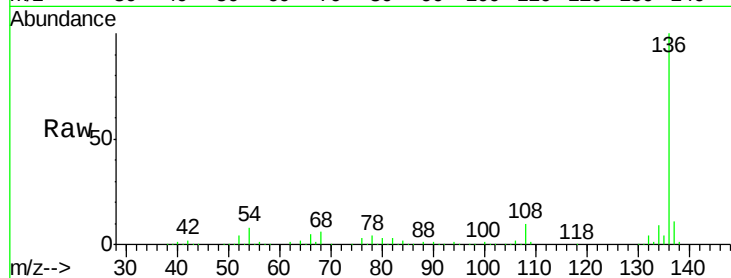

#23
Nitrobenzene-d5
Concen: 106.10 ng
RT: 7.50 min Scan# 469
Delta R.T. 0.00 min
Lab File: BF081866.D
Acq: 29 Sep 2015 5:02

Tgt Ion:	82	Resp:	767402
Ion	Ratio	Lower	Upper
82	100		
128	42.1	51.0	76.6#
54	56.6	47.5	71.3

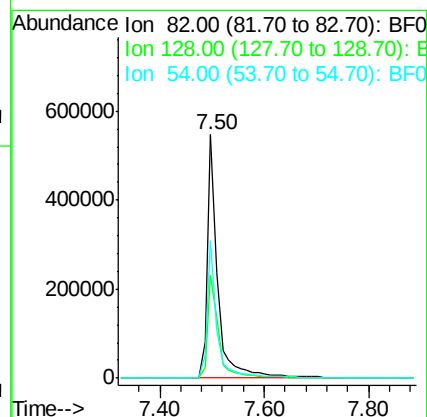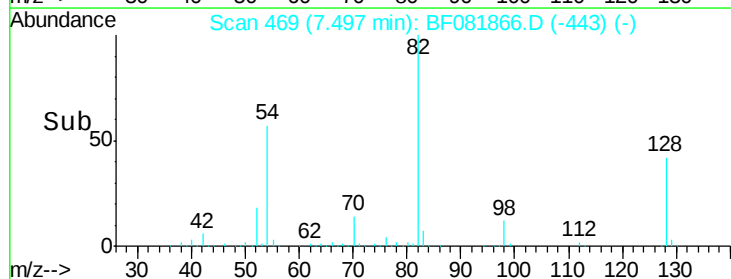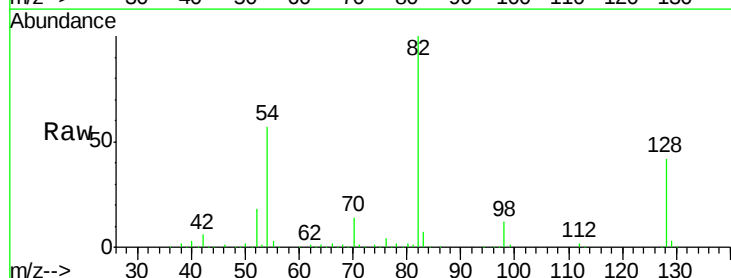

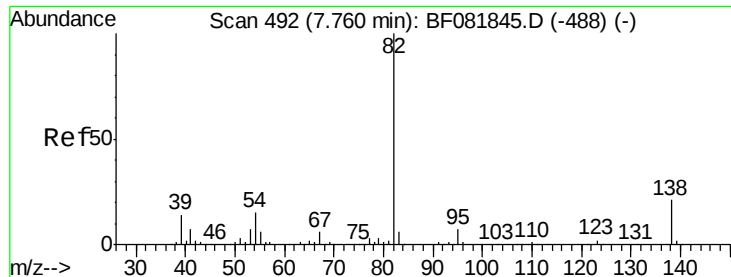

#25

Isophorone

Concen: 49.18 ng

RT: 7.50 min Scan# 469

Delta R.T. -0.26 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02

Instrument :

BNA_F

ClientSampleId :

LIP-12-9-16-15


Tgt Ion: 82 Resp: 705069

Ion Ratio Lower Upper

82 100

95 0.0 4.0 6.0#




138 0.0 18.3 27.5#

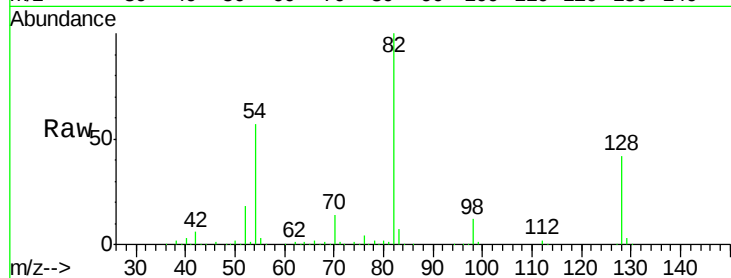

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 138.00 (137.70 to 138.70): E

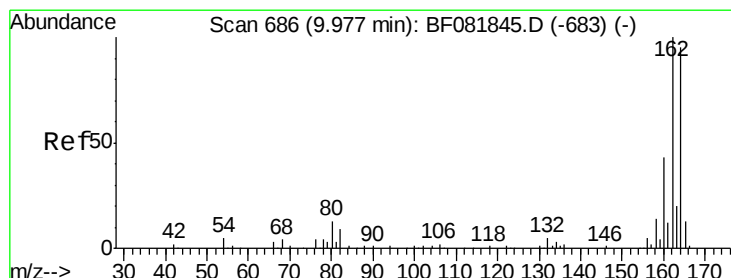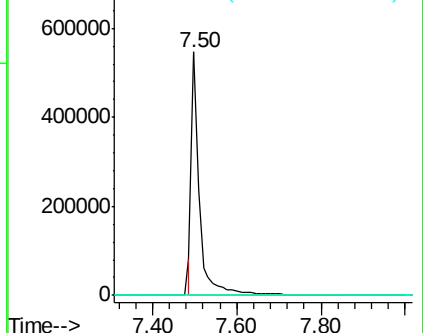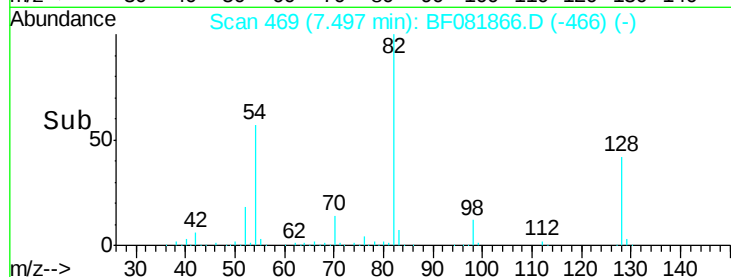

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.98 min Scan# 686

Delta R.T. 0.00 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02


Tgt Ion: 164 Resp: 231633

Ion Ratio Lower Upper

164 100

162 103.1 75.2 112.8



160 45.8 31.5 47.3

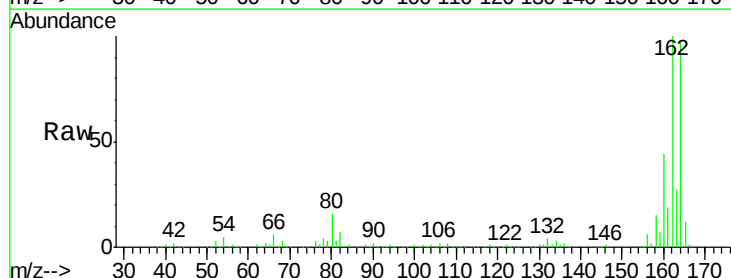


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



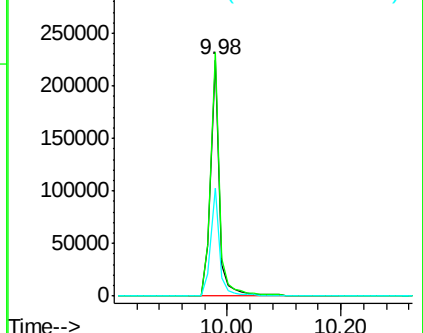
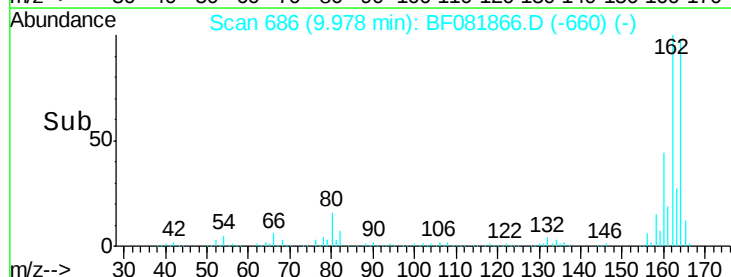


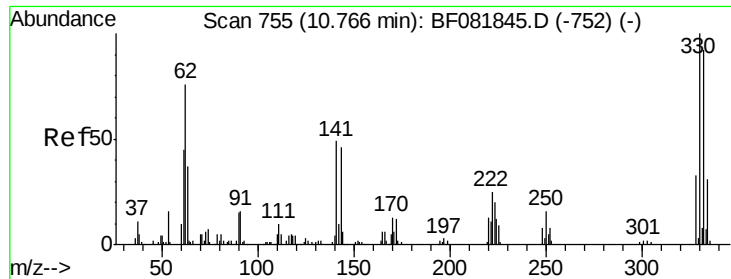

#41
 2,4,6-Tribromophenol
 Concen: 147.80 ng
 RT: 10.77 min Scan# 755
 Delta R.T. 0.00 min
 Lab File: BF081866.D
 Acq: 29 Sep 2015 5:02




Instrument :
 BNA_F
 ClientSampleId :
 LIP-12-9-16-15


Tgt Ion:330 Resp: 346718
 Ion Ratio Lower Upper
 330 100
 332 95.3 76.6 114.8
 141 33.6 29.7 44.5

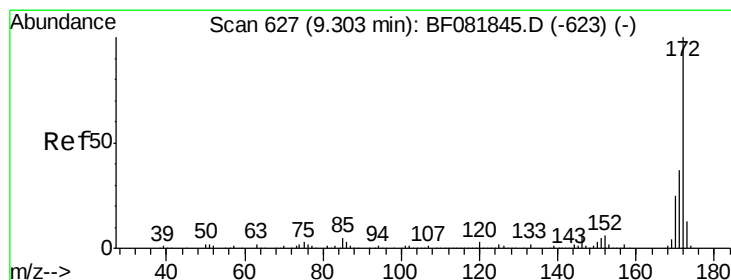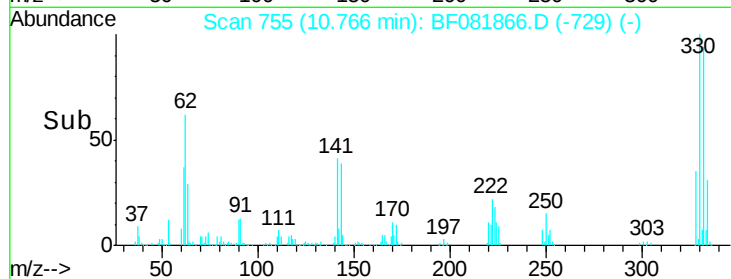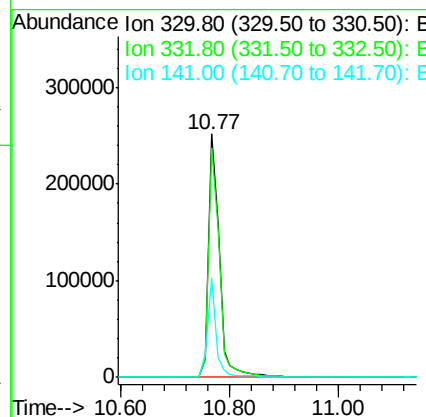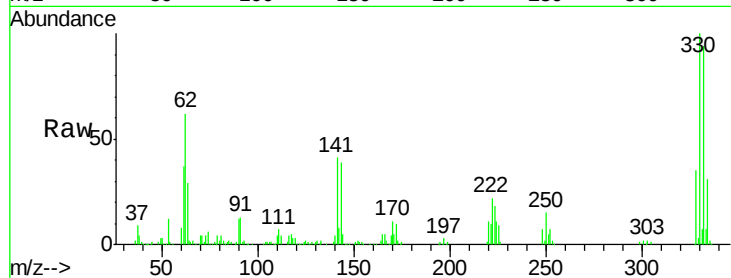

#44
 2-Fluorobiphenyl
 Concen: 118.86 ng
 RT: 9.30 min Scan# 627
 Delta R.T. 0.00 min
 Lab File: BF081866.D
 Acq: 29 Sep 2015 5:02

Tgt Ion:172 Resp: 1520349
 Ion Ratio Lower Upper
 172 100
 171 36.6 26.1 39.1
 170 25.0 17.4 26.2


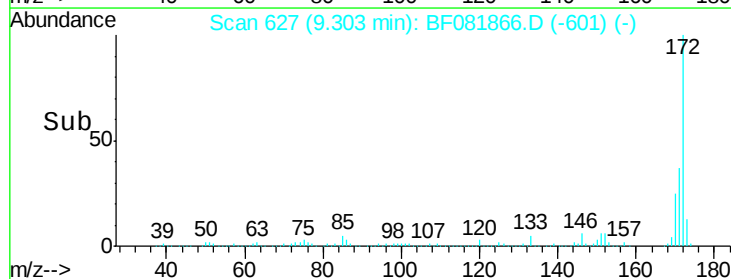
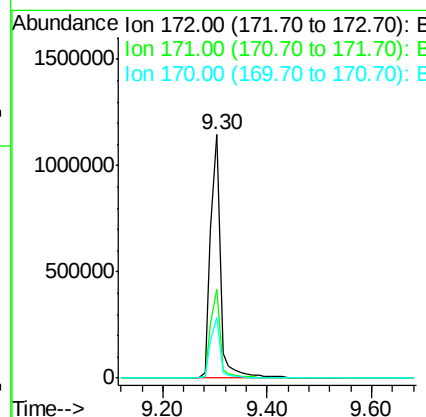
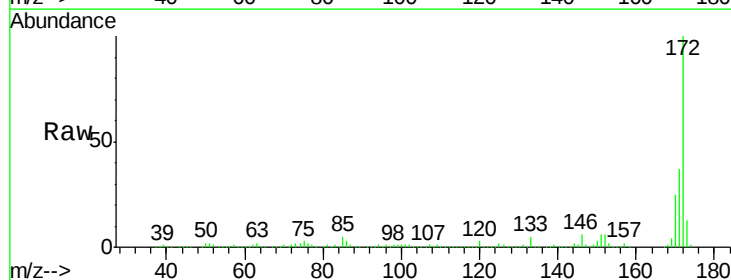


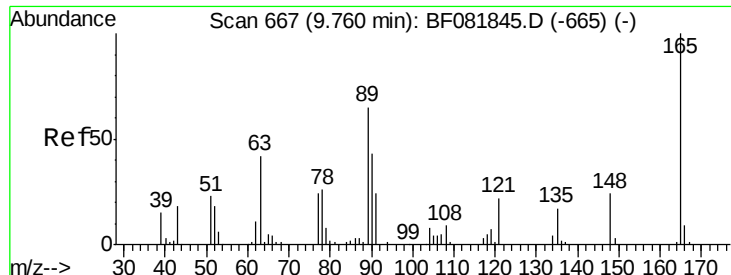

#50
 2,6-Dinitrotoluene
 Concen: 8.16 ng
 RT: 9.98 min Scan# 686
 Delta R.T. 0.22 min
 Lab File: BF081866.D
 Acq: 29 Sep 2015 5:02




Instrument :
 BNA_F
 ClientSampleId :
 LIP-12-9-16-15


Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	32.3	48.5#
89	1.3	28.6	43.0#

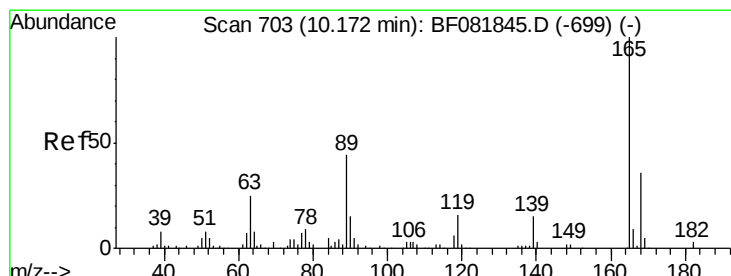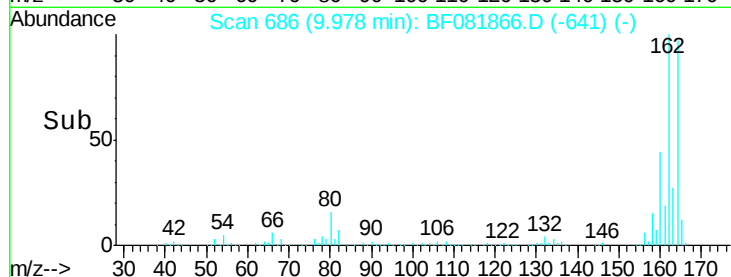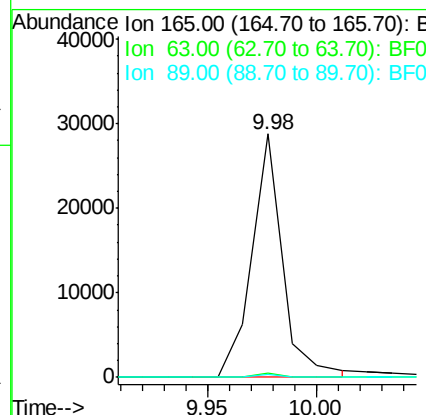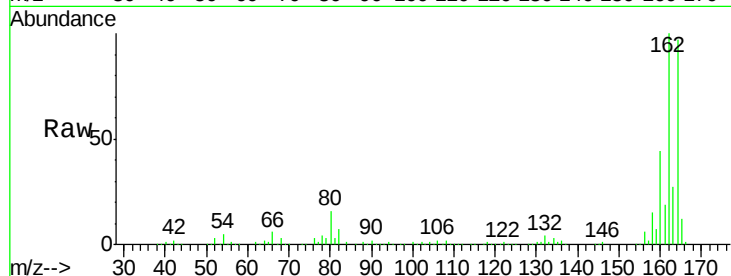

#56
 2,4-Dinitrotoluene
 Concen: 6.66 ng
 RT: 9.98 min Scan# 686
 Delta R.T. -0.19 min
 Lab File: BF081866.D
 Acq: 29 Sep 2015 5:02

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	29.8	44.6#
89	1.3	44.5	66.7#
182	0.0	3.0	4.4#

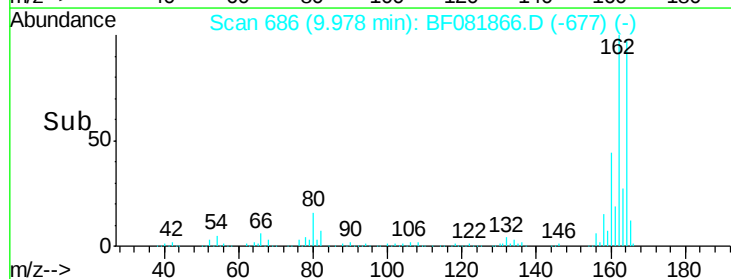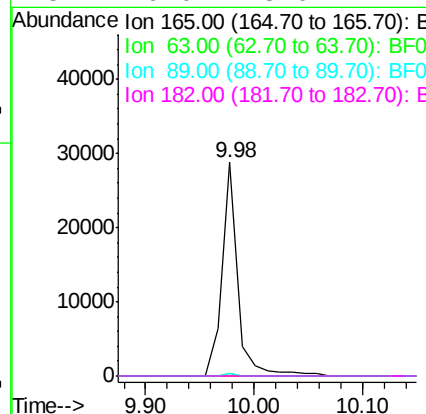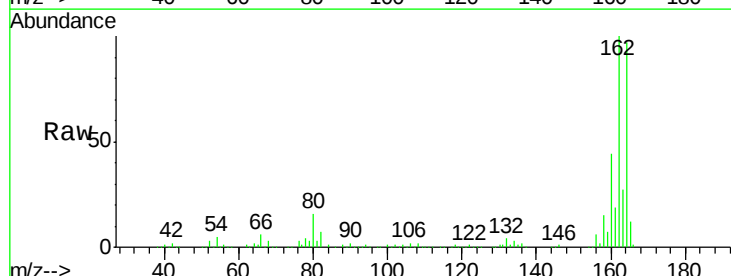


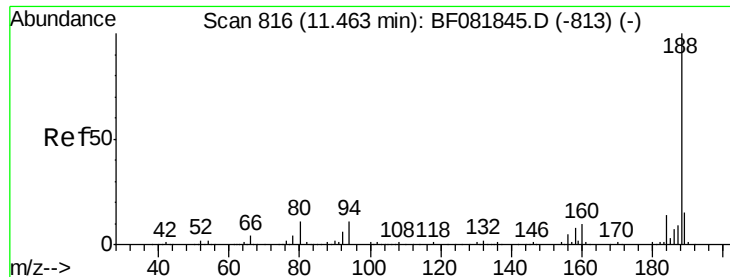




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.46 min Scan# 816
Delta R.T. 0.00 min
Lab File: BF081866.D
Acq: 29 Sep 2015 5:02

Instrument :
BNA_F
ClientSampleId :
LIP-12-9-16-15

Tgt Ion:188 Resp: 432445
Ion Ratio Lower Upper
188 100
94 9.3 11.1 16.7#
80 10.0 11.0 16.4#

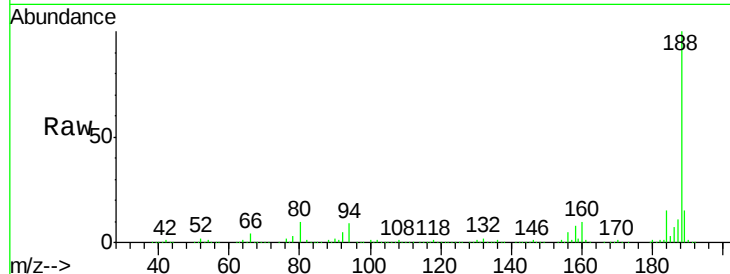


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

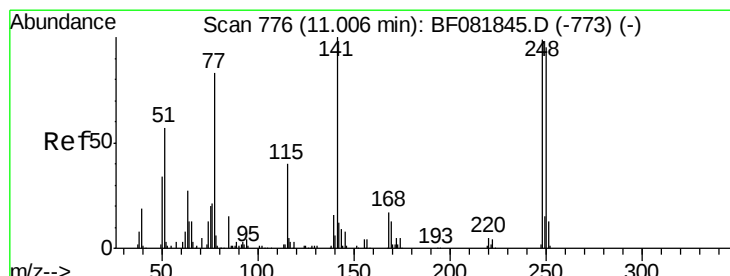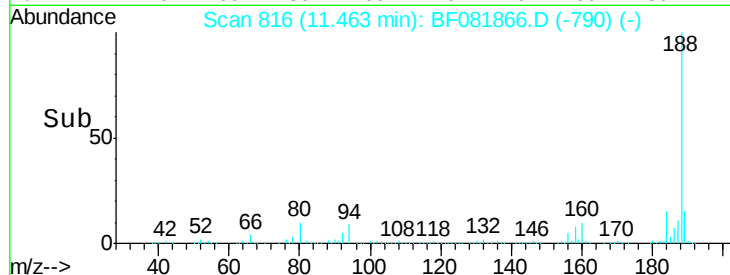
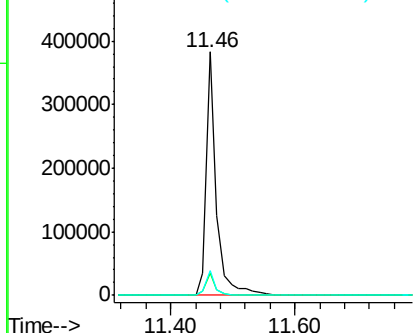



#66
4-Bromophenyl-phenylether
Concen: 4.97 ng
RT: 10.77 min Scan# 755
Delta R.T. -0.24 min
Lab File: BF081866.D
Acq: 29 Sep 2015 5:02

Tgt Ion:248 Resp: 21653
Ion Ratio Lower Upper
248 100
250 199.8 78.5 117.7#
141 542.5 59.0 88.6#

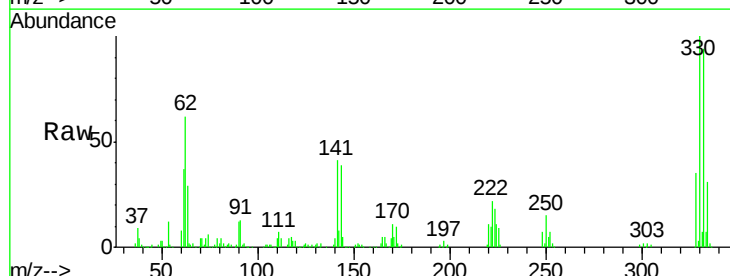

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

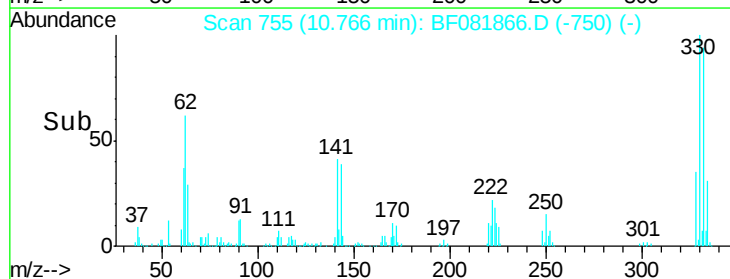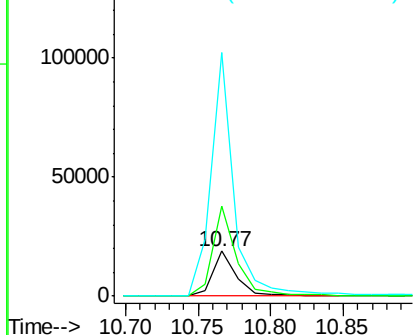

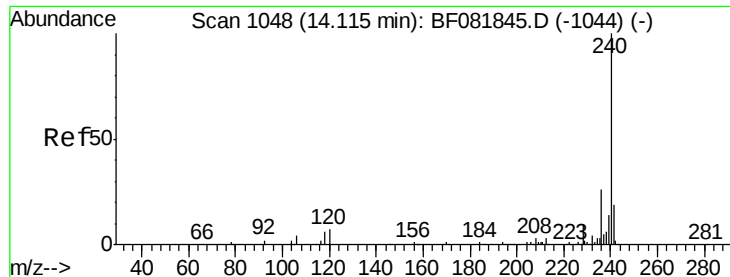

#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.10 min Scan# 1047

Delta R.T. -0.01 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02

Instrument :

BNA_F

ClientSampleId :

LIP-12-9-16-15


Tgt Ion:240 Resp: 370874

Ion Ratio Lower Upper

240 100

120 12.9 16.2 24.2#




236 26.2 18.4 27.6

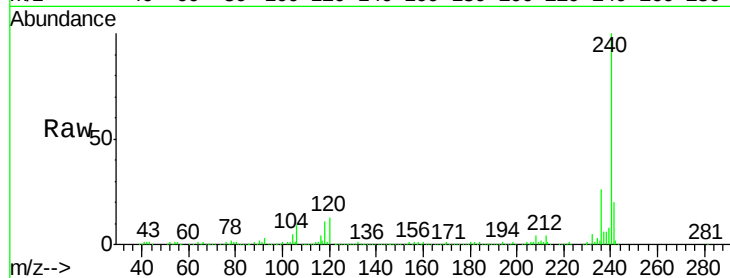

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

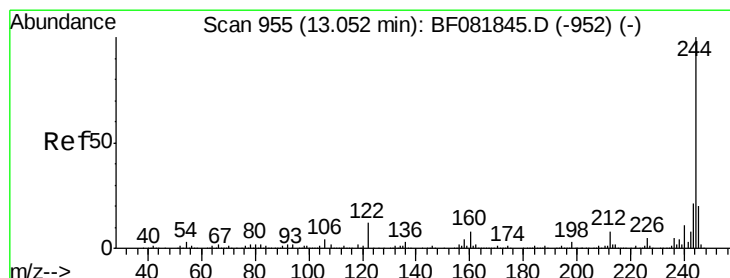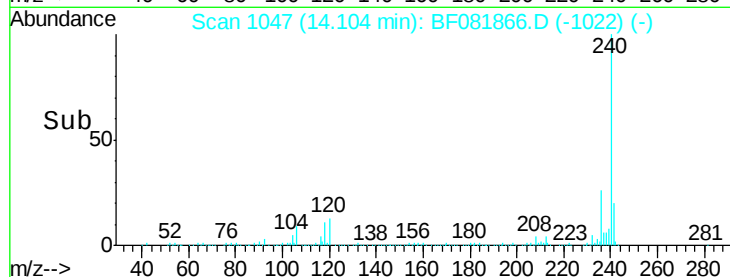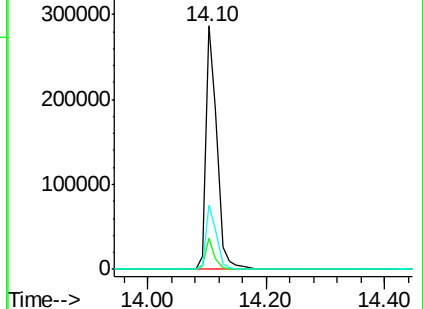

#78

Terphenyl-d14

Concen: 127.71 ng

RT: 13.05 min Scan# 955

Delta R.T. 0.00 min

Lab File: BF081866.D

Acq: 29 Sep 2015 5:02


Tgt Ion:244 Resp: 1269376

Ion Ratio Lower Upper

244 100

212 7.9 4.3 6.5#



122 12.2 17.4 26.2#

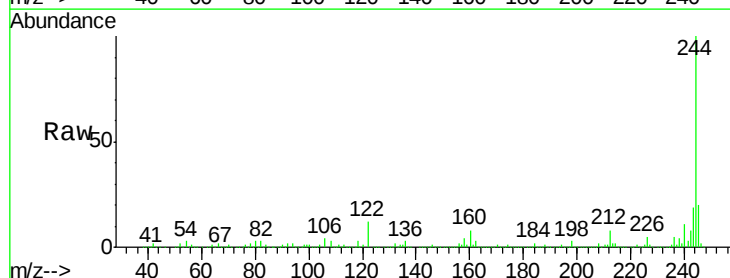


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

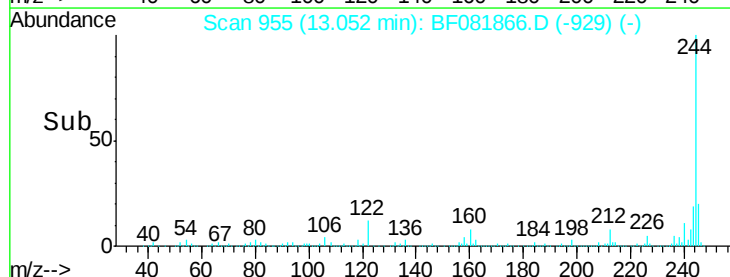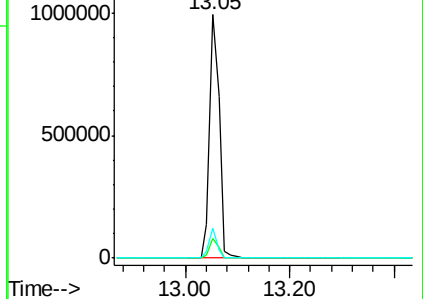

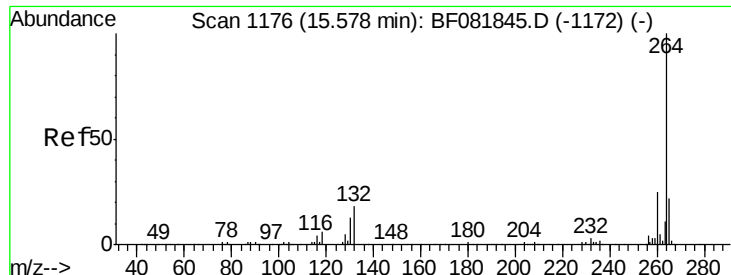

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.58 min Scan# 1176
Delta R.T. 0.00 min
Lab File: BF081866.D
Acq: 29 Sep 2015 5:02

Instrument :
BNA_F
ClientSampleId :
LIP-12-9-16-15

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.3	16.7	25.1
265	21.8	17.2	25.8

