
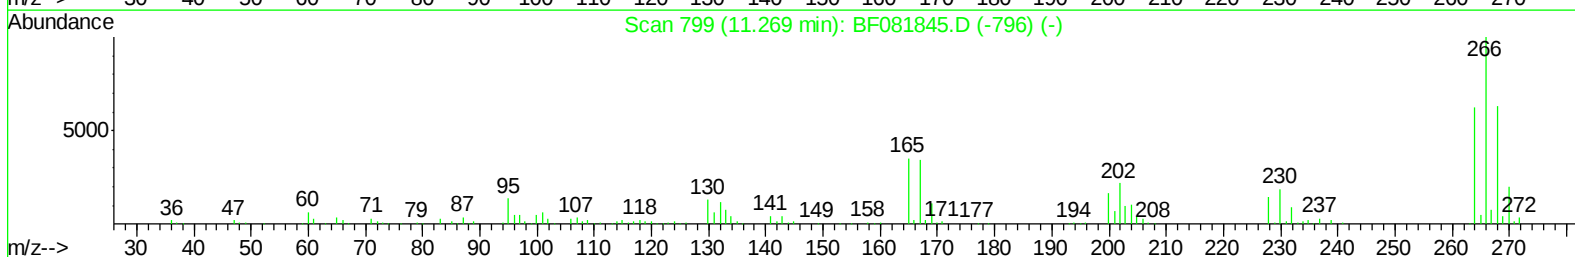
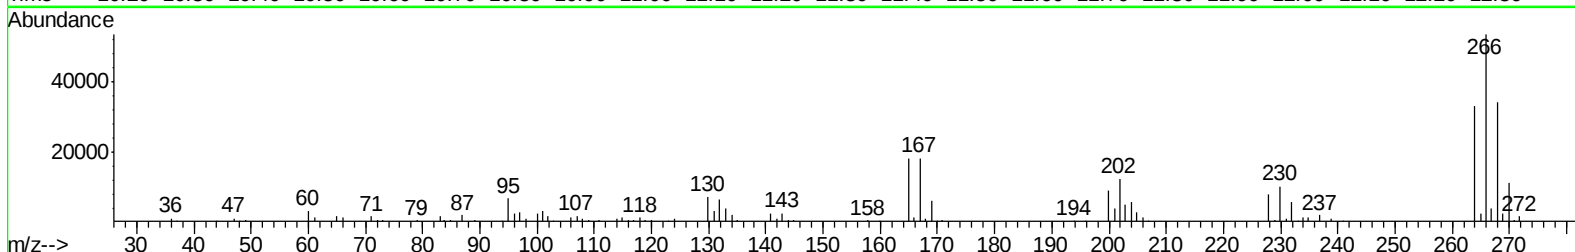


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF093015\
Data File : BF081910.D
Acq On : 30 Sep 2015 19:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 01 06:47:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 05:22:05 2015
Response via : Initial Calibration

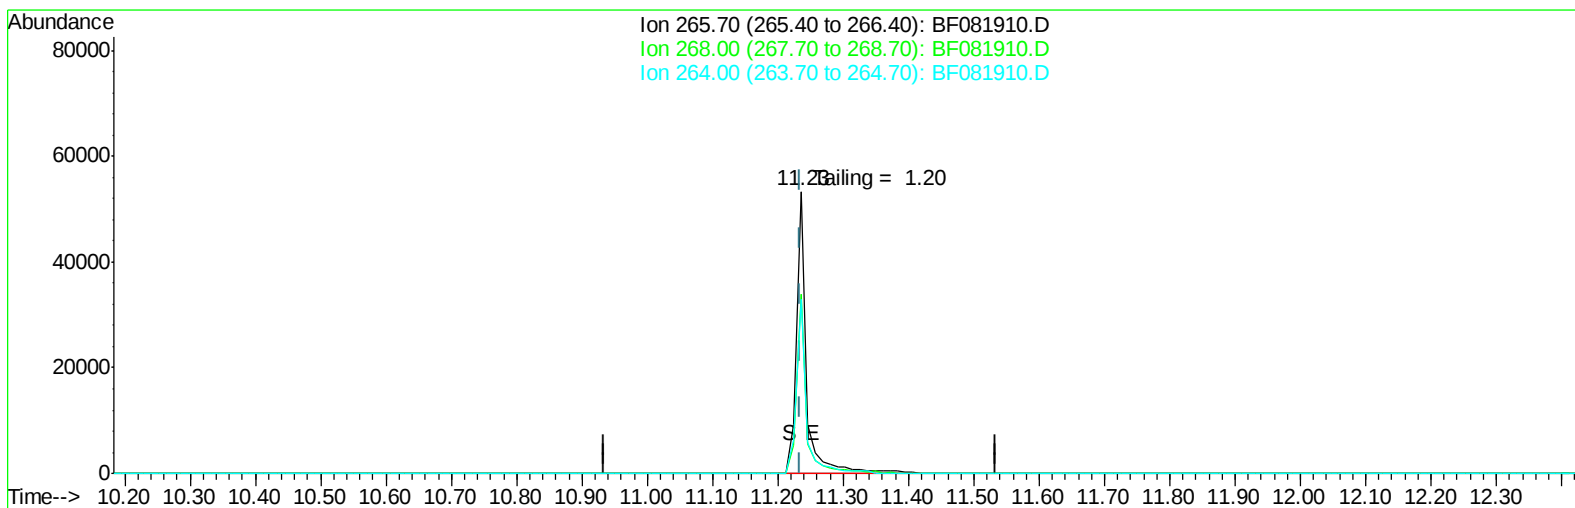

TIC: BF081910.D

(69) Pentachlorophenol (C)

11.235min (-0.000) 32998.60ng




response 59265

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.73
264.00	62.70	61.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF093015\
Data File : BF081910.D
Acq On : 30 Sep 2015 19:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 01 06:47:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 05:22:05 2015
Response via : Initial Calibration

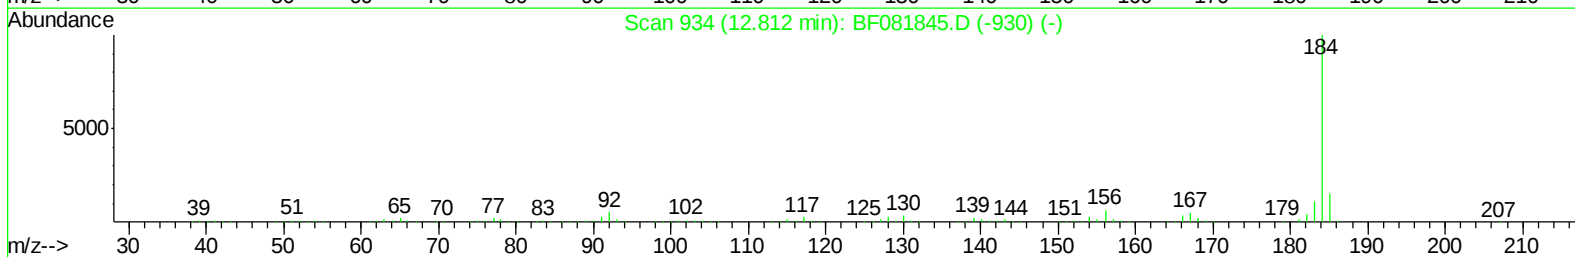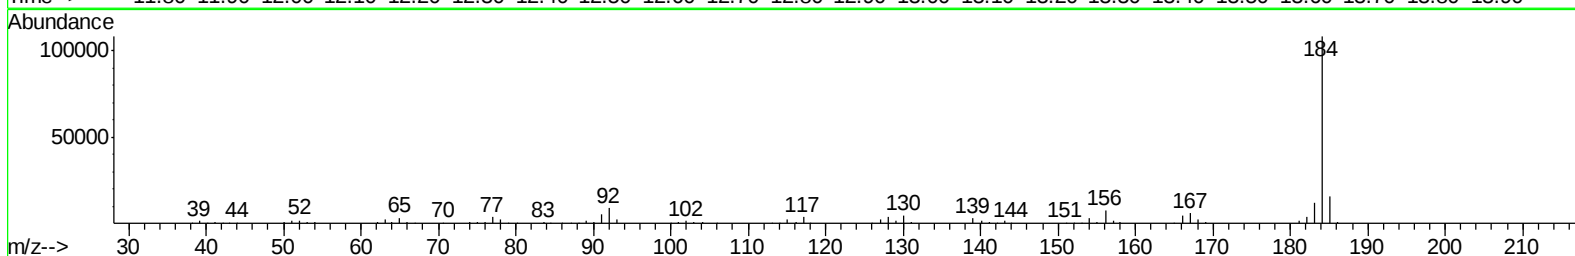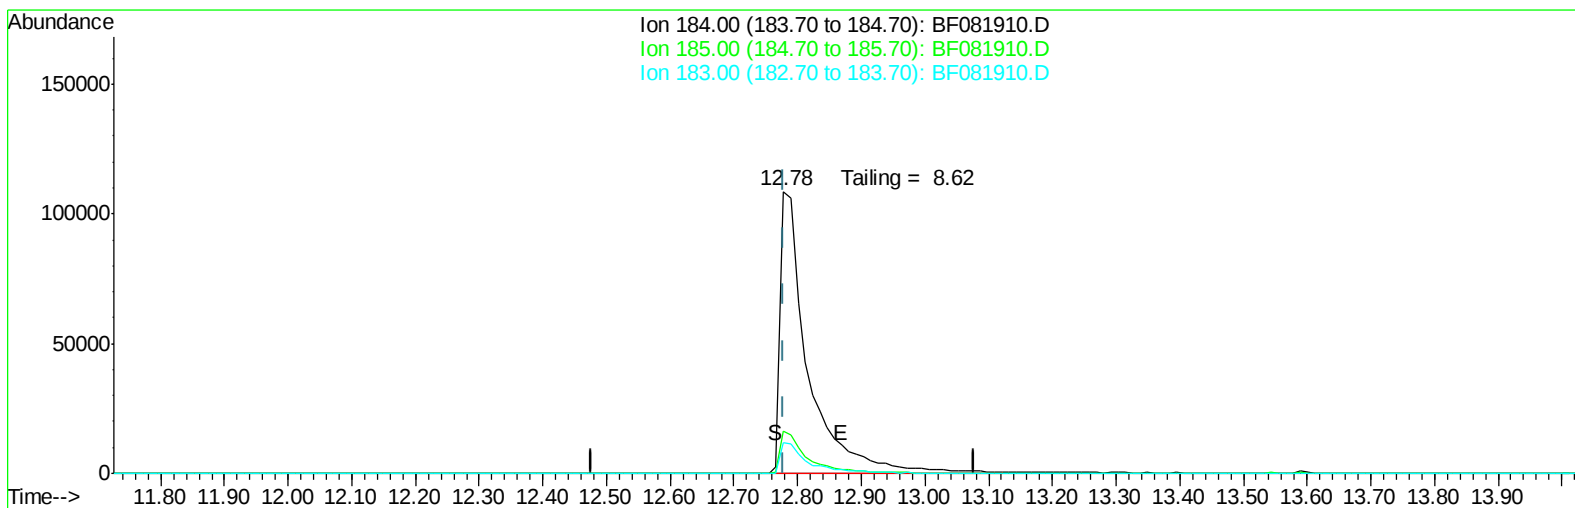

TIC: BF081910.D

(76) Benzidine

12.778min (-0.000) 0.00ng




response 324169

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.97
183.00	9.50	10.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF093015\
Data File : BF081910.D
Acq On : 30 Sep 2015 19:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 01 06:47:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 05:22:05 2015
Response via : Initial Calibration

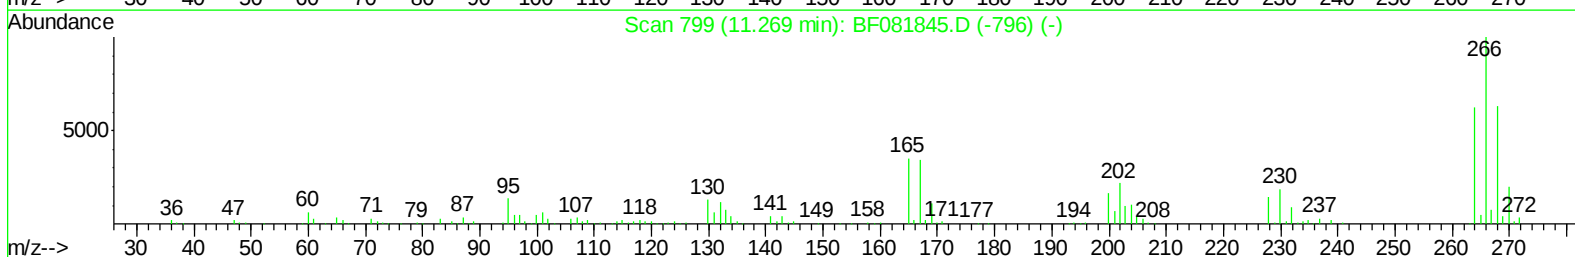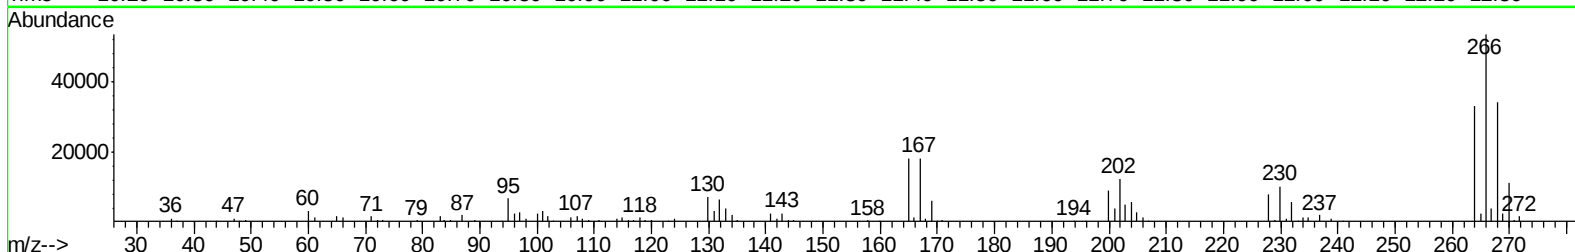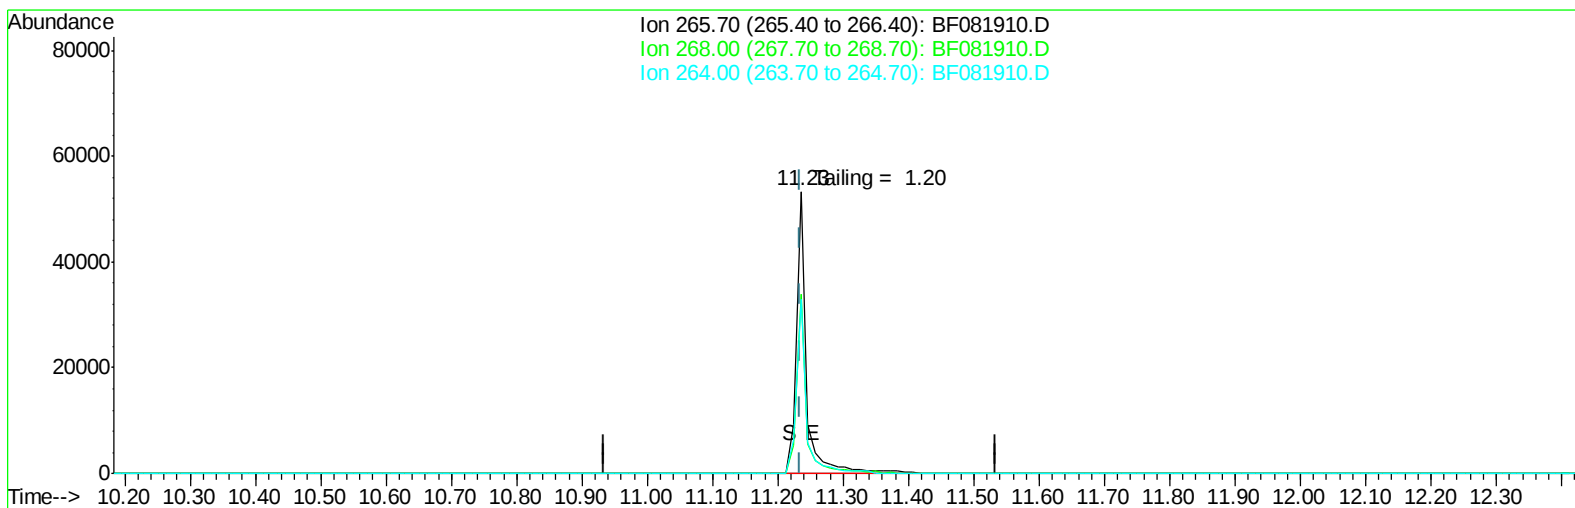

TIC: BF081910.D

(69) Pentachlorophenol (C)

11.235min (-0.000) 32998.60ng




response 59265

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.73
264.00	62.70	61.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF093015\
Data File : BF081910.D
Acq On : 30 Sep 2015 19:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 01 06:47:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 05:22:05 2015
Response via : Initial Calibration

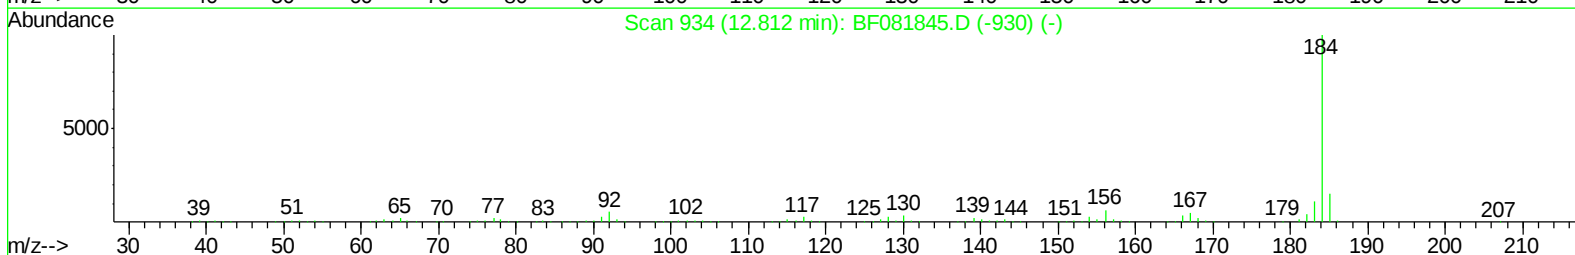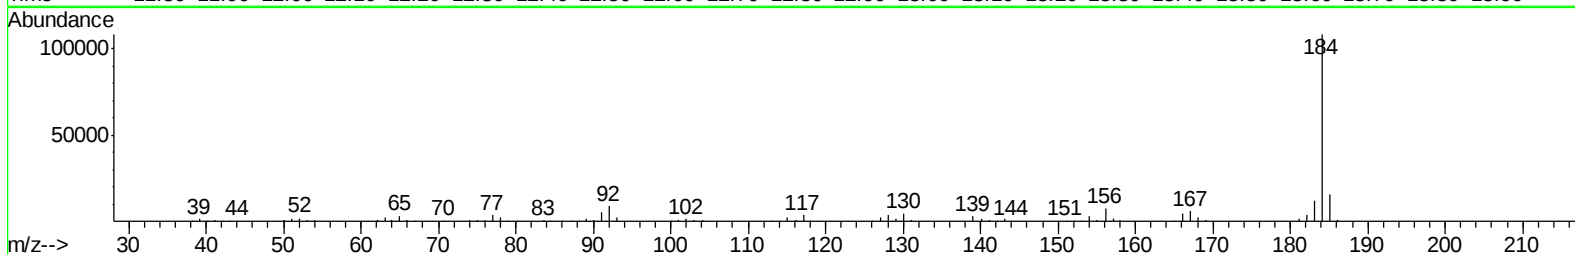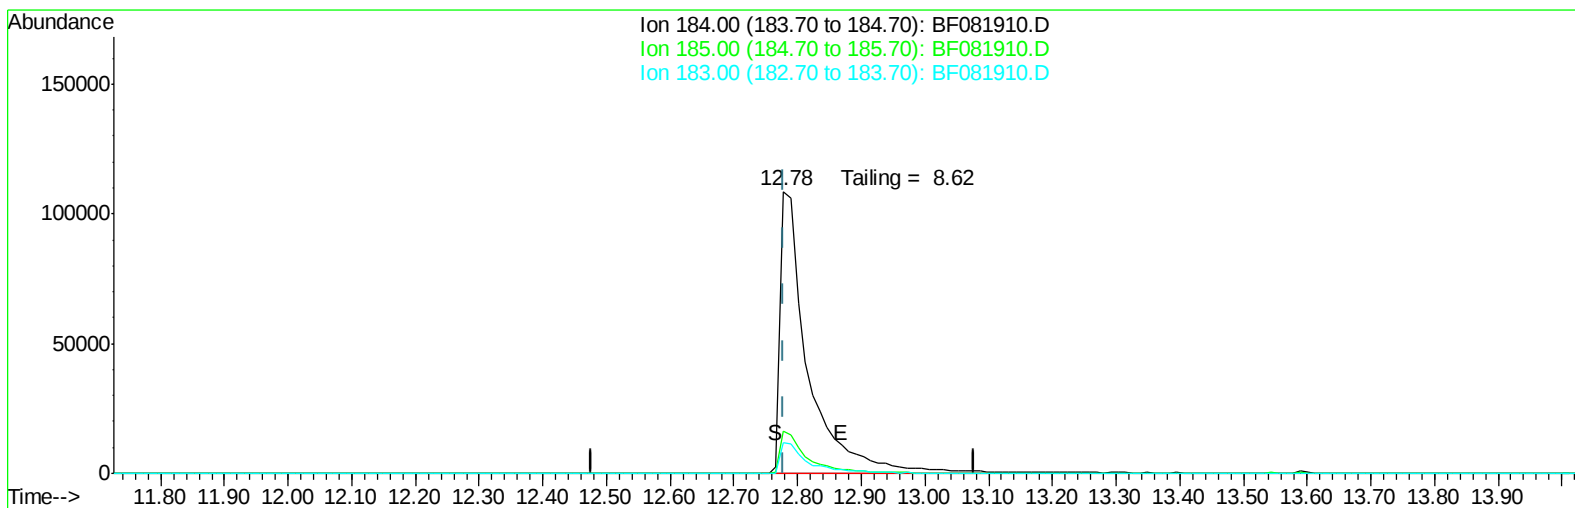

TIC: BF081910.D

(76) Benzidine

12.778min (-0.000) 0.00ng

response 324169

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.97
183.00	9.50	10.90
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF093015\
 Data File : BF081910.D
 Acq On : 30 Sep 2015 19:17
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 01 06:47:34 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 01 05:22:05 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-6.90
21) Naphthalene-d8	0.00	136	0	0.00	ng	-8.19
38) Acenaphthene-d10	0.00	164	0	0.00	ng	-9.95
63) Phenanthrene-d10	11.68	188	277	20.00	ng	0.24
75) Chrysene-d12	0.00	240	0	0.00	ng	-14.08
86) Perylene-d12	0.00	264	0	0.00	ng	-15.53
System Monitoring Compounds						
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	0.00	82	0	0.00	ng	
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	0.00	172	0	0.00	ng	
78) Terphenyl-d14	13.02	244	1454	0.00	ng	0.00
Target Compounds						
68) Atrazine	11.23	200	10507	4040.54	ng	Qvalue # 27
69) Pentachlorophenol	11.23	266	59265	32998.60	ng	98
70) Phenanthrene	11.68	178	211	14.71	ng	# 1
71) Anthracene	11.68	178	211	14.99	ng	# 1
72) Carbazole	11.68	167	3556	279.07	ng	# 79
73) Di-n-butylphthalate	11.99	149	2962	233.87	ng	# 78
74) Fluoranthene	12.88	202	906	61.06	ng	60

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF093015\
Data File : BF081910.D
Acq On : 30 Sep 2015 19:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 01 06:47:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 05:22:05 2015
Response via : Initial Calibration

