
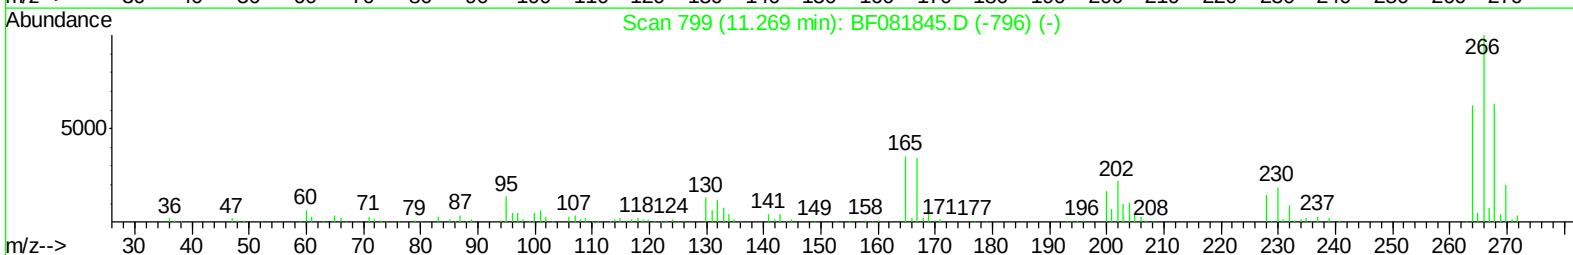
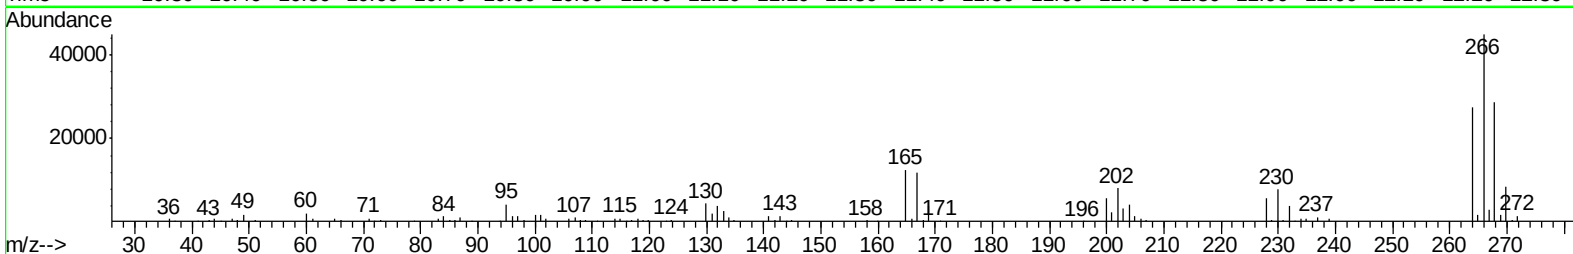


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092815\
Data File : BF081841.D
Acq On : 28 Sep 2015 12:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 18:37:46 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration

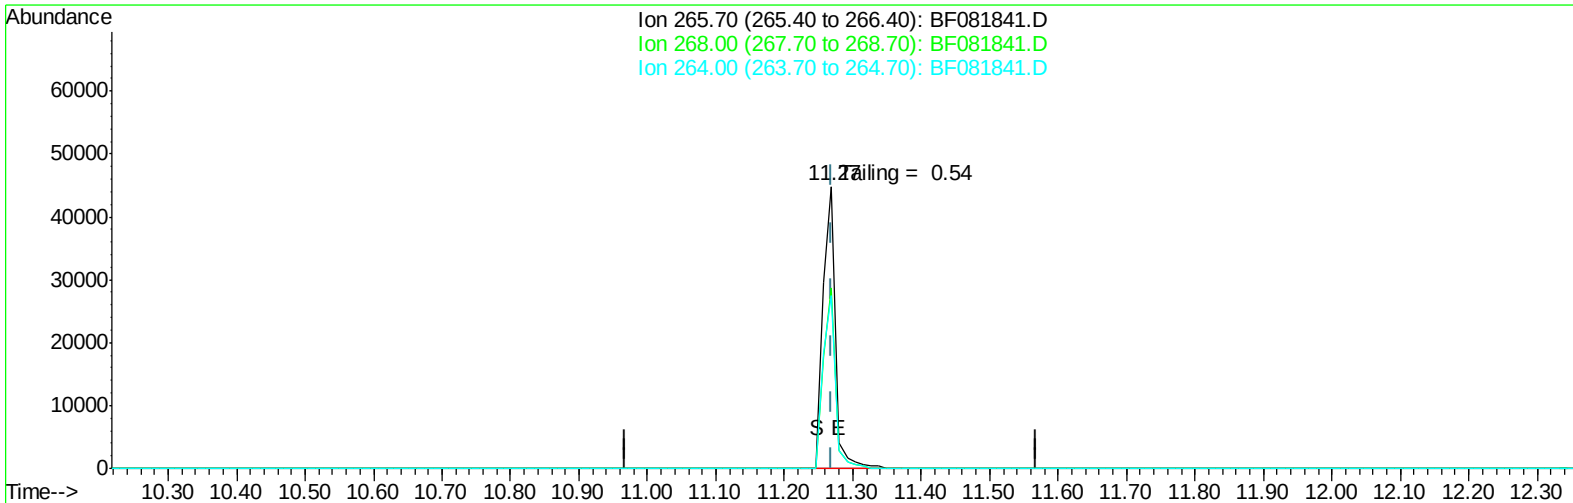

TIC: BF081841.D

(69) Pentachlorophenol (C)




11.269min (+0.000) 0.00ng

response 56487

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	64.11
264.00	62.70	61.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092815\
 Data File : BF081841.D
 Acq On : 28 Sep 2015 12:33
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 18:37:46 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 18:10:42 2015
 Response via : Initial Calibration

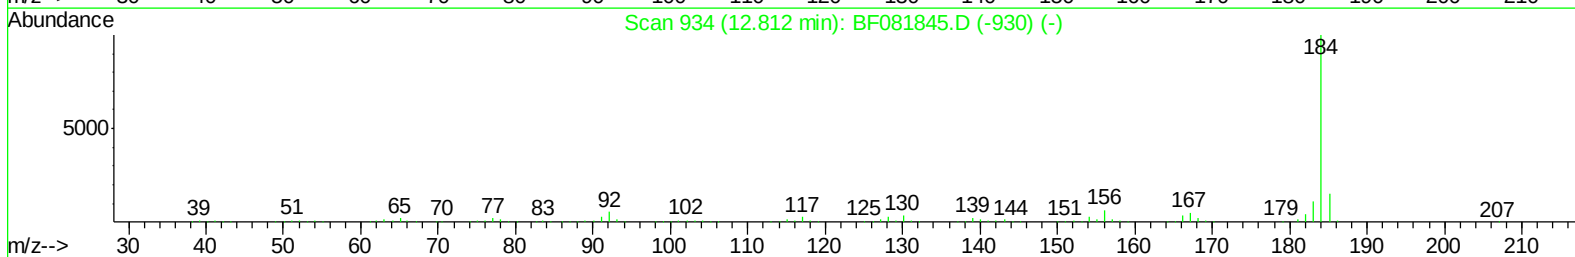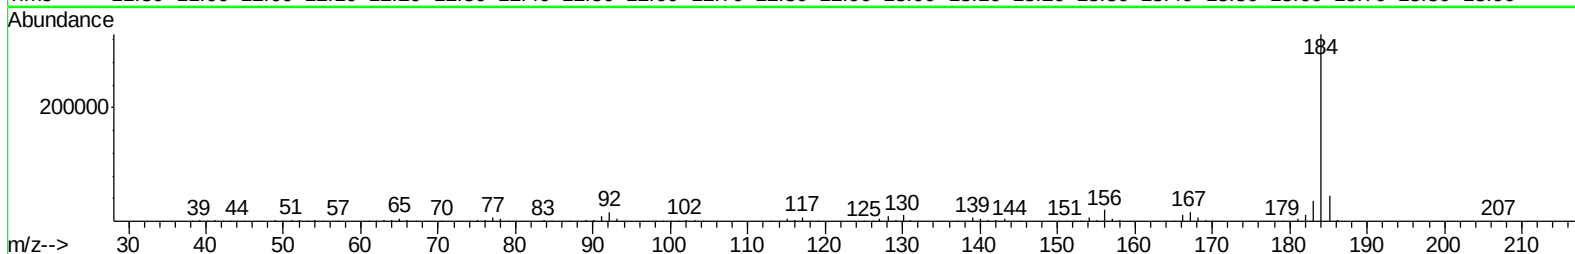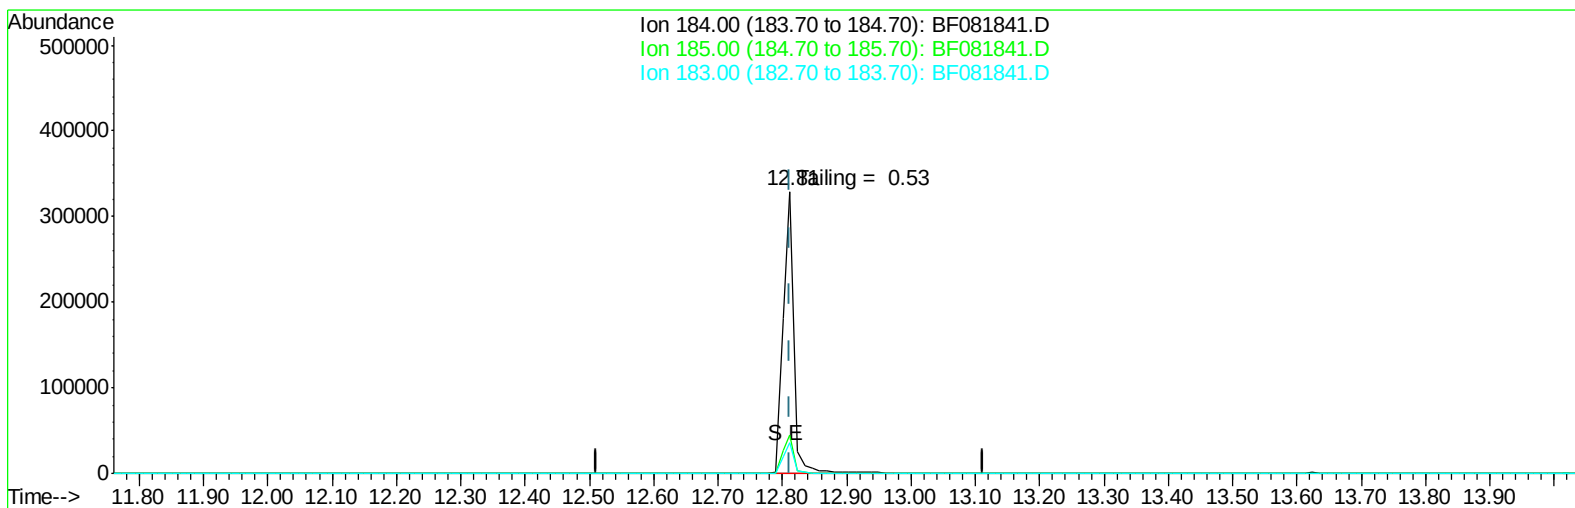

TIC: BF081841.D

(76) Benzidine

12.812min (+0.000) 0.00ng

response 392053

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.87
183.00	9.50	10.93
0.00	0.00	0.00