


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092815\
Data File : BF081841.D
Acq On : 28 Sep 2015 12:33
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 28 18:10:42 2015

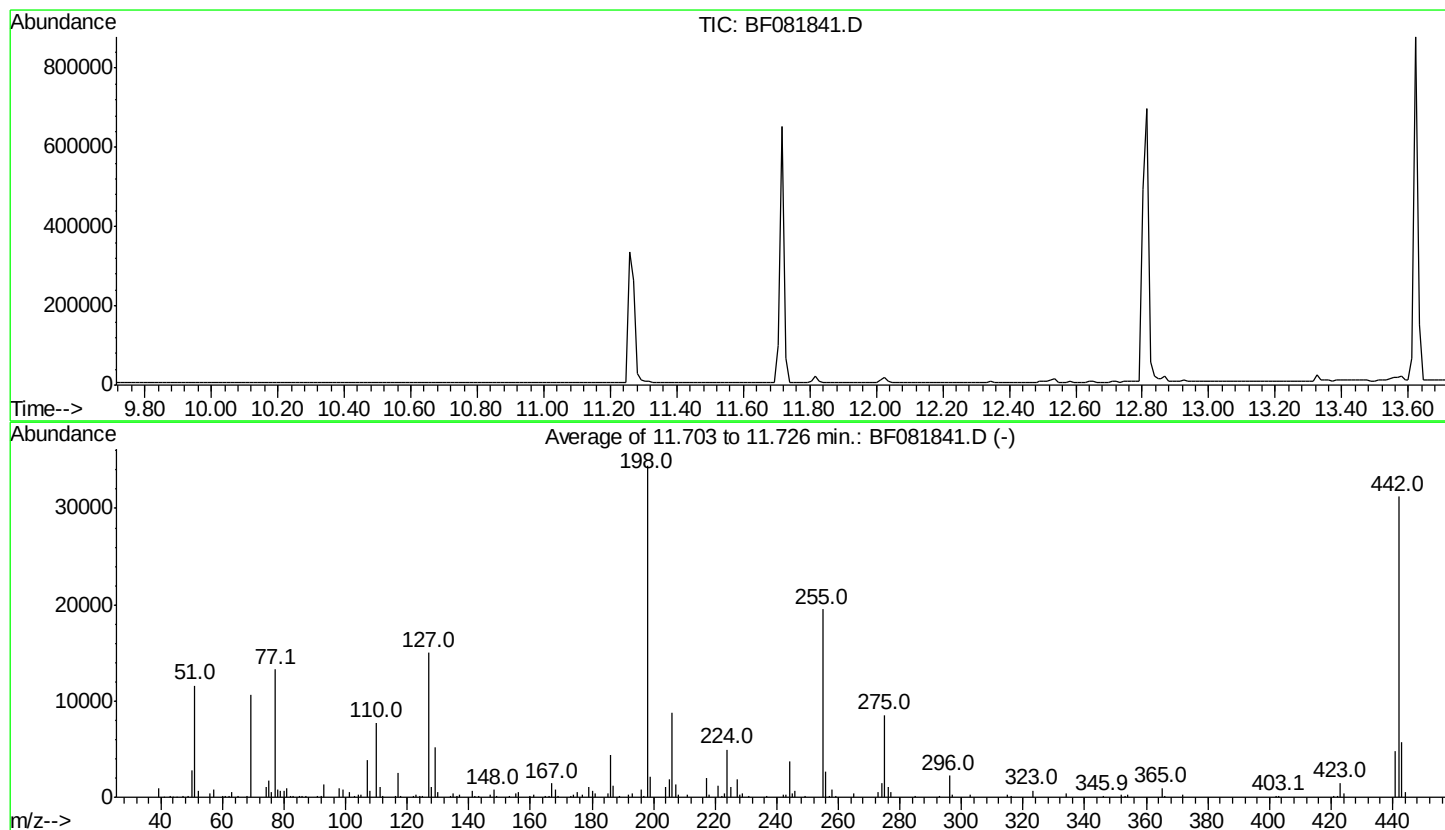

AutoFind: Scans 837, 838, 839; Background Corrected with Scan 834

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	11599	PASS
68	69	0.00	2	1.0	111	PASS
69	198	0.00	100	31.1	10711	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.5	14987	PASS
197	198	0.00	2	0.5	164	PASS
198	198	100	100	100.0	34453	PASS
199	198	5	9	6.4	2194	PASS
275	198	10	60	24.8	8555	PASS
365	198	1	100	2.9	991	PASS
441	442	0.01	24	15.3	4781	PASS
442	198	50	100	90.6	31231	PASS
443	442	15	24	18.4	5756	PASS