
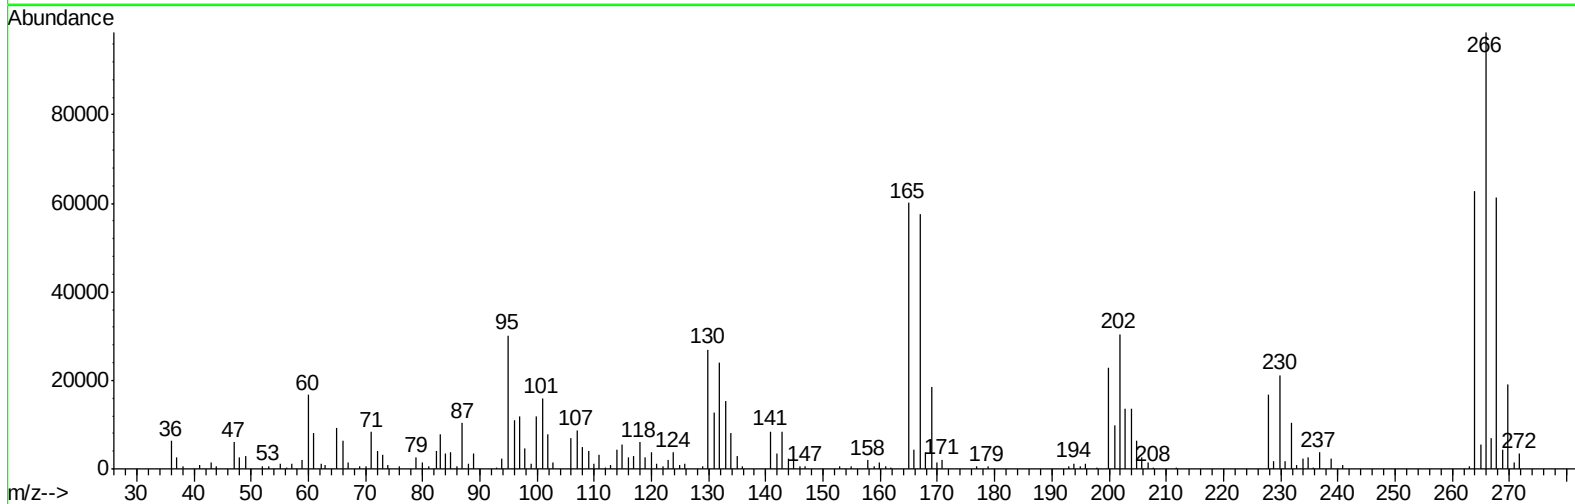


Data Path : Z:\HPCHEM1\BNA F\Data\BF092817\
Data File : BF098898.D
Acq On : 28 Sep 2017 10:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 07:07:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

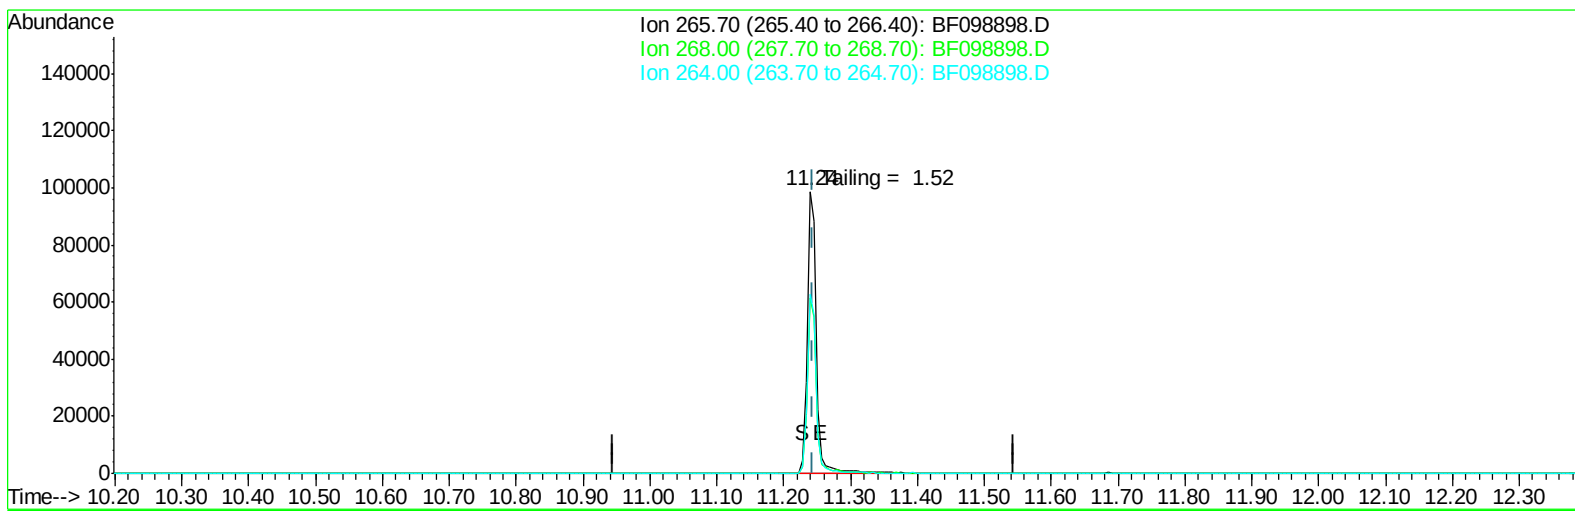

TIC: BF098898.D

(69) Pentachlorophenol (C)



11.239min (-0.006) 11286.51ng

response 94510

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.26
264.00	61.90	63.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF092817\
Data File : BF098898.D
Acq On : 28 Sep 2017 10:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 07:07:00 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

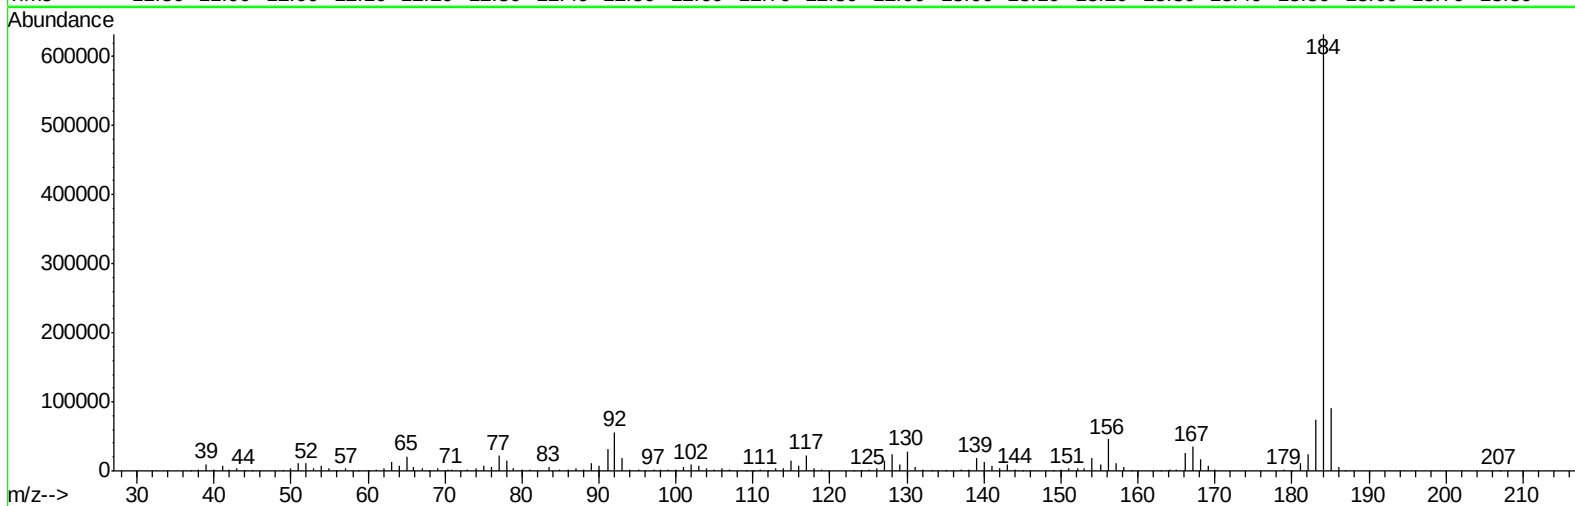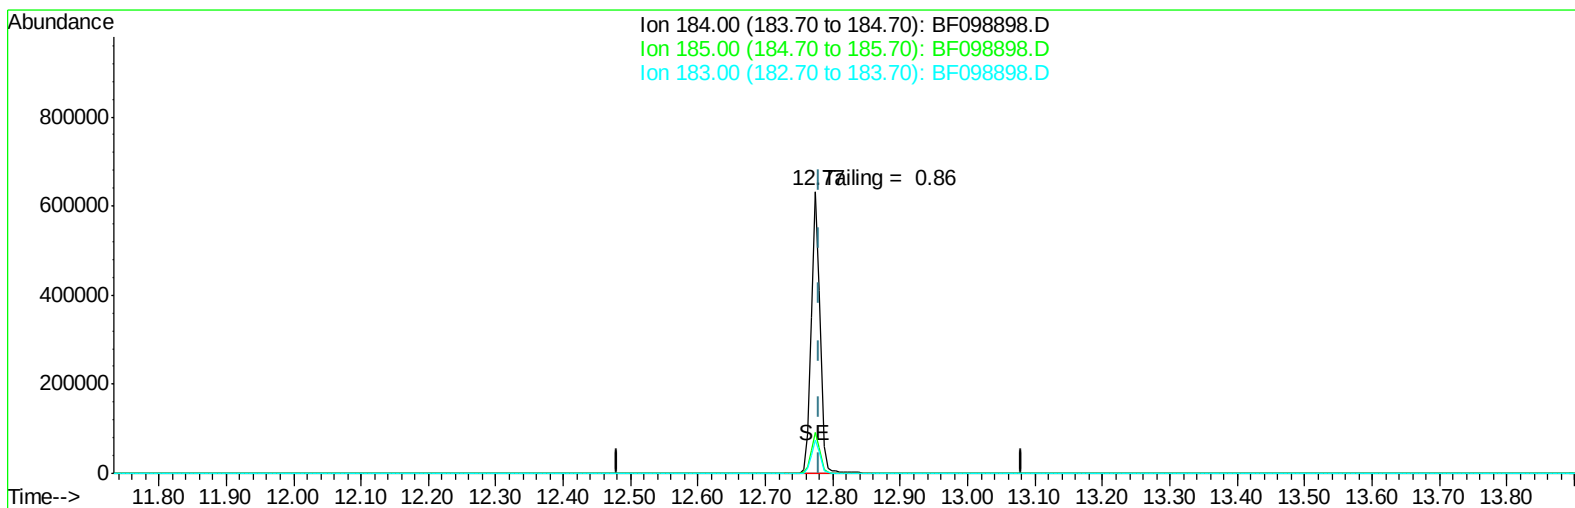

TIC: BF098898.D

(76) Benzidine

12.774min (-0.006) 12594.41ng

response 566441

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.50
183.00	11.60	11.67
0.00	0.00	0.00