
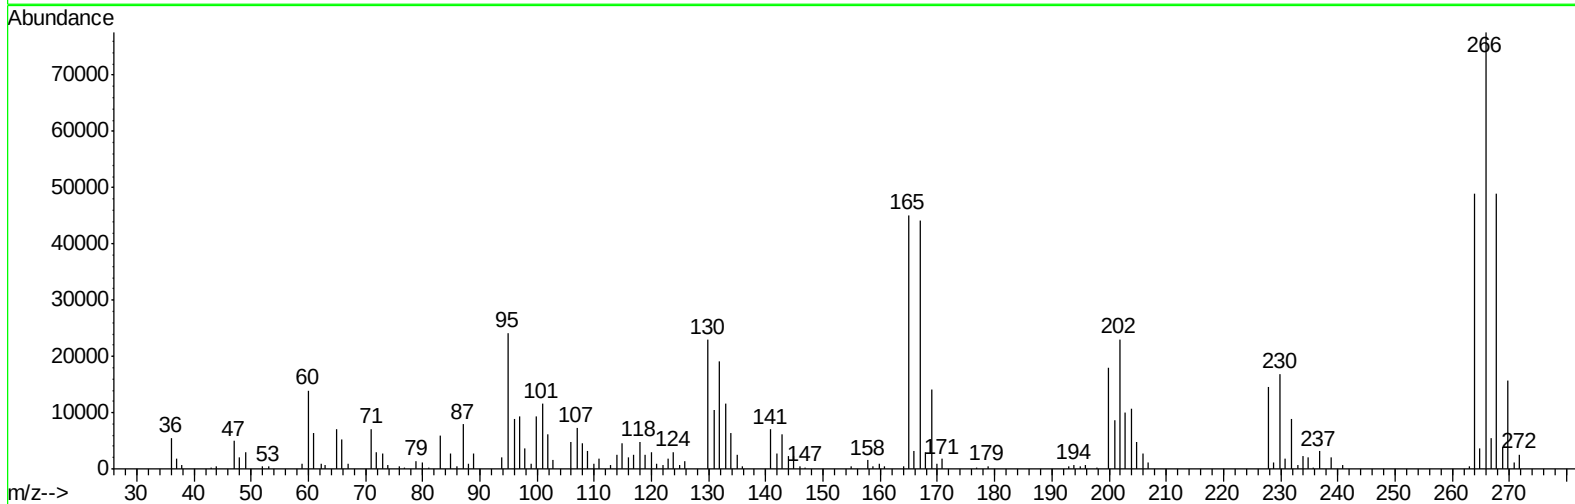


Data Path : Z:\HPCHEM1\BNA F\Data\BF092817\
Data File : BF098912.D
Acq On : 28 Sep 2017 17:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 07:08:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

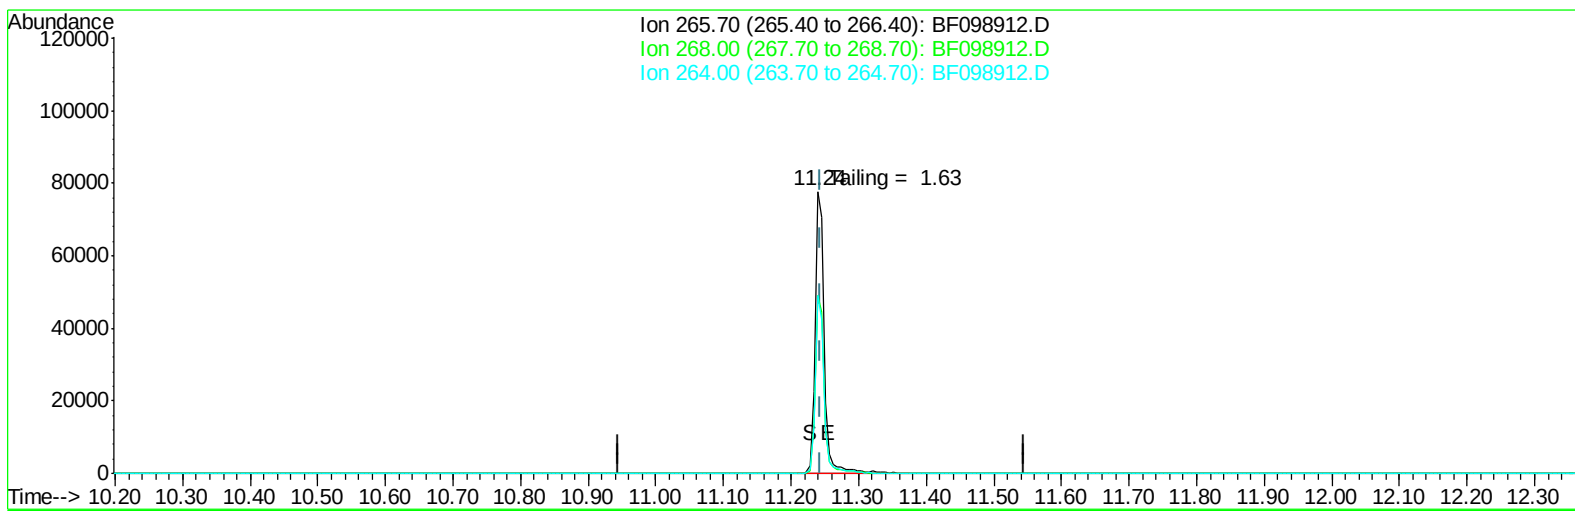

TIC: BF098912.D

(69) Pentachlorophenol (C)



11.239min (-0.006) 80757.08ng

response 74612

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.00
264.00	61.90	63.12
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF092817\
Data File : BF098912.D
Acq On : 28 Sep 2017 17:39
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 07:08:15 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

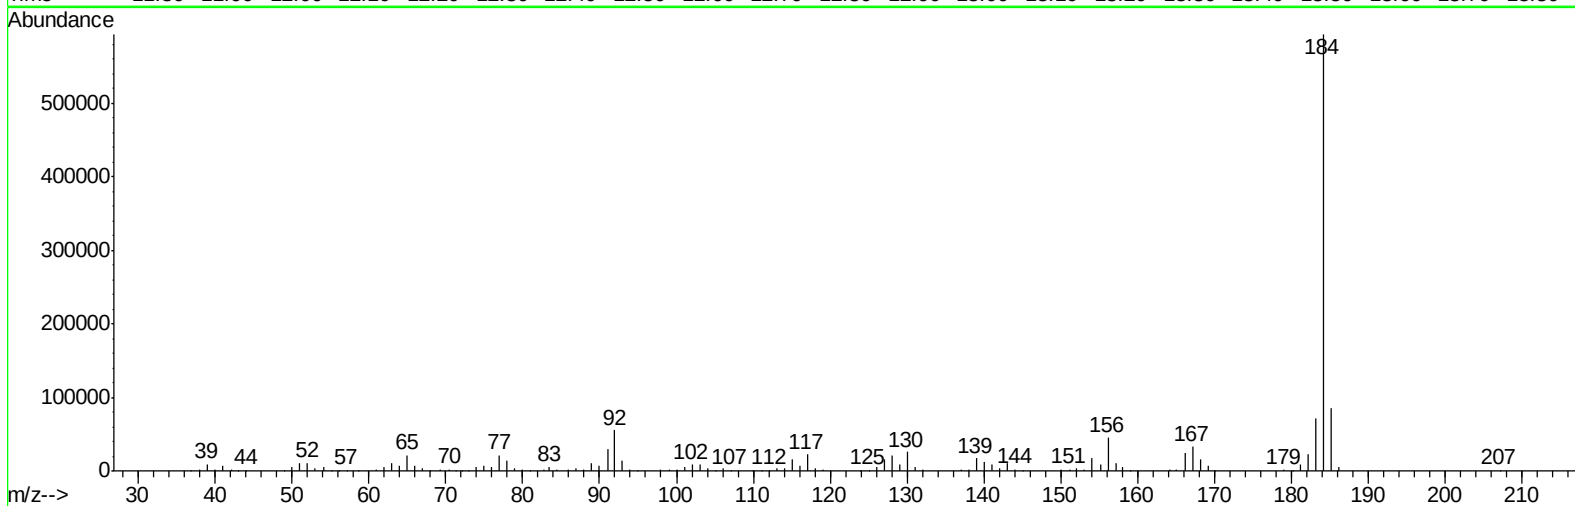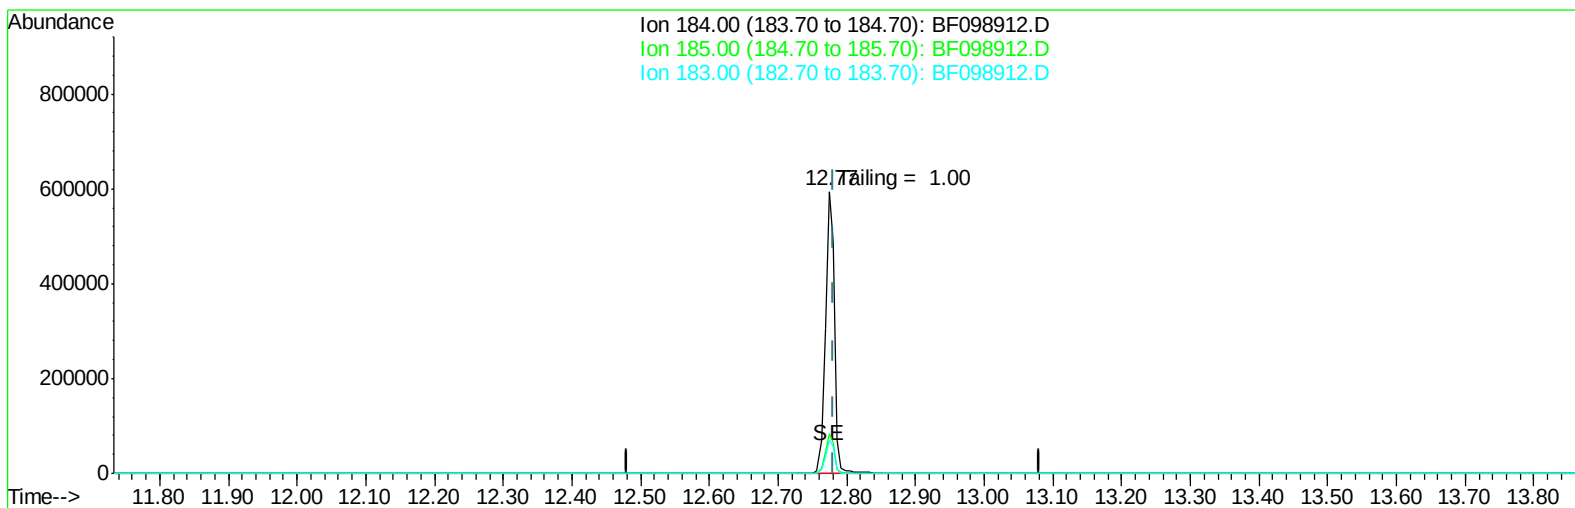

TIC: BF098912.D

(76) Benzidine

12.774min (-0.006) 0.00ng

response 553243

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.29
183.00	11.60	11.91
0.00	0.00	0.00