


Data Path : Z:\HPCHEM1\BNA_F\Data\BF092817\
 Data File : BF098898.D
 Acq On : 28 Sep 2017 10:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

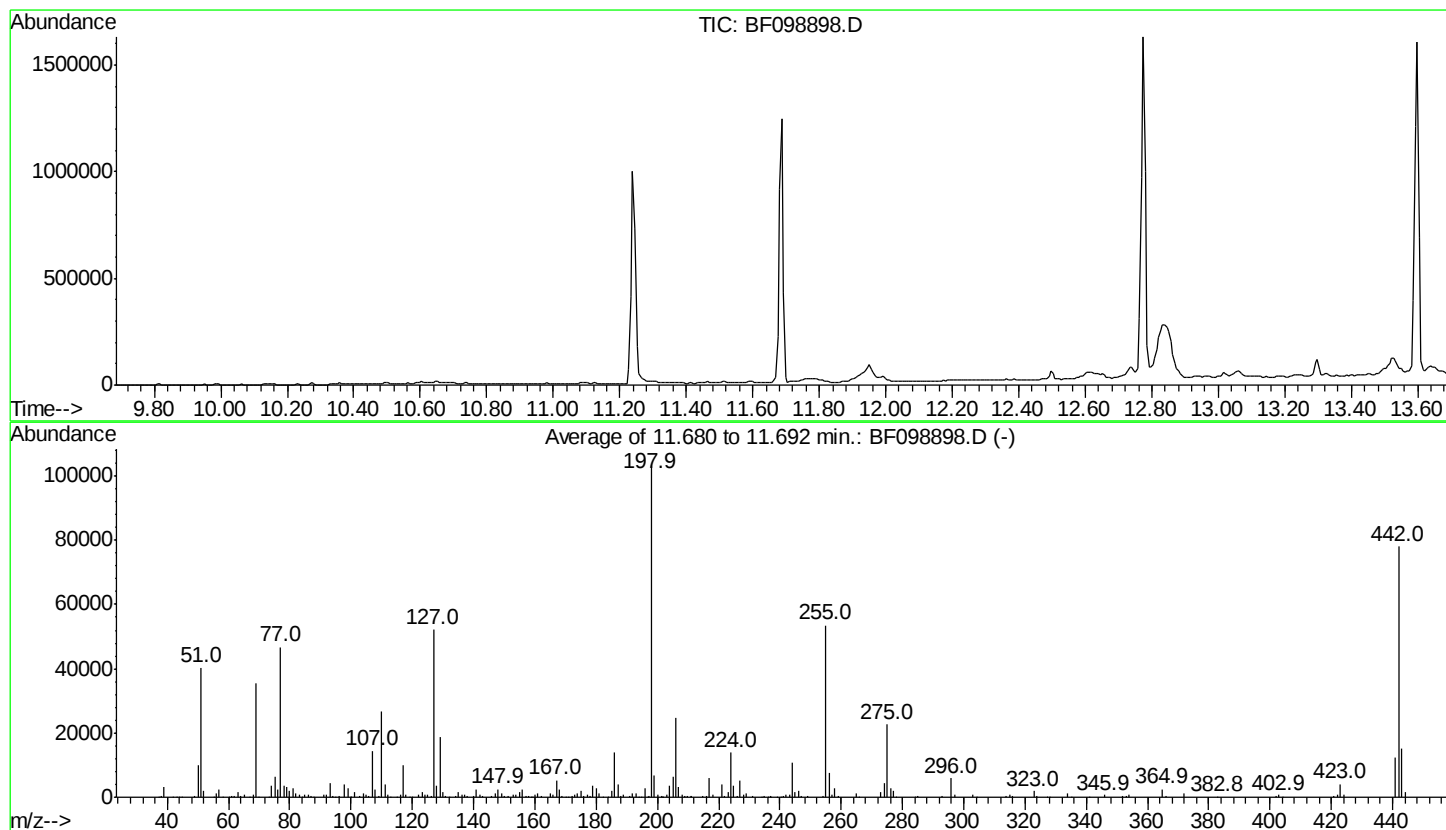

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.0	40277	PASS
68	69	0.00	2	1.9	674	PASS
69	198	0.00	100	34.5	35564	PASS
70	69	0.00	2	0.5	176	PASS
127	198	10	80	50.5	52077	PASS
197	198	0.00	2	0.6	576	PASS
198	198	100	100	100.0	103221	PASS
199	198	5	9	6.7	6889	PASS
275	198	10	60	21.9	22630	PASS
365	198	1	100	2.5	2561	PASS
441	442	0.01	24	15.8	12288	PASS
442	198	50	100	75.6	77989	PASS
443	442	15	24	19.3	15082	PASS