

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092818\
 Data File : BF109462.D
 Acq On : 29 Sep 2018 6:26
 Operator : JU/SJ
 Sample : J5133-15
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 092618-JETT-F-D-B

Quant Time: Oct 01 03:09:55 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	106193	20.00	ng	0.00
21) Naphthalene-d8	7.99	136	400273	20.00	ng	0.00
38) Acenaphthene-d10	9.74	164	190428	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	352193	20.00	ng	0.00
75) Chrysene-d12	13.84	240	209450	20.00	ng	0.00
86) Perylene-d12	15.24	264	217194	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.32	112	249430	38.69	ng	0.00
7) Phenol-d6	6.34	99	223595	27.18	ng	-0.02
23) Nitrobenzene-d5	7.27	82	646767	95.38	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	164420	87.59	ng	-0.01
44) 2-Fluorobiphenyl	9.07	172	1149874	91.07	ng	0.00
78) Terphenyl-d14	12.80	244	1042777	122.18	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
10) Phenol	6.35	94	25621	2.750	ng	93
19) n-Nitroso-di-n-propylamine	7.27	70	87492	16.230	ng	# 77
25) Isophorone	7.27	82	614178	50.300	ng	# 64
49) Dimethylphthalate	9.46	163	29197	2.108	ng	98
50) 2,6-Dinitrotoluene	9.74	165	24298	8.858	ng	# 26
56) 2,4-Dinitrotoluene	9.74	165	24298	7.001	ng	# 24
64) 4,6-Dinitro-2-methylphenol	10.52	198	139	6.605	ng	# 1
66) 4-Bromophenyl-phenylether	10.52	248	10056	2.571	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092818\
Data File : BF109462.D
Acq On : 29 Sep 2018 6:26
Operator : JU/SJ
Sample : J5133-15
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
092618-JETT-F-D-B

Quant Time: Oct 01 03:09:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

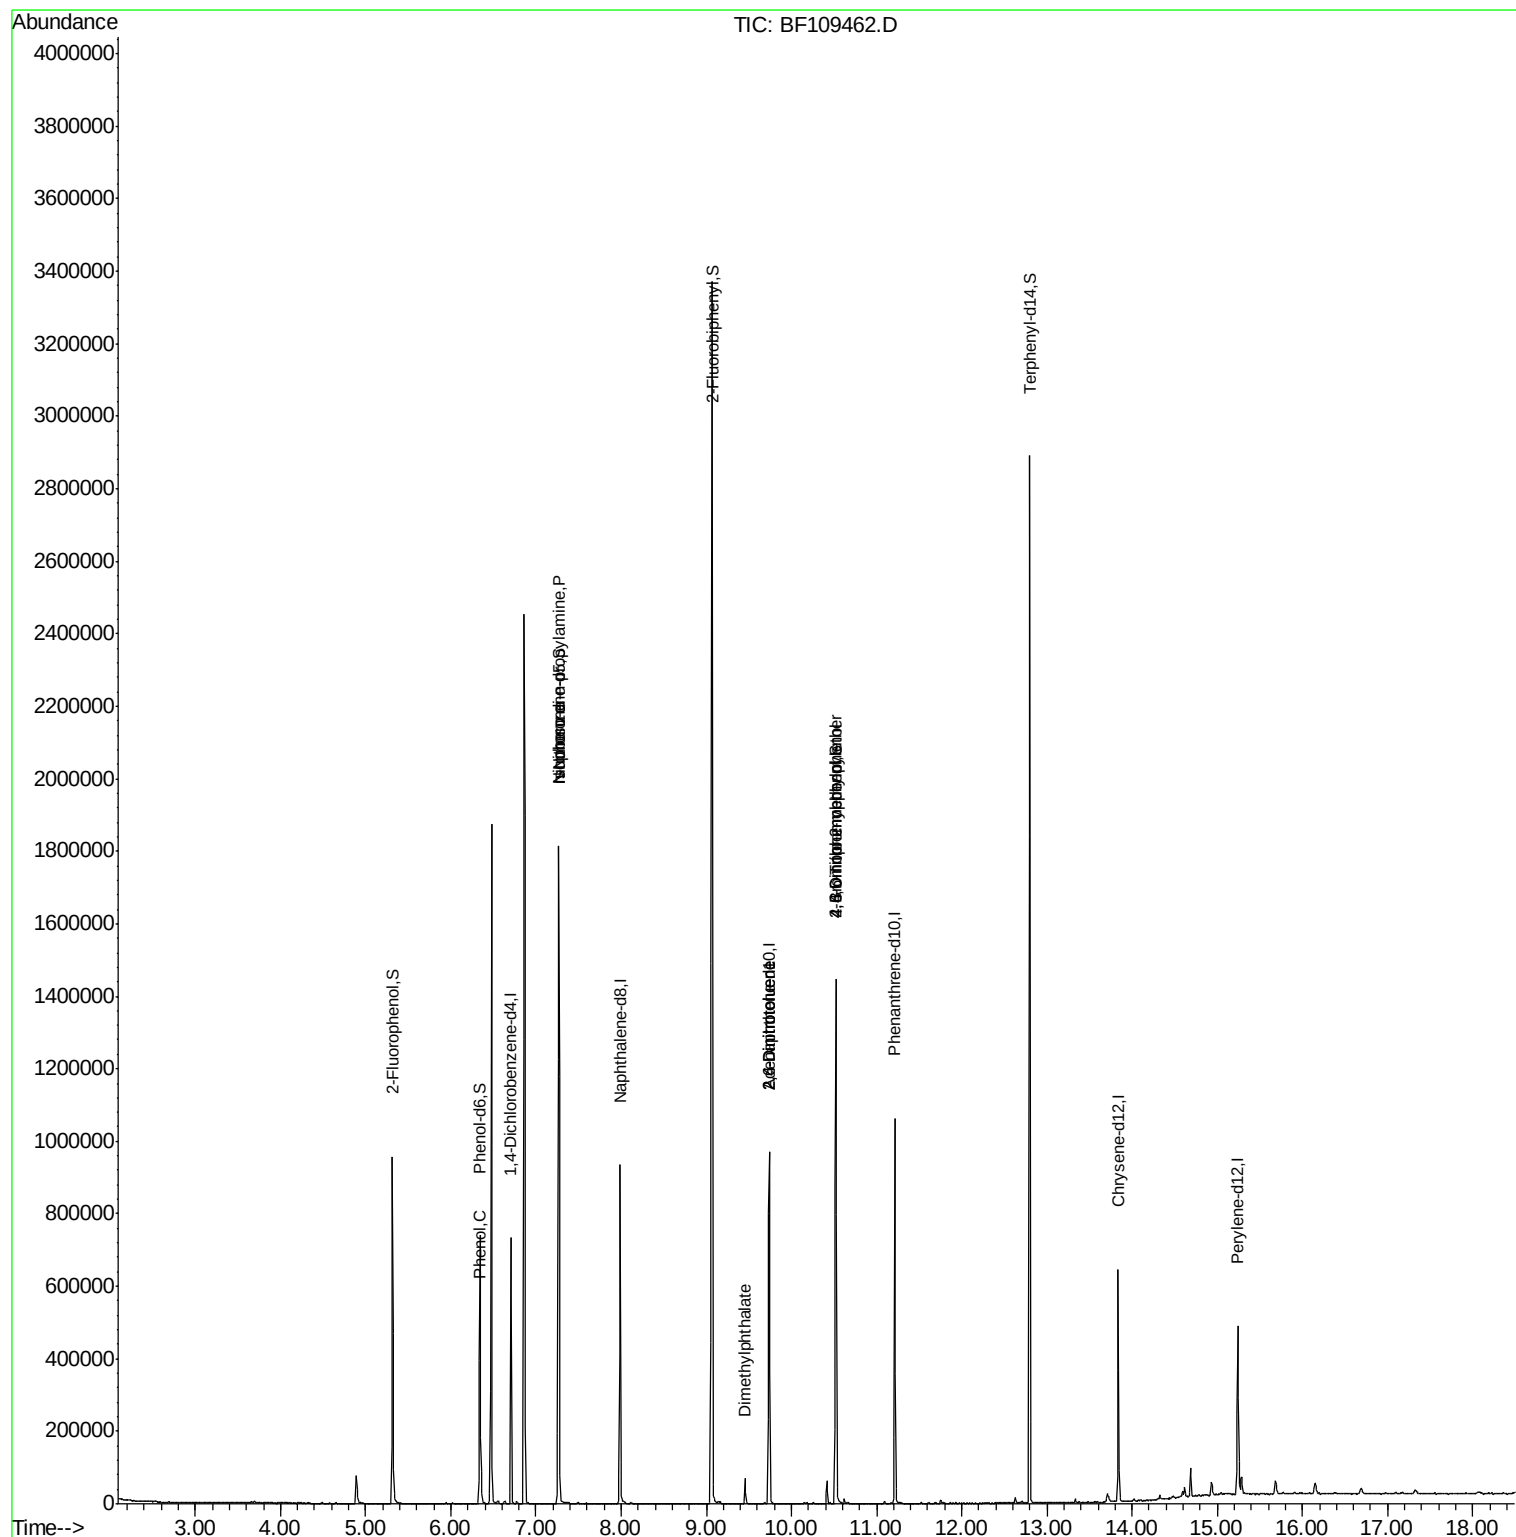


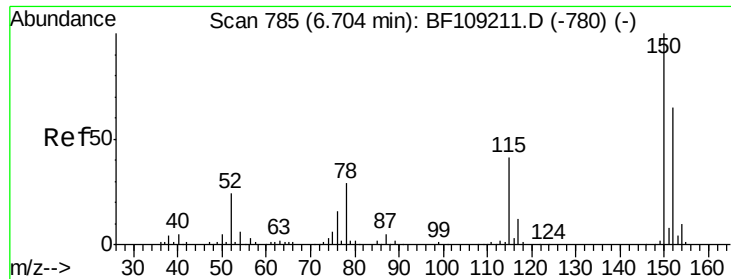




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.70 min Scan# 785
 Delta R.T. -0.01 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26

Instrument :
 BNA_F
 ClientSampleId :
 092618-JETT-F-D-B

Tgt Ion:152 Resp: 106193
 Ion Ratio Lower Upper
 152 100
 150 158.2 124.6 186.8
 115 63.0 50.1 75.1

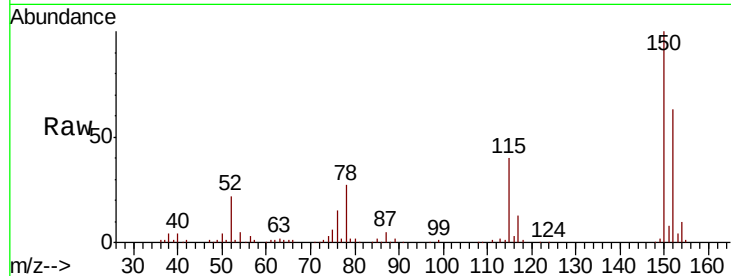


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

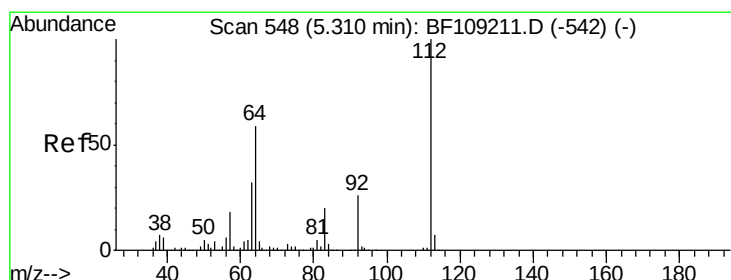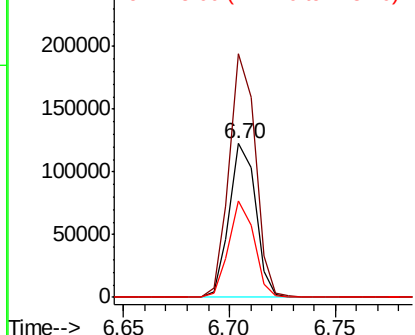
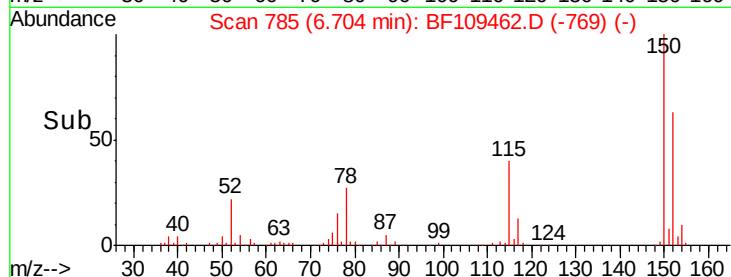



#5
 2-Fluorophenol
 Concen: 38.687 ng
 RT: 5.32 min Scan# 549
 Delta R.T. 0.00 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26

Tgt Ion:112 Resp: 249430
 Ion Ratio Lower Upper
 112 100
 64 57.4 47.9 71.9
 63 30.5 23.7 35.5

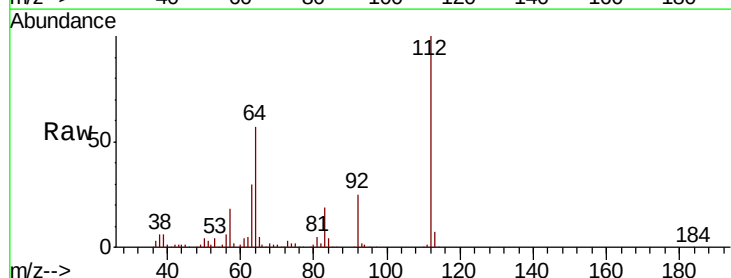

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

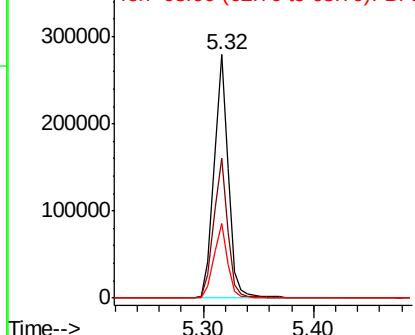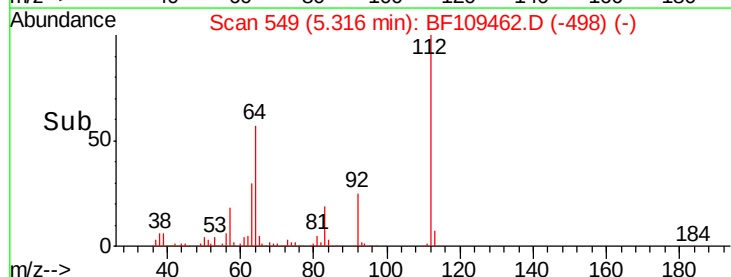

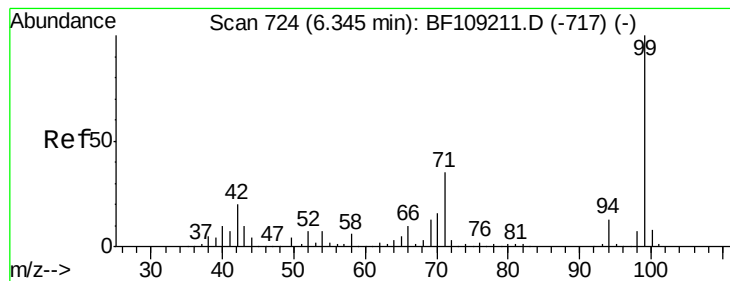

#7

Phenol-d6

Concen: 27.178 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.02 min

Lab File: BF109462.D

Acq: 29 Sep 2018 6:26

Instrument :

BNA_F

ClientSampleId :

092618-JETT-F-D-B



Tgt Ion: 99 Resp: 223595

Ion Ratio Lower Upper

99 100

42 18.3 14.5 21.7



71 33.8 25.4 38.0

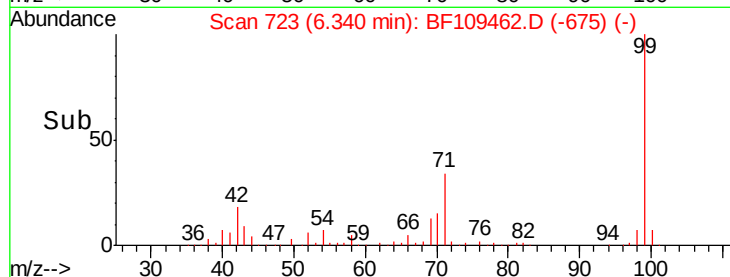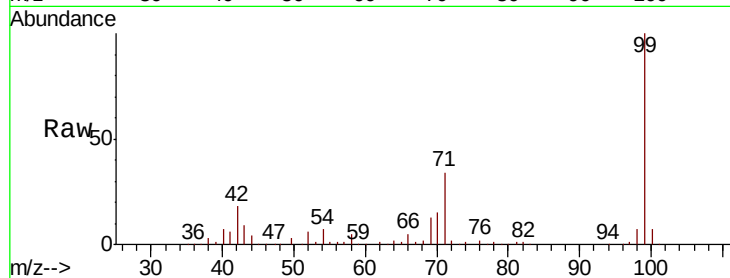

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

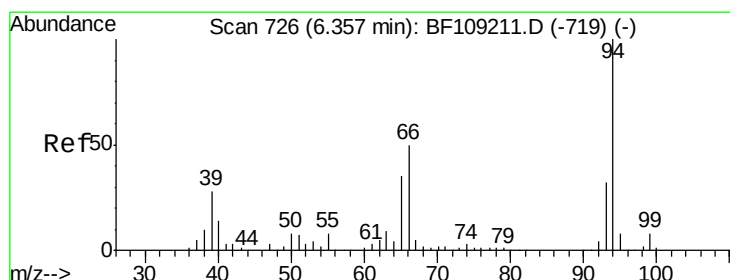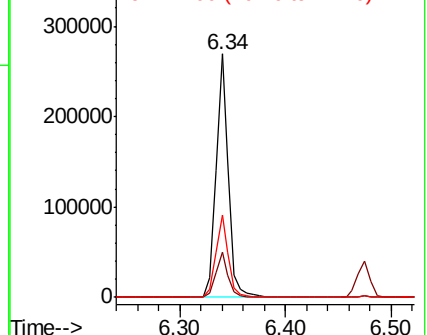

#10

Phenol

Concen: 2.750 ng

RT: 6.35 min Scan# 725

Delta R.T. -0.02 min

Lab File: BF109462.D

Acq: 29 Sep 2018 6:26



Tgt Ion: 94 Resp: 25621

Ion Ratio Lower Upper

94 100

65 29.2 7.9 47.9


66 42.3 16.2 56.2

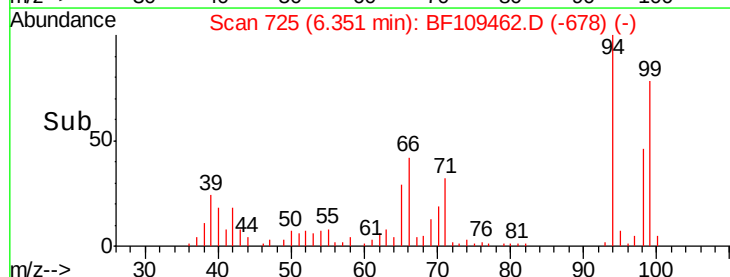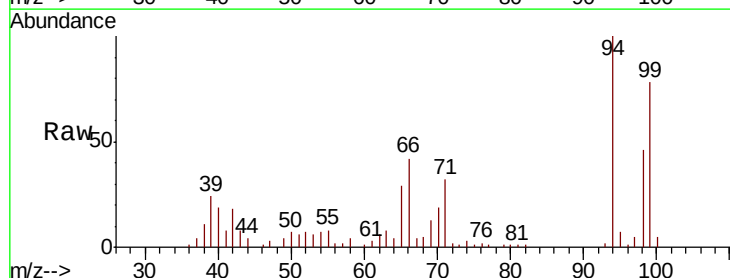


Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1




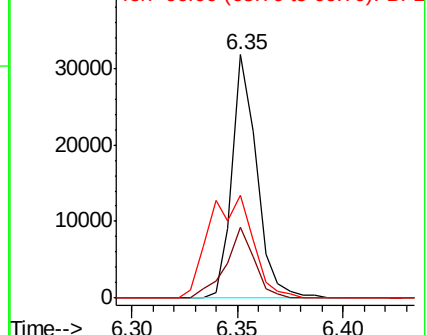


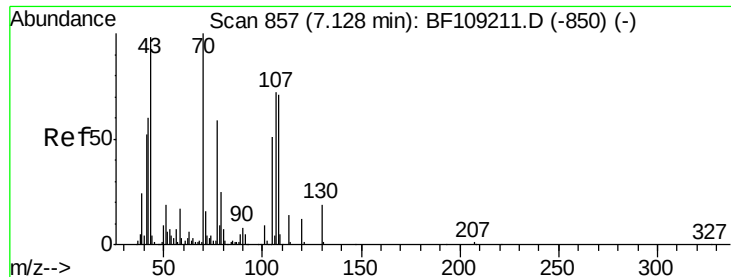

#19
n-Nitroso-di-n-propylamine
Concen: 16.230 ng
RT: 7.27 min Scan# 881
Delta R.T. 0.12 min
Lab File: BF109462.D
Acq: 29 Sep 2018 6:26




Instrument :
BNA_F
ClientSampleId :
092618-JETT-F-D-B


Tgt Ion:	70	Resp:	87492
Ion	Ratio	Lower	Upper
70	100		
42	46.7	47.5	71.3#
101	0.0	7.4	11.2#
130	2.0	16.6	25.0#

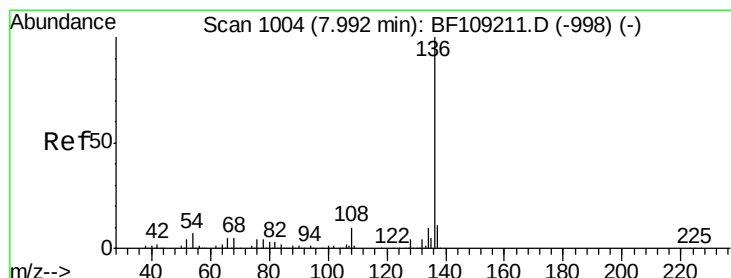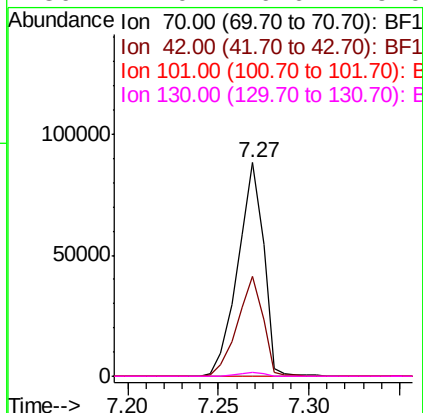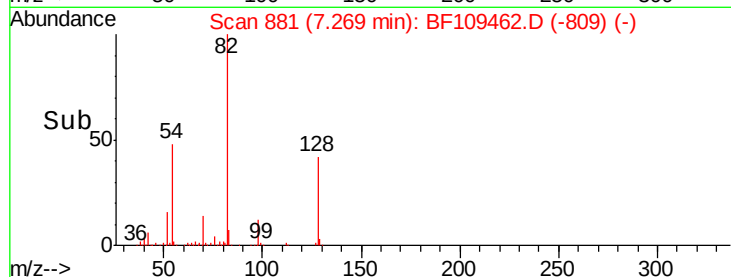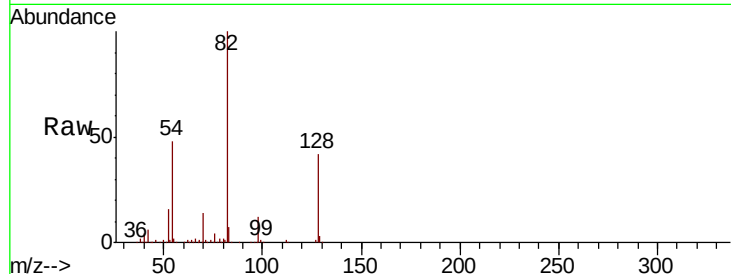

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.99 min Scan# 1003
Delta R.T. -0.01 min
Lab File: BF109462.D
Acq: 29 Sep 2018 6:26

Tgt Ion:	136	Resp:	400273
Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.9	13.3
54	7.2	6.6	9.8
68	5.5	5.0	7.4


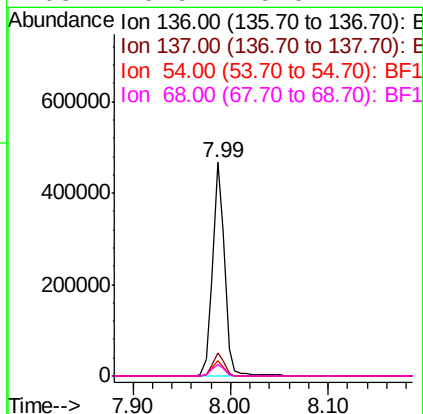
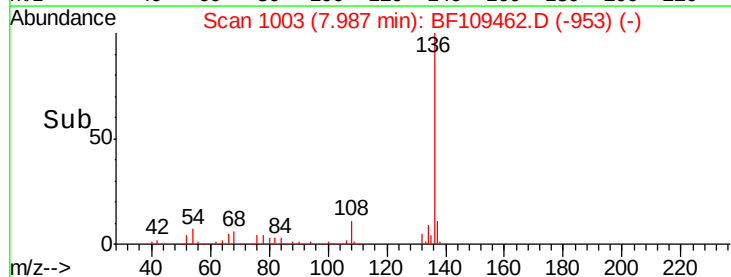
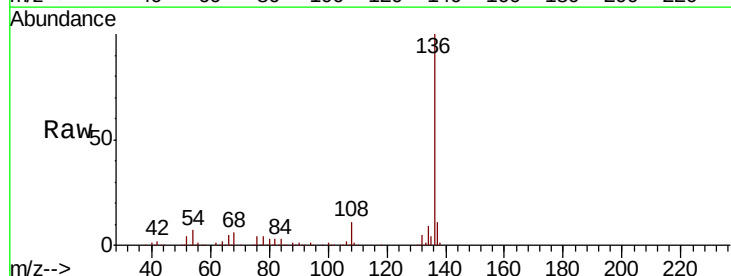


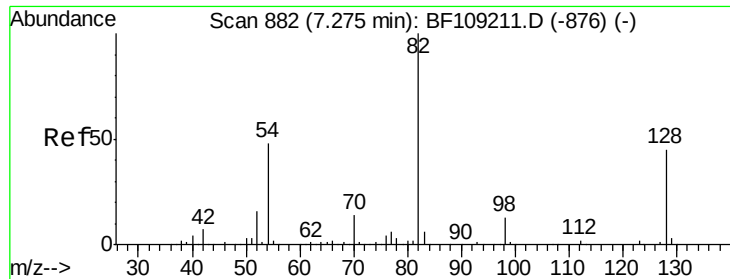

#23
 Nitrobenzene-d5
 Concen: 95.384 ng
 RT: 7.27 min Scan# 881
 Delta R.T. -0.01 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26




Instrument :
 BNA_F
 ClientSampleId :
 092618-JETT-F-D-B


Tgt Ion	Ratio	Lower	Upper
82	100		
128	42.2	36.1	54.1
54	47.9	41.4	62.2

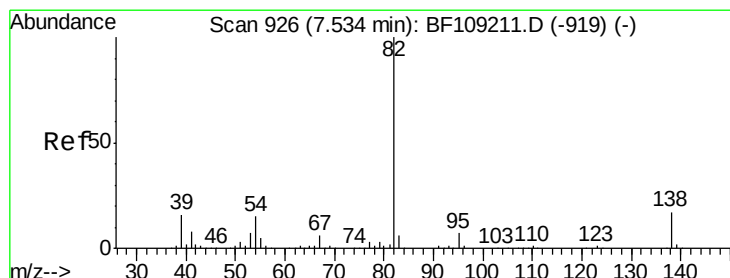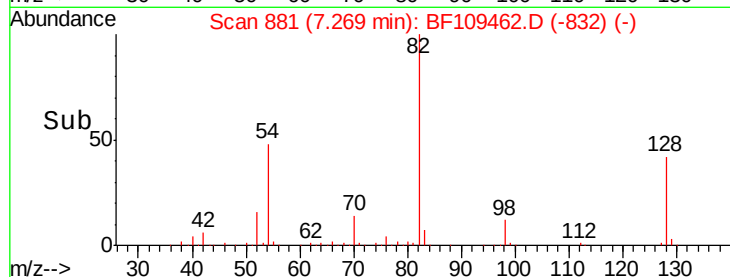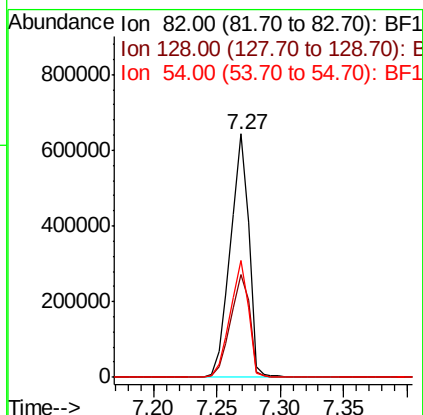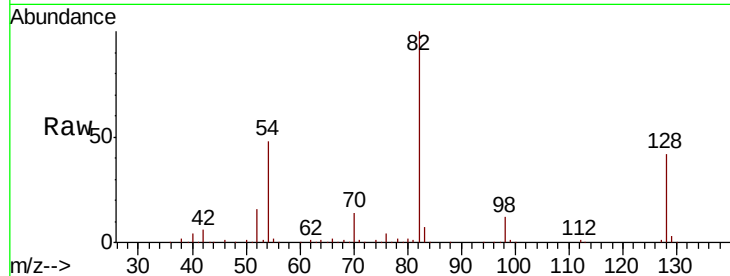

#25
 Isophorone
 Concen: 50.300 ng
 RT: 7.27 min Scan# 881
 Delta R.T. -0.28 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26

Tgt Ion	Ratio	Lower	Upper
82	100		
95	0.0	5.2	7.8#
138	0.0	14.9	22.3#

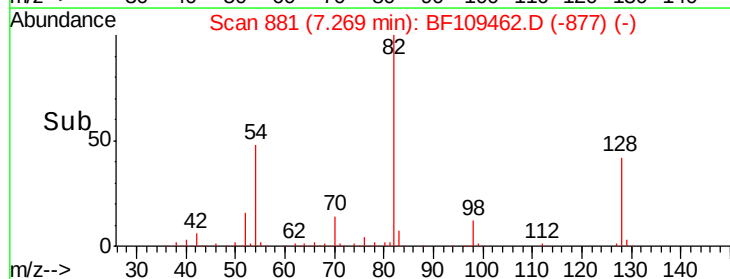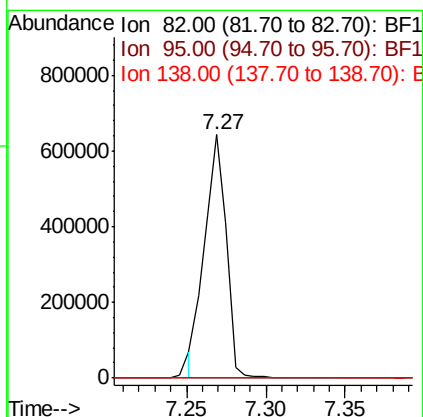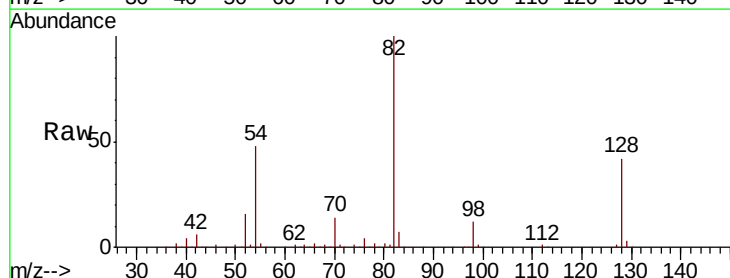


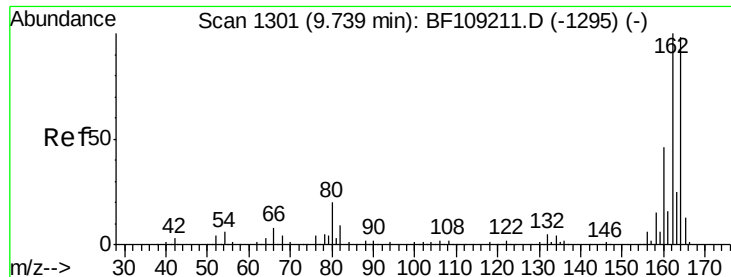




#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.74 min Scan# 1301
 Delta R.T. 0.00 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26

Instrument :
 BNA_F
 ClientSampleId :
 092618-JETT-F-D-B

Tgt Ion:164 Resp: 190428
 Ion Ratio Lower Upper
 164 100
 162 102.3 86.1 129.1
 160 47.4 38.3 57.5

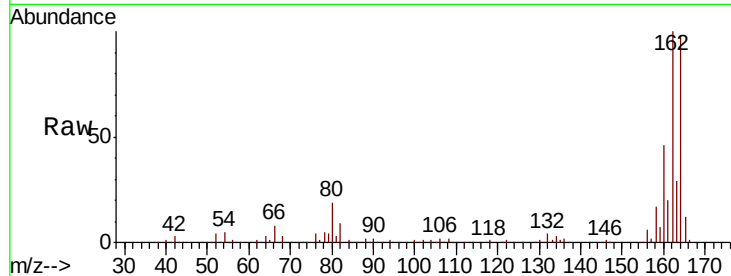


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

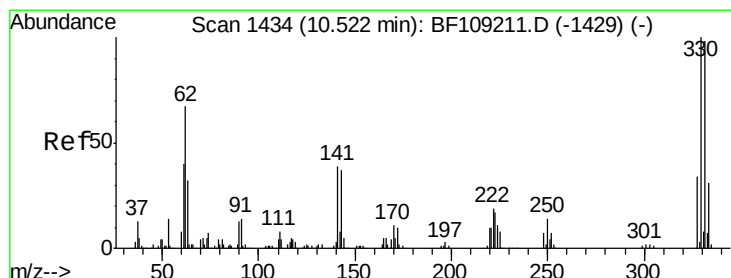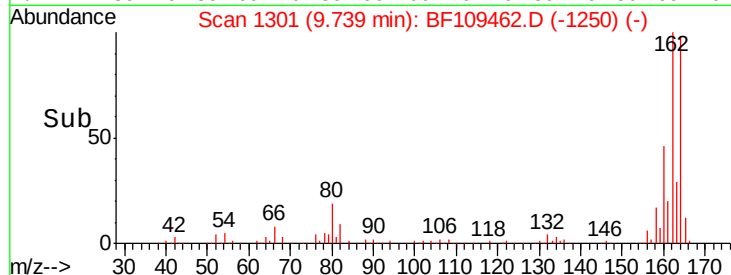
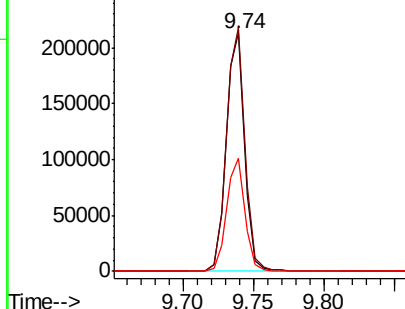



#41
 2,4,6-Tribromophenol
 Concen: 87.587 ng
 RT: 10.52 min Scan# 1434
 Delta R.T. -0.01 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26

Tgt Ion:330 Resp: 164420
 Ion Ratio Lower Upper
 330 100
 332 95.0 77.0 115.6
 141 33.6 29.9 44.9

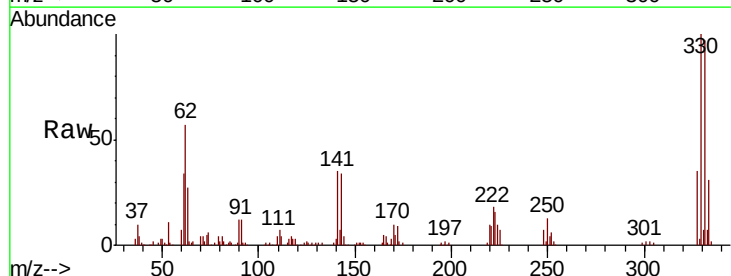

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

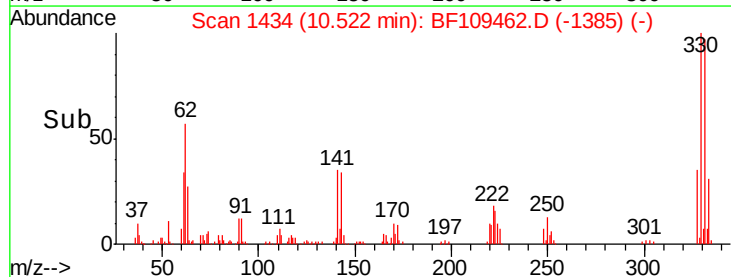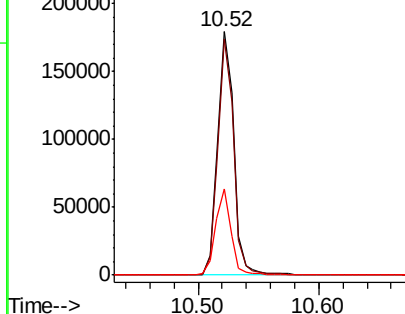


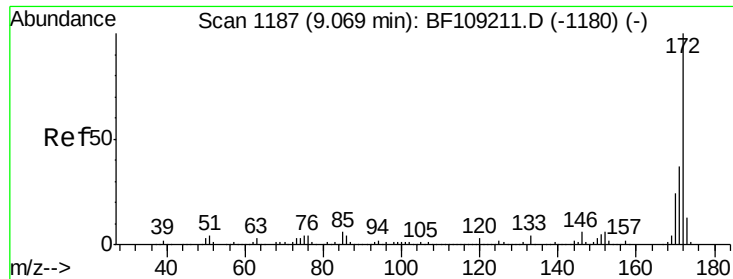




#44
2-Fluorobiphenyl
Concen: 91.070 ng
RT: 9.07 min Scan# 1187
Delta R.T. -0.01 min
Lab File: BF109462.D
Acq: 29 Sep 2018 6:26

Instrument :
BNA_F
ClientSampleId :
092618-JETT-F-D-B

Tgt Ion:172 Resp: 1149874
Ion Ratio Lower Upper
172 100
171 35.8 29.7 44.5
170 24.2 19.6 29.4

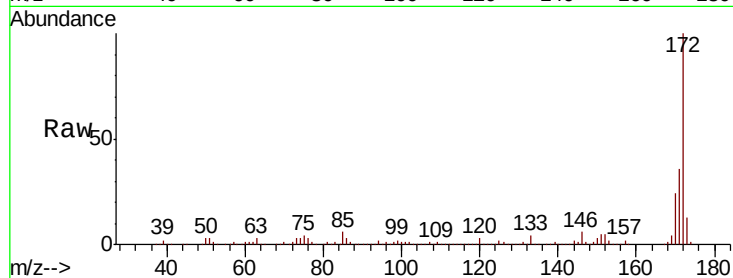


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

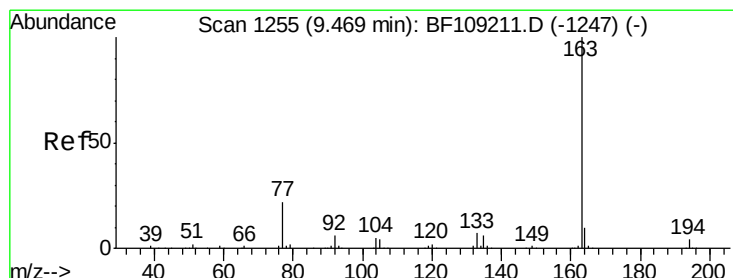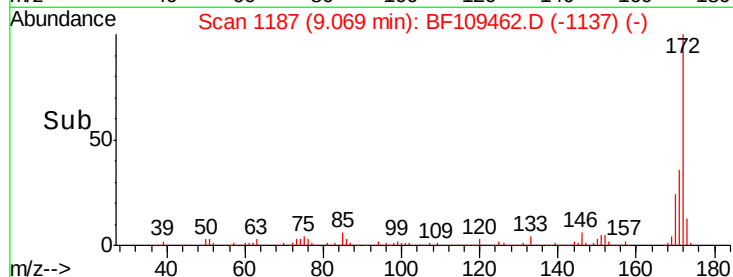
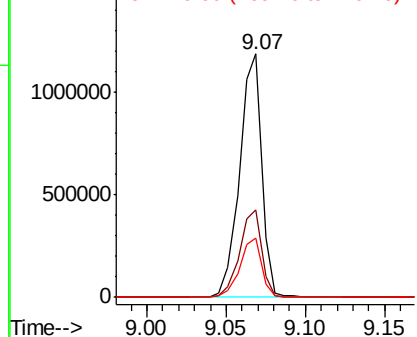



#49
Dimethylphthalate
Concen: 2.108 ng
RT: 9.46 min Scan# 1253
Delta R.T. -0.02 min
Lab File: BF109462.D
Acq: 29 Sep 2018 6:26

Tgt Ion:163 Resp: 29197
Ion Ratio Lower Upper
163 100
194 3.9 2.7 4.1
164 9.4 8.2 12.2

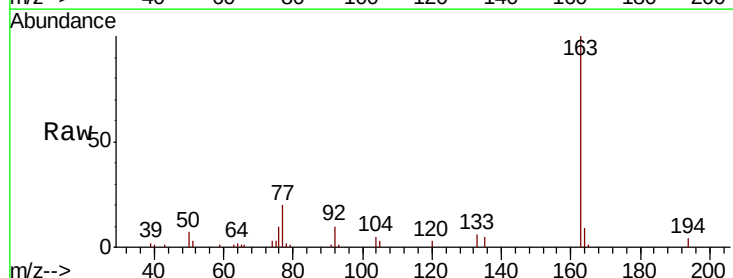

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

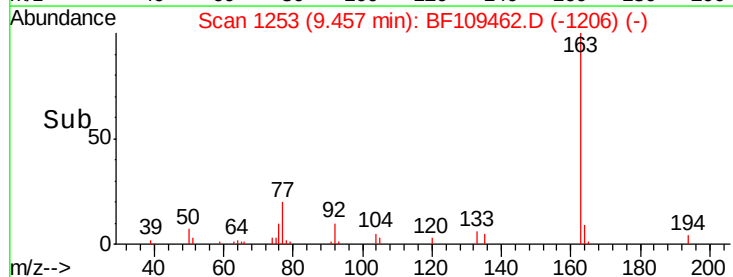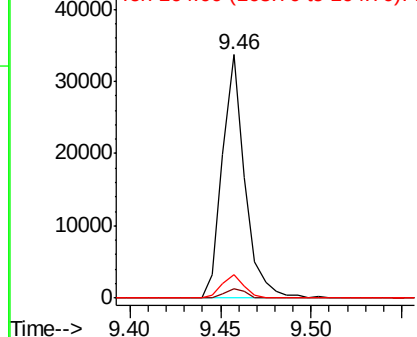


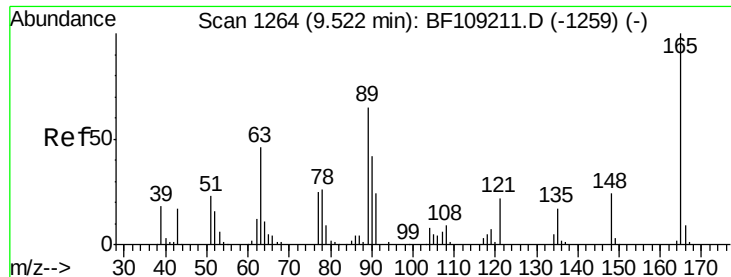




#50
 2,6-Dinitrotoluene
 Concen: 8.858 ng
 RT: 9.74 min Scan# 1301
 Delta R.T. 0.21 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26

Instrument :
 BNA_F
 ClientSampleId :
 092618-JETT-F-D-B

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	44.7	67.1#
89	1.8	44.0	66.0#

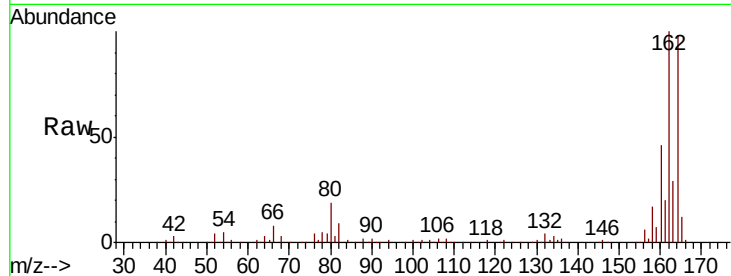




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1

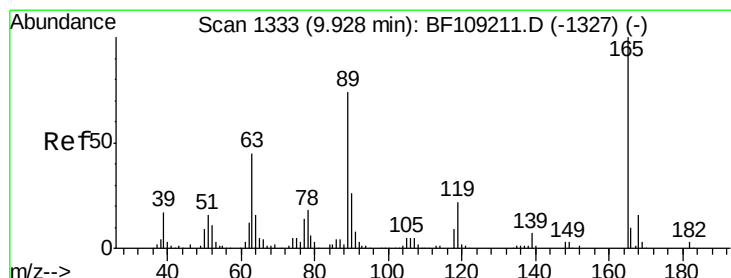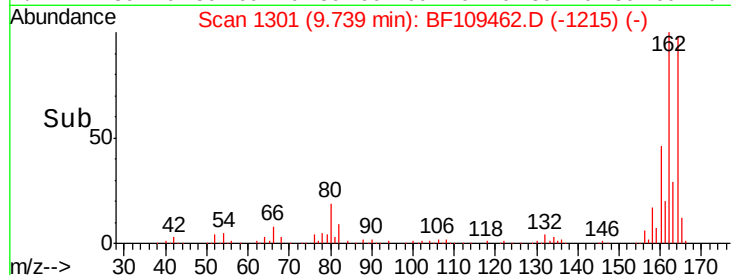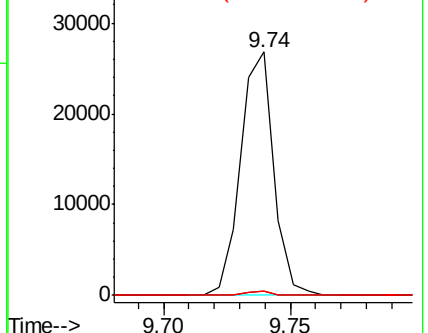


#56
 2,4-Dinitrotoluene
 Concen: 7.001 ng
 RT: 9.74 min Scan# 1301
 Delta R.T. -0.20 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	36.4	54.6#
89	1.8	57.8	86.6#
182	0.0	1.6	2.4#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E


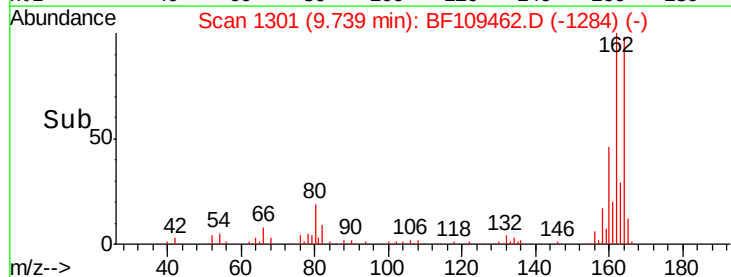
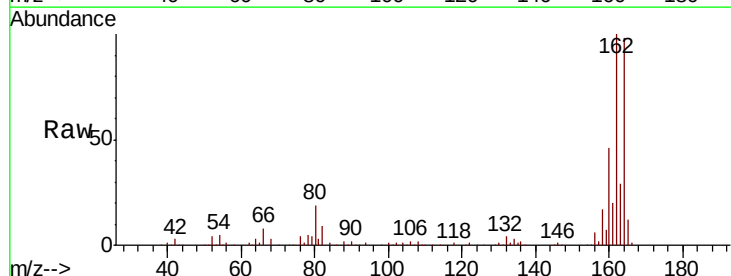
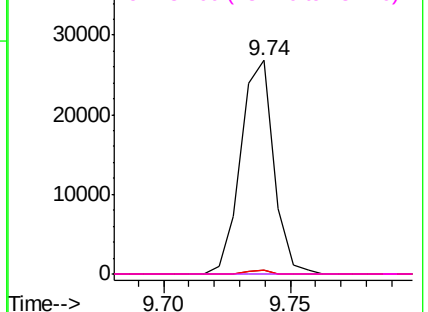


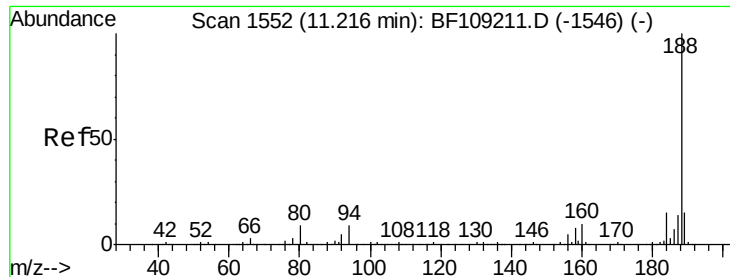

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.22 min Scan# 1552
 Delta R.T. 0.00 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26




Instrument :
 BNA_F
 ClientSampleId :
 092618-JETT-F-D-B


Tgt Ion	Ratio	Resp	Lower	Upper
188	100	352193		
94	8.8		8.5	12.7
80	8.8		9.2	13.8#

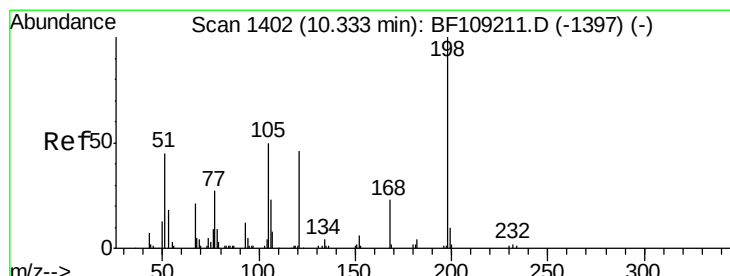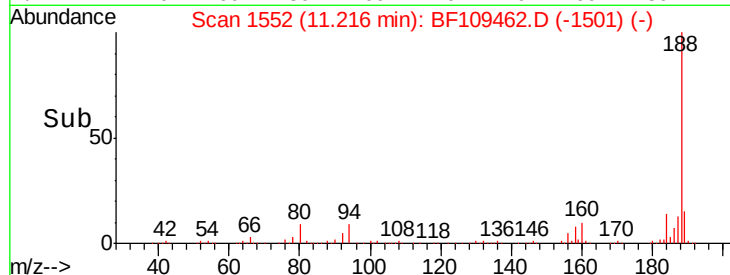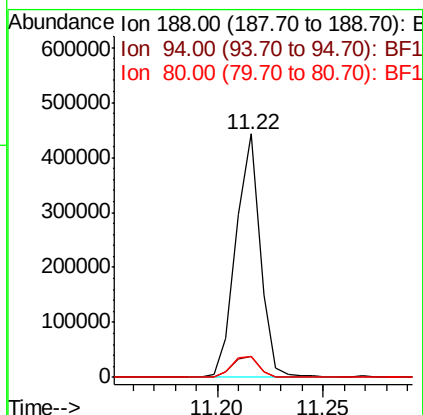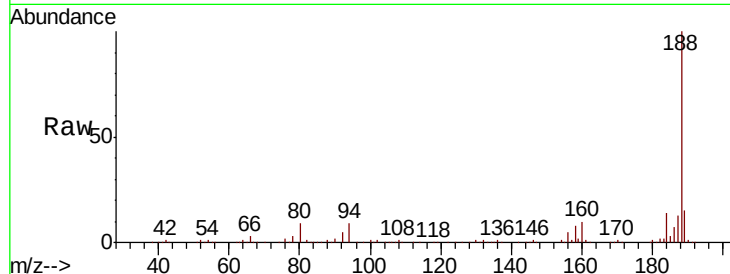

#64
 4,6-Dinitro-2-methylphenol
 Concen: 6.605 ng
 RT: 10.52 min Scan# 1434
 Delta R.T. 0.18 min
 Lab File: BF109462.D
 Acq: 29 Sep 2018 6:26

Tgt Ion	Ratio	Resp	Lower	Upper
198	100	139		
51	229.1		37.7	77.7#
105	208.4		36.3	76.3#

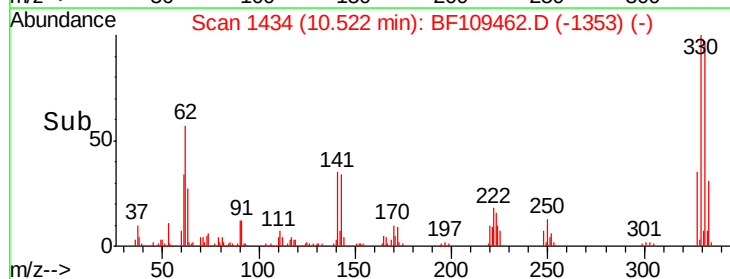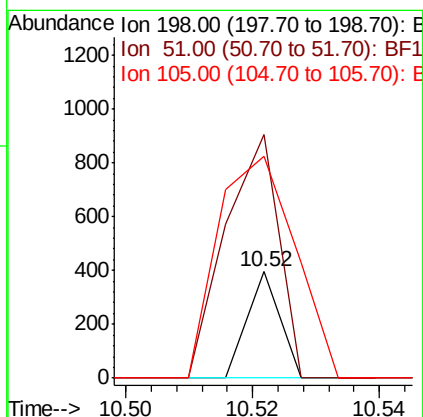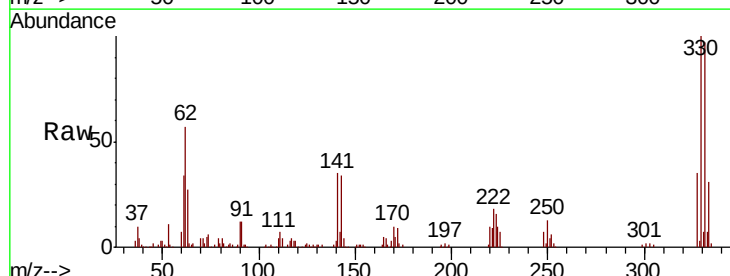


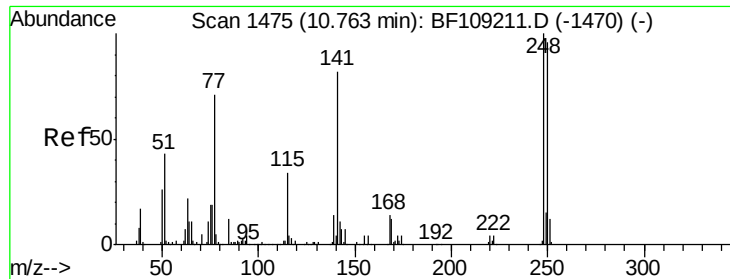




#66
4-Bromophenyl-phenylether
Concen: 2.571 ng
RT: 10.52 min Scan# 1434
Delta R.T. -0.25 min
Lab File: BF109462.D
Acq: 29 Sep 2018 6:26

Instrument :
BNA_F
ClientSampleId :
092618-JETT-F-D-B

Tgt Ion:248 Resp: 10056
Ion Ratio Lower Upper
248 100
250 198.0 76.9 115.3#
141 538.3 74.4 111.6#

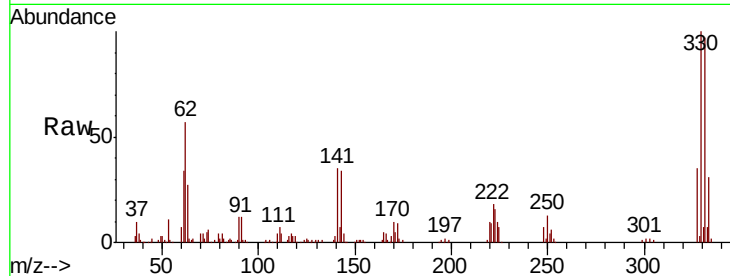


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

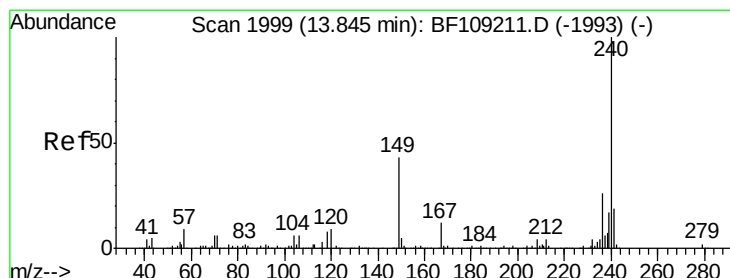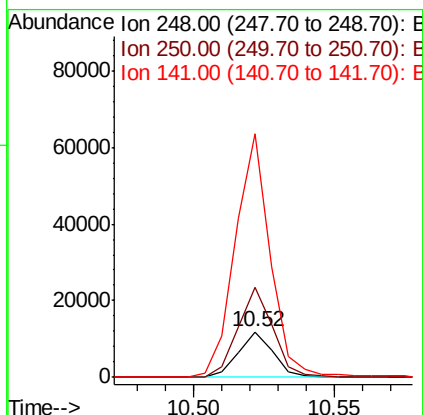
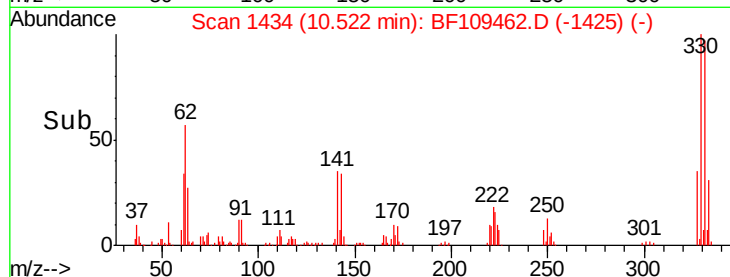



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.84 min Scan# 1998
Delta R.T. -0.01 min
Lab File: BF109462.D
Acq: 29 Sep 2018 6:26

Tgt Ion:240 Resp: 209450
Ion Ratio Lower Upper
240 100
120 11.4 9.5 14.3
236 25.9 20.7 31.1

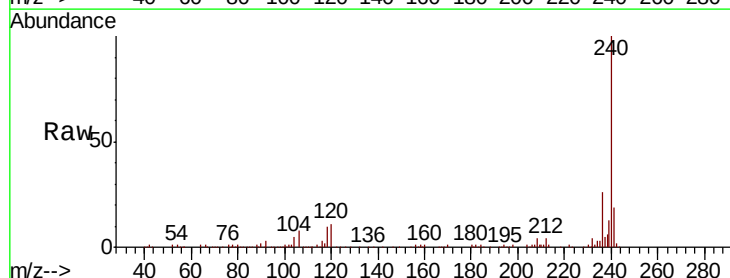

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

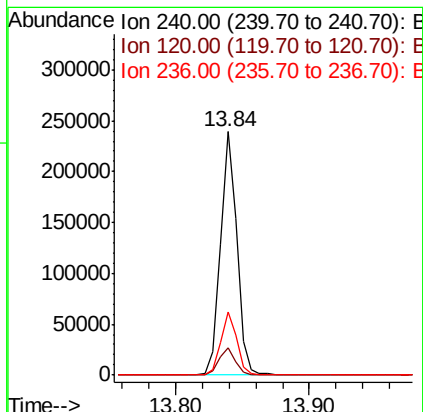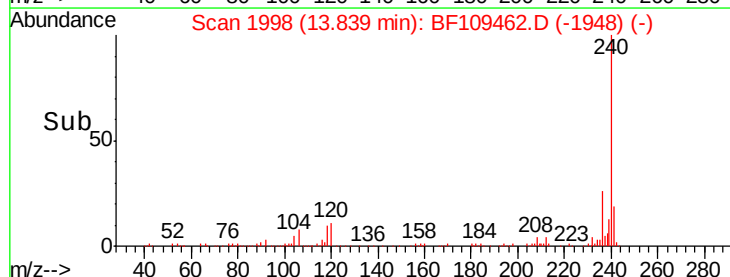

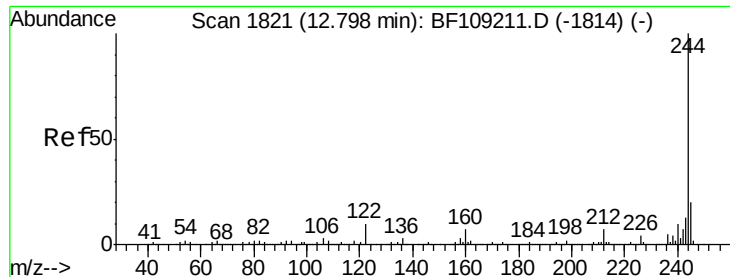

#78

Terphenyl-d14

Concen: 122.184 ng

RT: 12.80 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BF109462.D

Acq: 29 Sep 2018 6:26

Instrument :

BNA_F

ClientSampleId :

092618-JETT-F-D-B


Tgt Ion:244 Resp: 1042777

Ion Ratio Lower Upper

244 100

212 7.2 5.4 8.0




122 12.1 11.0 16.4

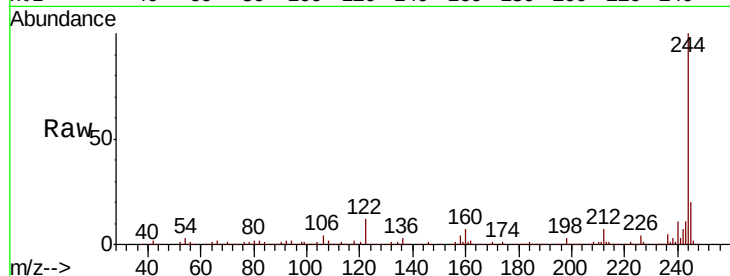

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

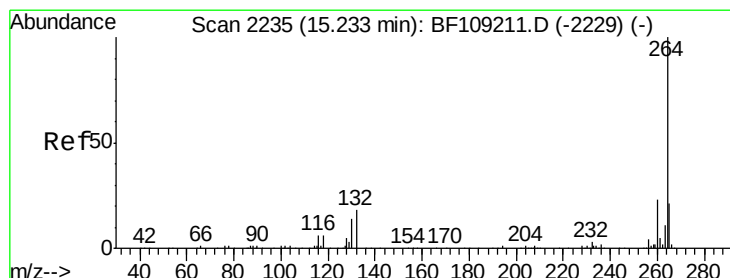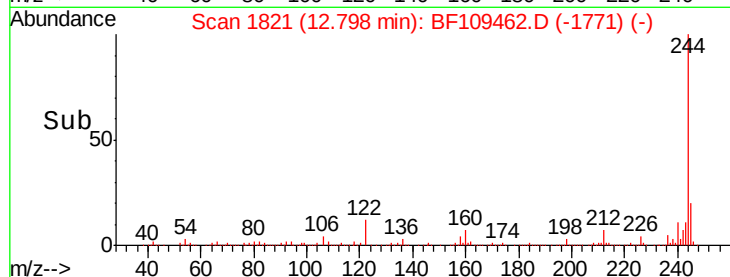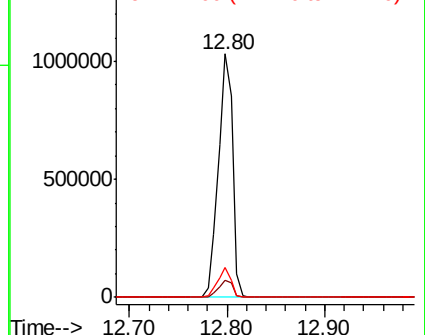

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.24 min Scan# 2237

Delta R.T. 0.01 min

Lab File: BF109462.D

Acq: 29 Sep 2018 6:26


Tgt Ion:264 Resp: 217194

Ion Ratio Lower Upper

264 100

260 23.5 19.2 28.8

265 21.5 17.5 26.3

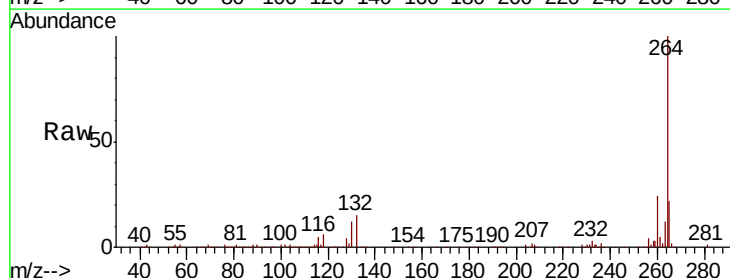

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

