
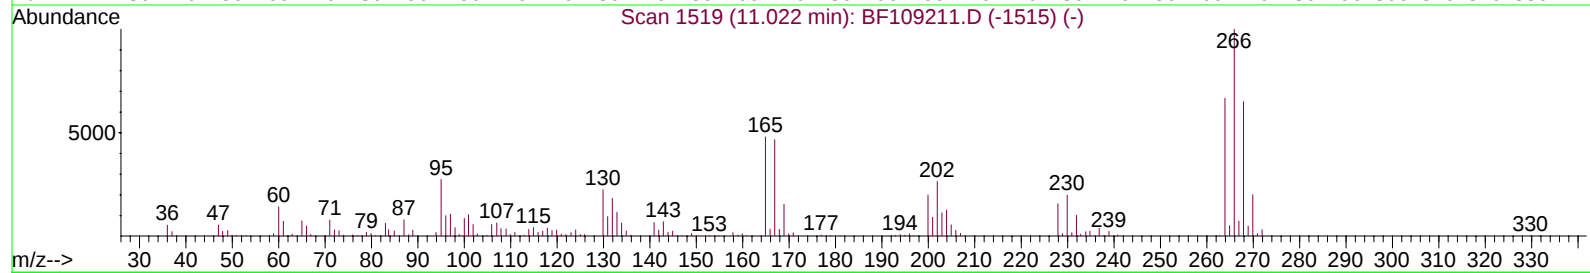
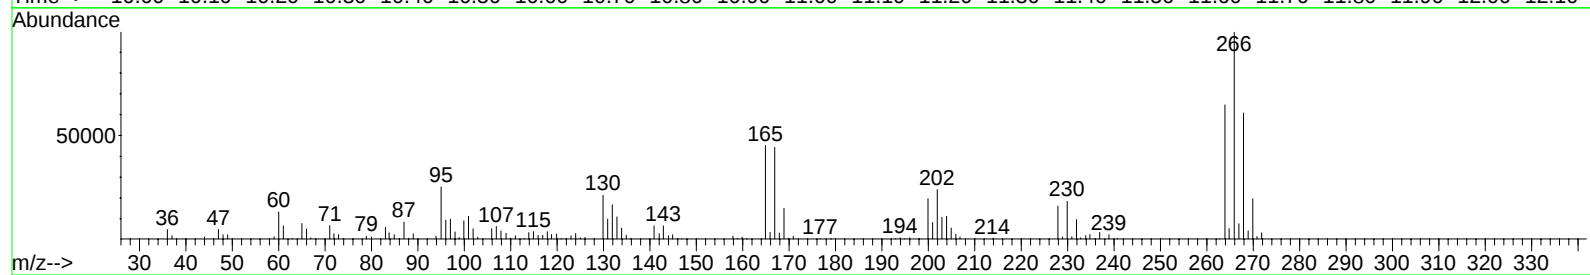


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092818\  
Data File  : BF109428.D  
Acq On     : 28 Sep 2018   12:34  
Operator   : JU/SJ  
Sample     : DFTPP  
Misc       :  
ALS Vial   : 1      Sample Multiplier: 1
```

Quant Time: Sep 28 19:16:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

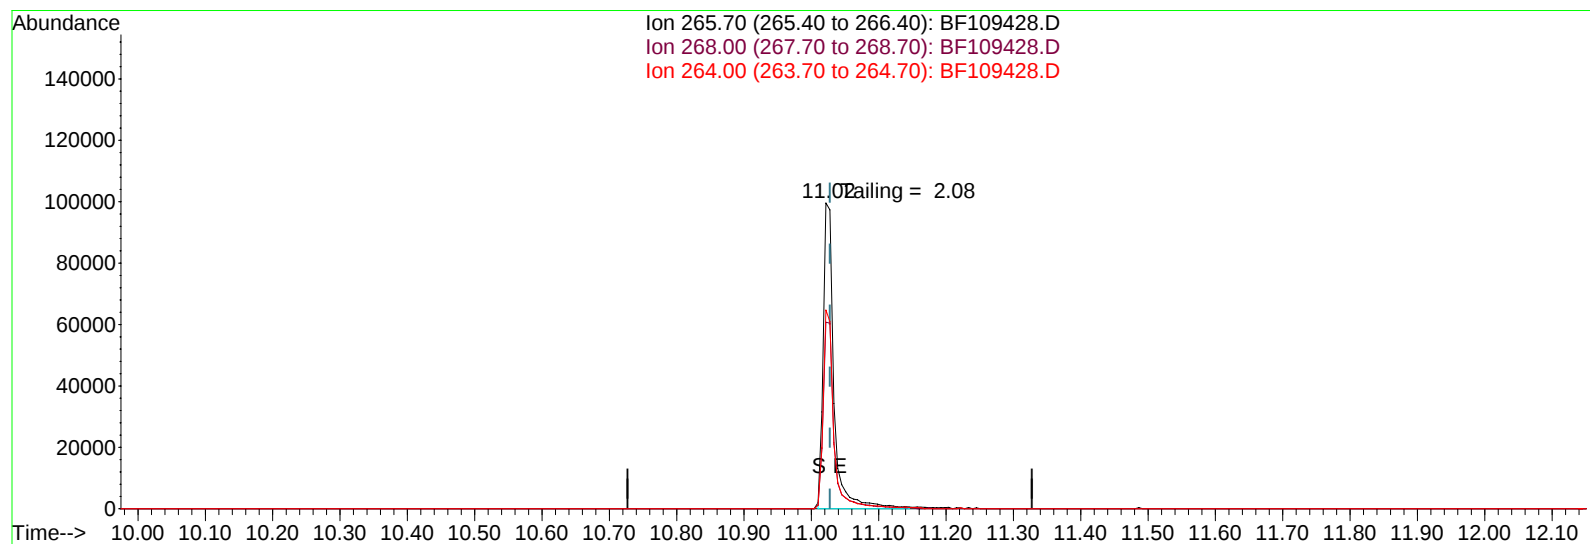

TIC: BF109428.D

(69) Pentachlorophenol (C)




11.022min (-0.006) 42855.64ng

response 111927

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.04
264.00	61.90	64.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092818\
Data File : BF109428.D
Acq On : 28 Sep 2018 12:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 19:16:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

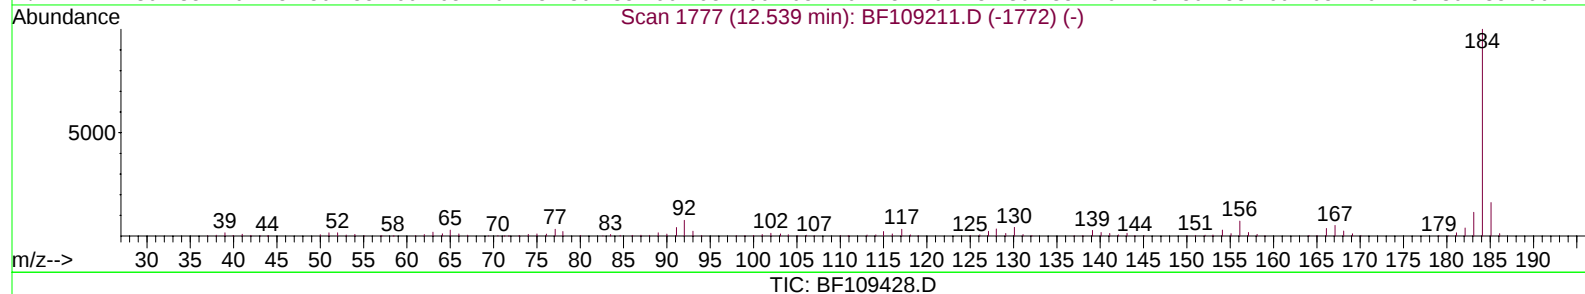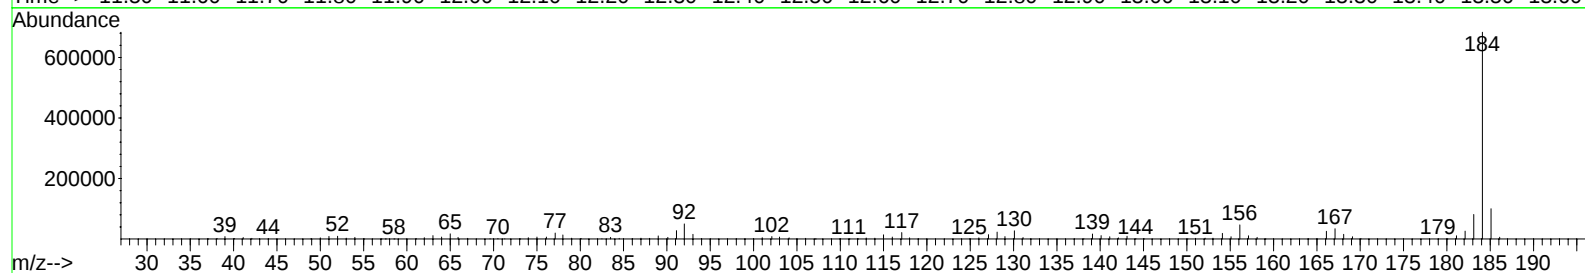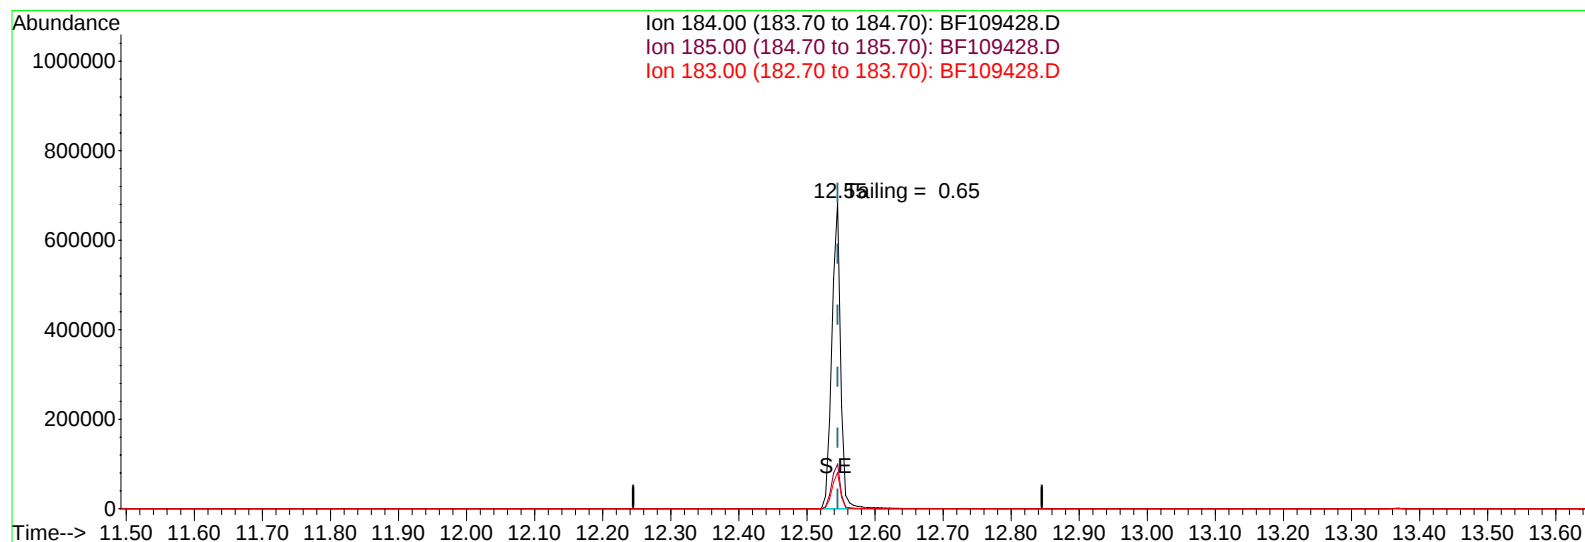

(76) Benzidine

12.545min (+0.000) 0.00ng

response 611522

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.68
183.00	11.60	11.88
0.00	0.00	0.00