
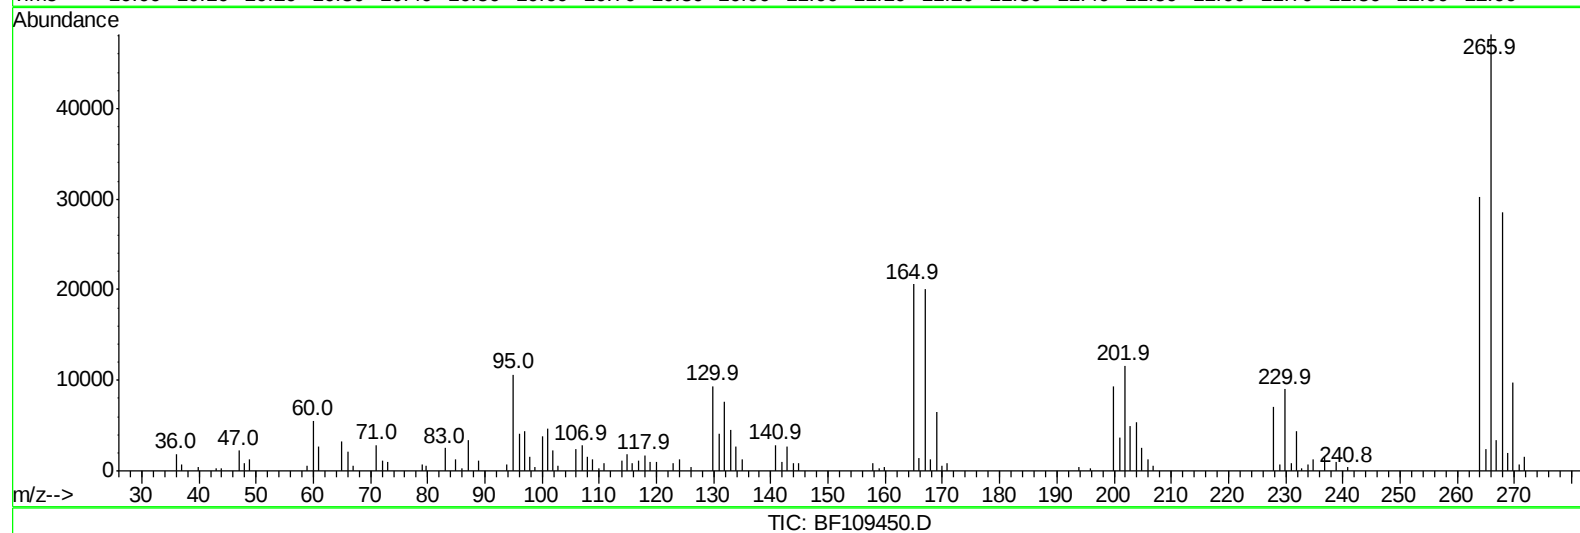


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092818\
Data File : BF109450.D
Acq On : 29 Sep 2018 1:08
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 08:47:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

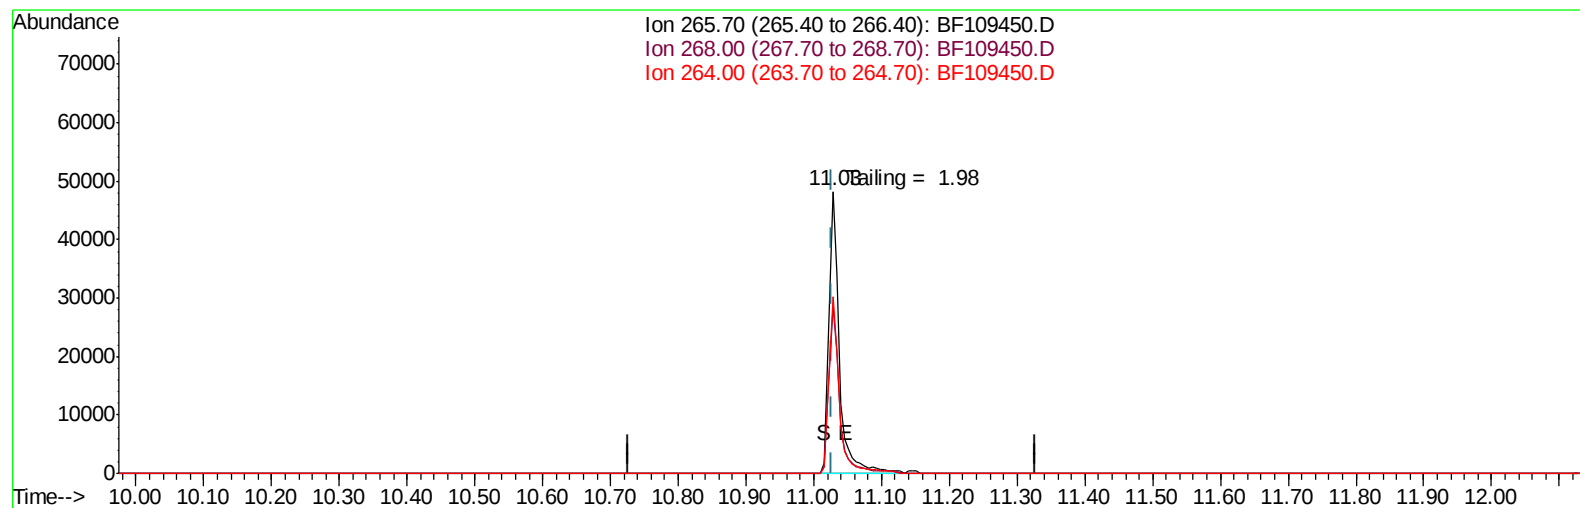

TIC: BF109450.D

(69) Pentachlorophenol (C)



11.028min (+0.000) 54233.07ng

response 49766

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.29
264.00	61.90	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF092818\
Data File : BF109450.D
Acq On : 29 Sep 2018 1:08
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 08:47:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

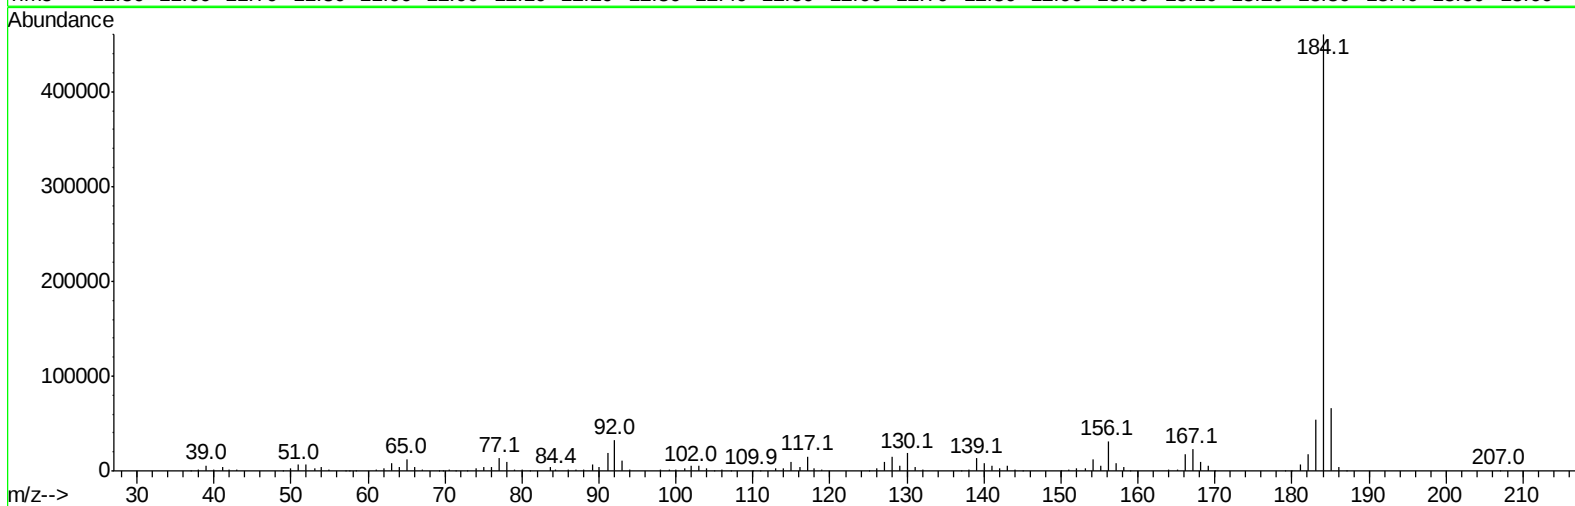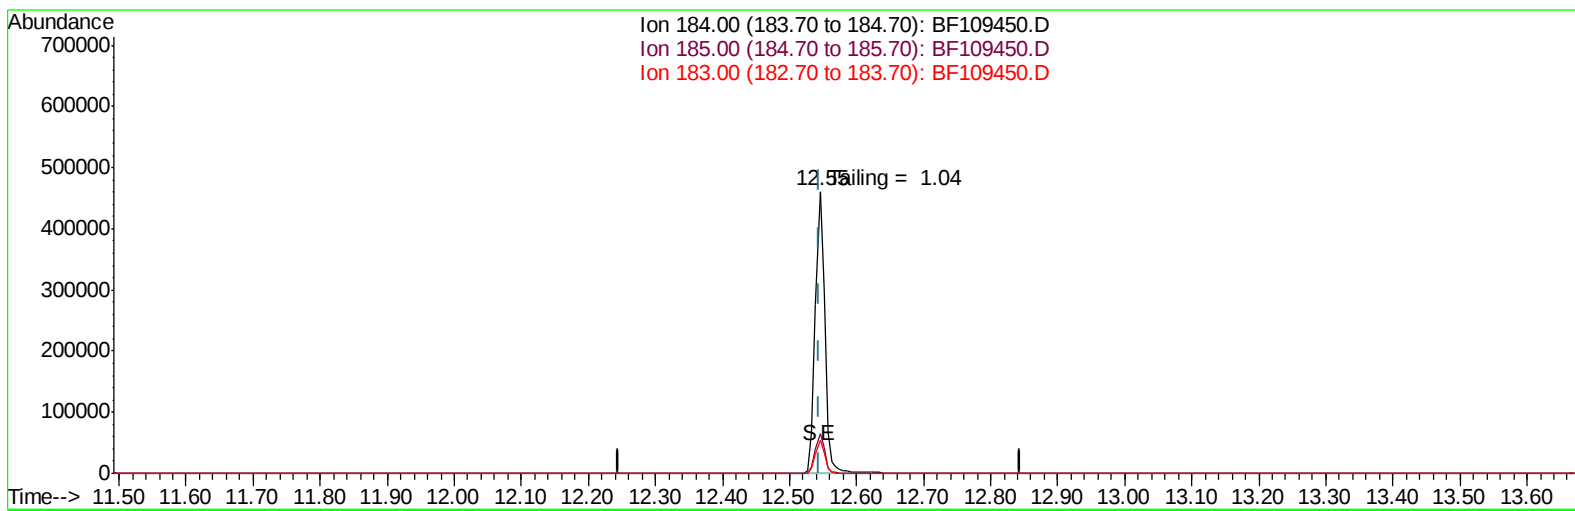

TIC: BF109450.D

(76) Benzidine

12.545min (+0.000) 0.00ng

response 435600

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.33
183.00	11.60	11.76
0.00	0.00	0.00