

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092818\
 Data File : BF109461.D
 Acq On : 29 Sep 2018 5:59
 Operator : JU/SJ
 Sample : J5133-14
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 092618-TIPC-F-U-S

Quant Time: Oct 01 03:54:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	113613	20.00	ng	0.00
21) Naphthalene-d8	7.99	136	418555	20.00	ng	0.00
38) Acenaphthene-d10	9.74	164	203025	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	367655	20.00	ng	0.00
75) Chrysene-d12	13.84	240	220866	20.00	ng	0.00
86) Perylene-d12	15.24	264	221482	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	275924	40.00	ng	0.00
7) Phenol-d6	6.34	99	227597	25.86	ng	-0.02
23) Nitrobenzene-d5	7.27	82	718104	101.28	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	183321	91.60	ng	-0.01
44) 2-Fluorobiphenyl	9.07	172	1224357	90.95	ng	0.00
78) Terphenyl-d14	12.80	244	1088863	120.99	ng	0.00
Target Compounds						
10) Phenol	6.35	94	39366	3.949	ng	95
49) Dimethylphthalate	9.46	163	66142	4.479	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092818\
Data File : BF109461.D
Acq On : 29 Sep 2018 5:59
Operator : JU/SJ
Sample : J5133-14
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
092618-TIPC-F-U-S

Quant Time: Oct 01 03:54:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

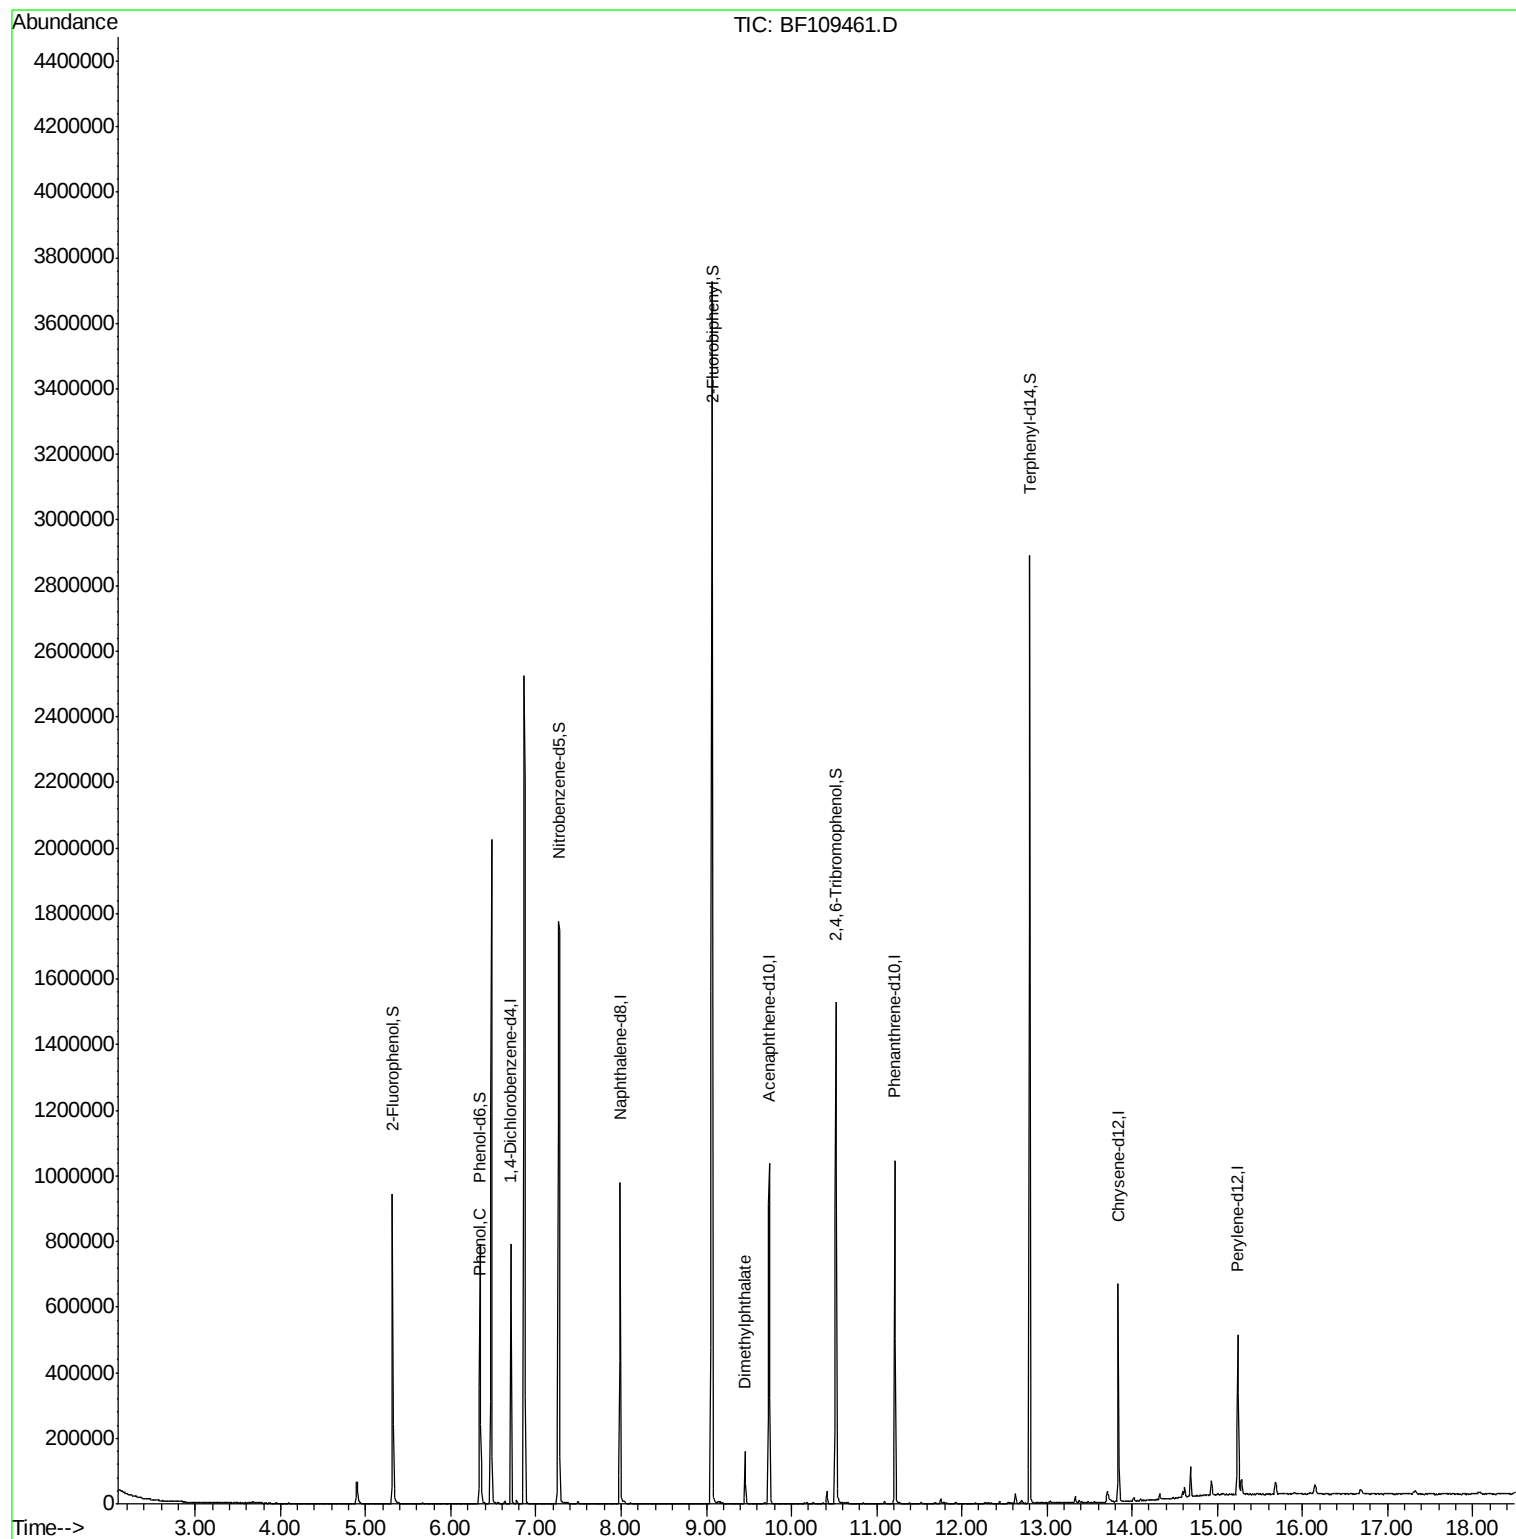




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF109461.D
Acq: 29 Sep 2018 5:59

Instrument :
BNA_F
ClientSampleId :
092618-TIPC-F-U-S

Tot Ion:152 Resp: 113613
Ion Ratio Lower Upper
152 100
150 156.5 124.6 186.8
115 61.7 50.1 75.1

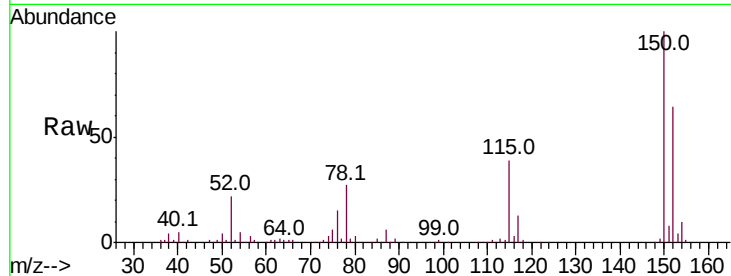


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

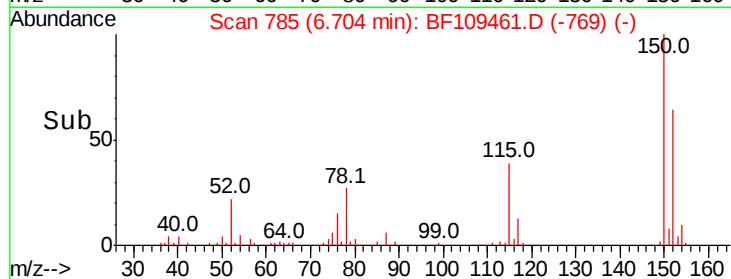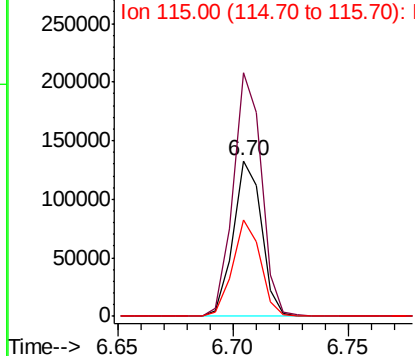



#5

2-Fluorophenol
Concen: 40.001 ng
RT: 5.32 min Scan# 550
Delta R.T. 0.01 min
Lab File: BF109461.D
Acq: 29 Sep 2018 5:59

Tgt Ion:112 Resp: 275924
Ion Ratio Lower Upper
112 100
64 53.5 47.9 71.9
63 28.8 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

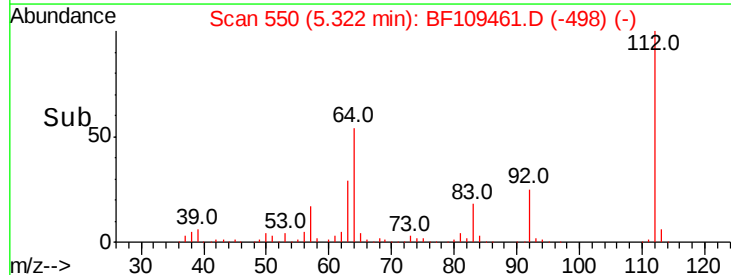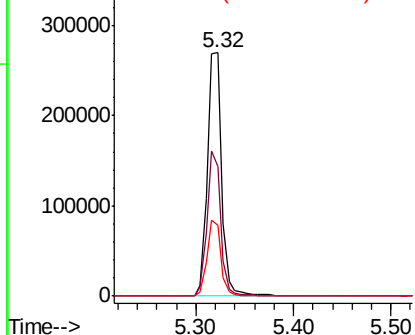



#7

Phenol-d6

Concen: 25.858 ng

RT: 6.34 min Scan# 723

Delta R.T. -0.02 min

Lab File: BF109461.D

Acq: 29 Sep 2018 5:59

Instrument :


BNA_F

ClientSampleId :

092618-TIPC-F-U-S

Tot Ion: 99 Resp: 227597

Ion	Ratio	Lower	Upper
99	100		
42	18.8	14.5	21.7
71	34.0	25.4	38.0






Abundance

Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

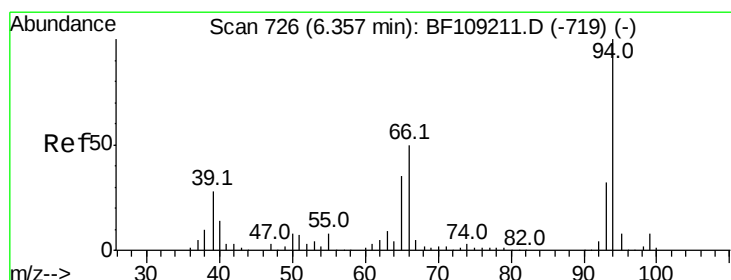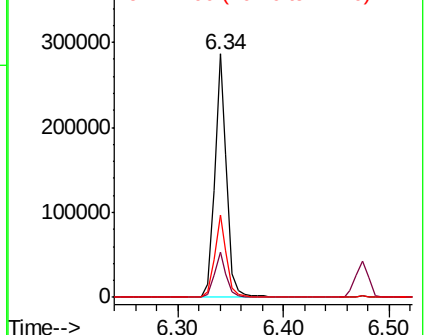

#10

Phenol

Concen: 3.949 ng

RT: 6.35 min Scan# 725


Delta R.T. -0.02 min

Lab File: BF109461.D

Acq: 29 Sep 2018 5:59

Tgt Ion: 94 Resp: 39366

Ion	Ratio	Lower	Upper
94	100		
65	28.9	7.9	47.9
66	40.5	16.2	56.2





Abundance

Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1

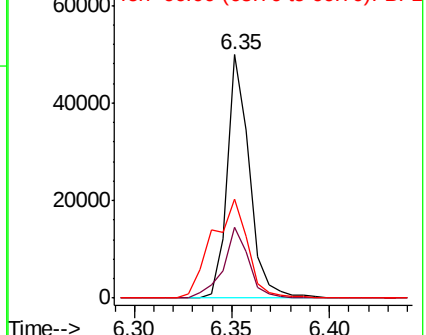



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.99 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF109461.D

Acq: 29 Sep 2018 5:59

Instrument :

BNA_F

ClientSampleId :

092618-TIPC-F-U-S

Tot Ion:136 Resp: 418555


Ion Ratio Lower Upper

136 100

137 10.9 8.9 13.3

54 7.5 6.6 9.8

68 5.7 5.0 7.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

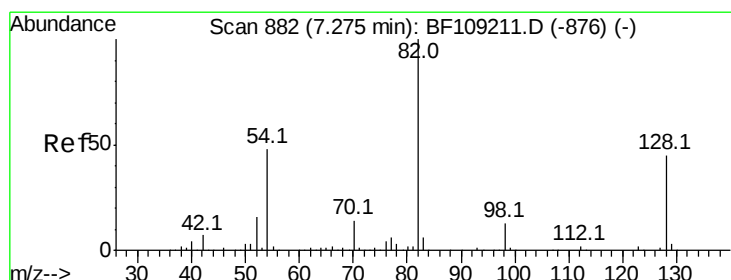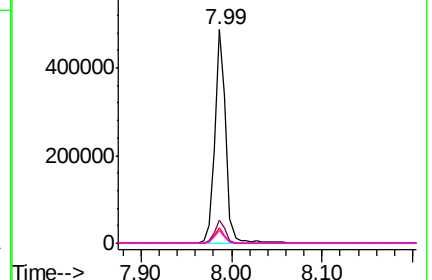

#23

Nitrobenzene-d5

Concen: 101.279 ng

RT: 7.27 min Scan# 881

Delta R.T. -0.01 min

Lab File: BF109461.D

Acq: 29 Sep 2018 5:59


Tgt Ion: 82 Resp: 718104

Ion Ratio Lower Upper

82 100

128 42.4 36.1 54.1



54 49.3 41.4 62.2




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1



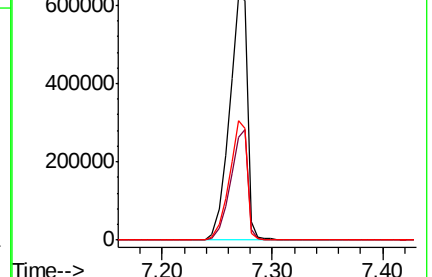



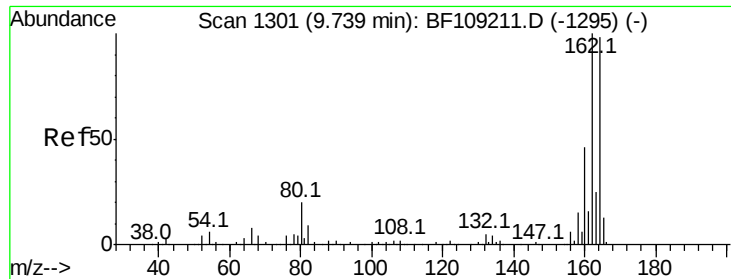

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.74 min Scan# 1301
 Delta R.T. 0.00 min
 Lab File: BF109461.D
 Acq: 29 Sep 2018 5:59




Instrument :
 BNA_F
 ClientSampleId :
 092618-TIPC-F-U-S


Tot Ion	Ratio	Lower	Upper
164	100		
162	105.3	86.1	129.1
160	46.9	38.3	57.5

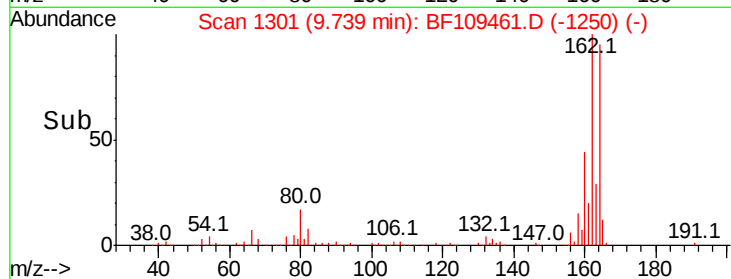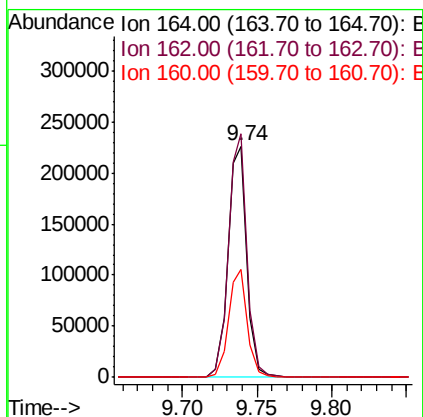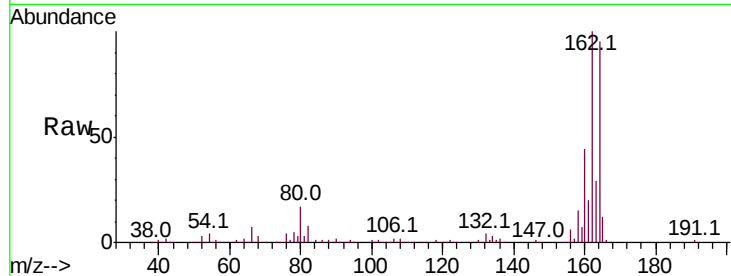

#41
 2,4,6-Tribromophenol
 Concen: 91.596 ng
 RT: 10.52 min Scan# 1434
 Delta R.T. -0.01 min
 Lab File: BF109461.D
 Acq: 29 Sep 2018 5:59

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.4	77.0	115.6
141	33.1	29.9	44.9

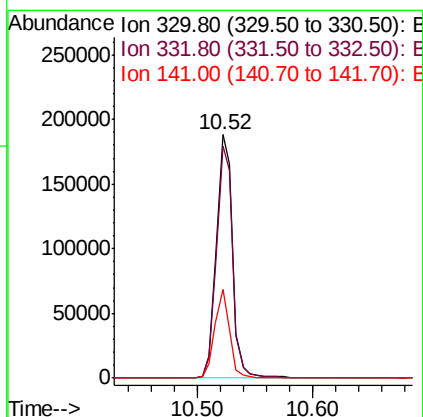







#44
2-Fluorobiphenyl
Concen: 90.953 ng
RT: 9.07 min Scan# 1187
Delta R.T. -0.01 min
Lab File: BF109461.D
Acq: 29 Sep 2018 5:59

Instrument :
BNA_F
ClientSampleId :
092618-TIPC-F-U-S

Tot Ion:172 Resp: 1224357
Ion Ratio Lower Upper
172 100
171 36.5 29.7 44.5
170 24.6 19.6 29.4




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E


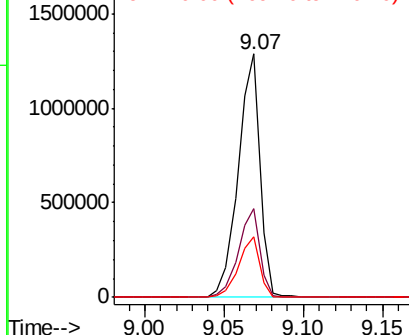



#49
Dimethylphthalate
Concen: 4.479 ng
RT: 9.46 min Scan# 1253
Delta R.T. -0.02 min
Lab File: BF109461.D
Acq: 29 Sep 2018 5:59

Tgt Ion:163 Resp: 66142
Ion Ratio Lower Upper
163 100
194 4.0 2.7 4.1
164 10.7 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

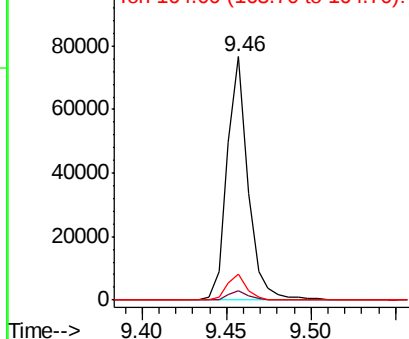

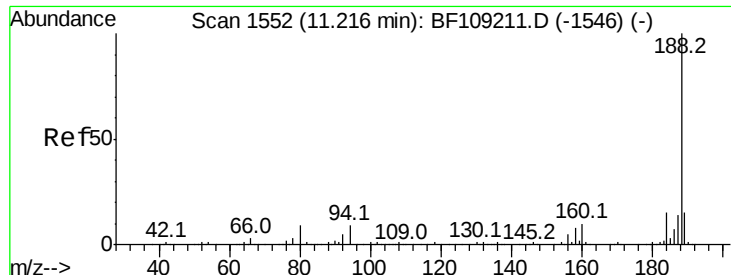

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.22 min Scan# 1552

Delta R.T. 0.00 min

Lab File: BF109461.D

Acq: 29 Sep 2018 5:59

Instrument :

BNA_F

ClientSampleId :

092618-TIPC-F-U-S


Tot Ion:188 Resp: 367655

Ion Ratio Lower Upper

188 100

94 8.6 8.5 12.7




80 9.5 9.2 13.8

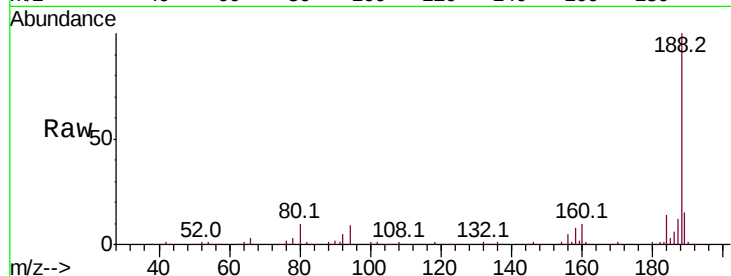

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

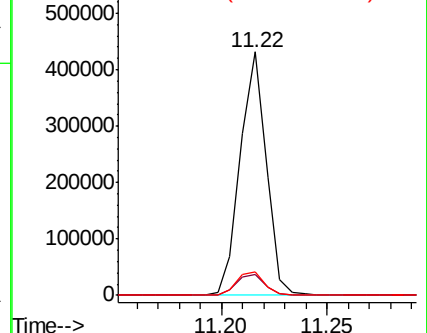

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.84 min Scan# 1998

Delta R.T. -0.01 min

Lab File: BF109461.D

Acq: 29 Sep 2018 5:59


Tgt Ion:240 Resp: 220866

Ion Ratio Lower Upper

240 100

120 11.1 9.5 14.3



236 25.2 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

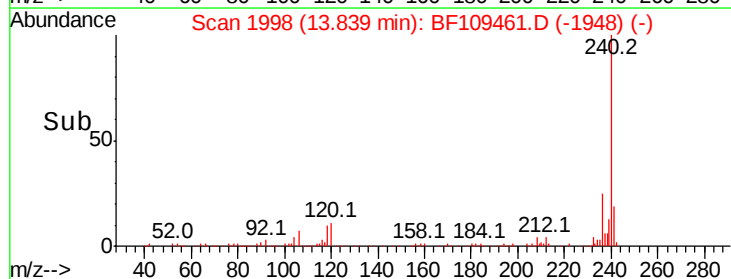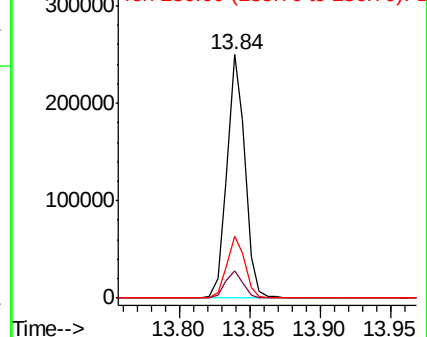


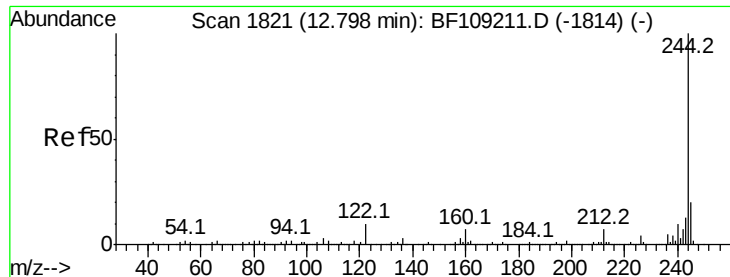




#78
 Terphenyl-d14
 Concen: 120.990 ng
 RT: 12.80 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BF109461.D
 Acq: 29 Sep 2018 5:59

Instrument :
 BNA_F
 ClientSampleId :
 092618-TIPC-F-U-S

Tot Ion:244 Resp: 1088863
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.4 8.0
 122 12.2 11.0 16.4

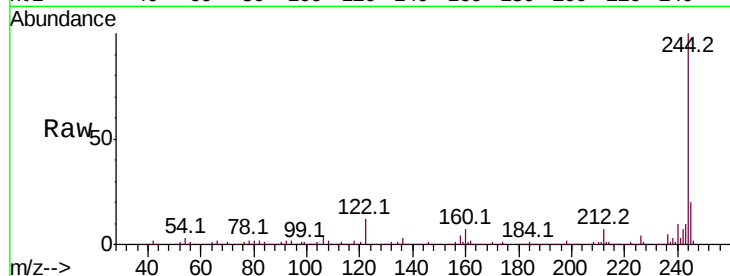


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

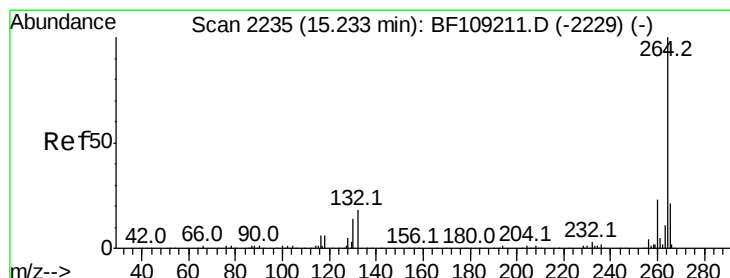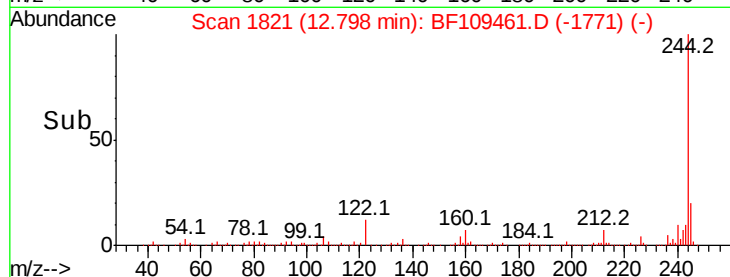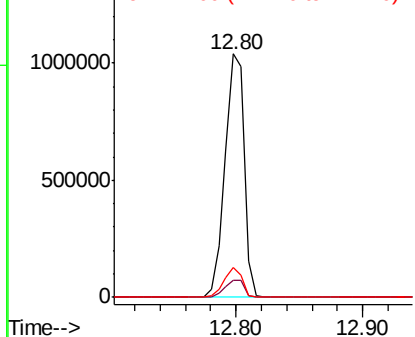

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.24 min Scan# 2237
 Delta R.T. 0.01 min
 Lab File: BF109461.D
 Acq: 29 Sep 2018 5:59

Tgt Ion:264 Resp: 221482
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.2 28.8
 265 21.1 17.5 26.3

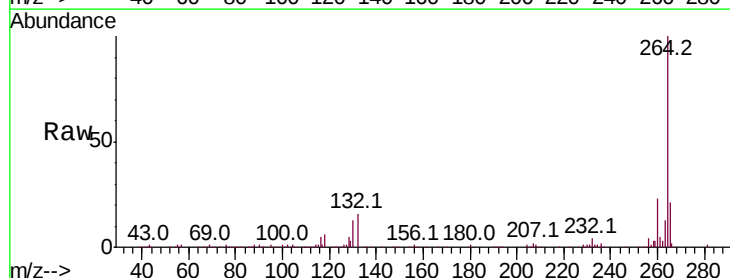

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

