


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092818\
 Data File : BF109428.D
 Acq On : 28 Sep 2018 12:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 22 13:32:18 2018

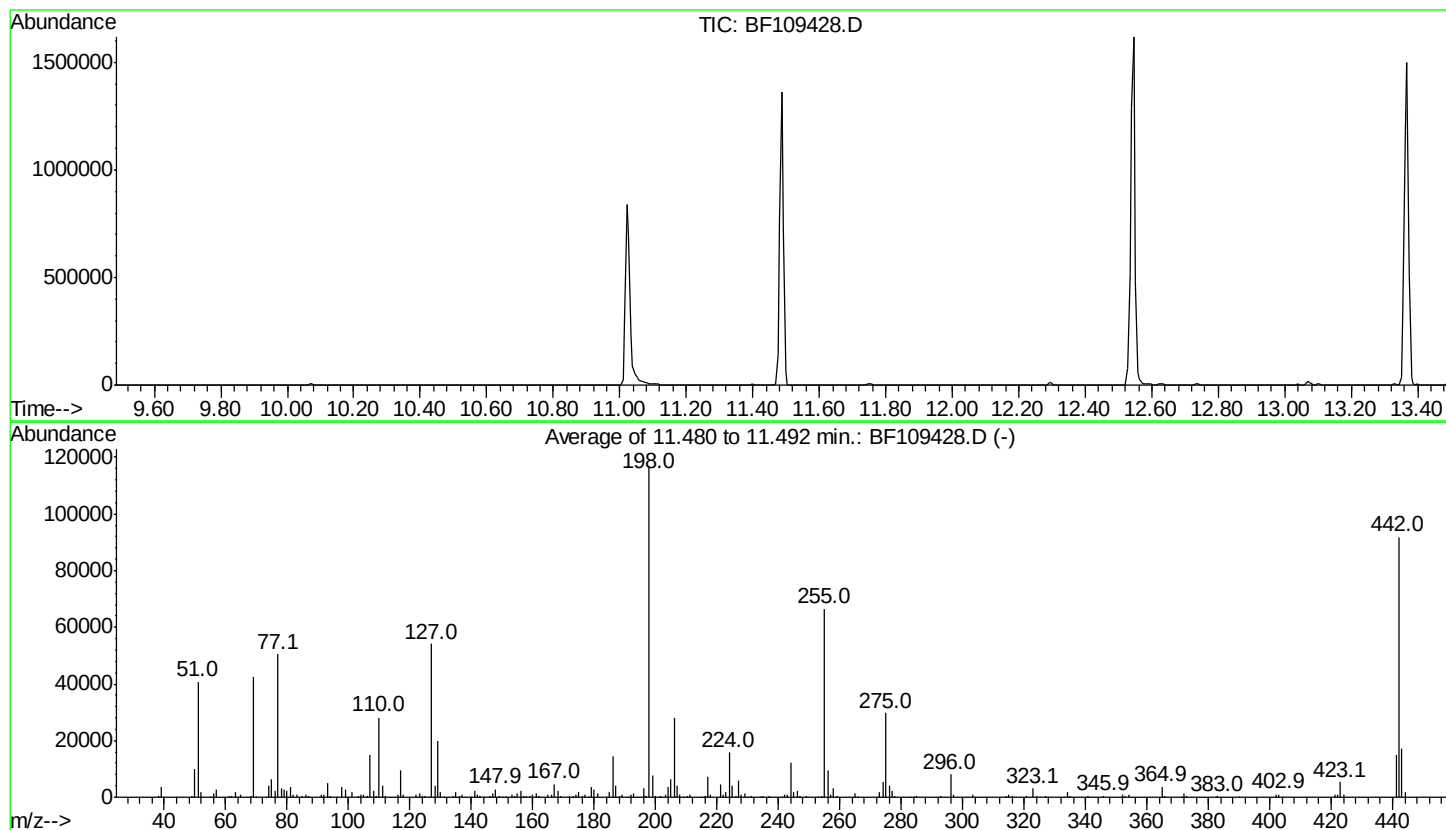

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	40778	PASS
68	69	0.00	2	1.6	665	PASS
69	198	0.00	100	36.5	42690	PASS
70	69	0.00	2	0.3	113	PASS
127	198	10	80	46.2	54082	PASS
197	198	0.00	2	0.5	561	PASS
198	198	100	100	100.0	117048	PASS
199	198	5	9	6.6	7740	PASS
275	198	10	60	25.5	29805	PASS
365	198	1	100	3.1	3684	PASS
441	198	0.01	100	12.6	14773	PASS
442	198	50	100	78.4	91730	PASS
443	442	15	24	18.9	17348	PASS