


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092820\
 Data File : BF121701.D
 Acq On : 28 Sep 2020 8:56
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 29 11:12:14 2020

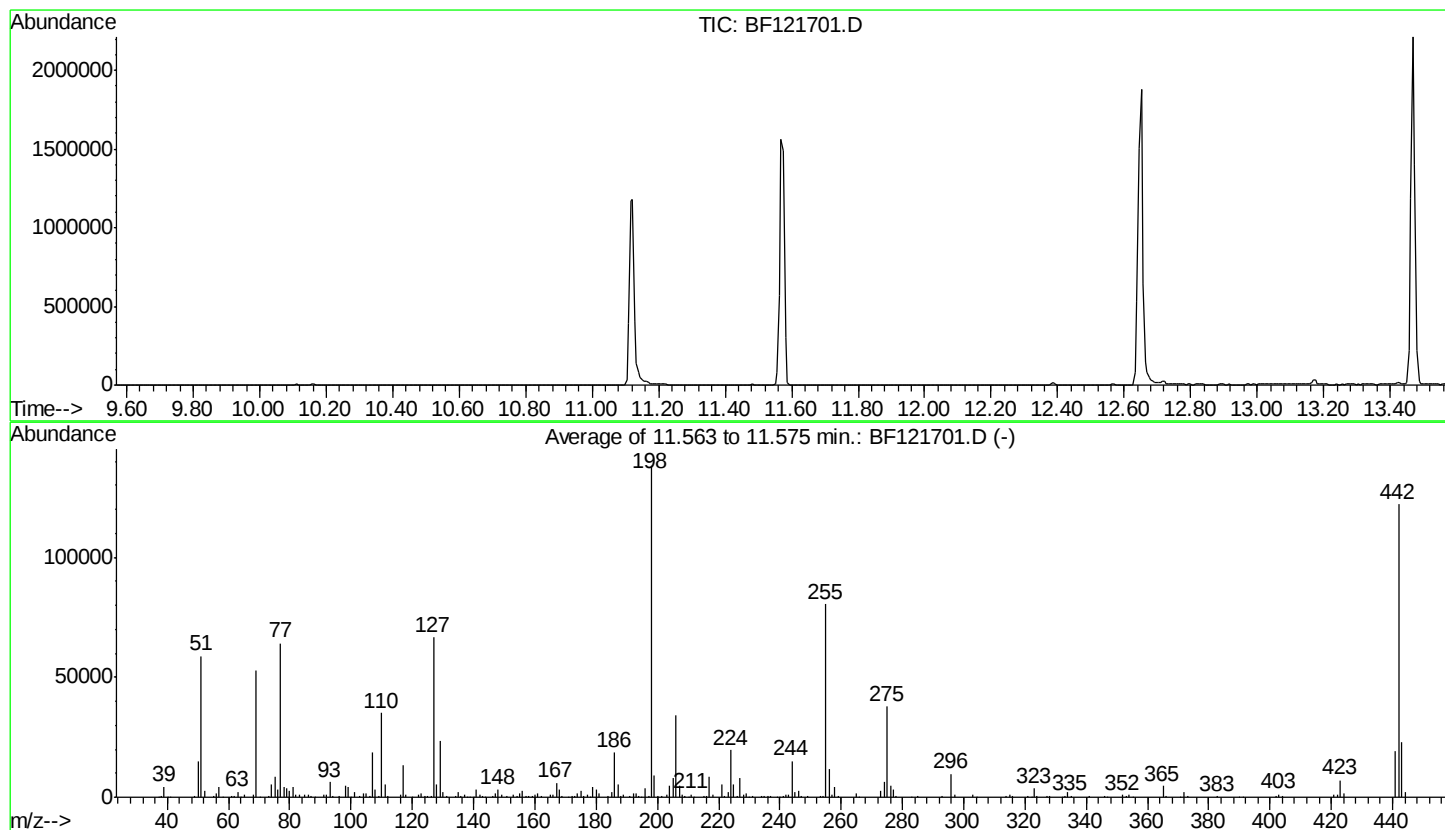

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	58797	PASS
68	69	0.00	2	1.9	1022	PASS
69	198	0.00	100	38.1	52616	PASS
70	69	0.00	2	0.3	165	PASS
127	198	10	80	48.2	66546	PASS
197	198	0.00	2	0.3	376	PASS
198	198	100	100	100.0	138165	PASS
199	198	5	9	6.7	9285	PASS
275	198	10	60	27.3	37744	PASS
365	198	1	100	3.4	4733	PASS
441	198	0.01	100	14.0	19404	PASS
442	198	50	100	88.3	122010	PASS
443	442	15	24	19.0	23137	PASS