

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092915\
 Data File : BF081909.D
 Acq On : 30 Sep 2015 12:38
 Operator : UM/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC

Quant Time: Sep 30 13:12:25 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 18:10:42 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.93	152	114888	20.00	ng	-0.01
21) Naphthalene-d8	8.21	136	283918	20.00	ng	-0.01
38) Acenaphthene-d10	9.97	164	149161	20.00	ng	-0.01
63) Phenanthrene-d10	11.45	188	354294	20.00	ng	-0.01
75) Chrysene-d12	14.10	240	335781	20.00	ng	-0.01
86) Perylene-d12	15.57	264	405450	20.00	ng	-0.01

System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	448347	70.84	ng	-0.01
7) Phenol-d6	6.55	99	609569	76.54	ng	-0.01
23) Nitrobenzene-d5	7.49	82	550518	129.25	ng	-0.01
41) 2,4,6-Tribromophenol	10.75	330	147517	97.65	ng	-0.01
44) 2-Fluorobiphenyl	9.29	172	775029	87.43	ng	-0.01
78) Terphenyl-d14	13.04	244	939583	92.67	ng	-0.01

Target Compounds				Qvalue		
2) 1,4-Dioxane	2.54	88	114844	41.73	ng	86
3) Pyridine	3.29	79	274184	38.26	ng	86
4) n-Nitrosodimethylamine	3.25	42	112915	34.69	ng	100
6) Aniline	6.58	93	396482	37.06	ng	# 86
8) 2-Chlorophenol	6.71	128	267200	38.23	ng	96
9) Benzaldehyde	6.47	77	182071	34.91	ng	# 78
10) Phenol	6.56	94	352852	39.50	ng	71
11) bis(2-Chloroethyl)ether	6.66	93	278541	40.21	ng	90
12) 1,3-Dichlorobenzene	7.10	146	276493	33.49	ng	97
13) 1,4-Dichlorobenzene	7.10	146	289585	33.59	ng	97
14) 1,2-Dichlorobenzene	7.10	146	302353	39.36	ng	99
15) Benzyl Alcohol	7.06	79	192884	33.55	ng	# 73
16) 2,2'-oxybis(1-Chloropropan	7.20	45	379918	38.79	ng	81
17) 2-Methylphenol	7.18	107	222512	39.27	ng	# 88
18) Hexachloroethane	7.43	117	95458	35.37	ng	92
19) n-Nitroso-di-n-propylamine	7.34	70	188222	38.89	ng	# 77
20) 3+4-Methylphenols	7.33	107	248547	34.73	ng	# 78
22) Acetophenone	7.34	105	362766	62.49	ng	# 84
24) Nitrobenzene	7.51	77	306568	66.29	ng	# 68
25) Isophorone	7.75	82	482637	57.17	ng	# 91
26) 2-Nitrophenol	7.83	139	101754	45.84	ng	# 79
27) 2,4-Dimethylphenol	7.86	122	146886	37.61	ng	# 79
28) bis(2-Chloroethoxy)methane	7.95	93	185004	36.90	ng	# 92
29) 2,4-Dichlorophenol	8.07	162	148593	39.24	ng	98
30) 1,2,4-Trichlorobenzene	8.15	180	172421	40.78	ng	97
31) Naphthalene	8.23	128	500939	39.82	ng	97
32) Benzoic acid	7.98	122	68294	32.10	ng	# 67
33) 4-Chloroaniline	8.29	127	206138	37.89	ng	# 93
34) Hexachlorobutadiene	8.34	225	106082	42.43	ng	98
35) Caprolactam	8.66	113	42354	40.40	ng	90
36) 4-Chloro-3-methylphenol	8.77	107	153647	41.49	ng	92
37) 2-Methylnaphthalene	8.93	142	347758	40.50	ng	# 91
39) 1,2,4,5-Tetrachlorobenzene	9.09	216	178974	39.08	ng	98
40) Hexachlorocyclopentadiene	9.07	237	102031	43.27	ng	97

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092915\
 Data File : BF081909.D
 Acq On : 30 Sep 2015 12:38
 Operator : UM/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC

Quant Time: Sep 30 13:12:25 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 18:10:42 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) 2,4,6-Trichlorophenol	9.20	196	118879	37.87	ng	98
43) 2,4,5-Trichlorophenol	9.23	196	133326	41.30	ng #	91
45) 1,1'-Biphenyl	9.38	154	429568	37.33	ng	94
46) 2-Chloronaphthalene	9.42	162	352152	38.97	ng	98
47) 2-Nitroaniline	9.51	65	104736	39.48	ng #	62
48) Acenaphthylene	9.83	152	563841	38.99	ng	96
49) Dimethylphthalate	9.69	163	434025	42.15	ng #	98
50) 2,6-Dinitrotoluene	9.76	165	87512	39.15	ng	94
51) Acenaphthene	10.00	154	337274	39.27	ng	88
52) 3-Nitroaniline	9.93	138	103632	40.07	ng #	83
53) 2,4-Dinitrophenol	10.03	184	31109	42.29	ng #	51
54) Dibenzofuran	10.17	168	475875	39.21	ng #	86
55) 4-Nitrophenol	10.08	139	62171	33.27	ng #	49
56) 2,4-Dinitrotoluene	10.16	165	126698	44.46	ng #	98
57) Fluorene	10.51	166	454941	52.78	ng	91
58) 2,3,4,6-Tetrachlorophenol	10.29	232	115252	45.01	ng	98
59) Diethylphthalate	10.39	149	504241	52.43	ng	98
60) 4-Chlorophenyl-phenylether	10.50	204	210989	47.48	ng #	77
61) 4-Nitroaniline	10.55	138	125883	48.55	ng #	54
62) Azobenzene	10.66	77	454047	48.38	ng	87
64) 4,6-Dinitro-2-methylphenol	10.56	198	63386	40.89	ng	97
65) n-Nitrosodiphenylamine	10.63	169	422828	39.44	ng	91
66) 4-Bromophenyl-phenylether	10.99	248	138365	38.73	ng #	82
67) Hexachlorobenzene	11.06	284	160521	39.82	ng #	78
68) Atrazine	11.15	200	137480	41.33	ng	83
69) Pentachlorophenol	11.26	266	91266	39.73	ng	99
70) Phenanthrene	11.47	178	652969	38.04	ng	96
71) Anthracene	11.53	178	755893	41.98	ng	97
72) Carbazole	11.69	167	657722	40.36	ng	96
73) Di-n-butylphthalate	12.01	149	777889	46.92	ng #	98
74) Fluoranthene	12.66	202	756077	39.84	ng	92
76) Benzidine	12.80	184	358886	35.47	ng	97
77) Pyrene	12.90	202	738071	36.79	ng	97
79) Butylbenzylphthalate	13.52	149	366161	48.51	ng #	91
80) Benzo(a)anthracene	14.09	228	671619	37.14	ng	96
81) 3,3'-Dichlorobenzidine	14.06	252	245033	40.13	ng #	93
82) Chrysene	14.09	228	671619	40.51	ng	98
83) Bis(2-ethylhexyl)phthalate	14.07	149	471279	49.77	ng #	91
84) Di-n-octyl phthalate	14.69	149	783870	50.87	ng #	93
85) Indeno(1,2,3-cd)pyrene	17.03	276	821241	58.06	ng #	86
87) Benzo(b)fluoranthene	15.13	252	844484	36.48	ng #	88
88) Benzo(k)fluoranthene	15.13	252	844484	39.80	ng #	89
89) Benzo(a)pyrene	15.50	252	719562	35.84	ng #	88
90) Dibenzo(a,h)anthracene	17.04	278	681247	40.44	ng #	81
91) Benzo(g,h,i)perylene	17.46	276	516327	29.91	ng #	75


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092915\
Data File : BF081909.D
Acq On : 30 Sep 2015 12:38
Operator : UM/IZ
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC

Quant Time: Sep 30 13:12:25 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration





#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.93 min Scan# 419

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:152 Resp: 114888

Ion Ratio Lower Upper

152 100

150 159.9 124.7 187.1


115 53.4 39.0 58.4




Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E



Time-->



#2

1,4-Dioxane

Concen: 41.73 ng

RT: 2.54 min Scan# 35

Delta R.T. -0.00 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion: 88 Resp: 114844

Ion Ratio Lower Upper

88 100

58 81.9 77.7 116.5


43 27.1 26.6 40.0




Abundance Ion 88.00 (87.70 to 88.70): BF0

Ion 58.00 (57.70 to 58.70): BF0

Ion 43.00 (42.70 to 43.70): BF0



Time-->



#3

Pyridine

Concen: 38.26 ng

RT: 3.29 min Scan# 101

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC





Tgt Ion: 79 Resp: 274184

Ion Ratio Lower Upper

79 100

52 78.5 76.8 115.2

51 37.0 32.2 48.4



#4

n-Nitrosodimethylamine

Concen: 34.69 ng

RT: 3.25 min Scan# 97

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38




Tgt Ion: 42 Resp: 112915

Ion Ratio Lower Upper

42 100

74 131.7 105.0 157.6

44 7.4 6.6 10.0





#5

2-Fluorophenol

Concen: 70.84 ng

RT: 5.51 min Scan# 295

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion: 112 Resp: 448347

Ion Ratio Lower Upper

112 100

64 63.4 39.7 59.5#




63 33.2 17.4 26.0#



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0



#6

Aniline

Concen: 37.06 ng

RT: 6.58 min Scan# 389

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion: 93 Resp: 396482

Ion Ratio Lower Upper

93 100

66 43.5 27.2 40.8#



65 22.2 14.7 22.1#




Abundance Ion 93.00 (92.70 to 93.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

Ion 65.00 (64.70 to 65.70): BF0





#7

Phenol-d6

Concen: 76.54 ng

RT: 6.55 min Scan# 386

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC





Tgt Ion: 99 Resp: 609569

Ion Ratio Lower Upper

99 100

42 17.3 13.7 20.5

71 32.7 14.2 21.2#



#8

2-Chlorophenol

Concen: 38.23 ng

RT: 6.71 min Scan# 400

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38




Tgt Ion: 128 Resp: 267200


Ion Ratio Lower Upper

128 100

130 34.3 12.2 52.2

64 37.4 20.5 60.5





#9

Benzaldehyde

Concen: 34.91 ng

RT: 6.47 min Scan# 379

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC





Tgt Ion: 77 Resp: 182071

Ion Ratio Lower Upper

77 100

105 96.7 91.6 131.6

106 90.7 102.6 142.6#



#10

Phenol

Concen: 39.50 ng

RT: 6.56 min Scan# 387

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38




Tgt Ion: 94 Resp: 352852

Ion Ratio Lower Upper

94 100

65 29.4 0.7 40.7

66 39.0 0.8 40.8









#11
bis(2-Chloroethyl)ether
Concen: 40.21 ng
RT: 6.66 min Scan# 396
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38




Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC


Tgt Ion: 93 Resp: 278541
Ion Ratio Lower Upper
93 100
63 73.4 65.6 105.6
95 32.1 13.6 53.6



#12
1,3-Dichlorobenzene
Concen: 33.49 ng
RT: 7.10 min Scan# 434
Delta R.T. 0.23 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Tgt Ion: 146 Resp: 276493
Ion Ratio Lower Upper
146 100
148 65.7 51.0 76.4
75 21.3 15.0 22.6









#13
 1,4-Dichlorobenzene
 Concen: 33.59 ng
 RT: 7.10 min Scan# 434
 Delta R.T. 0.15 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC


Tgt Ion:146 Resp: 289585
 Ion Ratio Lower Upper
 146 100
 148 65.7 51.8 77.6
 111 34.6 24.9 37.3



#14
 1,2-Dichlorobenzene
 Concen: 39.36 ng
 RT: 7.10 min Scan# 434
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion:146 Resp: 302353
 Ion Ratio Lower Upper
 146 100
 148 65.7 52.7 79.1
 111 34.6 28.8 43.2





#15

Benzyl Alcohol

Concen: 33.55 ng

RT: 7.06 min Scan# 431

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC





Tgt Ion: 79 Resp: 192884

Ion Ratio Lower Upper

79 100

108 71.1 88.6 132.8#

77 63.6 47.0 70.4



#16

2,2'-oxybis(1-Chloropropane)

Concen: 38.79 ng

RT: 7.20 min Scan# 443

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38




Tgt Ion: 45 Resp: 379918

Ion Ratio Lower Upper

45 100

77 15.1 0.0 28.1

79 12.4 0.0 26.0









#17
2-Methylphenol
Concen: 39.27 ng
RT: 7.18 min Scan# 441
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38




Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC

Tgt Ion	Ratio	Lower	Upper
107	100		
108	115.5	96.6	145.0
77	41.7	23.3	34.9#
79	43.3	22.0	33.0#



#18
Hexachloroethane
Concen: 35.37 ng
RT: 7.43 min Scan# 463
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Tgt Ion	Ratio	Lower	Upper
117	100		
119	93.8	83.8	125.6
201	73.2	55.1	82.7









#19
n-Nitroso-di-n-propylamine
Concen: 38.89 ng
RT: 7.34 min Scan# 455
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38




Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC


Tgt Ion: 70 Resp: 188222
Ion Ratio Lower Upper
70 100
42 58.1 63.8 95.6#
101 8.9 9.2 13.8#
130 18.9 27.3 40.9#



#20
3+4-Methylphenols
Concen: 34.73 ng
RT: 7.33 min Scan# 454
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Tgt Ion: 107 Resp: 248547
Ion Ratio Lower Upper
107 100
108 89.4 74.6 114.6
77 66.9 0.7 40.7#
79 29.2 0.0 38.9





#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.21 min Scan# 531

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC

Tgt Ion:136 Resp: 283918


Ion Ratio Lower Upper

136 100

137 11.1 9.0 13.6

54 9.4 8.2 12.2

68 5.3 5.8 8.6#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



#22

Acetophenone

Concen: 62.49 ng

RT: 7.34 min Scan# 455

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Tgt Ion:105 Resp: 362766


Ion Ratio Lower Upper

105 100

71 9.9 4.7 7.1#

51 29.0 22.0 33.0

120 21.4 30.1 45.1#






Abundance Ion 105.00 (104.70 to 105.70): E

Ion 71.00 (70.70 to 71.70): BF0

Ion 51.00 (50.70 to 51.70): BF0

Ion 120.00 (119.70 to 120.70): E









#23
 Nitrobenzene-d5
 Concen: 129.25 ng
 RT: 7.49 min Scan# 468
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC


Tgt Ion: 82 Resp: 550518
 Ion Ratio Lower Upper
 82 100
 128 40.8 51.0 76.6#
 54 56.1 47.5 71.3



#24
 Nitrobenzene
 Concen: 66.29 ng
 RT: 7.51 min Scan# 470
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion: 77 Resp: 306568
 Ion Ratio Lower Upper
 77 100
 123 43.6 59.8 89.8#
 65 13.6 10.2 15.4





#25

Isophorone

Concen: 57.17 ng

RT: 7.75 min Scan# 491

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC





Tgt Ion: 82 Resp: 482637

Ion Ratio Lower Upper

82 100

95 7.2 4.0 6.0#

138 18.3 18.3 27.5



#26

2-Nitrophenol

Concen: 45.84 ng

RT: 7.83 min Scan# 498

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38




Tgt Ion: 139 Resp: 101754


Ion Ratio Lower Upper

139 100

109 26.6 11.0 16.4#

65 40.1 24.7 37.1#





#27

2,4-Dimethylphenol

Concen: 37.61 ng

RT: 7.86 min Scan# 501

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:122 Resp: 146886

Ion Ratio Lower Upper

122 100

107 116.0 71.8 107.6#




121 59.2 42.3 63.5



Abundance Ion 122.00 (121.70 to 122.70): E

Ion 107.00 (106.70 to 107.70): E

Ion 121.00 (120.70 to 121.70): E



#28

bis(2-Chloroethoxy)methane

Concen: 36.90 ng

RT: 7.95 min Scan# 509

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion: 93 Resp: 185004

Ion Ratio Lower Upper

93 100

95 31.9 27.5 41.3



123 10.5 13.7 20.5#




Abundance Ion 93.00 (92.70 to 93.70): BF0

Ion 95.00 (94.70 to 95.70): BF0

Ion 123.00 (122.70 to 123.70): E









#29
 2,4-Dichlorophenol
 Concen: 39.24 ng
 RT: 8.07 min Scan# 519
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC

Tgt Ion	Ratio	Lower	Upper
162	100		
164	64.8	44.9	84.9
98	29.4	13.0	53.0




Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 98.00 (97.70 to 98.70): BF0






#30
 1,2,4-Trichlorobenzene
 Concen: 40.78 ng
 RT: 8.15 min Scan# 526
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion	Ratio	Lower	Upper
180	100		
182	93.1	77.1	115.7
145	30.0	23.3	34.9



Abundance Ion 180.00 (179.70 to 180.70): E
 Ion 182.00 (181.70 to 182.70): E
 Ion 145.00 (144.70 to 145.70): E





#31

Naphthalene

Concen: 39.82 ng

RT: 8.23 min Scan# 533

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:128 Resp: 500939

Ion Ratio Lower Upper

128 100

129 11.5 8.4 12.6




127 13.4 9.9 14.9



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E



#32

Benzoic acid

Concen: 32.10 ng

RT: 7.98 min Scan# 511

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion:122 Resp: 68294

Ion Ratio Lower Upper

122 100

105 120.6 76.1 116.1#



77 95.6 40.5 80.5#




Abundance Ion 122.00 (121.70 to 122.70): E

Ion 105.00 (104.70 to 105.70): E

Ion 77.00 (76.70 to 77.70): BF0









#33
4-Chloroaniline
Concen: 37.89 ng
RT: 8.29 min Scan# 538
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38




Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC


Tgt Ion:	127	Resp:	206138
Ion	Ratio	Lower	Upper
127	100		
129	33.1	25.8	38.6
65	28.3	17.9	26.9#
92	17.8	10.5	15.7#



#34
Hexachlorobutadiene
Concen: 42.43 ng
RT: 8.34 min Scan# 543
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Tgt Ion:	225	Resp:	106082
Ion	Ratio	Lower	Upper
225	100		
223	64.4	50.2	75.2
227	63.5	52.2	78.2









#35
 Caprolactam
 Concen: 40.40 ng
 RT: 8.66 min Scan# 571
 Delta R.T. 0.00 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC


Tgt Ion:113 Resp: 42354
 Ion Ratio Lower Upper
 113 100
 55 185.6 152.4 192.4
 56 137.2 104.6 144.6



#36
 4-Chloro-3-methylphenol
 Concen: 41.49 ng
 RT: 8.77 min Scan# 580
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion:107 Resp: 153647
 Ion Ratio Lower Upper
 107 100
 144 28.3 25.4 38.0
 142 88.2 77.3 115.9









#37
 2-Methylnaphthalene
 Concen: 40.50 ng
 RT: 8.93 min Scan# 594
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC


Tgt Ion	Ratio	Lower	Upper
142	100		
141	89.1	67.5	101.3
115	34.6	18.2	27.2#



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.97 min Scan# 685
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.1	75.2	112.8
160	45.9	31.5	47.3





#39

1,2,4,5-Tetrachlorobenzene

Concen: 39.08 ng

RT: 9.09 min Scan# 608

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC

Tgt Ion:216 Resp: 178974



Ion Ratio Lower Upper

216 100

214 78.8 63.5 95.3

179 22.2 16.6 24.8

108 18.3 16.3 24.5





Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E



#40

Hexachlorocyclopentadiene

Concen: 43.27 ng

RT: 9.07 min Scan# 607

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38



Tgt Ion:237 Resp: 102031

Ion Ratio Lower Upper

237 100

235 63.1 42.0 82.0


272 12.5 0.0 36.1




Abundance Ion 236.80 (236.50 to 237.50): E

Ion 234.90 (234.60 to 235.60): E

Ion 271.75 (271.45 to 272.45): E









#41
 2,4,6-Tribromophenol
 Concen: 97.65 ng
 RT: 10.75 min Scan# 754
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC

Tgt Ion:330 Resp: 147517
 Ion Ratio Lower Upper
 330 100
 332 96.0 76.6 114.8
 141 36.5 29.7 44.5




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E





#42
 2,4,6-Trichlorophenol
 Concen: 37.87 ng
 RT: 9.20 min Scan# 618
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion:196 Resp: 118879
 Ion Ratio Lower Upper
 196 100
 198 96.2 75.7 113.5
 200 29.3 23.9 35.9



Abundance Ion 196.00 (195.70 to 196.70): E
 Ion 198.00 (197.70 to 198.70): E
 Ion 200.00 (199.70 to 200.70): E






#43
 2,4,5-Trichlorophenol
 Concen: 41.30 ng
 RT: 9.23 min Scan# 621
 Delta R.T. -0.02 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC

Tgt Ion	Ratio	Lower	Upper
196	100		
198	93.6	75.4	113.0
97	61.0	33.3	49.9
132	33.6	24.6	37.0






Abundance

Ion 196.00 (195.70 to 196.70): E

Ion 198.00 (197.70 to 198.70): E


Ion 97.00 (96.70 to 97.70): BF0

Ion 132.00 (131.70 to 132.70): E



#44
 2-Fluorobiphenyl
 Concen: 87.43 ng
 RT: 9.29 min Scan# 626
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	26.1	39.1
170	24.2	17.4	26.2






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E









#45
 1,1'-Biphenyl
 Concen: 37.33 ng
 RT: 9.38 min Scan# 634
 Delta R.T. -0.02 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC


Tgt Ion	Ratio	Lower	Upper
154	100		
153	40.9	17.1	57.1
76	13.0	0.0	31.6



#46
 2-Chloronaphthalene
 Concen: 38.97 ng
 RT: 9.42 min Scan# 637
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion	Ratio	Lower	Upper
162	100		
127	35.1	27.6	41.4
164	33.3	25.4	38.2





#47

2-Nitroaniline

Concen: 39.48 ng

RT: 9.51 min Scan# 645

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC





Tgt Ion: 65 Resp: 104736

Ion Ratio Lower Upper

65 100

92 60.8 55.4 83.0

138 80.6 115.5 173.3#



#48

Acenaphthylene

Concen: 38.99 ng

RT: 9.83 min Scan# 673

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38




Tgt Ion: 152 Resp: 563841


Ion Ratio Lower Upper

152 100

151 20.7 14.6 22.0

153 13.5 10.3 15.5





#49

Dimethylphthalate

Concen: 42.15 ng

RT: 9.69 min Scan# 661

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC





Tgt Ion:163 Resp: 434025

Ion Ratio Lower Upper

163 100

194 3.6 4.4 6.6#

164 10.3 8.3 12.5



#50

2,6-Dinitrotoluene

Concen: 39.15 ng

RT: 9.76 min Scan# 667

Delta R.T. 0.00 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38




Tgt Ion:165 Resp: 87512


Ion Ratio Lower Upper

165 100

63 33.8 32.3 48.5

89 35.8 28.6 43.0





#51

Acenaphthene

Concen: 39.27 ng

RT: 10.00 min Scan# 688

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:154 Resp: 337274

Ion Ratio Lower Upper

154 100

153 115.1 82.1 123.1




152 54.9 37.9 56.9



Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E



#52

3-Nitroaniline

Concen: 40.07 ng

RT: 9.93 min Scan# 682

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion:138 Resp: 103632

Ion Ratio Lower Upper

138 100

108 9.1 5.7 8.5#



92 100.5 67.7 101.5



Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BF0









#53
2,4-Dinitrophenol
Concen: 42.29 ng
RT: 10.03 min Scan# 691
Delta R.T. 0.00 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38




Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC


Tgt Ion:184 Resp: 31109
Ion Ratio Lower Upper
184 100
63 62.7 35.4 53.2#
154 84.5 32.2 48.4#



#54
Dibenzofuran
Concen: 39.21 ng
RT: 10.17 min Scan# 703
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Tgt Ion:168 Resp: 475875
Ion Ratio Lower Upper
168 100
139 41.3 24.2 36.2#
169 13.6 10.6 15.8





#55

4-Nitrophenol

Concen: 33.27 ng

RT: 10.08 min Scan# 695

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:139 Resp: 62171

Ion Ratio Lower Upper

139 100

109 74.1 12.7 52.7#




65 97.3 45.9 85.9#



Abundance Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): BF0



#56

2,4-Dinitrotoluene

Concen: 44.46 ng

RT: 10.16 min Scan# 702

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Tgt Ion:165 Resp: 126698


Ion Ratio Lower Upper

165 100

63 34.9 29.8 44.6

89 54.9 44.5 66.7

182 2.5 3.0 4.4#






Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0

Ion 182.00 (181.70 to 182.70): E





#57

Fluorene

Concen: 52.78 ng

RT: 10.51 min Scan# 733

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:166 Resp: 454941

Ion Ratio Lower Upper

166 100

165 100.1 72.6 109.0




167 13.8 10.6 16.0



Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E



#58

2,3,4,6-Tetrachlorophenol

Concen: 45.01 ng

RT: 10.29 min Scan# 713

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Tgt Ion:232 Resp: 115252


Ion Ratio Lower Upper

232 100

131 46.2 38.5 57.7

130 2.1 1.8 2.6

166 30.8 25.0 37.6






Abundance Ion 232.00 (231.70 to 232.70): E

Ion 131.00 (130.70 to 131.70): E

Ion 130.00 (129.70 to 130.70): E

Ion 166.00 (165.70 to 166.70): E





#59

Diethylphthalate

Concen: 52.43 ng

RT: 10.39 min Scan# 722

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:149 Resp: 504241

Ion Ratio Lower Upper

149 100

177 22.6 17.5 26.3




150 12.6 9.4 14.2



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 177.00 (176.70 to 177.70): E

Ion 150.00 (149.70 to 150.70): E



#60

4-Chlorophenyl-phenylether

Concen: 47.48 ng

RT: 10.50 min Scan# 732

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion:204 Resp: 210989

Ion Ratio Lower Upper

204 100

206 32.6 24.8 37.2



141 77.8 42.2 63.4#




Abundance Ion 204.00 (203.70 to 204.70): E

Ion 206.00 (205.70 to 206.70): E

Ion 141.00 (140.70 to 141.70): E









#61
4-Nitroaniline
Concen: 48.55 ng
RT: 10.55 min Scan# 736
Delta R.T. 0.00 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38




Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC


Tgt Ion:138 Resp: 125883
Ion Ratio Lower Upper
138 100
92 45.6 12.6 52.6
108 70.6 12.4 52.4#



#62
Azobenzene
Concen: 48.38 ng
RT: 10.66 min Scan# 746
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Tgt Ion: 77 Resp: 454047
Ion Ratio Lower Upper
77 100
182 18.0 15.1 55.1
105 20.4 3.4 43.4
51 32.1 12.0 52.0









#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.45 min Scan# 815
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC

Tgt Ion:188 Resp: 354294
Ion Ratio Lower Upper
188 100
94 9.2 11.1 16.7#
80 10.2 11.0 16.4#




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0






#64
4,6-Dinitro-2-methylphenol
Concen: 40.89 ng
RT: 10.56 min Scan# 737
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Tgt Ion:198 Resp: 63386
Ion Ratio Lower Upper
198 100
51 57.3 39.6 79.6
105 51.1 28.5 68.5



Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF0
Ion 105.00 (104.70 to 105.70): E









#65
 n-Nitrosodiphenylamine
 Concen: 39.44 ng
 RT: 10.63 min Scan# 743
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC

Tgt Ion:169 Resp: 422828
 Ion Ratio Lower Upper
 169 100
 168 68.5 48.9 73.3
 167 37.5 26.2 39.4



#66
 4-Bromophenyl-phenylether
 Concen: 38.73 ng
 RT: 10.99 min Scan# 775
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion:248 Resp: 138365
 Ion Ratio Lower Upper
 248 100
 250 96.8 78.5 117.7
 141 107.2 59.0 88.6#









#67
Hexachlorobenzene
Concen: 39.82 ng
RT: 11.06 min Scan# 781
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC

Tgt Ion:284 Resp: 160521
Ion Ratio Lower Upper
284 100
142 19.0 29.5 44.3#
249 28.8 19.5 29.3




Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E






#68
Atrazine
Concen: 41.33 ng
RT: 11.15 min Scan# 789
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Tgt Ion:200 Resp: 137480
Ion Ratio Lower Upper
200 100
173 25.6 13.2 53.2
215 47.2 41.8 81.8



Abundance Ion 200.00 (199.70 to 200.70): E
Ion 173.00 (172.70 to 173.70): E
Ion 215.00 (214.70 to 215.70): E









#69
 Pentachlorophenol
 Concen: 39.73 ng
 RT: 11.26 min Scan# 798
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC

Tgt Ion: 266 Resp: 91266
 Ion Ratio Lower Upper
 266 100
 268 62.5 49.8 74.6
 264 63.3 50.2 75.2




Abundance Ion 265.70 (265.40 to 266.40): E
 Ion 268.00 (267.70 to 268.70): E
 Ion 264.00 (263.70 to 264.70): E






#70
 Phenanthrene
 Concen: 38.04 ng
 RT: 11.47 min Scan# 817
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion: 178 Resp: 652969
 Ion Ratio Lower Upper
 178 100
 176 19.5 13.8 20.8
 179 15.9 12.2 18.2



Abundance Ion 178.00 (177.70 to 178.70): E
 Ion 176.00 (175.70 to 176.70): E
 Ion 179.00 (178.70 to 179.70): E









#71
 Anthracene
 Concen: 41.98 ng
 RT: 11.53 min Scan# 822
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC


Tgt Ion:178 Resp: 755893
 Ion Ratio Lower Upper
 178 100
 176 19.7 14.1 21.1
 179 15.7 12.2 18.2



#72
 Carbazole
 Concen: 40.36 ng
 RT: 11.69 min Scan# 836
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion:167 Resp: 657722
 Ion Ratio Lower Upper
 167 100
 166 21.9 15.7 23.5
 139 12.5 9.5 14.3





#73

Di-n-butylphthalate

Concen: 46.92 ng

RT: 12.01 min Scan# 864

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:149 Resp: 777889

Ion Ratio Lower Upper




149 100

150 9.6 7.4 11.2

104 5.2 2.4 3.6#



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 104.00 (103.70 to 104.70): E



#74

Fluoranthene

Concen: 39.84 ng

RT: 12.66 min Scan# 921

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion:202 Resp: 756077

Ion Ratio Lower Upper



202 100


101 11.9 0.0 38.3

203 17.9 0.0 37.3



Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 203.00 (202.70 to 203.70): E





#75

Chrysene-d12

Concen: 20.00 ng

RT: 14.10 min Scan# 1047

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:240 Resp: 335781

Ion Ratio Lower Upper

240 100

120 6.5 16.2 24.2#




236 25.8 18.4 27.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



#76

Benzidine

Concen: 35.47 ng

RT: 12.80 min Scan# 933

Delta R.T. -0.01 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion:184 Resp: 358886

Ion Ratio Lower Upper

184 100

185 15.8 11.8 17.6



183 10.9 7.6 11.4




Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E









#77
 Pyrene
 Concen: 36.79 ng
 RT: 12.90 min Scan# 942
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC

Tgt Ion: 202 Resp: 738071
 Ion Ratio Lower Upper
 202 100
 200 21.3 15.0 22.4
 203 17.3 14.1 21.1



#78
 Terphenyl-d14
 Concen: 92.67 ng
 RT: 13.04 min Scan# 954
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion: 244 Resp: 939583
 Ion Ratio Lower Upper
 244 100
 212 8.0 4.3 6.5#
 122 11.0 17.4 26.2#









#79
Butylbenzylphthalate
Concen: 48.51 ng
RT: 13.52 min Scan# 996
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38




Instrument :
BNA_F
ClientSampleId :
SSTDCCC040EC

Tgt Ion:149 Resp: 366161
Ion Ratio Lower Upper
149 100
91 53.8 48.6 72.8
206 23.1 14.9 22.3#



#80
Benzo(a)anthracene
Concen: 37.14 ng
RT: 14.09 min Scan# 1046
Delta R.T. -0.01 min
Lab File: BF081909.D
Acq: 30 Sep 2015 12:38

Tgt Ion:228 Resp: 671619
Ion Ratio Lower Upper
228 100
226 27.8 20.0 30.0
229 20.0 15.4 23.2









#81
 3,3'-Dichlorobenzidine
 Concen: 40.13 ng
 RT: 14.06 min Scan# 1043
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC

Tgt Ion: 252 Resp: 245033
 Ion Ratio Lower Upper
 252 100
 254 65.0 51.4 77.2
 126 8.6 16.4 24.6#



#82
 Chrysene
 Concen: 40.51 ng
 RT: 14.09 min Scan# 1046
 Delta R.T. -0.04 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion: 228 Resp: 671619
 Ion Ratio Lower Upper
 228 100
 226 27.8 21.0 31.4
 229 20.0 15.6 23.4









#83
 Bis(2-ethylhexyl)phthalate
 Concen: 49.77 ng
 RT: 14.07 min Scan# 1044
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC


Tgt Ion:149 Resp: 471279
 Ion Ratio Lower Upper
 149 100
 167 25.0 24.2 36.2
 279 2.4 3.8 5.6#



#84
 Di-n-octyl phthalate
 Concen: 50.87 ng
 RT: 14.69 min Scan# 1098
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion:149 Resp: 783870
 Ion Ratio Lower Upper
 149 100
 167 1.4 1.0 1.6
 43 9.5 10.2 15.2#









#85
 Indeno(1,2,3-cd)pyrene
 Concen: 58.06 ng
 RT: 17.03 min Scan# 1303
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38




Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040EC


Tgt Ion: 276 Resp: 821241
 Ion Ratio Lower Upper
 276 100
 138 24.1 25.7 38.5#
 277 25.0 15.6 23.4#



#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.57 min Scan# 1175
 Delta R.T. -0.01 min
 Lab File: BF081909.D
 Acq: 30 Sep 2015 12:38

Tgt Ion: 264 Resp: 405450
 Ion Ratio Lower Upper
 264 100
 260 23.7 16.7 25.1
 265 21.0 17.2 25.8





#87

Benzo(b)fluoranthene

Concen: 36.48 ng

RT: 15.13 min Scan# 1137

Delta R.T. -0.02 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:252 Resp: 844484

Ion Ratio Lower Upper

252 100

253 22.4 17.5 26.3




125 10.4 17.1 25.7#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

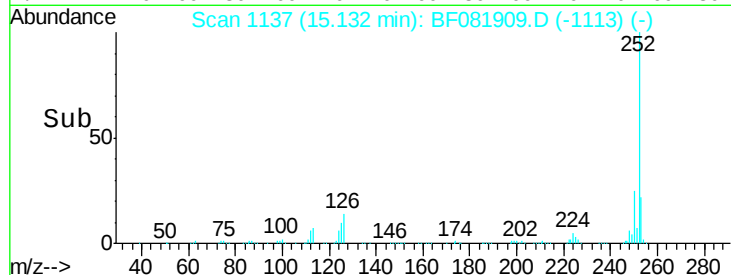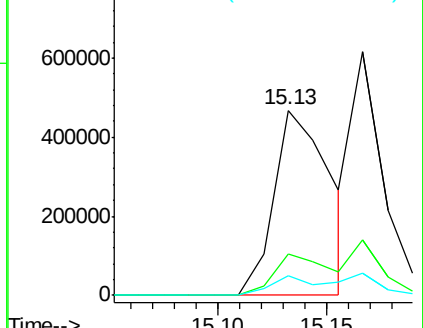

#88

Benzo(k)fluoranthene

Concen: 39.80 ng

RT: 15.13 min Scan# 1137

Delta R.T. -0.05 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion:252 Resp: 844484

Ion Ratio Lower Upper

252 100

253 22.4 17.0 25.4



125 10.4 16.0 24.0#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

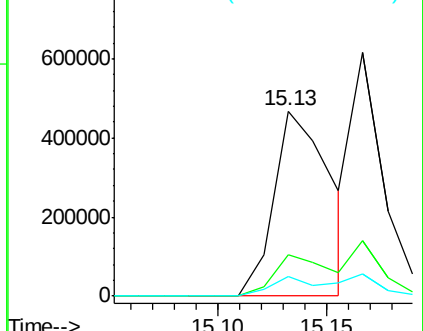



#89

Benzo(a)pyrene

Concen: 35.84 ng

RT: 15.50 min Scan# 1169

Delta R.T. -0.02 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040EC


Tgt Ion:252 Resp: 719562

Ion Ratio Lower Upper

252 100

253 21.9 17.2 25.8




125 11.7 18.0 27.0#



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

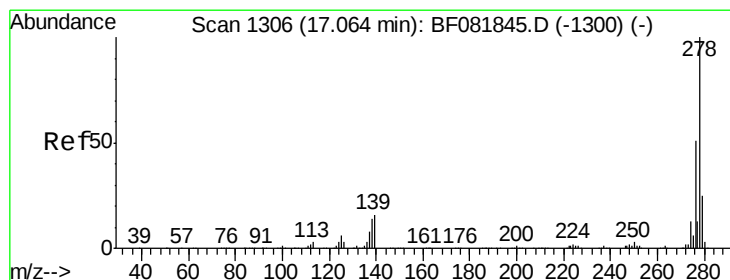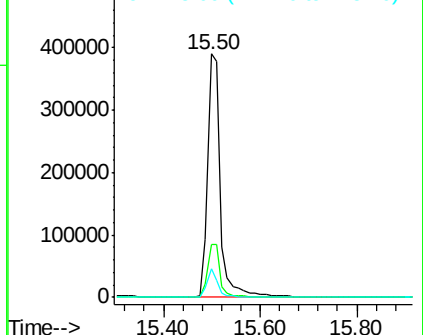

#90

Dibenzo(a,h)anthracene

Concen: 40.44 ng

RT: 17.04 min Scan# 1304

Delta R.T. -0.02 min

Lab File: BF081909.D

Acq: 30 Sep 2015 12:38


Tgt Ion:278 Resp: 681247

Ion Ratio Lower Upper

278 100

139 15.7 26.3 39.5#



279 23.8 18.2 27.4



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

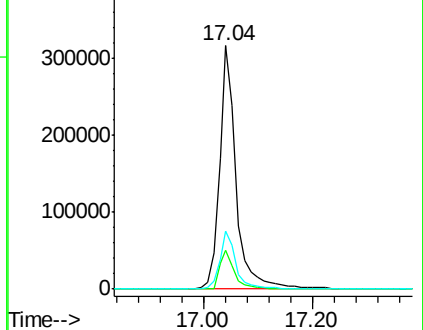



#91

Benzo(g,h,i)perylene

Concen: 29.91 ng

RT: 17.46 min Scan# 1341

Delta R.T. -0.02 min

Lab File: BF081909.D


Acq: 30 Sep 2015 12:38

Instrument :


BNA_F

ClientSampleId :

SSTDCCC040EC



Tgt Ion:	276	Resp:	516327
Ion Ratio	Lower	Upper	
276	100		
277	23.9	17.8	26.6
138	20.2	34.6	51.8#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

