
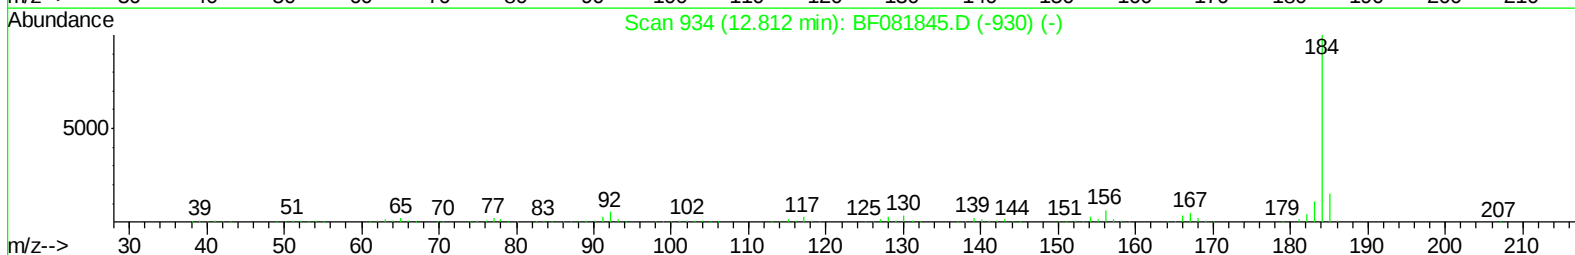
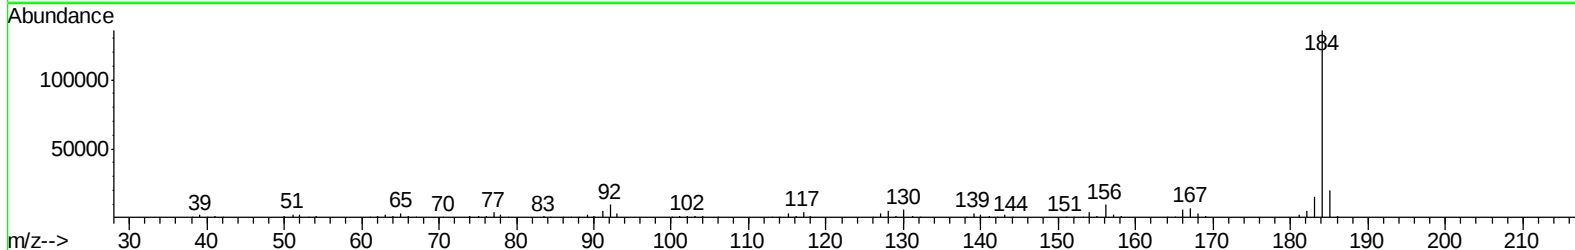


Data Path : Z:\HPCHEM1\BNA F\Data\BF092915\
 Data File : BF081893.D
 Acq On : 30 Sep 2015 2:44
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 09:02:49 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 28 18:10:42 2015
 Response via : Initial Calibration

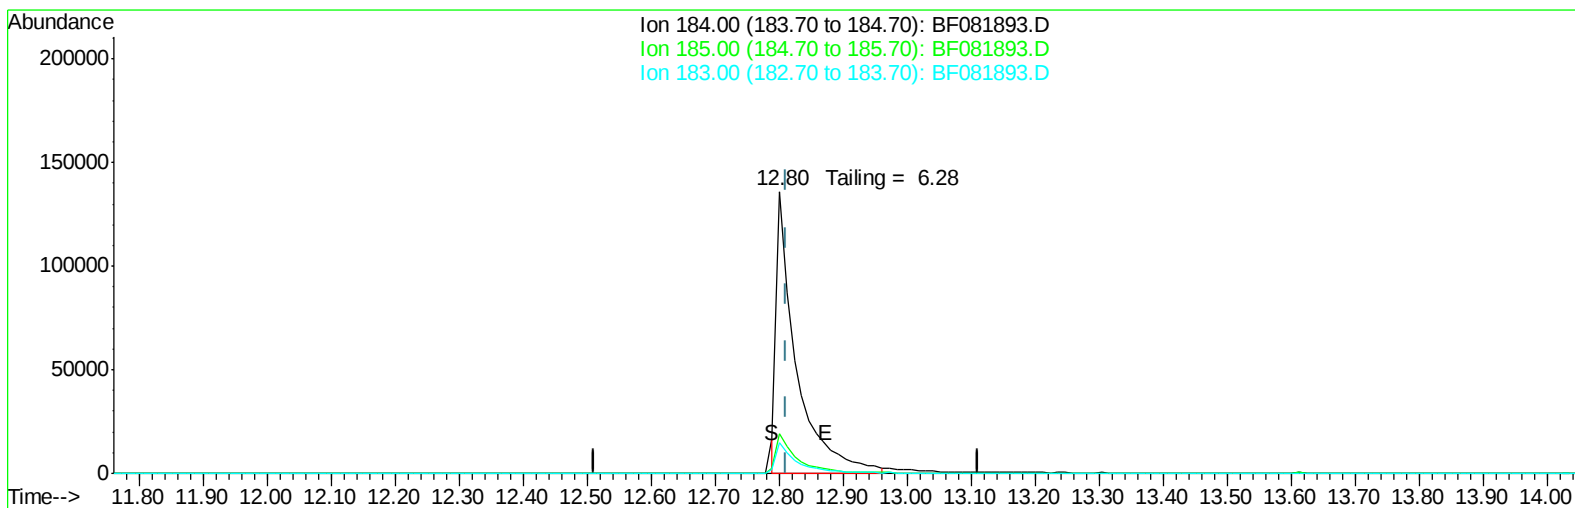

TIC: BF081893.D

(76) Benzidine




12.801min (-0.011) 0.00ng

response 310350

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.27
183.00	9.50	11.06
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF092915\
Data File : BF081893.D
Acq On : 30 Sep 2015 2:44
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 09:02:49 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 28 18:10:42 2015
Response via : Initial Calibration

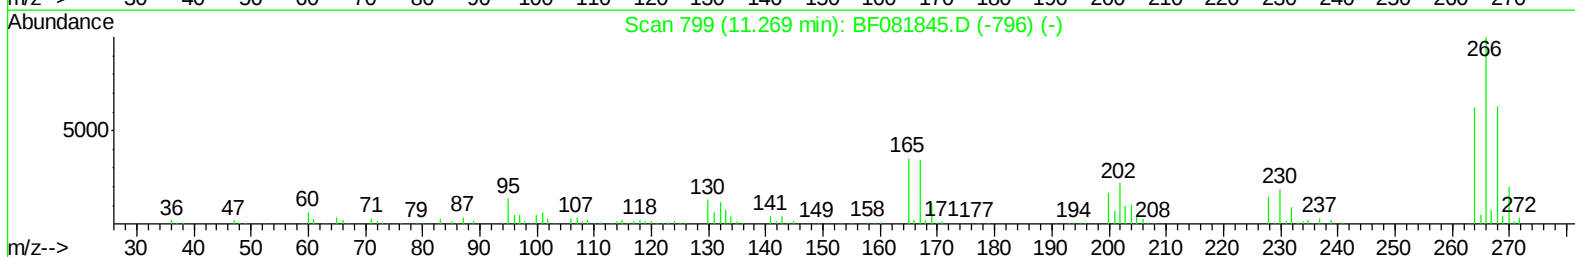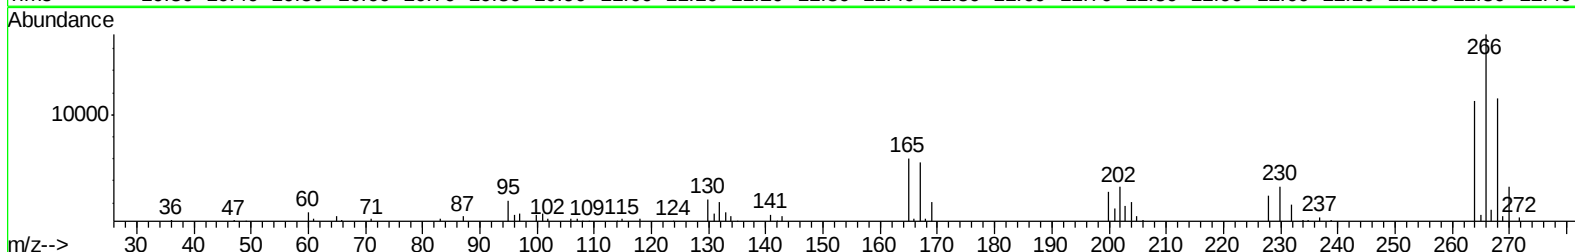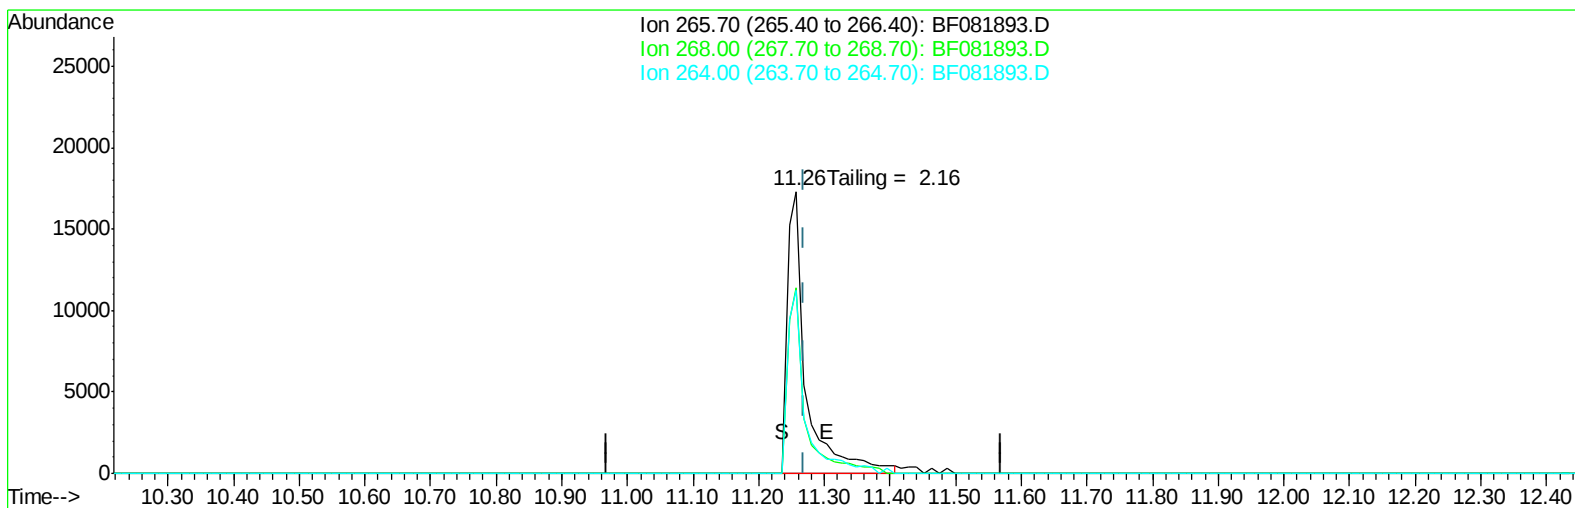

TIC: BF081893.D

(69) Pentachlorophenol (C)

11.258min (-0.011) 23328.70ng

response 35999

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	66.11
264.00	62.70	65.22
0.00	0.00	0.00