

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092915\
 Data File : BF081890.D
 Acq On : 29 Sep 2015 20:33
 Operator : UM/IZ
 Sample : PB85767BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB85767BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.109	257	260	271	rBV	225604	272589	9.54%	1.639%
2	5.520	293	296	298	rBV	813095	985309	34.49%	5.926%
3	6.537	383	385	395	rBV	708273	868483	30.40%	5.223%
4	6.686	395	398	400	rBV	909154	976161	34.17%	5.871%
5	6.926	417	419	430	rBV	246741	436286	15.27%	2.624%
6	7.074	430	432	446	rVB	1431188	1400370	49.02%	8.422%
7	7.486	466	468	494	rBV	874587	1078923	37.77%	6.489%
8	8.206	529	531	548	rBV	503634	619548	21.69%	3.726%
9	9.280	623	625	628	rBV	1764746	2270508	79.48%	13.655%
10	9.966	682	685	687	rBV	830909	851363	29.80%	5.120%
11	10.755	752	754	772	rBV	757286	1018919	35.67%	6.128%
12	11.452	813	815	828	rBV	865041	997877	34.93%	6.001%
13	13.041	952	954	957	rBV	2760691	2856822	100.00%	17.181%
14	14.092	1044	1046	1059	rBV	786752	1086951	38.05%	6.537%
15	15.567	1172	1175	1188	rBV	530871	907817	31.78%	5.460%




Sum of corrected areas: 16627926

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092915\
Data File : BF081890.D
Acq On : 29 Sep 2015 20:33
Operator : UM/IZ
Sample : PB85767BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85767BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

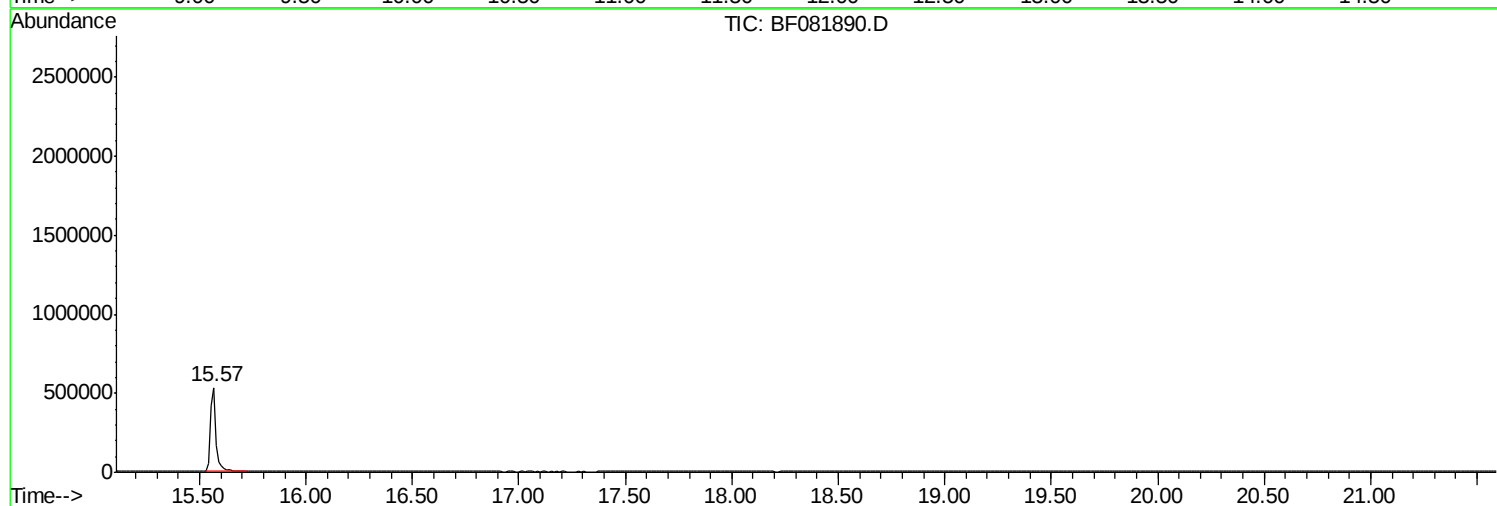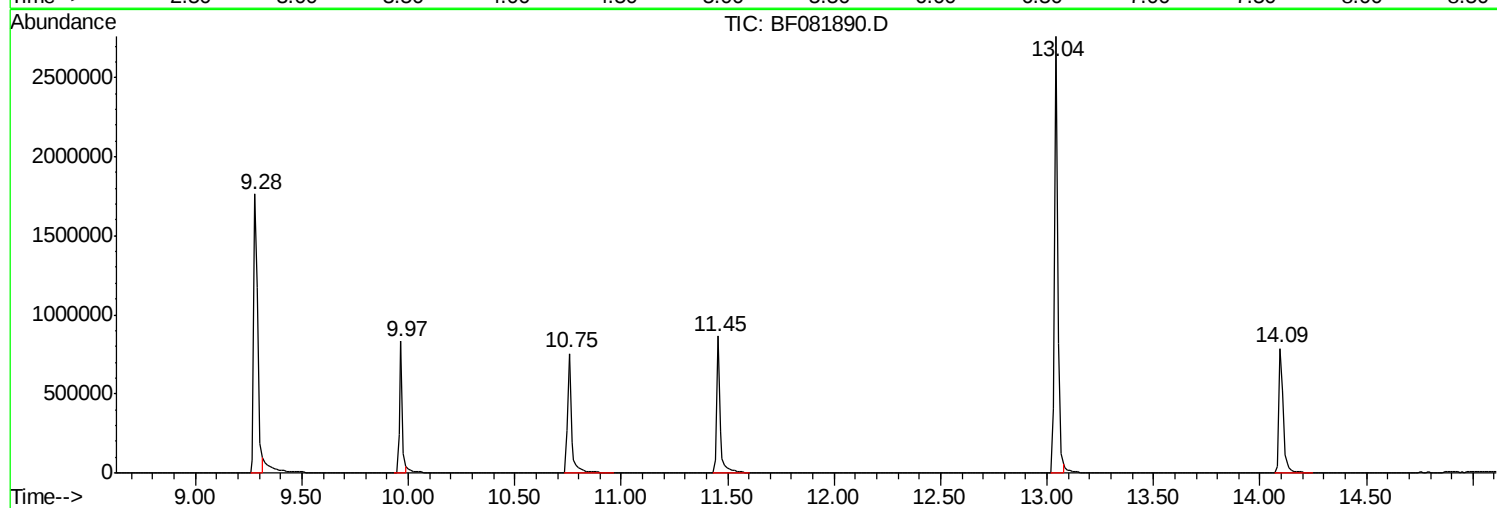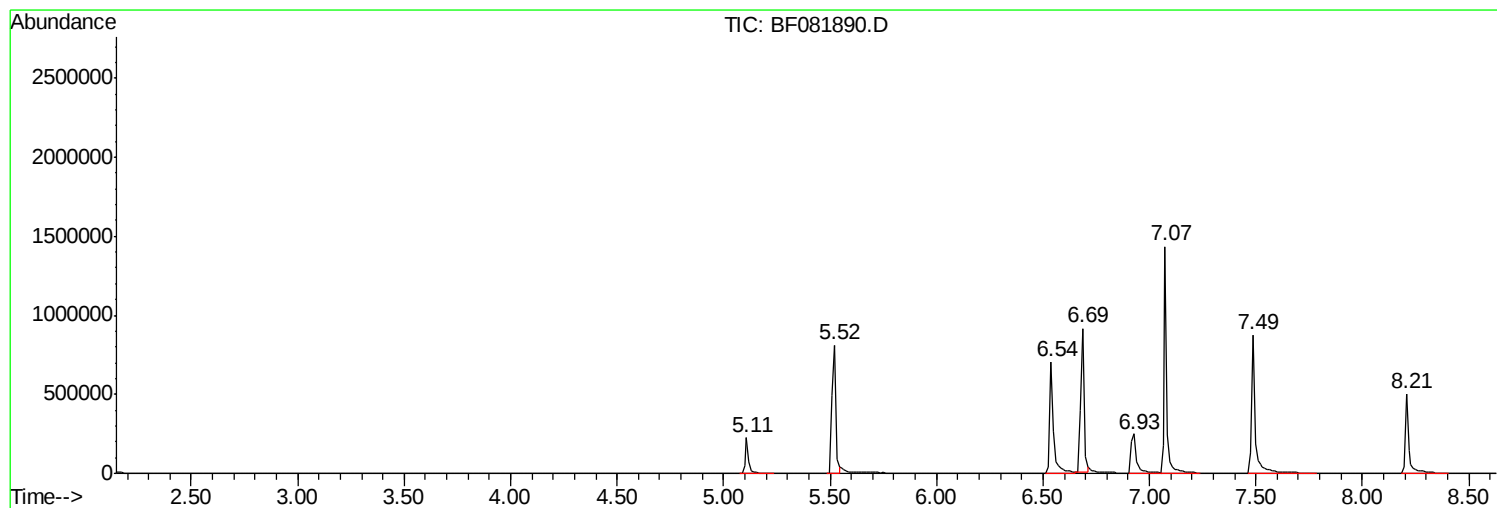

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092915\
Data File : BF081890.D
Acq On : 29 Sep 2015 20:33
Operator : UM/IZ
Sample : PB85767BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85767BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.11	12.50 ng	272589	1,4-Dichlorobenzene-d4	6.93

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2		Propane, 2-methyl-2-(1-methylethoxy)-	116	C7H16O	017348-59-3	36
3		Acetic acid, cyano-, 1,1-dimethyl-	141	C7H11NO2	001116-98-9	23
4		Acetone	58	C3H6O	000067-64-1	9
5		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

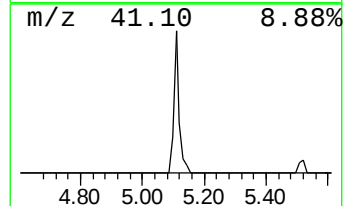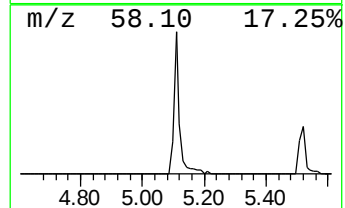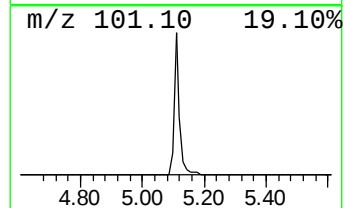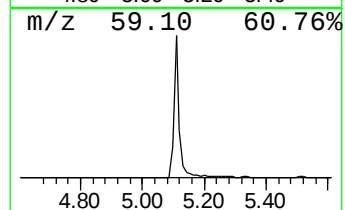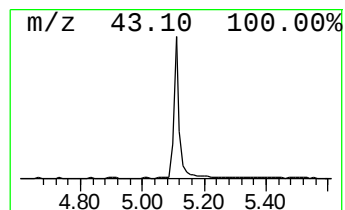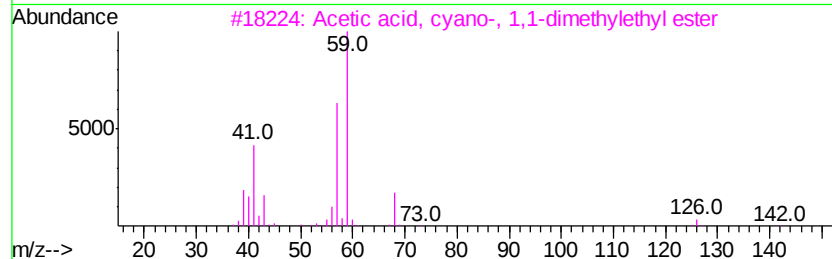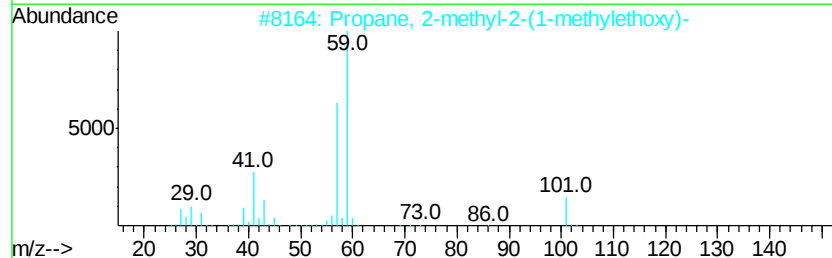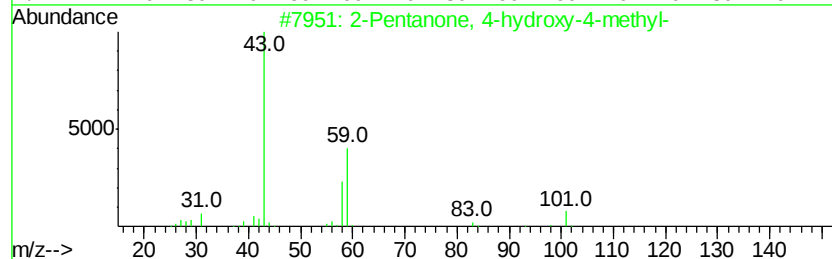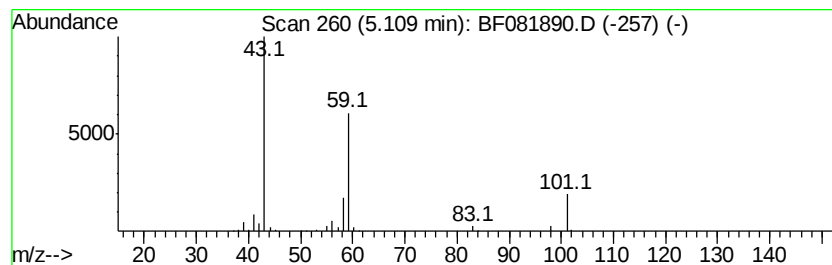

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092915\
Data File : BF081890.D
Acq On : 29 Sep 2015 20:33
Operator : UM/IZ
Sample : PB85767BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85767BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.69 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.69	44.75 ng	976161	1,4-Dichlorobenzene-d4	6.93

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
4		Xenon	132	Xe	007440-63-3	9
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

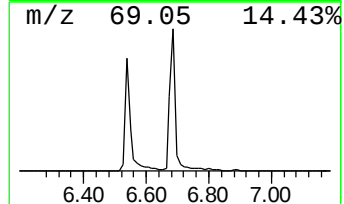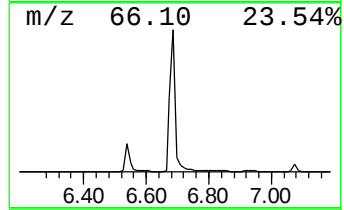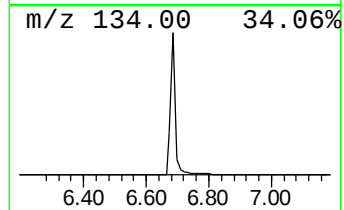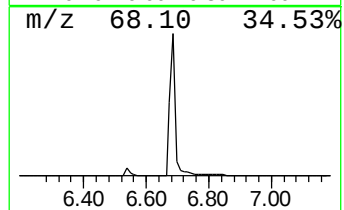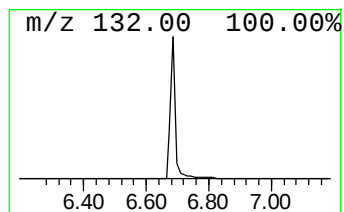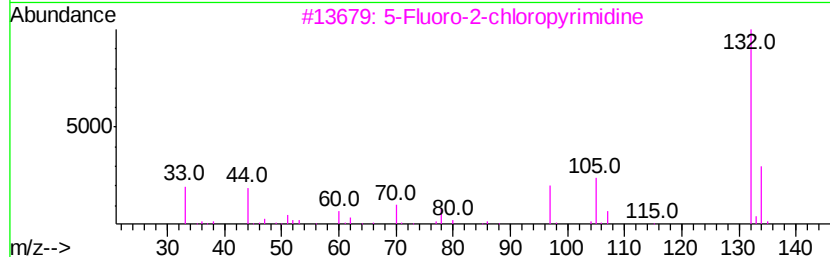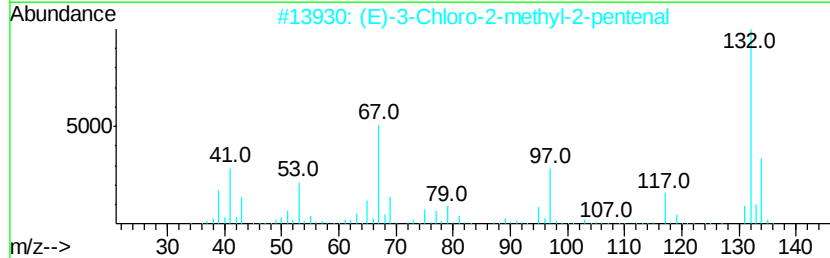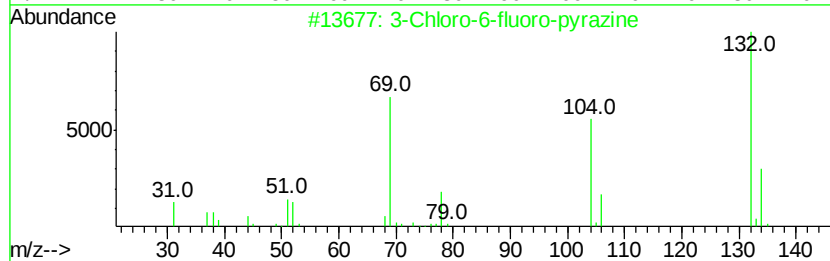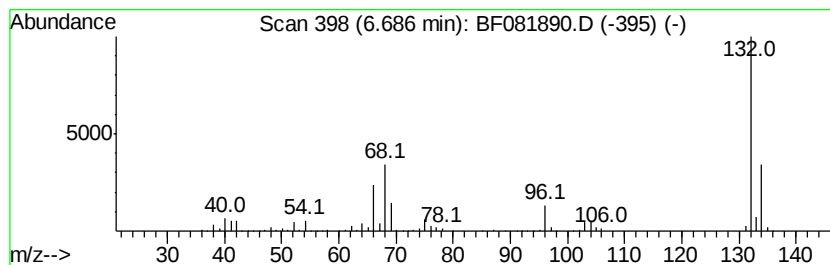

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092915\
Data File : BF081890.D
Acq On : 29 Sep 2015 20:33
Operator : UM/IZ
Sample : PB85767BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85767BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.11	12.5	ng	272589	1	6.93	436286	20.0
unknown6.69	6.69	44.8	ng	976161	1	6.93	436286	20.0