


Data Path : Z:\HPCHEM1\BNA_F\Data\BF092915\
 Data File : BF081893.D
 Acq On : 30 Sep 2015 2:44
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 28 18:10:42 2015

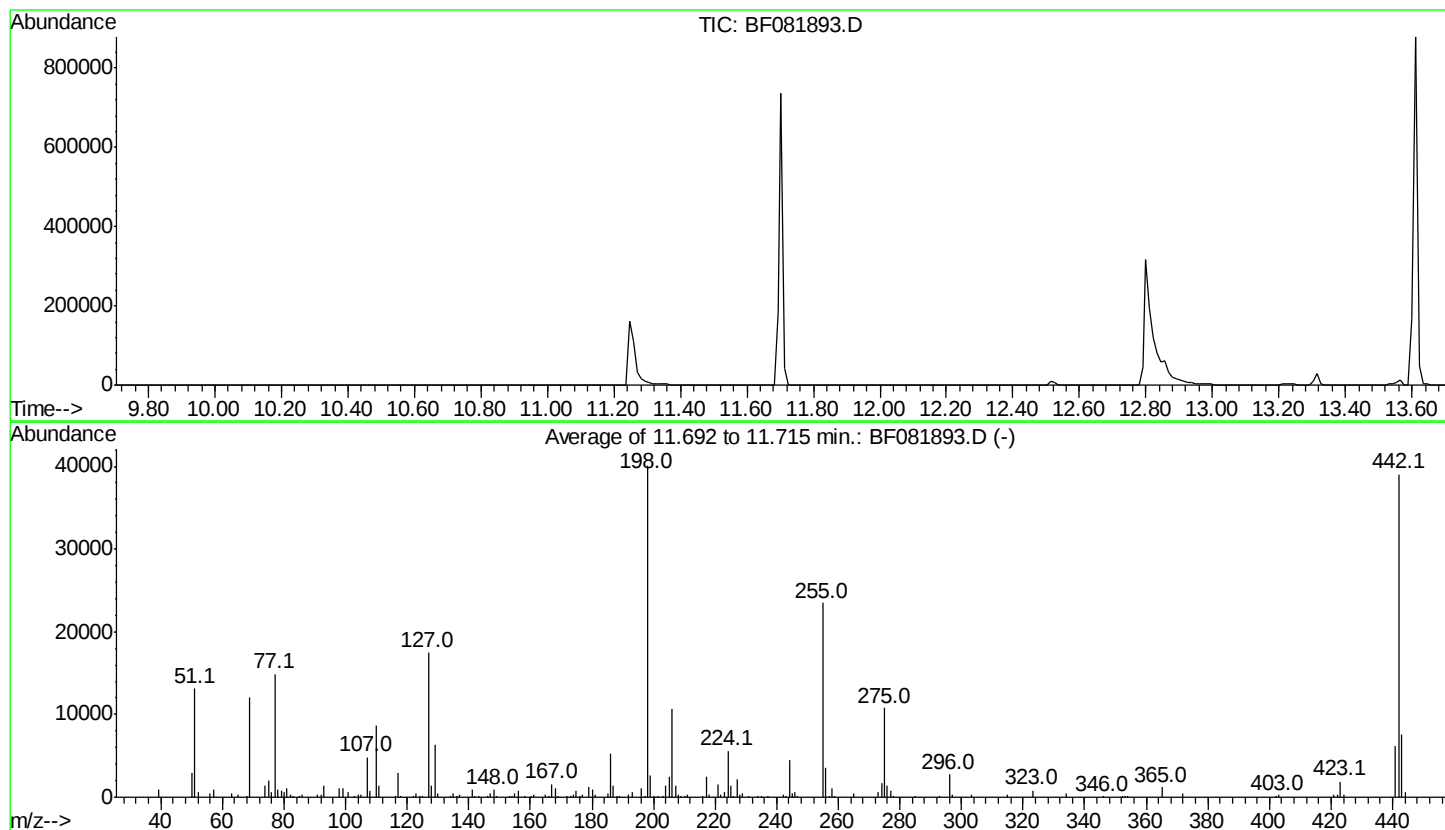

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	13127	PASS
68	69	0.00	2	0.9	106	PASS
69	198	0.00	100	30.2	12086	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.4	17414	PASS
197	198	0.00	2	0.5	202	PASS
198	198	100	100	100.0	40085	PASS
199	198	5	9	6.5	2622	PASS
275	198	10	60	27.0	10821	PASS
365	198	1	100	3.0	1206	PASS
441	442	0.01	24	15.9	6196	PASS
442	198	50	100	97.3	39000	PASS
443	442	15	24	19.3	7527	PASS