
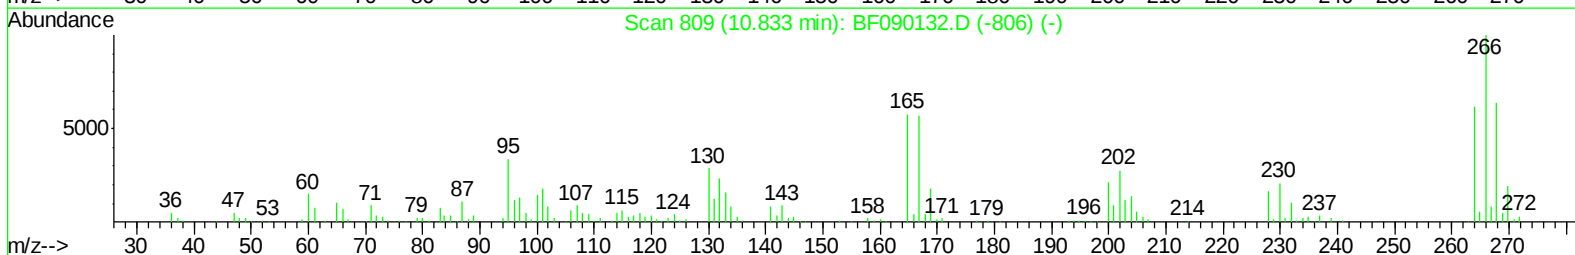
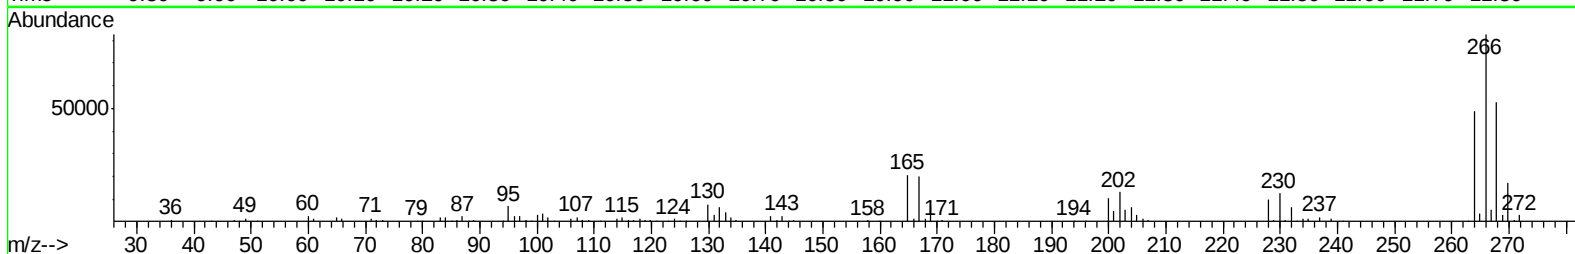


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092916\
Data File : BF090285.D
Acq On : 29 Sep 2016 9:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 07:04:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 15:58:38 2016
Response via : Initial Calibration

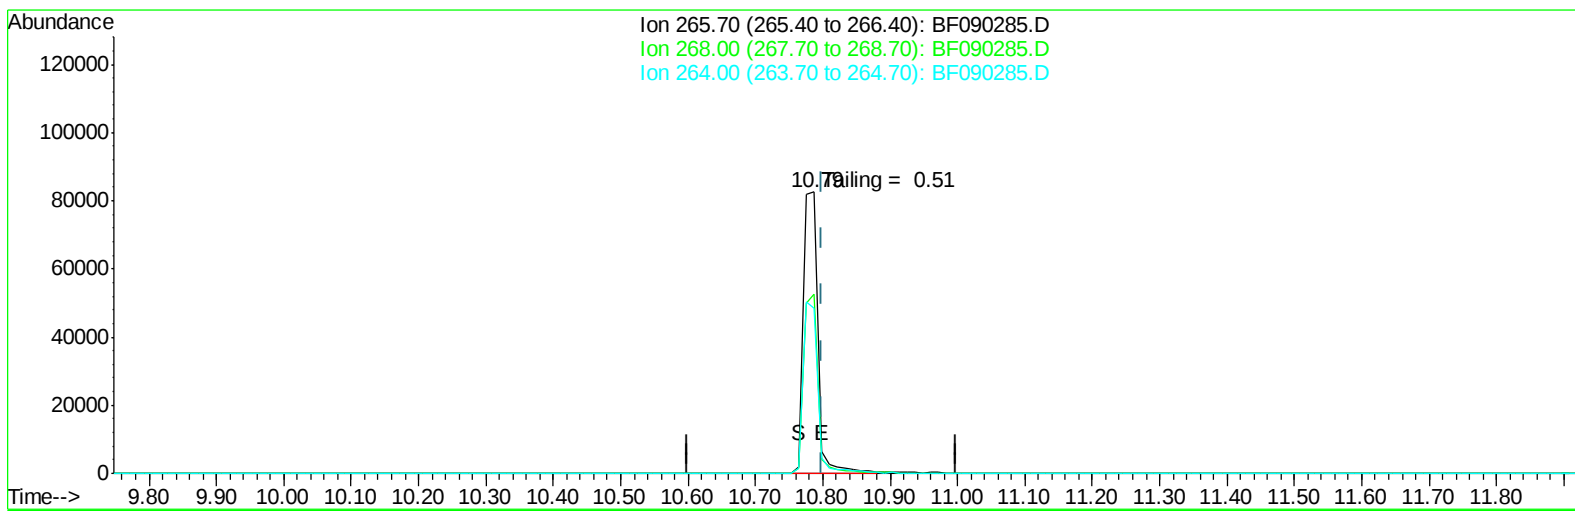

TIC: BF090285.D

(69) Pentachlorophenol (C)




10.788min (-0.011) 68947.96ng

response 126119

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	63.81
264.00	62.90	58.85
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092916\
Data File : BF090285.D
Acq On : 29 Sep 2016 9:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 07:04:56 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 15:58:38 2016
Response via : Initial Calibration

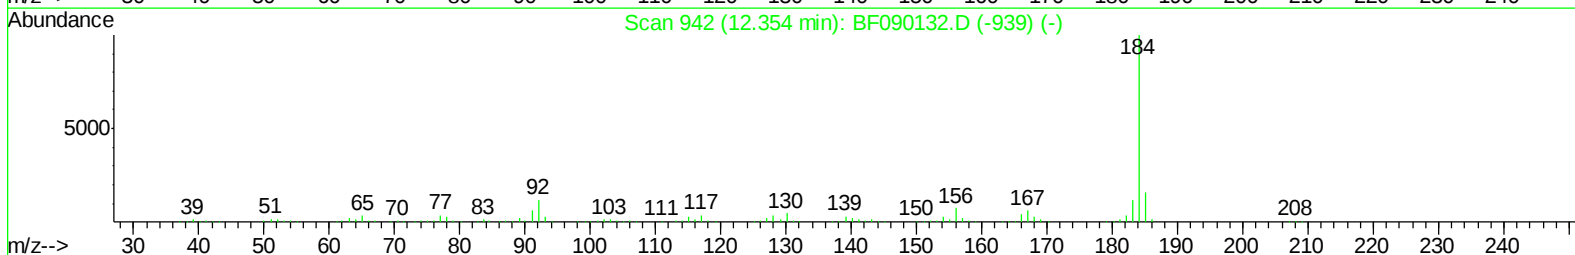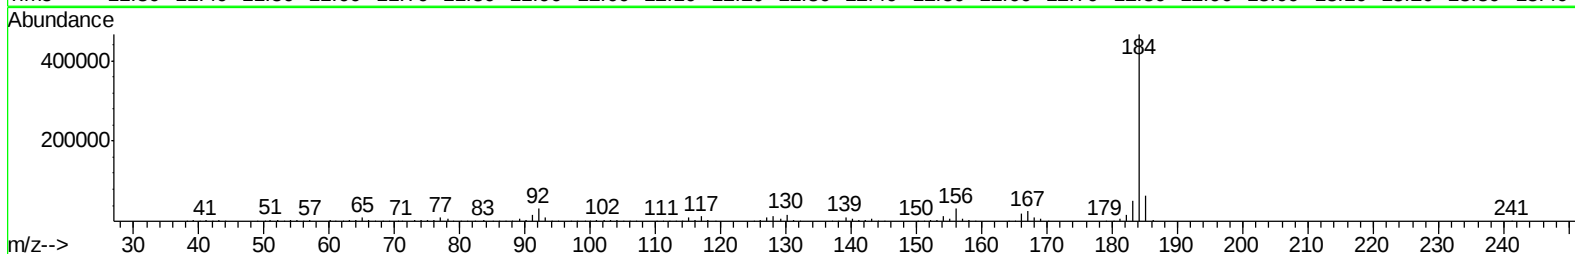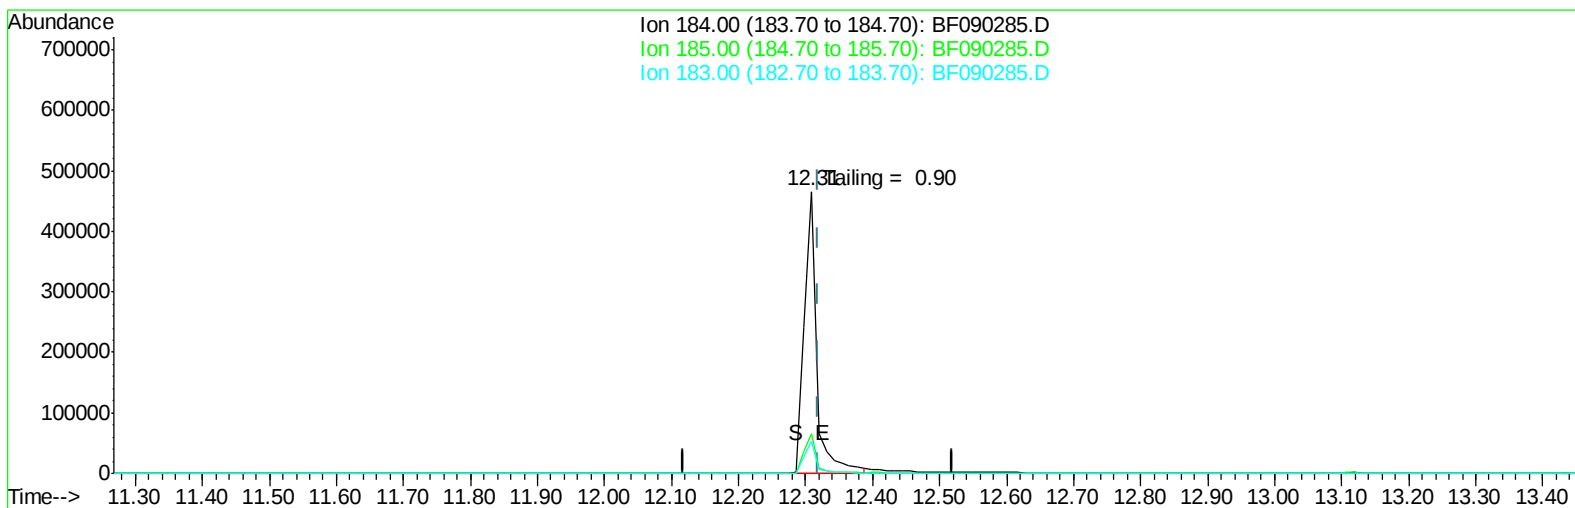

TIC: BF090285.D

(76) Benzidine

12.308min (-0.011) 32777.61ng

response 619864

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	14.06
183.00	11.50	11.32
0.00	0.00	0.00