
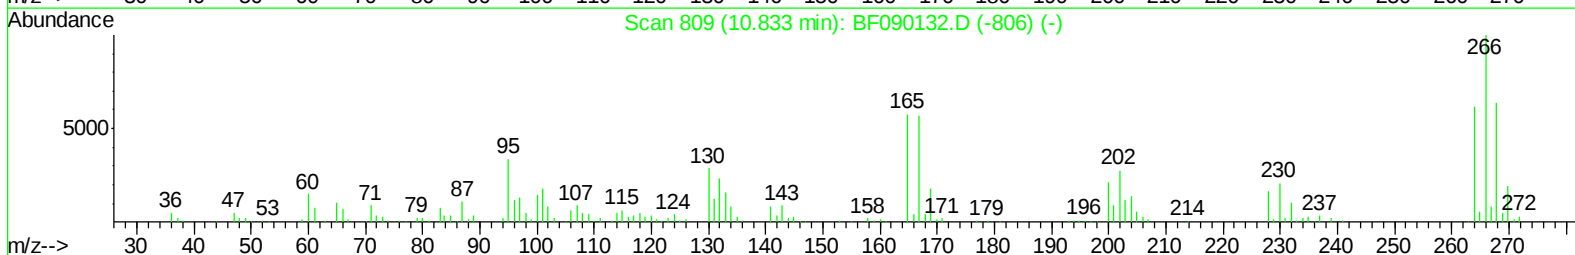
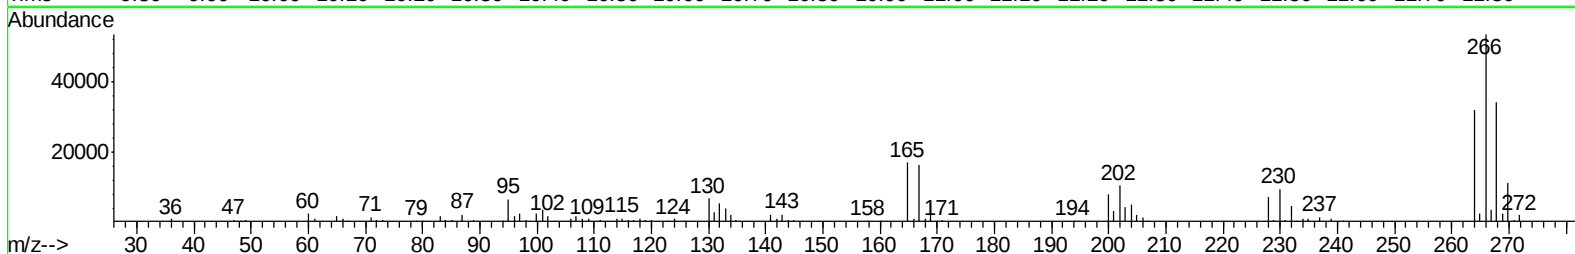


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092916\
Data File : BF090303.D
Acq On : 29 Sep 2016 23:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 07:05:44 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 15:58:38 2016
Response via : Initial Calibration

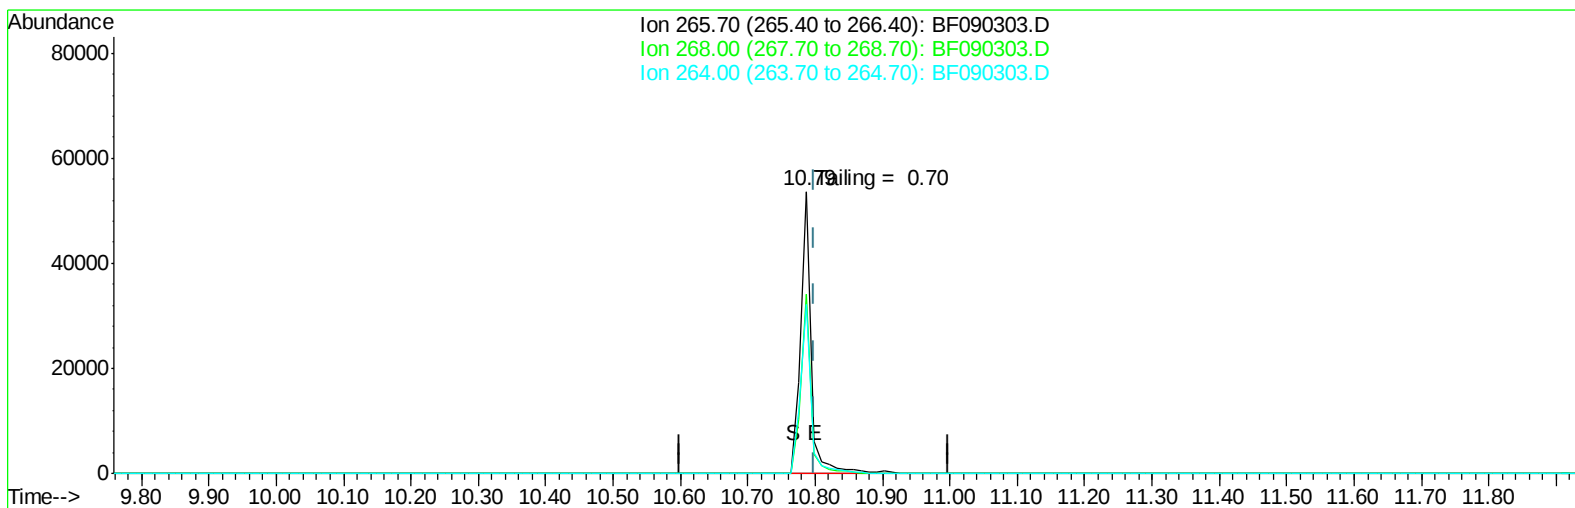

TIC: BF090303.D

(69) Pentachlorophenol (C)




10.788min (-0.012) 0.00ng

response 58398

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	63.68
264.00	62.90	60.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092916\
Data File : BF090303.D
Acq On : 29 Sep 2016 23:20
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 07:05:44 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 26 15:58:38 2016
Response via : Initial Calibration

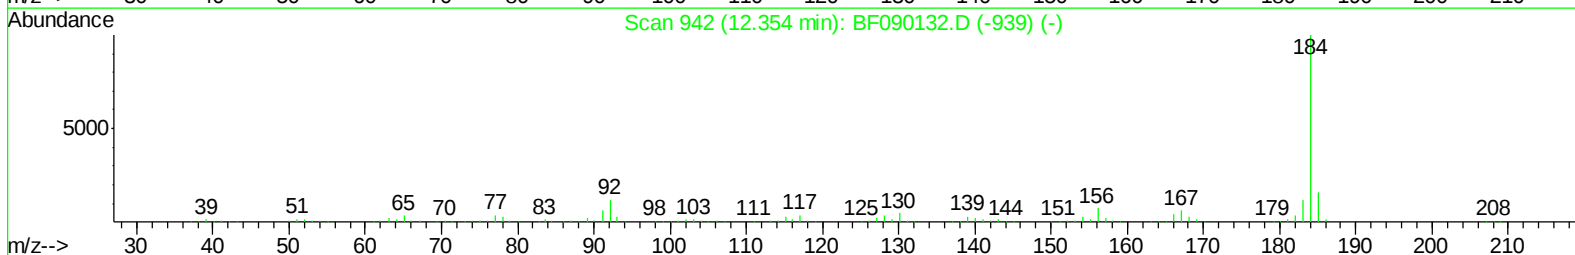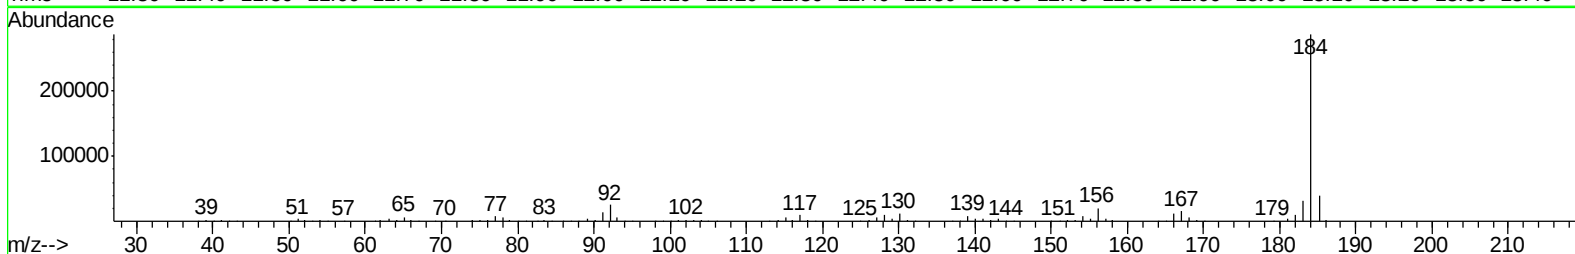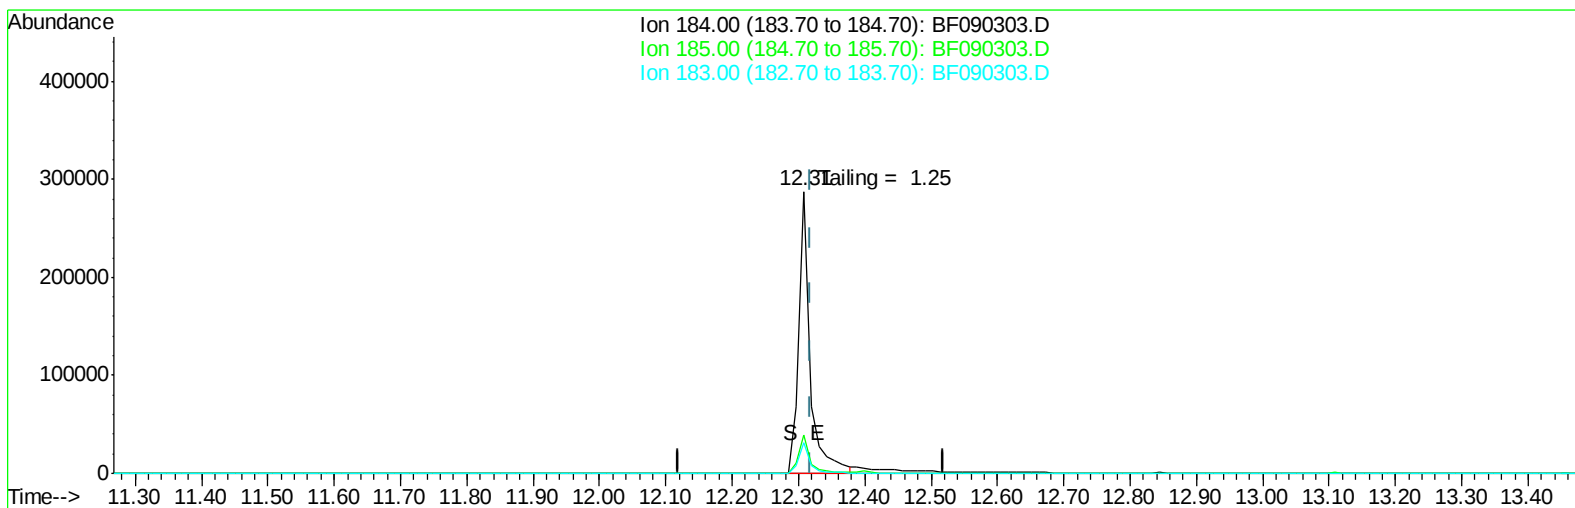

TIC: BF090303.D

(76) Benzidine

12.308min (-0.012) 0.00ng

response 366358

Ion	Exp%	Act%
184.00	100	100
185.00	16.50	13.86
183.00	11.50	10.87
0.00	0.00	0.00