


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092916\
Data File : BF090285.D
Acq On : 29 Sep 2016 9:38
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Sep 26 15:58:38 2016

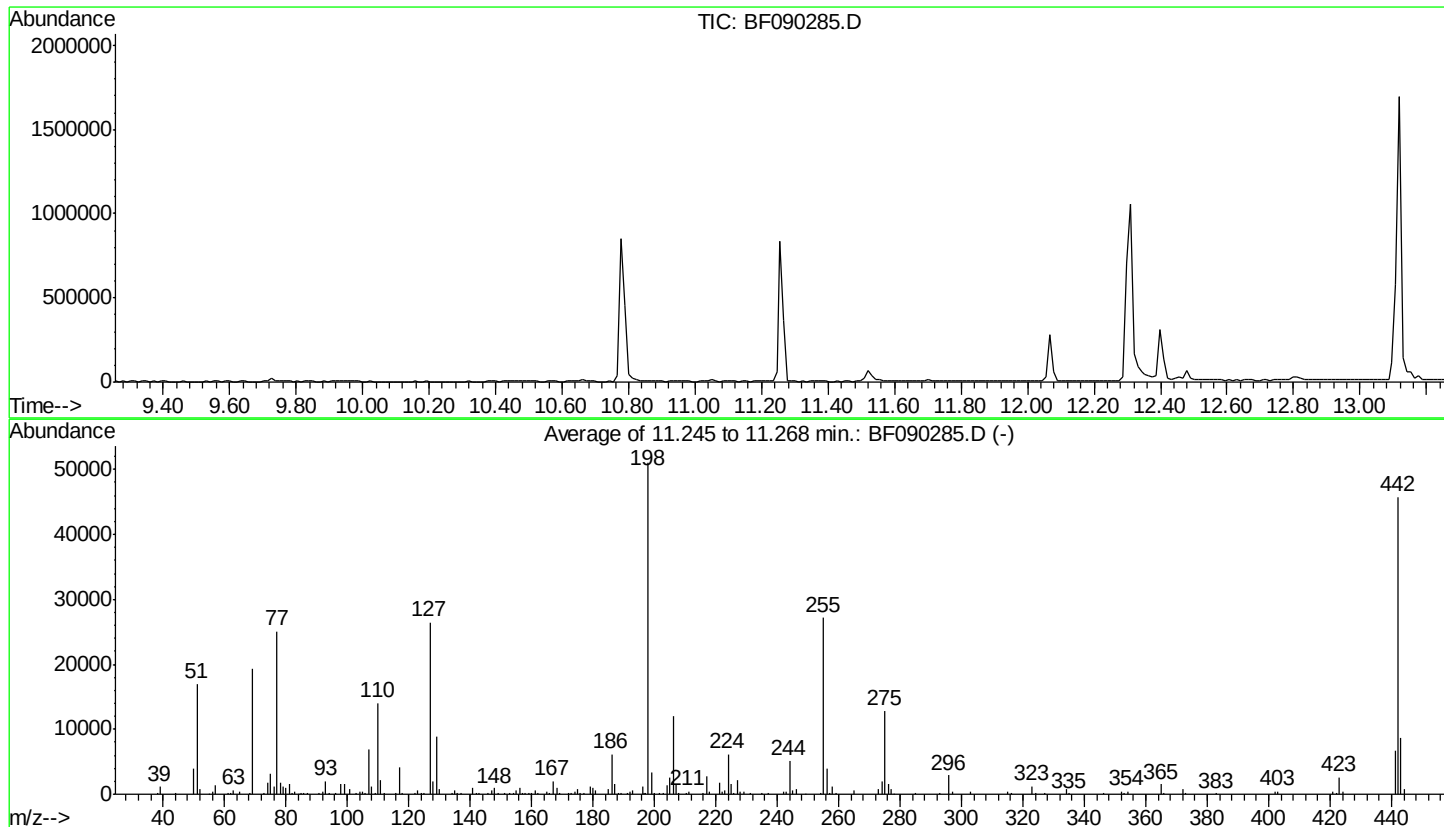

AutoFind: Scans 845, 846, 847; Background Corrected with Scan 841

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	16983	PASS
68	69	0.00	2	1.1	222	PASS
69	198	0.00	100	37.8	19306	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.8	26436	PASS
197	198	0.00	2	0.4	213	PASS
198	198	100	100	100.0	51051	PASS
199	198	5	9	6.7	3411	PASS
275	198	10	60	25.1	12812	PASS
365	198	1	100	2.9	1503	PASS
441	442	0.01	24	14.8	6783	PASS
442	198	50	100	89.7	45798	PASS
443	442	15	24	19.1	8750	PASS