


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF092916\
 Data File : BF090303.D
 Acq On : 29 Sep 2016 23:20
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 26 15:58:38 2016

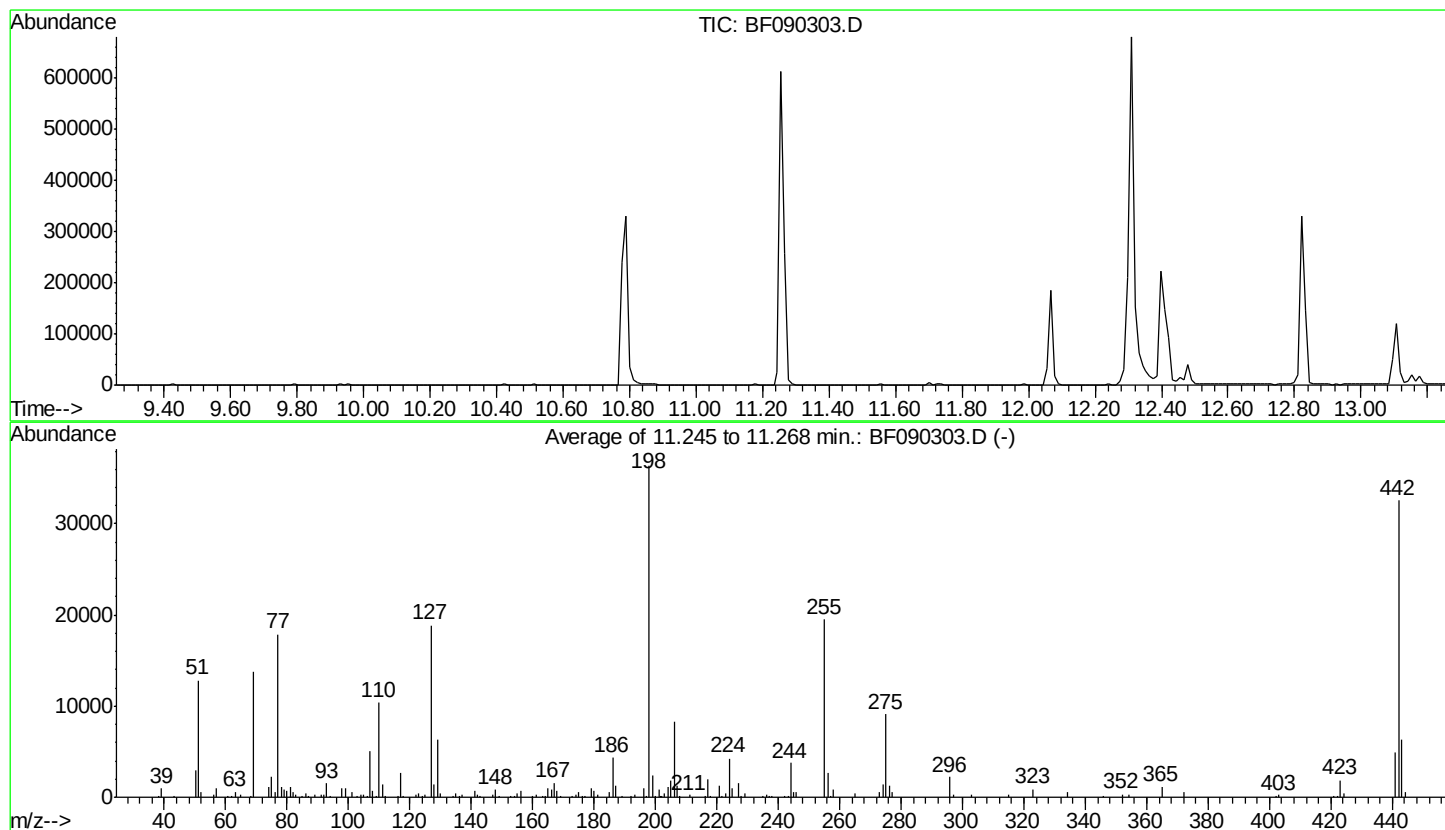

AutoFind: Scans 845, 846, 847; Background Corrected with Scan 842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	12799	PASS
68	69	0.00	2	1.4	192	PASS
69	198	0.00	100	37.8	13747	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	18898	PASS
197	198	0.00	2	0.5	190	PASS
198	198	100	100	100.0	36395	PASS
199	198	5	9	6.7	2429	PASS
275	198	10	60	25.0	9102	PASS
365	198	1	100	3.3	1199	PASS
441	442	0.01	24	15.1	4926	PASS
442	198	50	100	89.4	32536	PASS
443	442	15	24	19.3	6289	PASS