
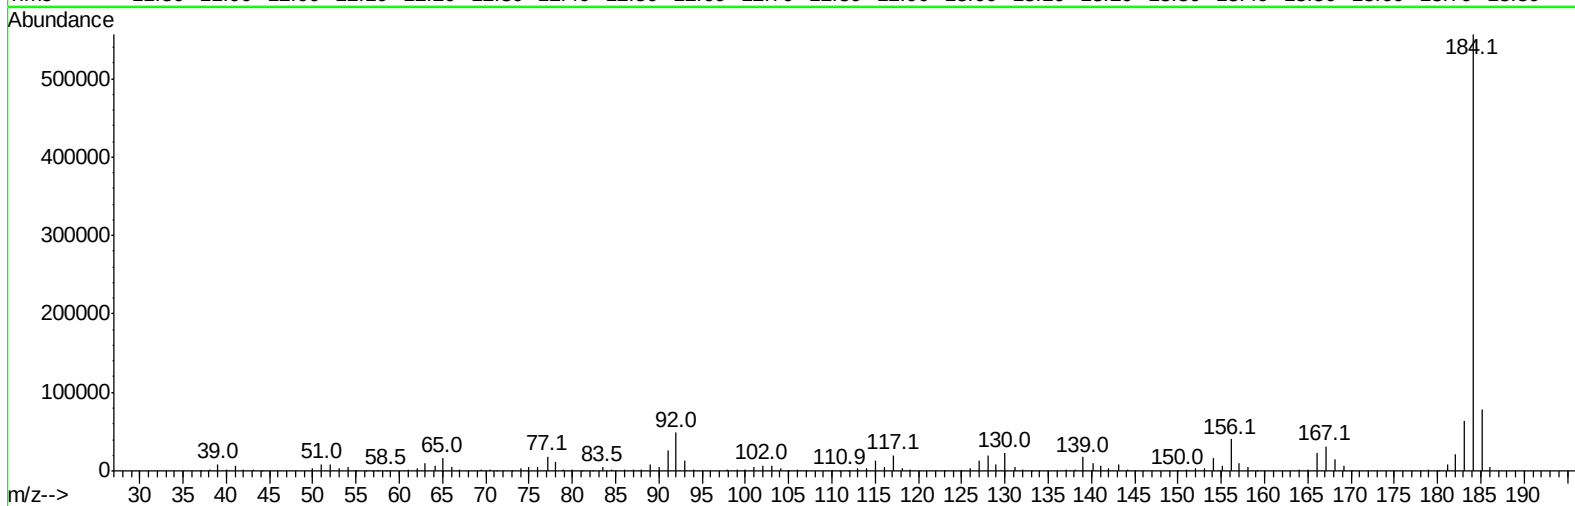


Data Path : Z:\HPCHEM1\BNA F\Data\BF092917\
Data File : BF098936.D
Acq On : 29 Sep 2017 8:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 22:57:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

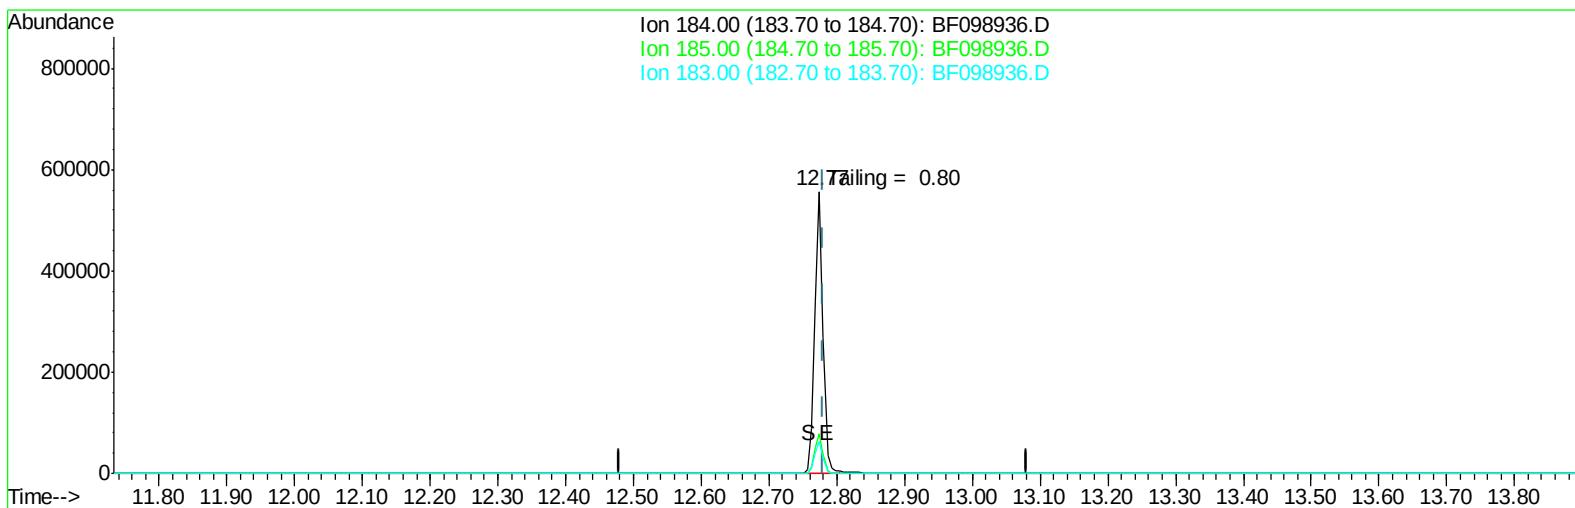

TIC: BF098936.D

(76) Benzidine



12.774min (-0.006) 0.00ng

response 470264

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.11
183.00	11.60	11.50
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF092917\
Data File : BF098936.D
Acq On : 29 Sep 2017 8:49
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 22:57:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

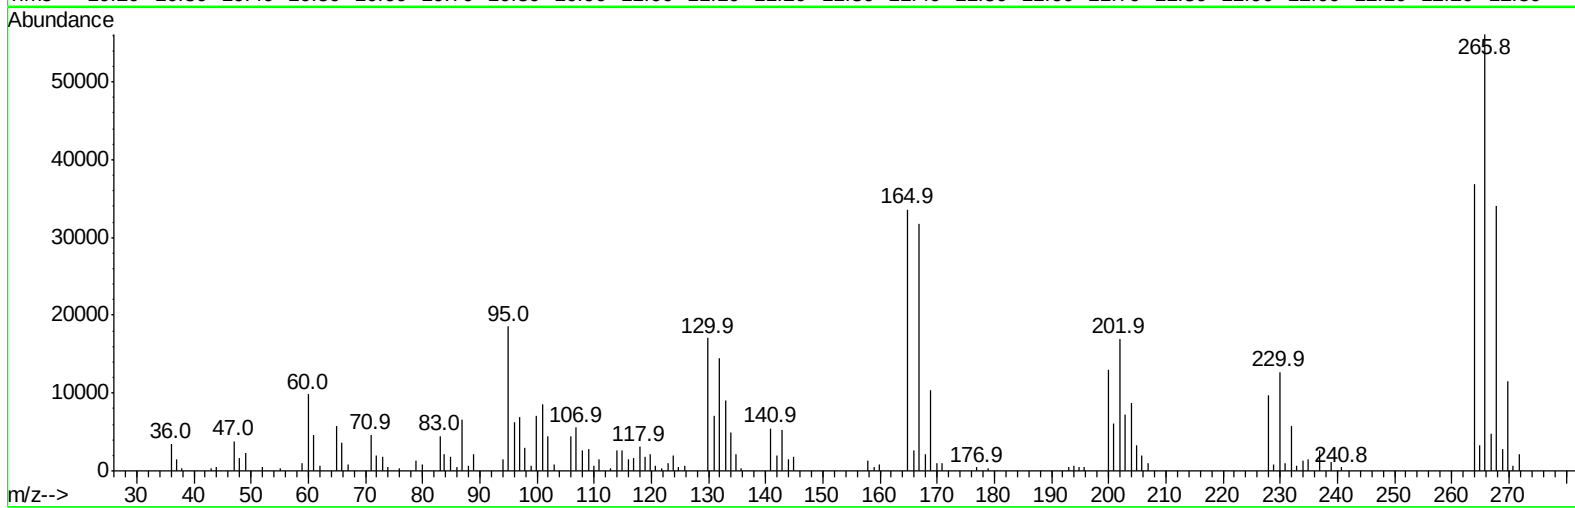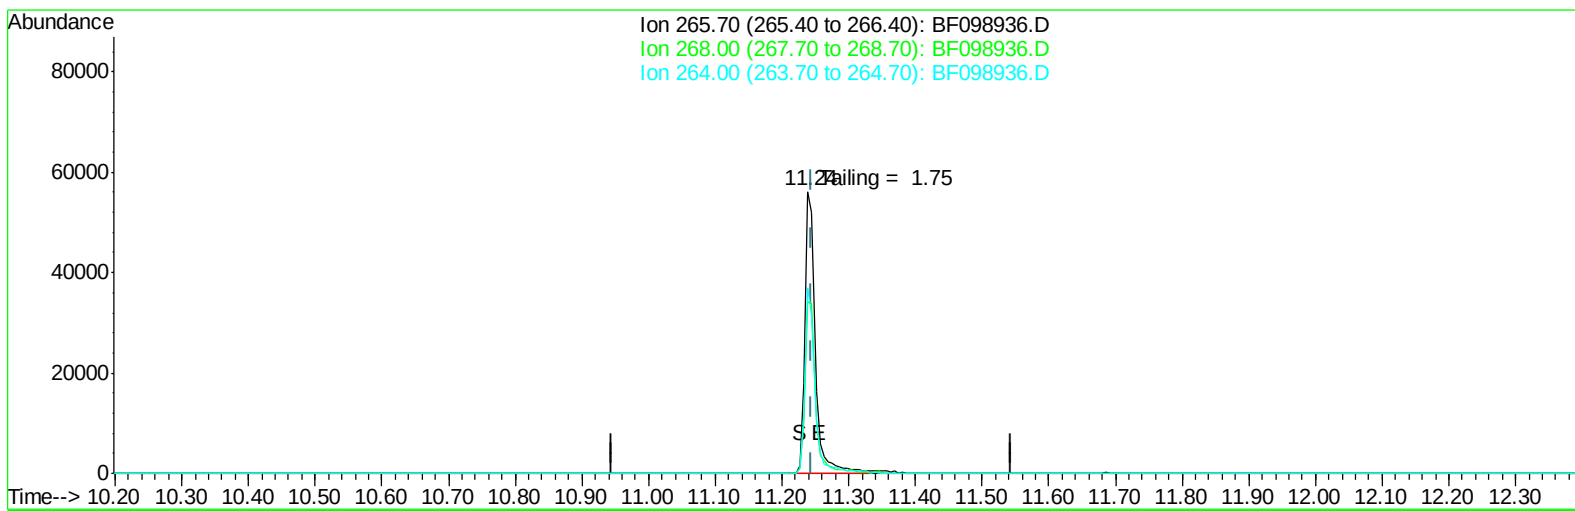

TIC: BF098936.D

(69) Pentachlorophenol (C)

11.239min (-0.006) 32499.74ng

response 59842

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.74
264.00	61.90	65.84
0.00	0.00	0.00