
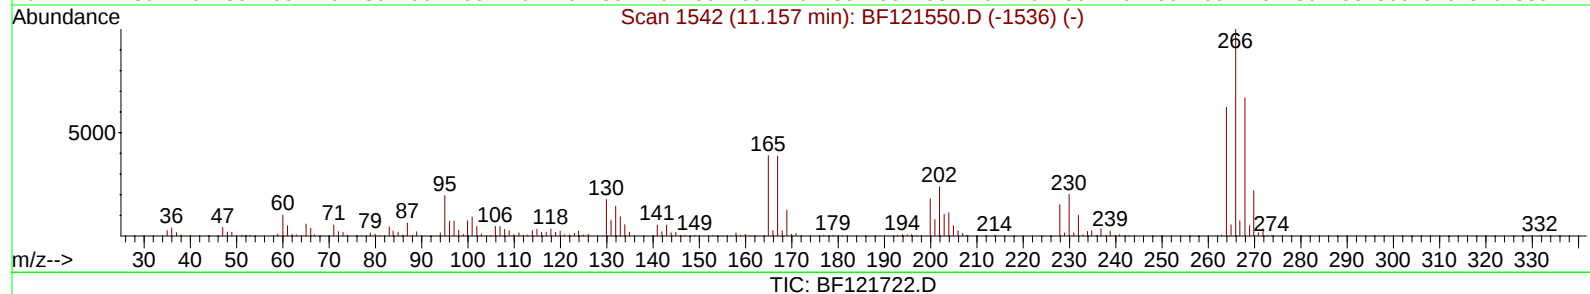
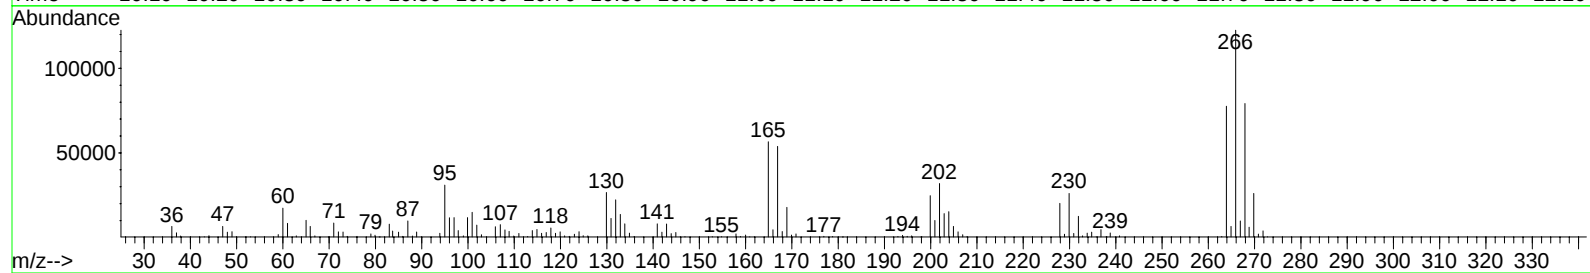


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092920\  
Data File : BF121722.D  
Acq On : 29 Sep 2020 10:12  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 18:38:39 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 29 11:12:14 2020  
Response via : Initial Calibration

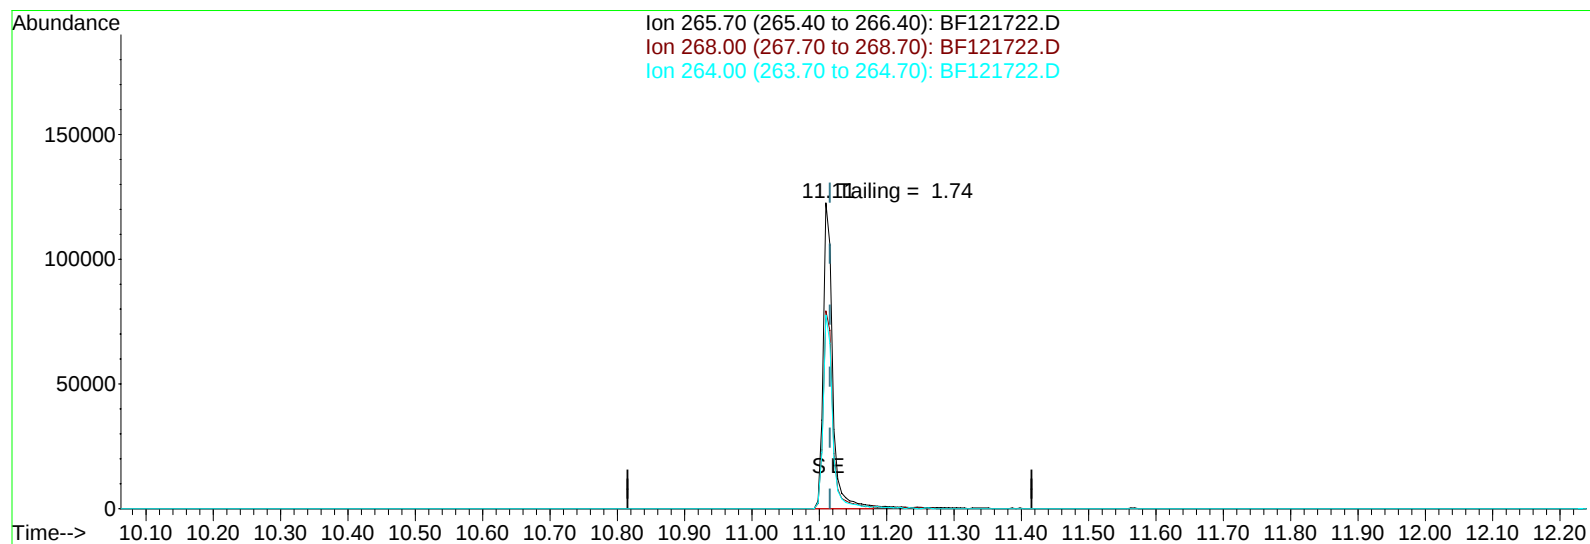

(70) Pentachlorophenol (C)

11.110min (-0.006) 61944.44ng

response 121078

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.50 | 64.67 |
| 264.00 | 62.60 | 63.30 |
| 0.00   | 0.00  | 0.00  |