


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092920\
 Data File : BF121722.D
 Acq On : 29 Sep 2020 10:12
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 29 11:12:14 2020

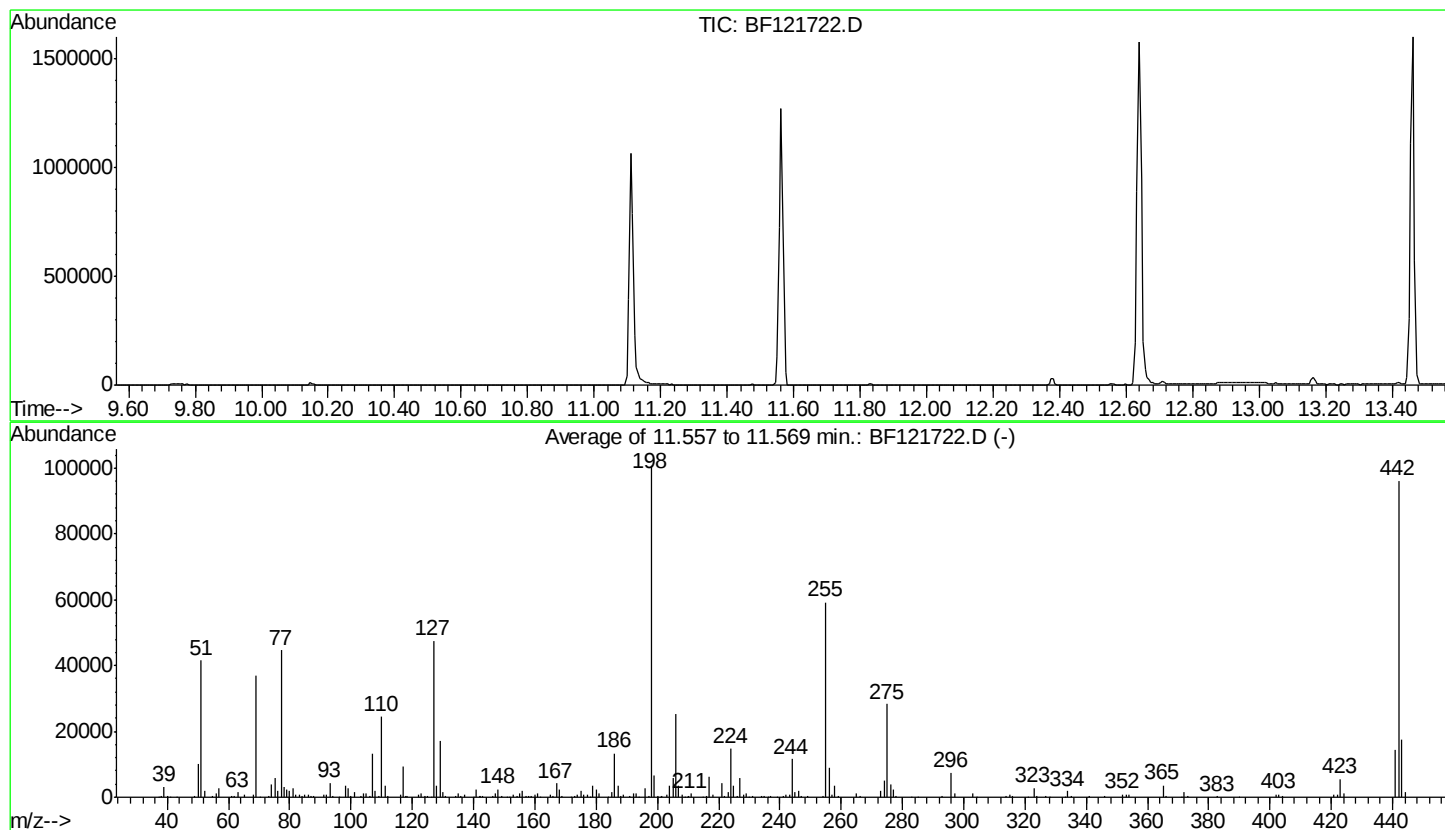

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	41469	PASS
68	69	0.00	2	1.7	619	PASS
69	198	0.00	100	36.8	37018	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	47.2	47501	PASS
197	198	0.00	2	0.6	594	PASS
198	198	100	100	100.0	100728	PASS
199	198	5	9	6.7	6746	PASS
275	198	10	60	28.1	28341	PASS
365	198	1	100	3.6	3652	PASS
441	198	0.01	100	14.5	14589	PASS
442	198	50	100	95.4	96045	PASS
443	442	15	24	18.1	17349	PASS