


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092921\
 Data File : BF125701.D
 Acq On : 29 Sep 2021 9:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 10:44:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

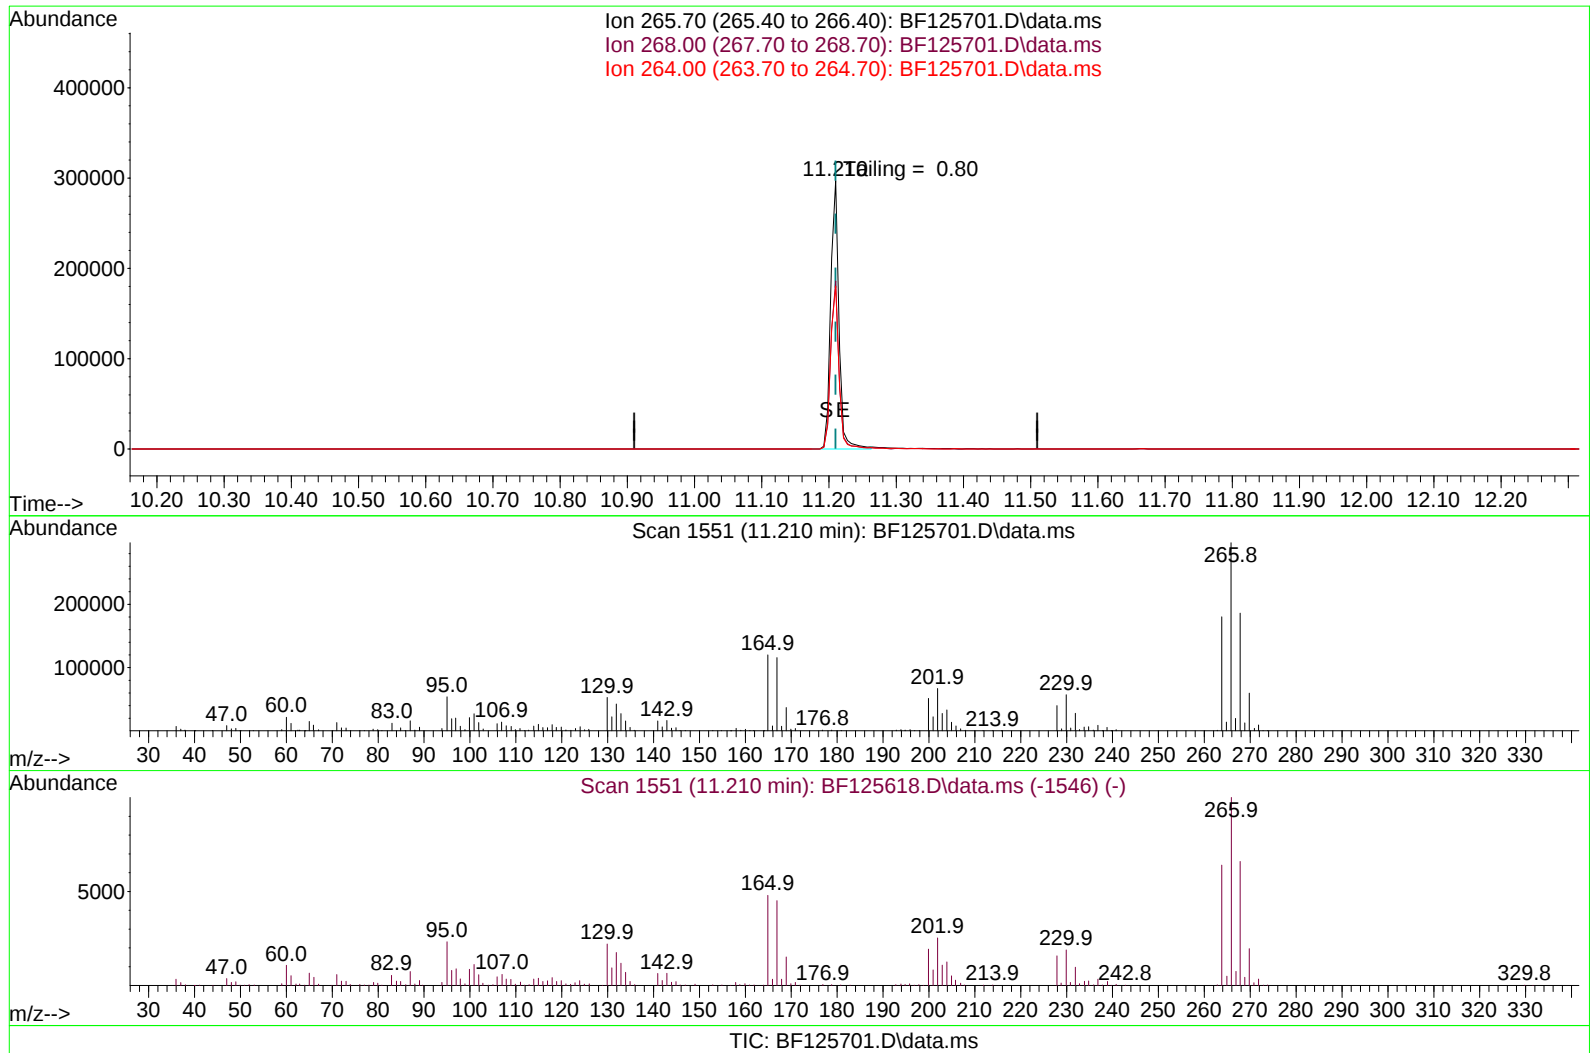




(70) Pentachlorophenol (C)

11.210min (-0.000) 38348.83 ng

response 256385

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.60
264.00	69.90	60.68
0.00	0.00	0.00

Quant Time: Sep 29 10:44:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration

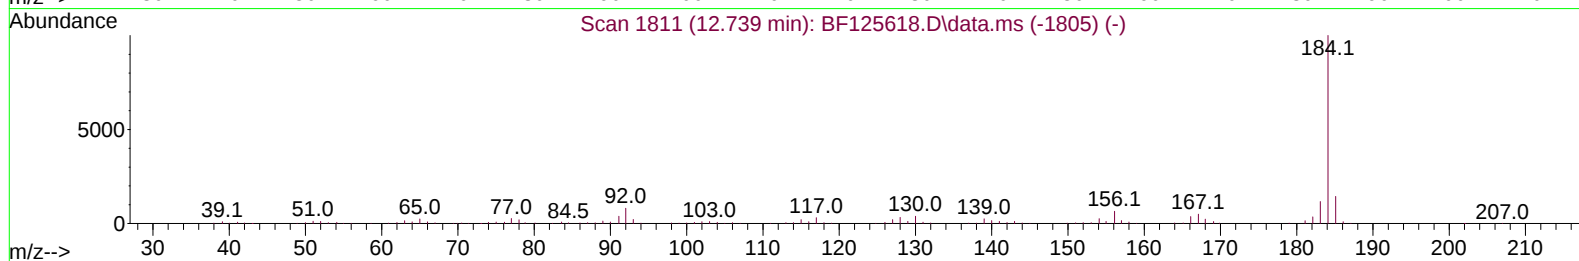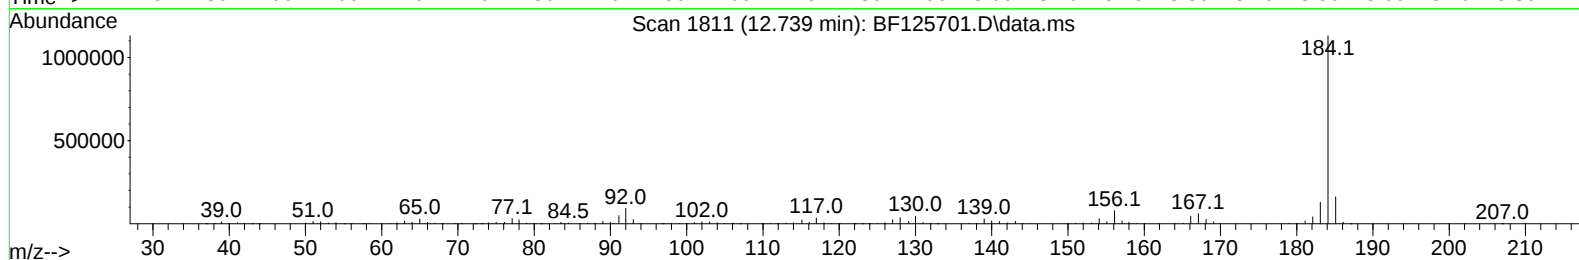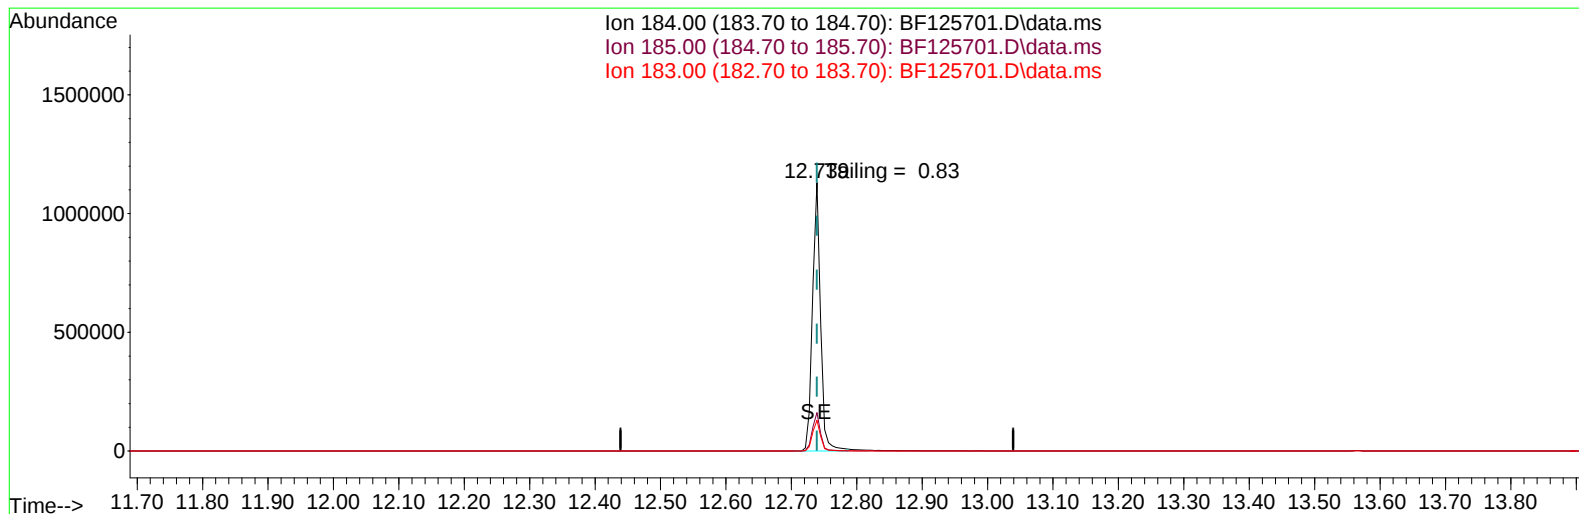

TIC: BF125701.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 318241.67 ng

response **986515**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	13.50	14.31
--------	-------	-------

183.00	10.10	11.47
--------	-------	-------

0.00 0.00 0.00