

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092921\
 Data File : BF125716.D
 Acq On : 29 Sep 2021 19:22
 Operator : JU/CG
 Sample : M3964-20
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CC-20

Quant Time: Sep 30 03:28:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	250046	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	991706	20.000	ng	# 0.00
39) Acenaphthene-d10	9.922	164	480354	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	714965	20.000	ng	0.00
76) Chrysene-d12	14.039	240	548148	20.000	ng	0.00
86) Perylene-d12	15.515	264	510461	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	1185234	78.096	ng	0.00
7) Phenol-d6	6.510	99	1415329	69.366	ng	0.00
23) Nitrobenzene-d5	7.445	82	816252	57.410	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	313793	70.064	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	1534931	52.264	ng	0.00
79) Terphenyl-d14	12.992	244	1401780	44.286	ng	0.00
Target Compounds						
26) 2-Nitrophenol	7.781	139	603	5.804	ng	# 85
74) Di-n-butylphthalate	11.963	149	398896	10.148	ng	99
80) Butylbenzylphthalate	13.463	149	60183	3.669	ng	95
84) Bis(2-ethylhexyl)phtha...	14.021	149	152076	8.098	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092921\
Data File : BF125716.D
Acq On : 29 Sep 2021 19:22
Operator : JU/CG
Sample : M3964-20
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CC-20

Quant Time: Sep 30 03:28:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration




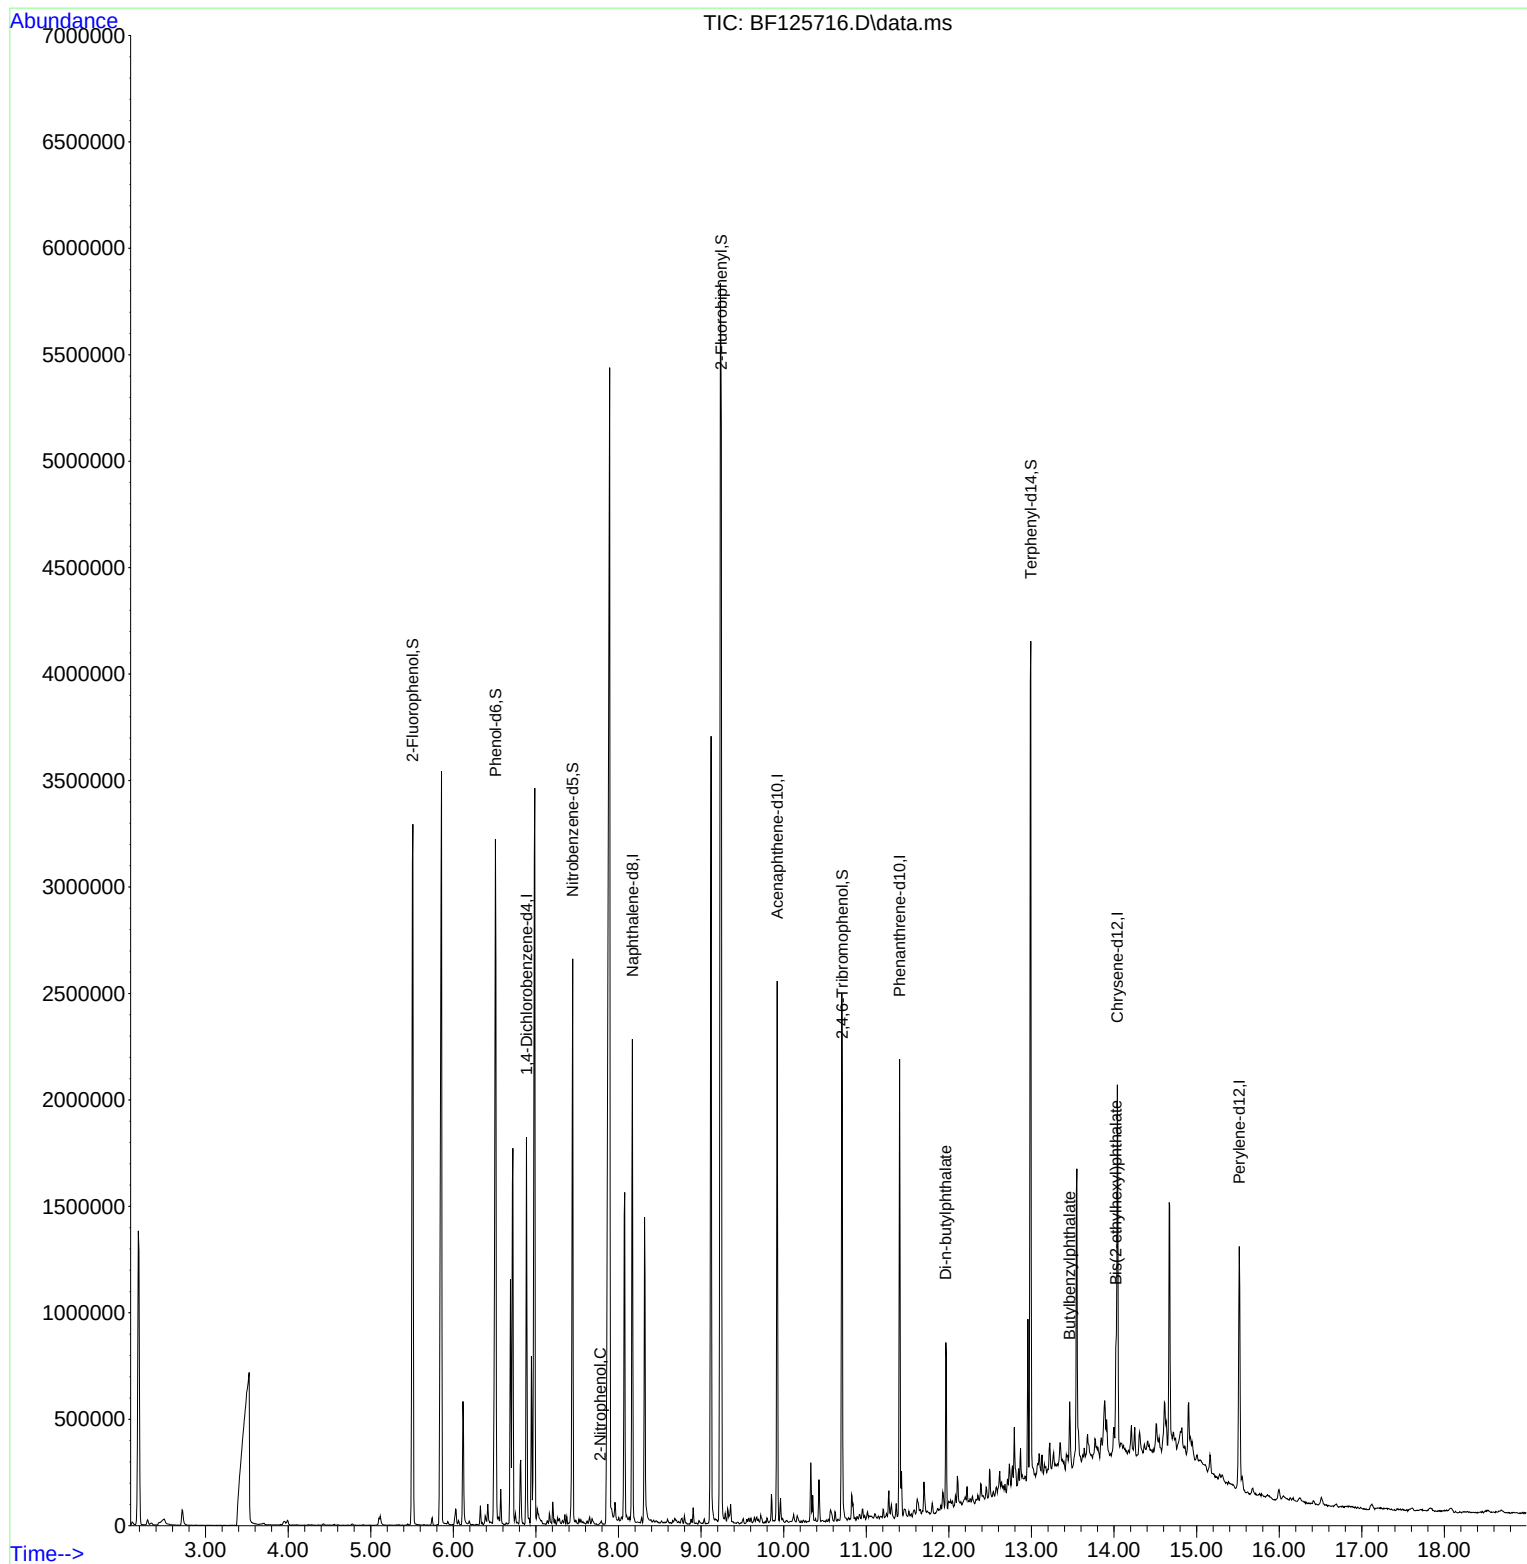




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.887 min Scan# 816
Delta R.T. -0.005 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22




Instrument :
BNA_F
ClientSampleId :
CC-20


Tgt Ion:152 Resp: 250046
Ion Ratio Lower Upper
152 100
150 161.0 117.6 176.4
115 59.4 47.1 70.7

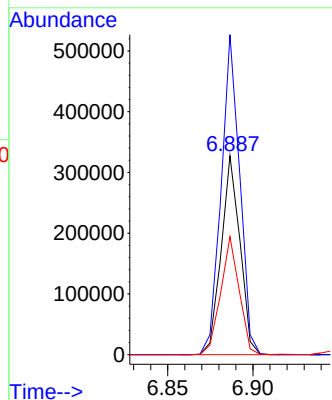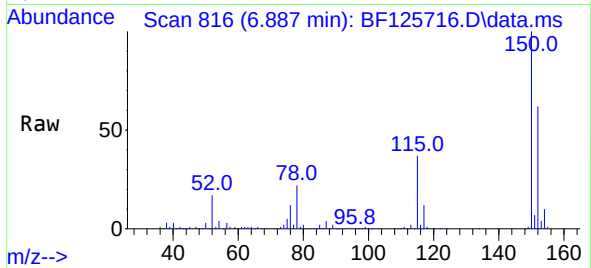

#5
2-Fluorophenol
Concen: 78.096 ng
RT: 5.510 min Scan# 582
Delta R.T. 0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22

Tgt Ion:112 Resp: 1185234
Ion Ratio Lower Upper
112 100
64 50.1 44.2 66.2
63 24.9 26.2 39.2#


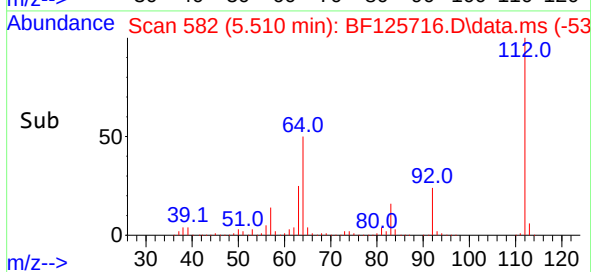
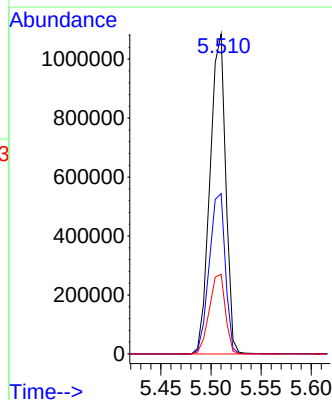





#7
Phenol-d6
Concen: 69.366 ng
RT: 6.510 min Scan# 752
Delta R.T. 0.000 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22




Instrument :
BNA_F
ClientSampleId :
CC-20


Tgt Ion: 99 Resp: 1415329
Ion Ratio Lower Upper
99 100
42 14.2 23.5 35.3#
71 29.2 25.6 38.4

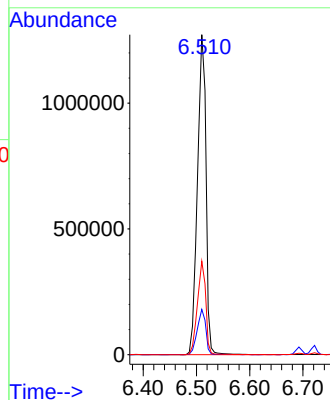

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1034
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22

Tgt Ion: 136 Resp: 991706
Ion Ratio Lower Upper
136 100
137 10.5 9.8 14.6
54 6.1 6.4 9.6#
68 5.6 3.3 4.9#


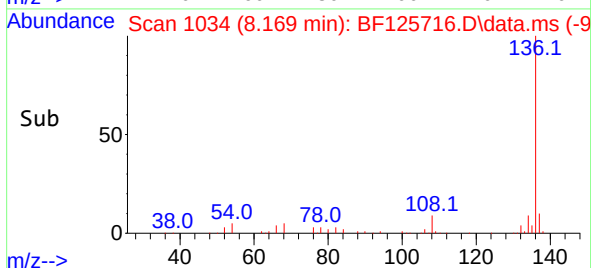
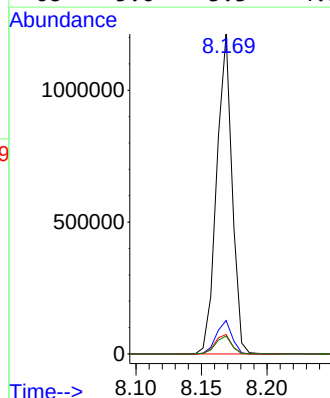





#23
Nitrobenzene-d5
Concen: 57.410 ng
RT: 7.445 min Scan# 911
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22




Instrument :
BNA_F
ClientSampled :
CC-20


Tgt Ion: 82 Resp: 816252
Ion Ratio Lower Upper
82 100
128 50.3 40.6 60.8
54 42.4 49.6 74.4#

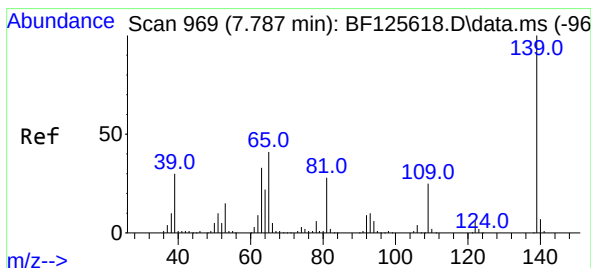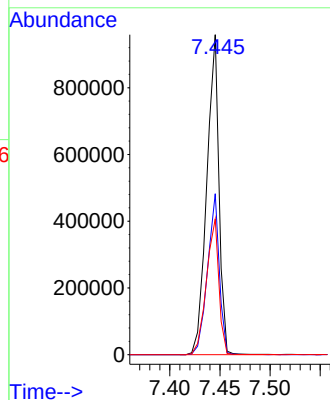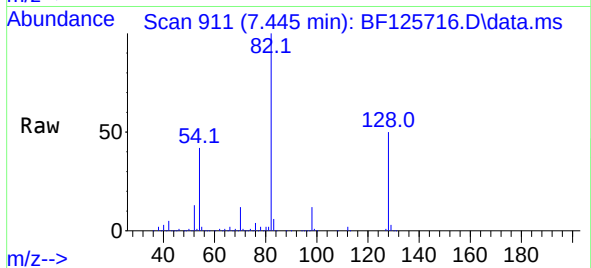

#26
2-Nitrophenol
Concen: 5.804 ng
RT: 7.781 min Scan# 968
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22

Tgt Ion:139 Resp: 603
Ion Ratio Lower Upper
139 100
109 49.8 26.0 39.0#
65 38.1 31.0 46.4


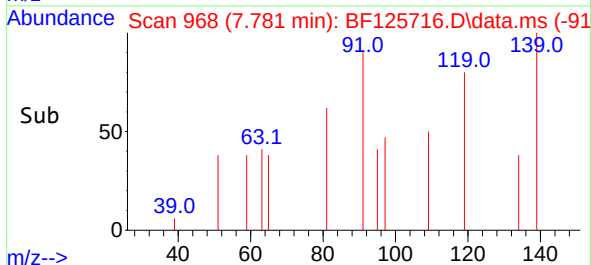
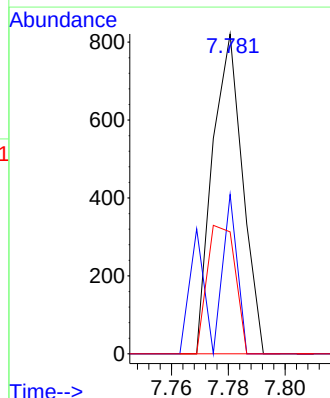
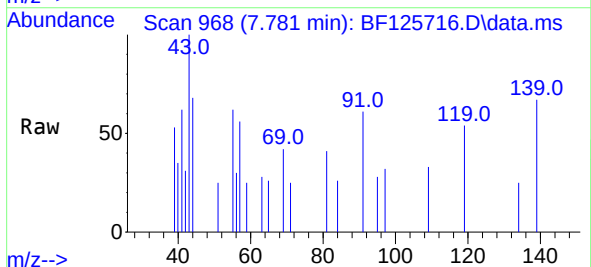




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.922 min Scan# 1332
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22




Instrument :
BNA_F
ClientSampleId :
CC-20


Tgt Ion:164 Resp: 480354
Ion Ratio Lower Upper
164 100
162 100.3 81.3 121.9
160 43.6 38.0 57.0

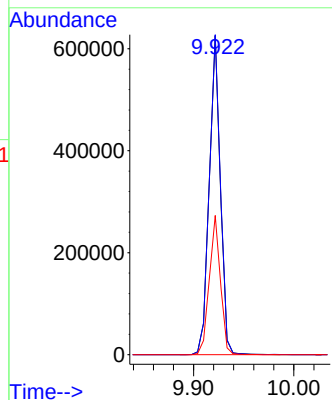

#42
2,4,6-Tribromophenol
Concen: 70.064 ng
RT: 10.710 min Scan# 1466
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22

Tgt Ion:330 Resp: 313793
Ion Ratio Lower Upper
330 100
332 95.8 76.2 114.4
141 31.5 44.6 66.8#


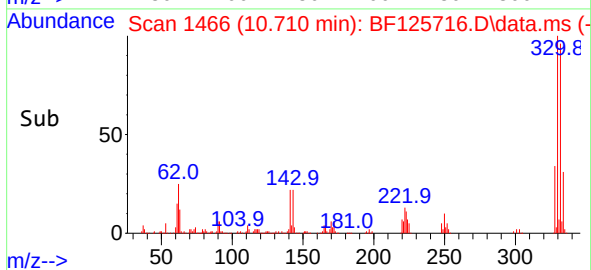
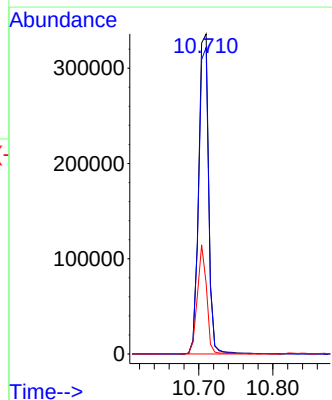





#45
2-Fluorobiphenyl
Concen: 52.264 ng
RT: 9.245 min Scan# 1217
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22




Instrument :
BNA_F
ClientSampled :
CC-20


Tgt Ion:172 Resp: 1534931
Ion Ratio Lower Upper
172 100
171 35.5 26.5 39.7
170 24.0 18.8 28.2

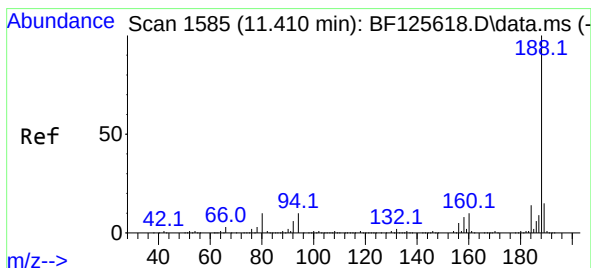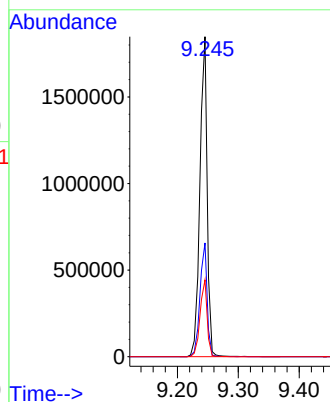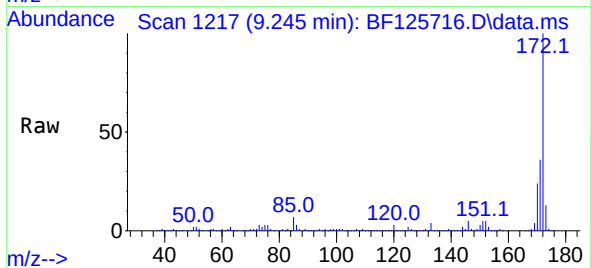

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 1584
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22

Tgt Ion:188 Resp: 714965
Ion Ratio Lower Upper
188 100
94 10.0 6.7 10.1
80 10.7 7.5 11.3


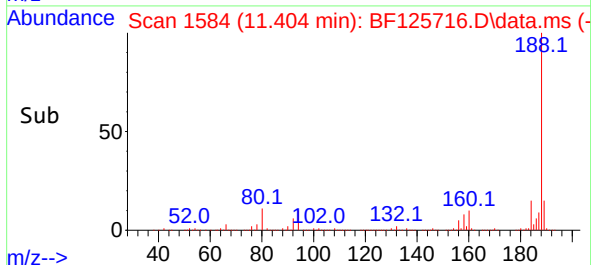
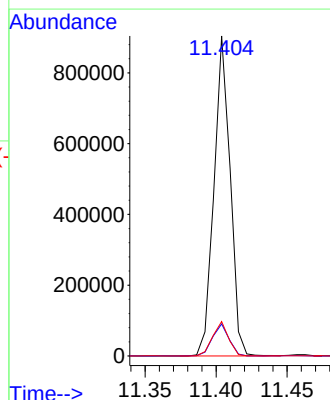
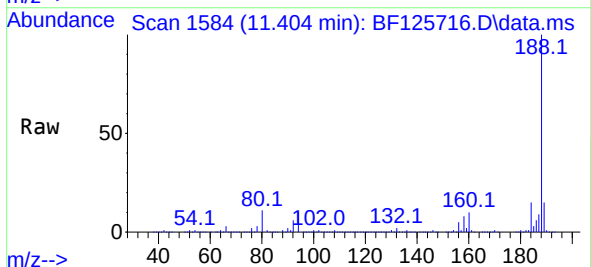




#74
Di-n-butylphthalate
Concen: 10.148 ng
RT: 11.963 min Scan# 1679
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22




Instrument :
BNA_F
ClientSampleId :
CC-20


Tgt Ion:149 Resp: 398896
Ion Ratio Lower Upper
149 100
150 9.4 7.4 11.2
104 4.4 4.1 6.1

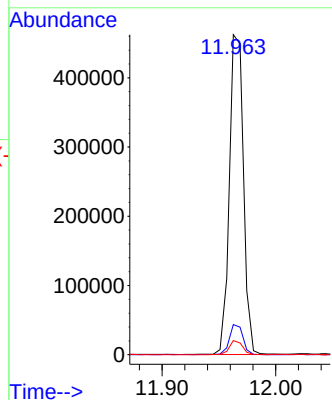

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.039 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22

Tgt Ion:240 Resp: 548148
Ion Ratio Lower Upper
240 100
120 14.2 10.8 16.2
236 25.1 21.6 32.4


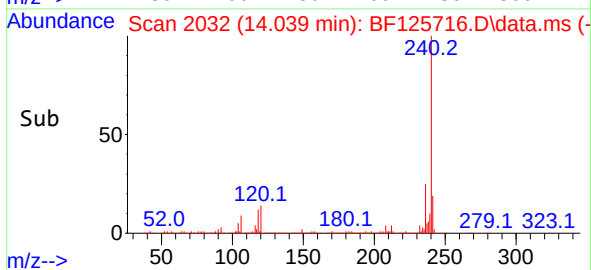
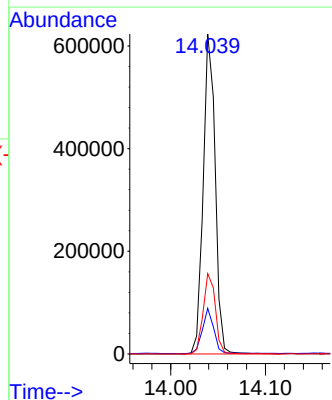





#79
Terphenyl-d14
Concen: 44.286 ng
RT: 12.992 min Scan# 1854
Delta R.T. 0.000 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22




Instrument :
BNA_F
ClientSampled :
CC-20


Tgt Ion:244 Resp: 1401780
Ion Ratio Lower Upper
244 100
212 6.2 5.9 8.9
122 10.8 9.0 13.4

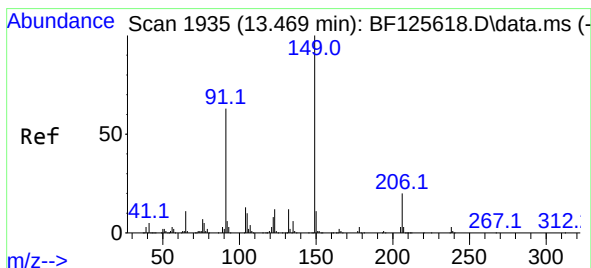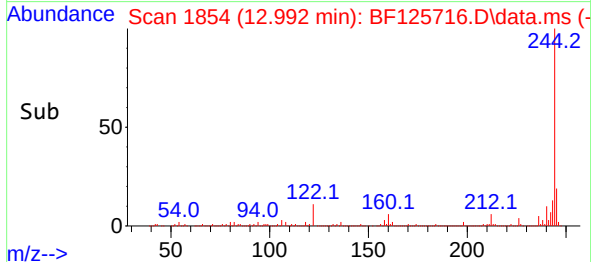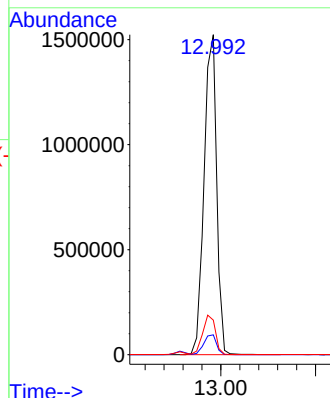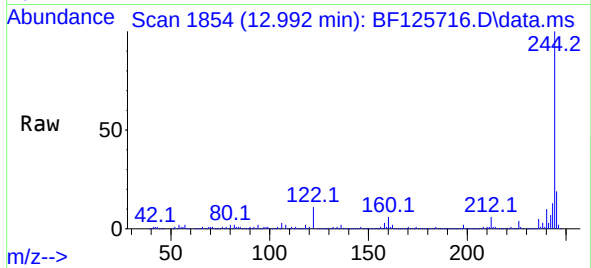

#80
Butylbenzylphthalate
Concen: 3.669 ng
RT: 13.463 min Scan# 1934
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22

Tgt Ion:149 Resp: 60183
Ion Ratio Lower Upper
149 100
91 69.3 51.8 77.8
206 19.4 14.5 21.7

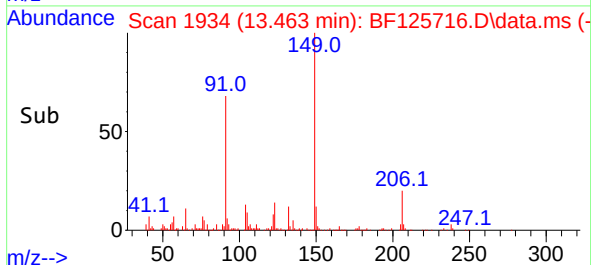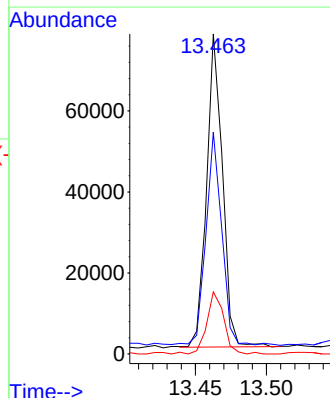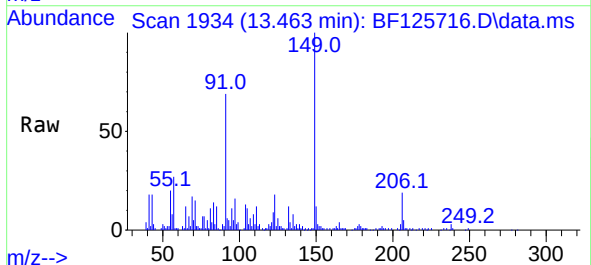







#84
Bis(2-ethylhexyl)phthalate
Concen: 8.098 ng
RT: 14.021 min Scan# 2029
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22

Instrument :
BNA_F
ClientSampled :
CC-20

Tgt Ion:149 Resp: 152076

Ion	Ratio	Lower	Upper
149	100		
167	27.1	21.4	32.0
279	3.3	2.6	4.0

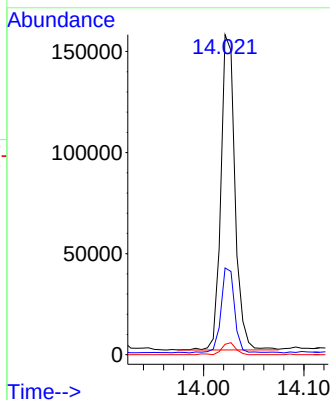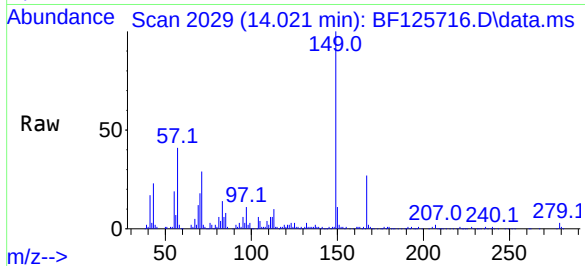

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.515 min Scan# 2283
Delta R.T. -0.006 min
Lab File: BF125716.D
Acq: 29 Sep 2021 19:22

Tgt Ion:264 Resp: 510461

Ion	Ratio	Lower	Upper
264	100		
260	23.5	19.6	29.4
265	21.1	17.2	25.8

