
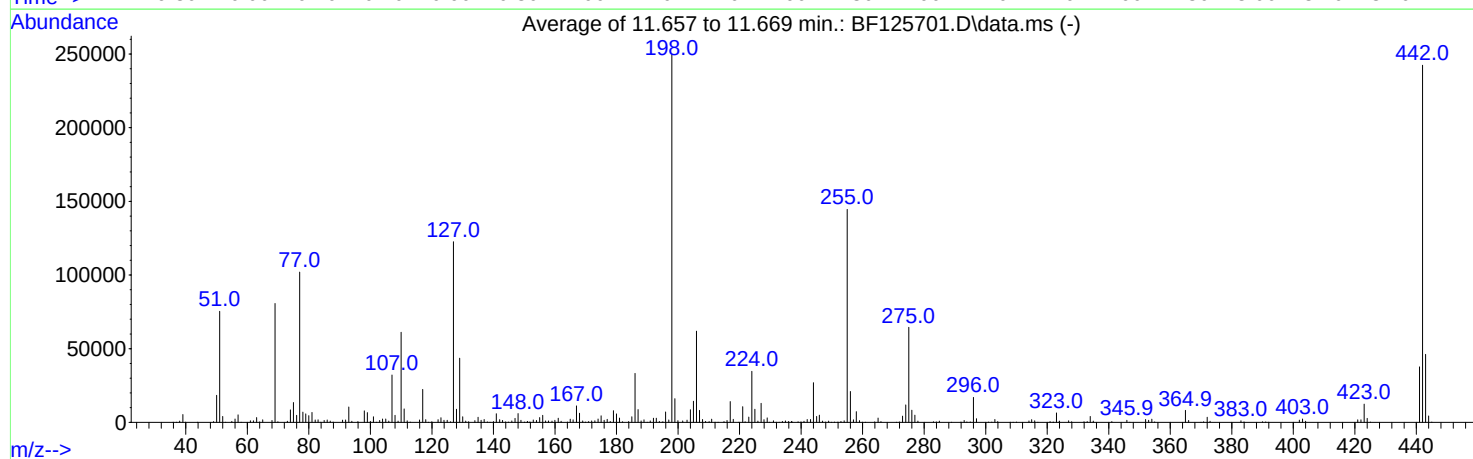


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092921\
 Data File : BF125701.D
 Acq On : 29 Sep 2021 9:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 15:38:32 2021

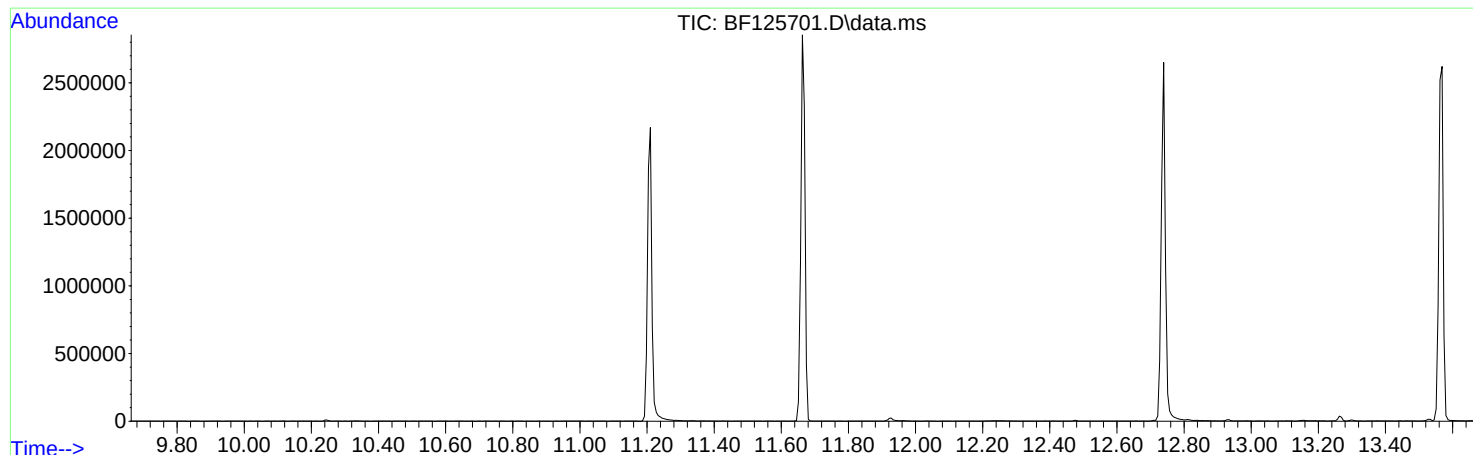


AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.2	75381	PASS
68	69	0.00	2	1.7	1361	PASS
69	198	0.00	100	32.3	80723	PASS
70	69	0.00	2	0.5	426	PASS
127	198	10	80	49.1	122595	PASS
197	198	0.00	2	0.7	1636	PASS
198	198	100	100	100.0	249664	PASS
199	198	5	9	6.5	16126	PASS
275	198	10	60	25.8	64493	PASS
365	198	1	100	3.3	8124	PASS
441	198	0.01	100	15.1	37687	PASS
442	442	50	100	100.0	242440	PASS
443	442	15	24	19.0	46129	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092921\
 Data File : BF125701.D
 Acq On : 29 Sep 2021 9:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 29 10:44:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

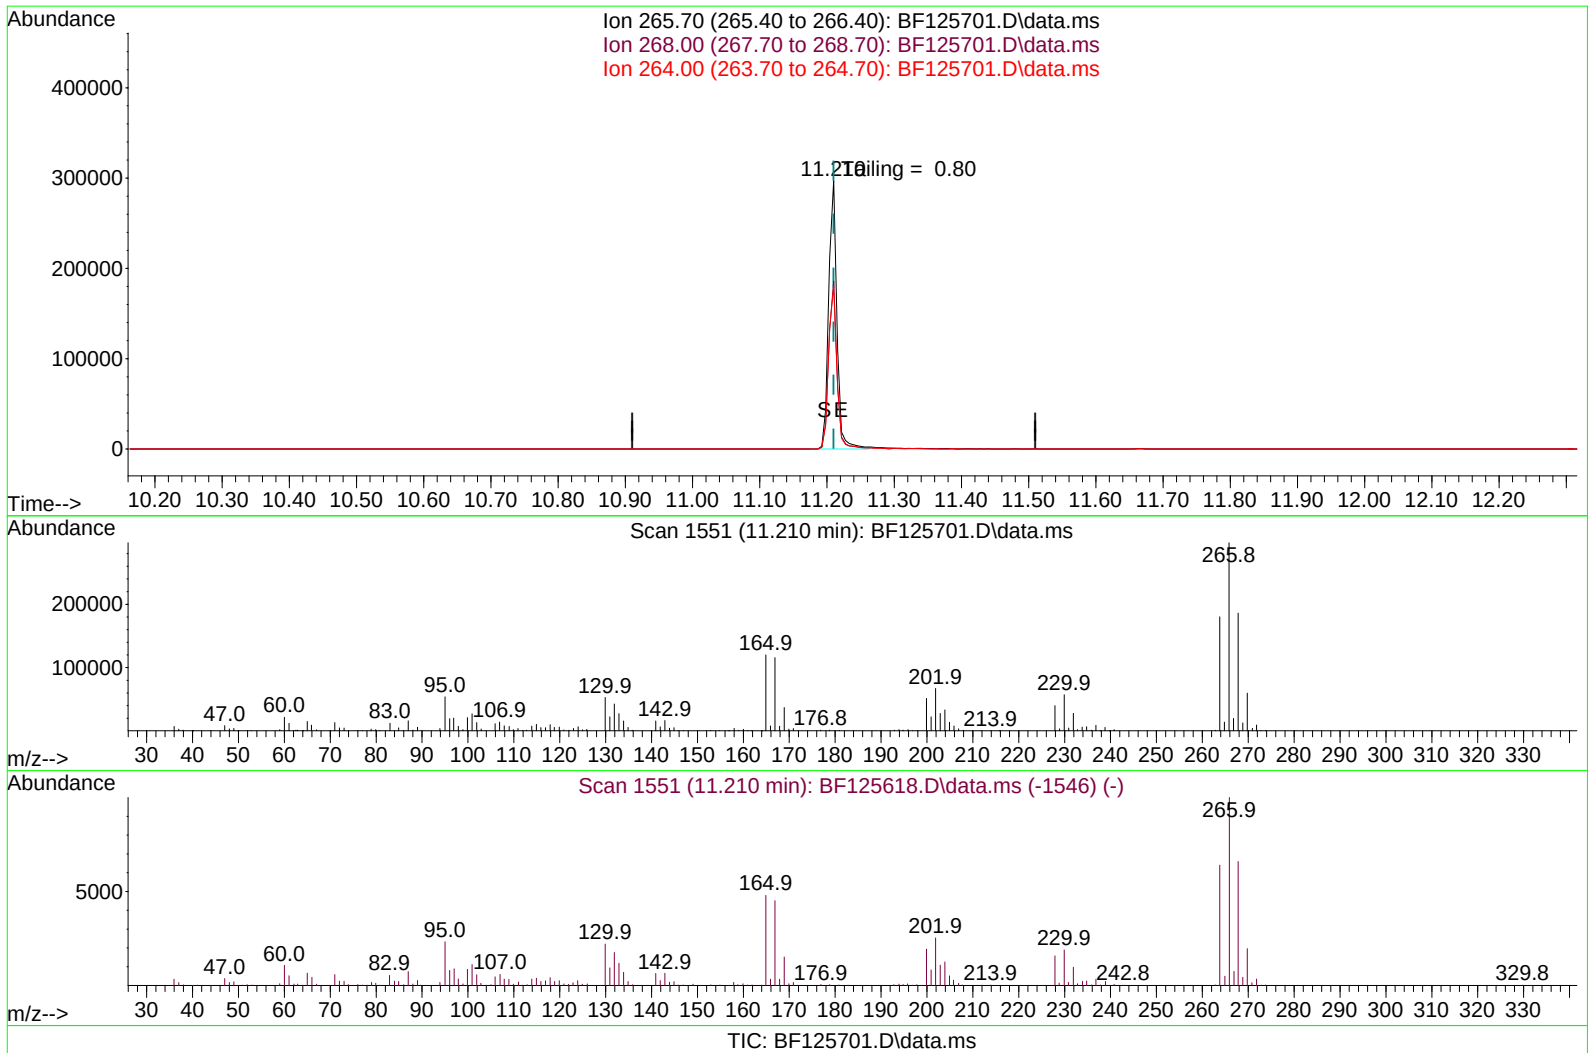

(70) Pentachlorophenol (C)

11.210min (-0.000) 38348.83 ng




response 256385

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.60
264.00	69.90	60.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092921\
 Data File : BF125701.D
 Acq On : 29 Sep 2021 9:00
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 29 10:44:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

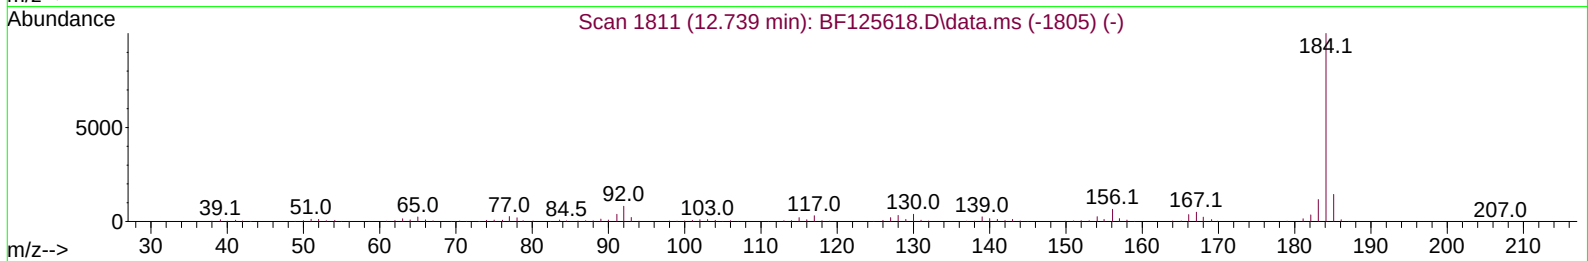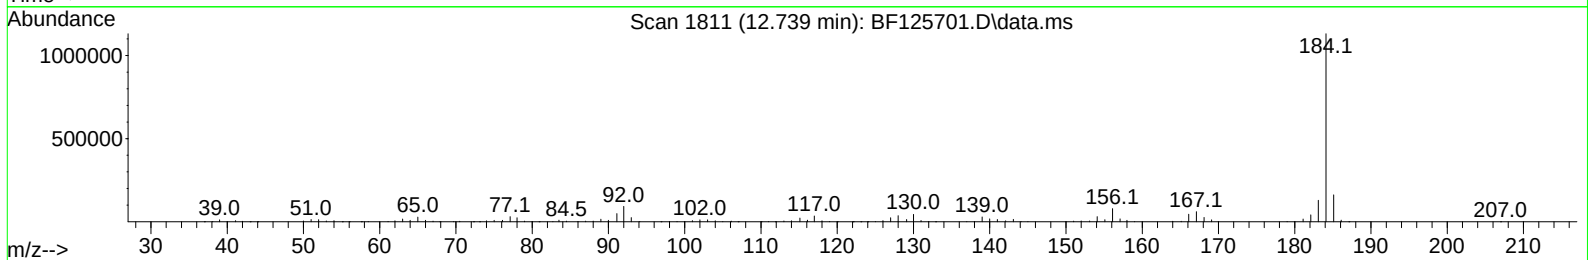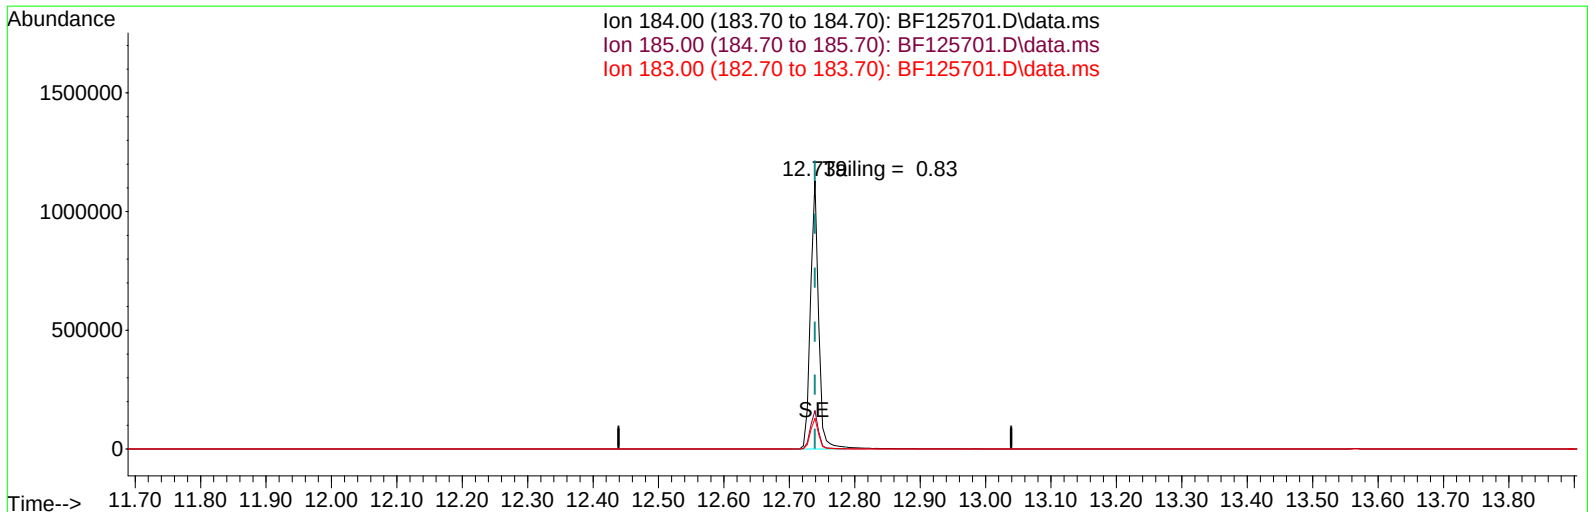

TIC: BF125701.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 318241.67 ng

response 986515

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.31
183.00	10.10	11.47
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
9/29/2021	BNA_F	<u>BF125701.D</u>
Compound Name	Response	Retention Time
DDT	479987	13.56
DDD	7533	13.26
DDE	1851	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9384	489371	1.92