
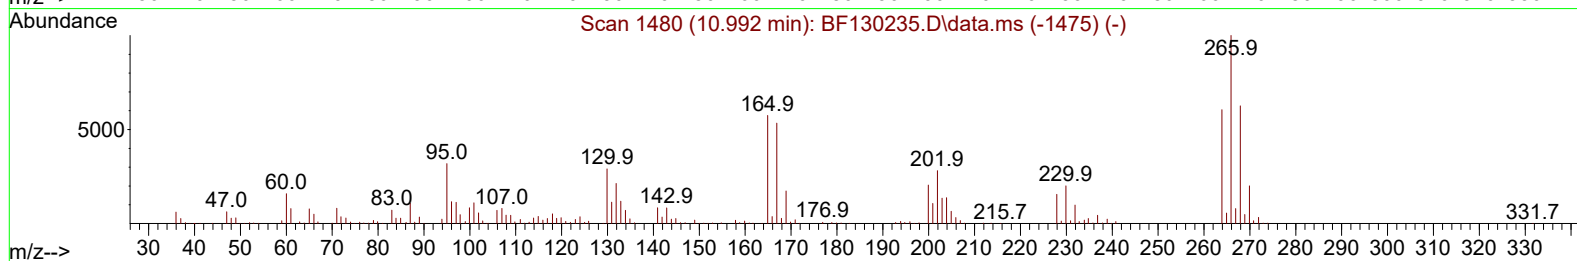
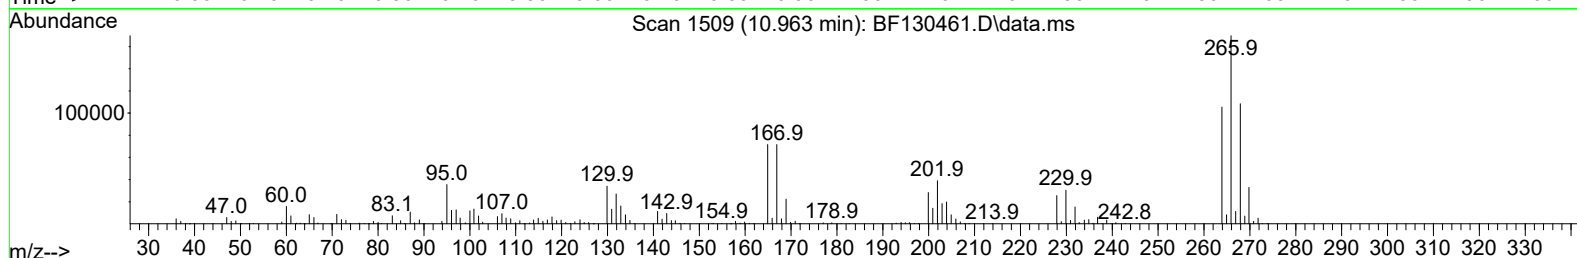


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092922\  
 Data File : BF130461.D  
 Acq On : 29 Sep 2022 10:25  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 05:01:43 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091422.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 28 02:59:31 2022  
 Response via : Initial Calibration

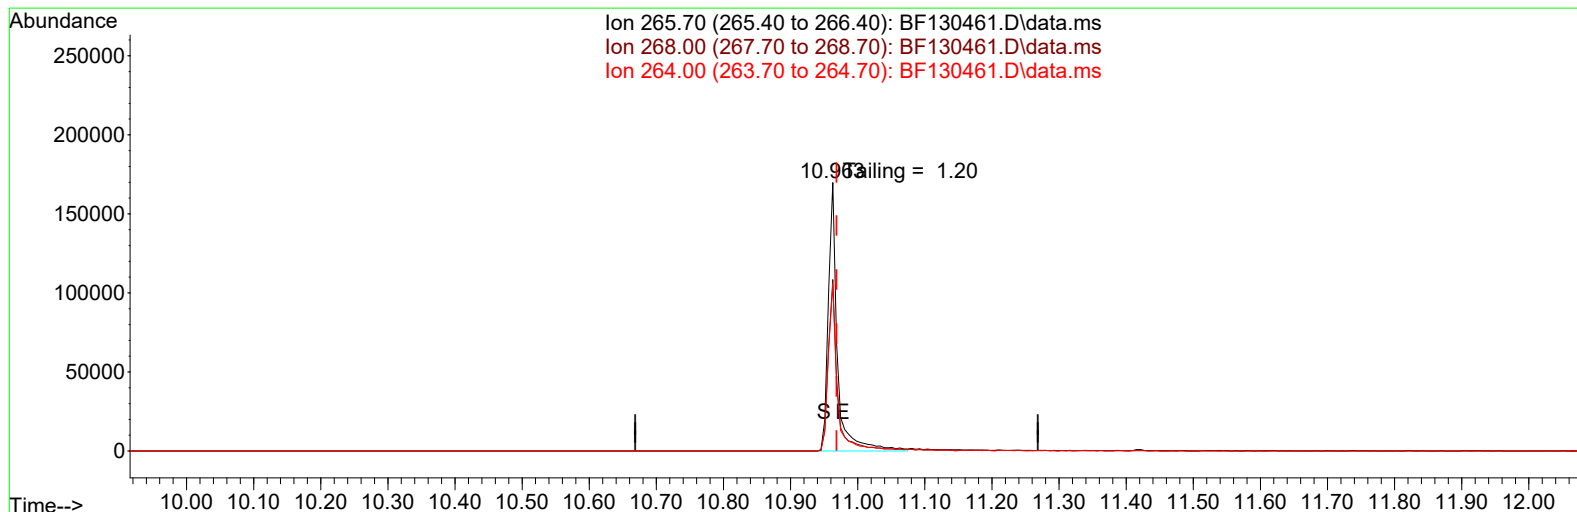

TIC: BF130461.D\data.ms

**(70) Pentachlorophenol (C)**




10.963min (-0.006) 182775.39 ng

response 161920

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.10  | 63.86  |
| 264.00 | 63.10  | 62.07  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092922\  
 Data File : BF130461.D  
 Acq On : 29 Sep 2022 10:25  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 05:01:43 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091422.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 28 02:59:31 2022  
 Response via : Initial Calibration

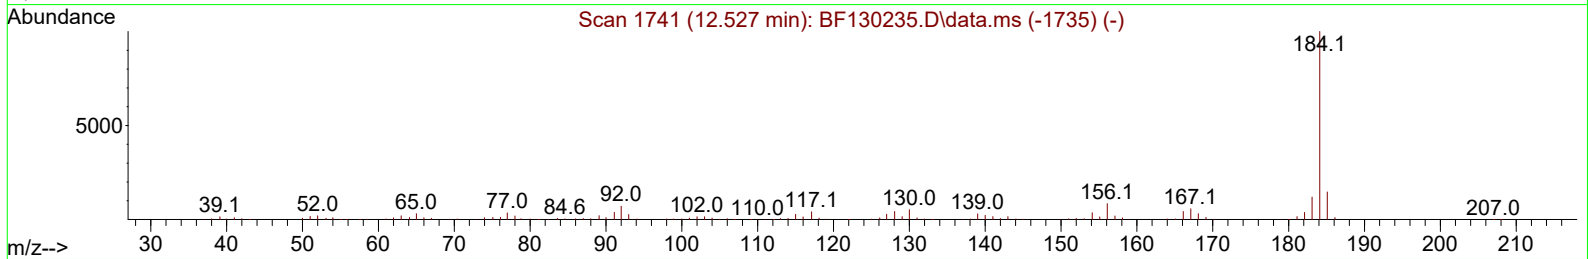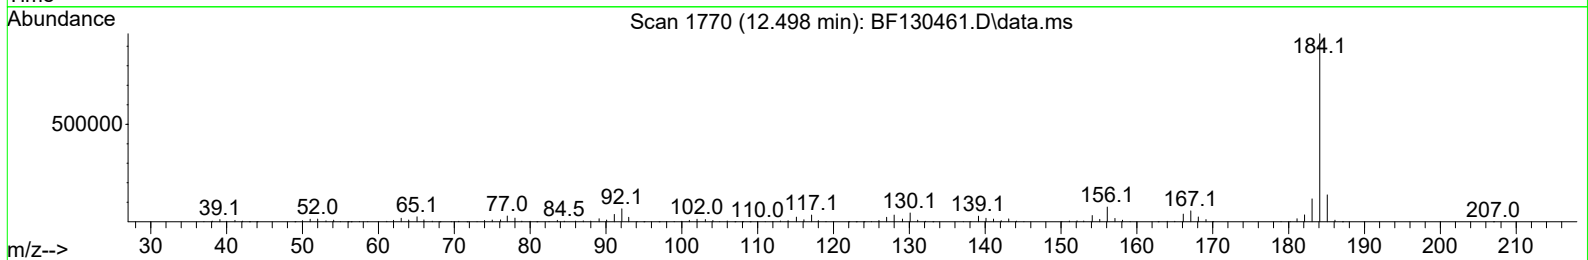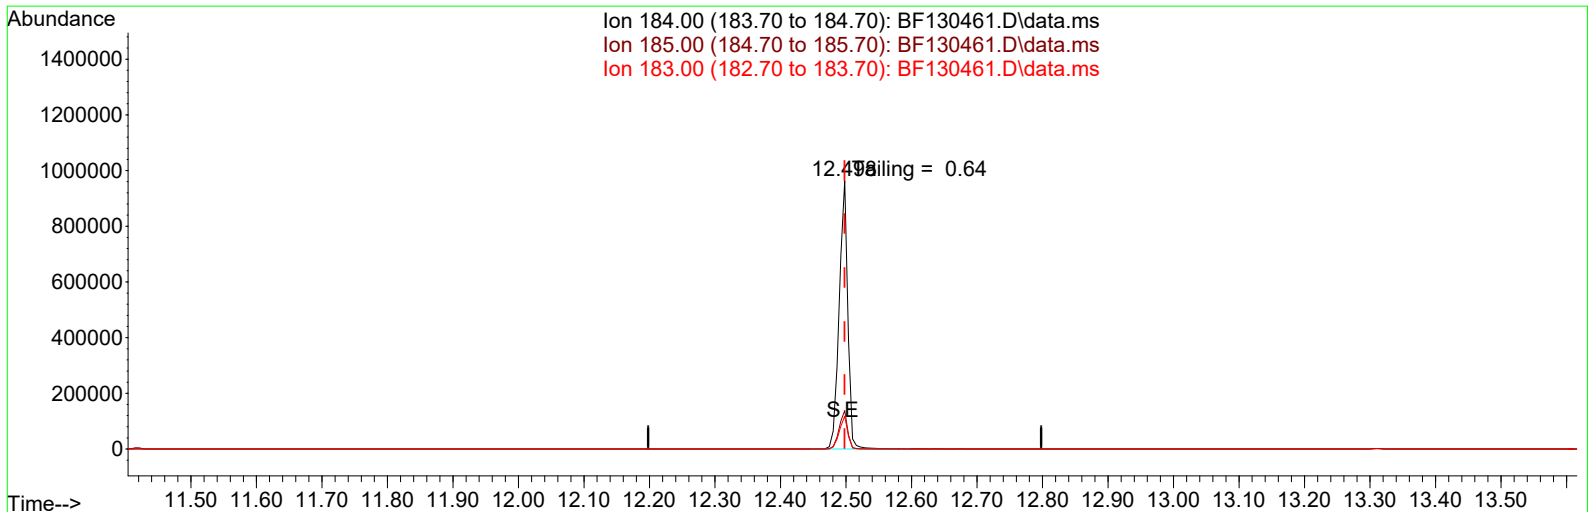

TIC: BF130461.D\data.ms

**(77) Benzidine**

12.498min (+ 0.000) 28482.65 ng

response 883877

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 14.31  |
| 183.00 | 11.40  | 12.21  |
| 0.00   | 0.00   | 0.00   |