
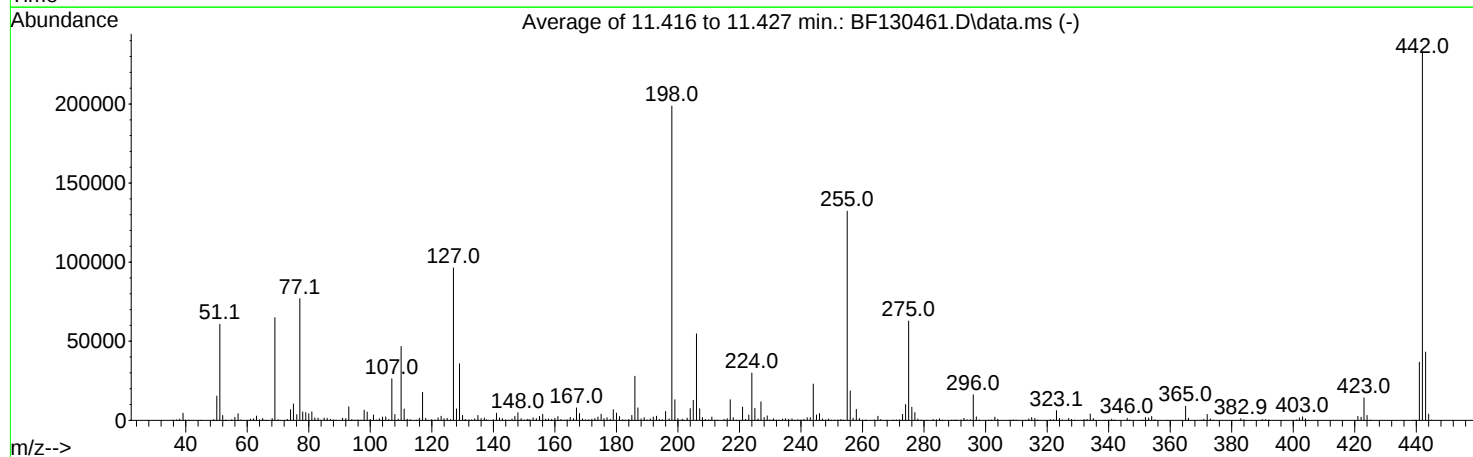


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092922\
 Data File : BF130461.D
 Acq On : 29 Sep 2022 10:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 02:59:31 2022

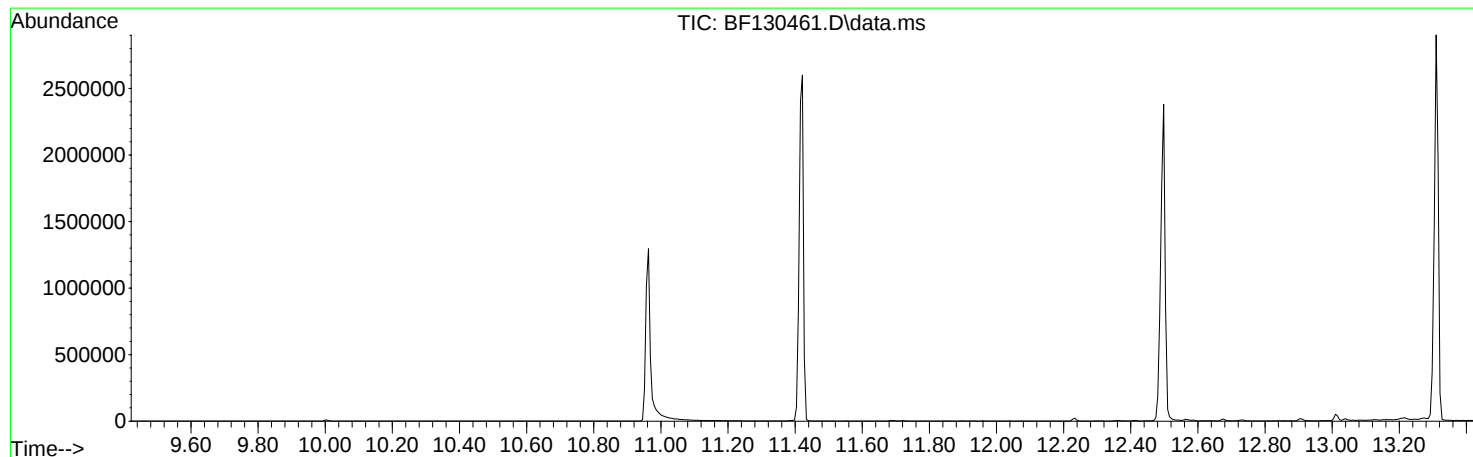




AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	60741	PASS
68	69	0.00	2	1.8	1194	PASS
69	198	0.00	100	32.7	64896	PASS
70	69	0.00	2	0.5	342	PASS
127	198	10	80	48.5	96369	PASS
197	198	0.00	2	0.5	921	PASS
198	198	100	100	100.0	198627	PASS
199	198	5	9	6.5	12978	PASS
275	198	10	60	31.6	62797	PASS
365	198	1	100	4.5	8910	PASS
441	198	0.01	100	18.5	36739	PASS
442	442	50	100	100.0	232597	PASS
443	442	15	24	18.6	43189	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092922\
 Data File : BF130461.D
 Acq On : 29 Sep 2022 10:25
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 30 05:01:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:59:31 2022
 Response via : Initial Calibration

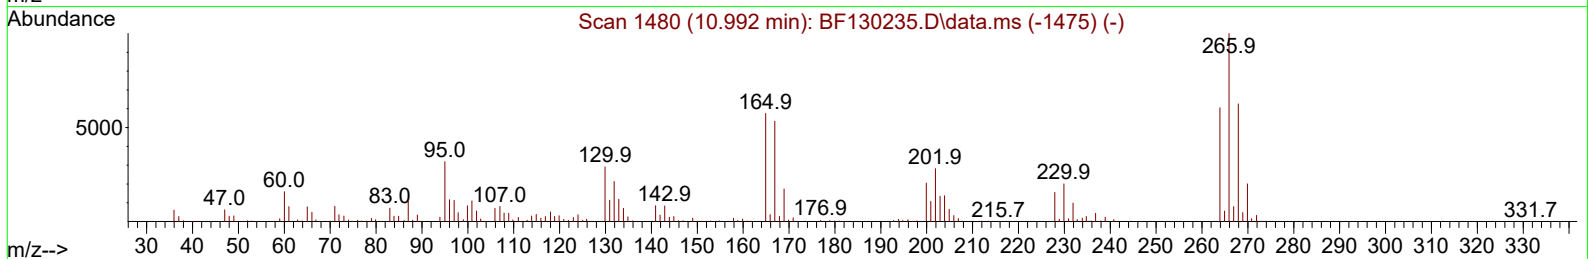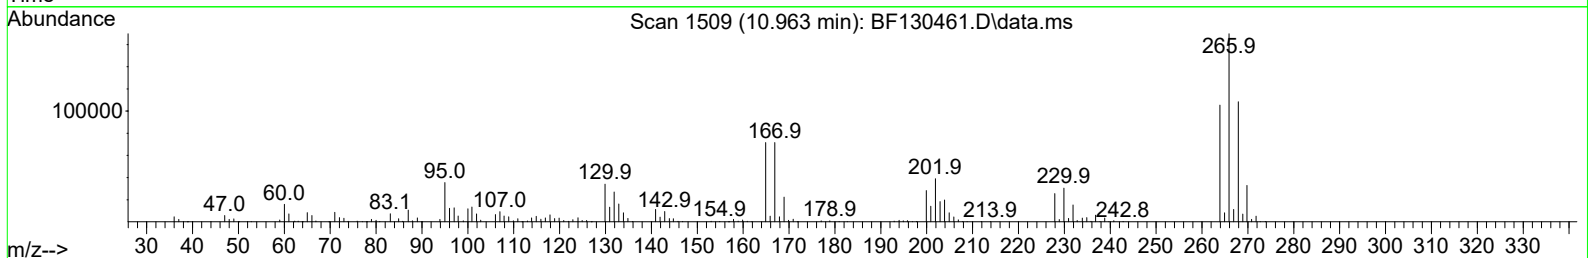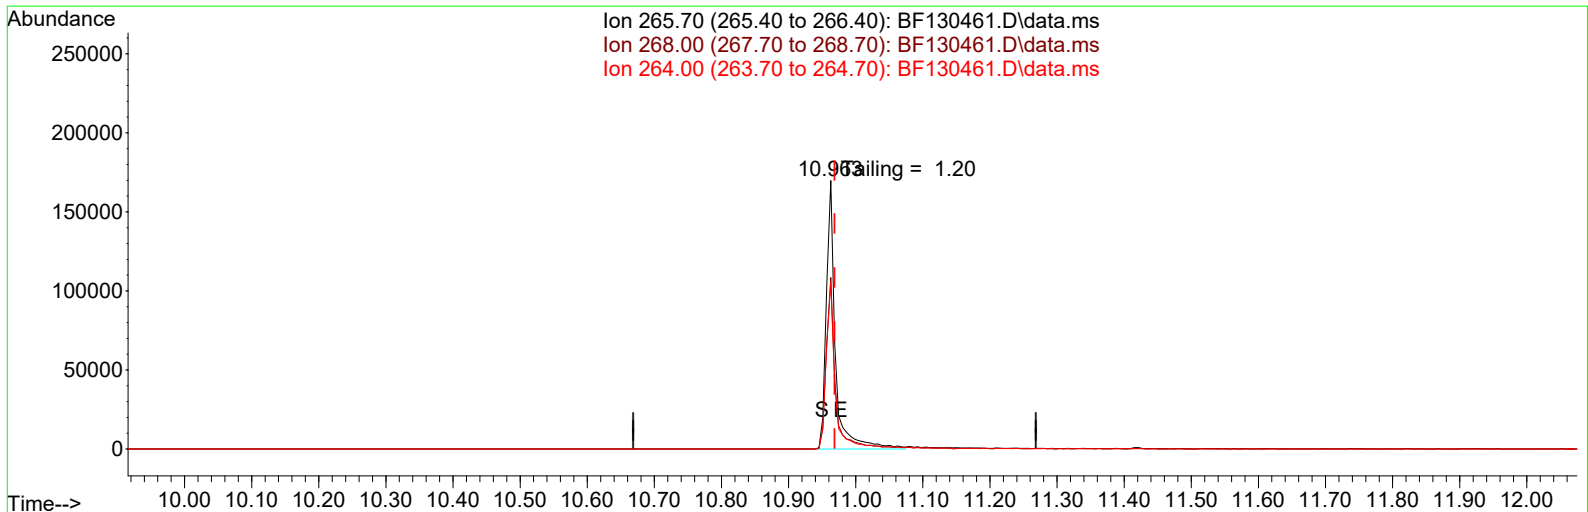

TIC: BF130461.D\data.ms

(70) Pentachlorophenol (C)

10.963min (-0.006) 182775.39 ng

response 161920

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.86
264.00	63.10	62.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/29/2022	BNA_F	<u>BF130461.D</u>
Compound Name	Response	Retention Time
DDT	475521	13.31
DDD	11304	13.01
DDE	1843	12.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13147	488668	2.69

Instrument :
BNA_F
ClientSampleId :
DFTPP