
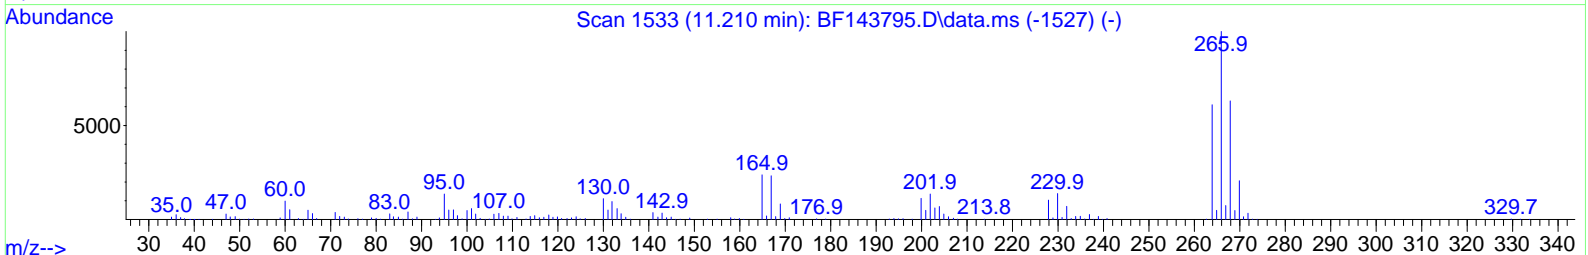
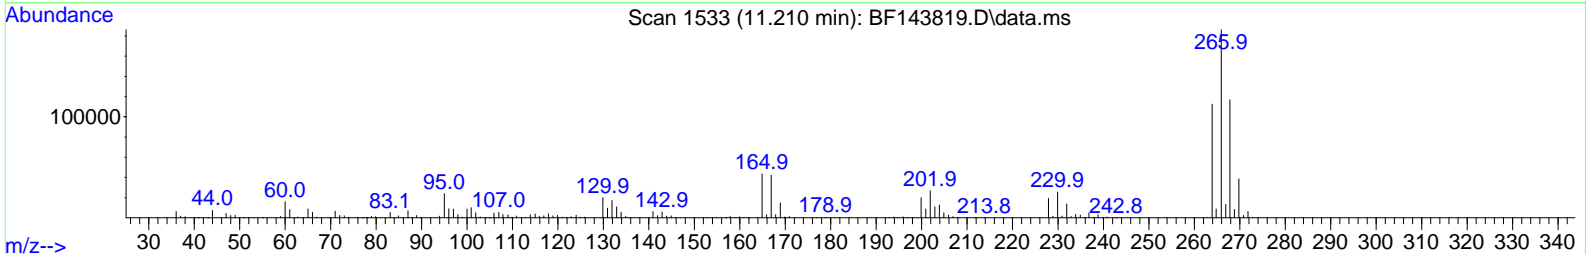


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092925\
 Data File : BF143819.D
 Acq On : 29 Sep 2025 10:40
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 11:22:46 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 24 05:00:00 2025
 Response via : Initial Calibration

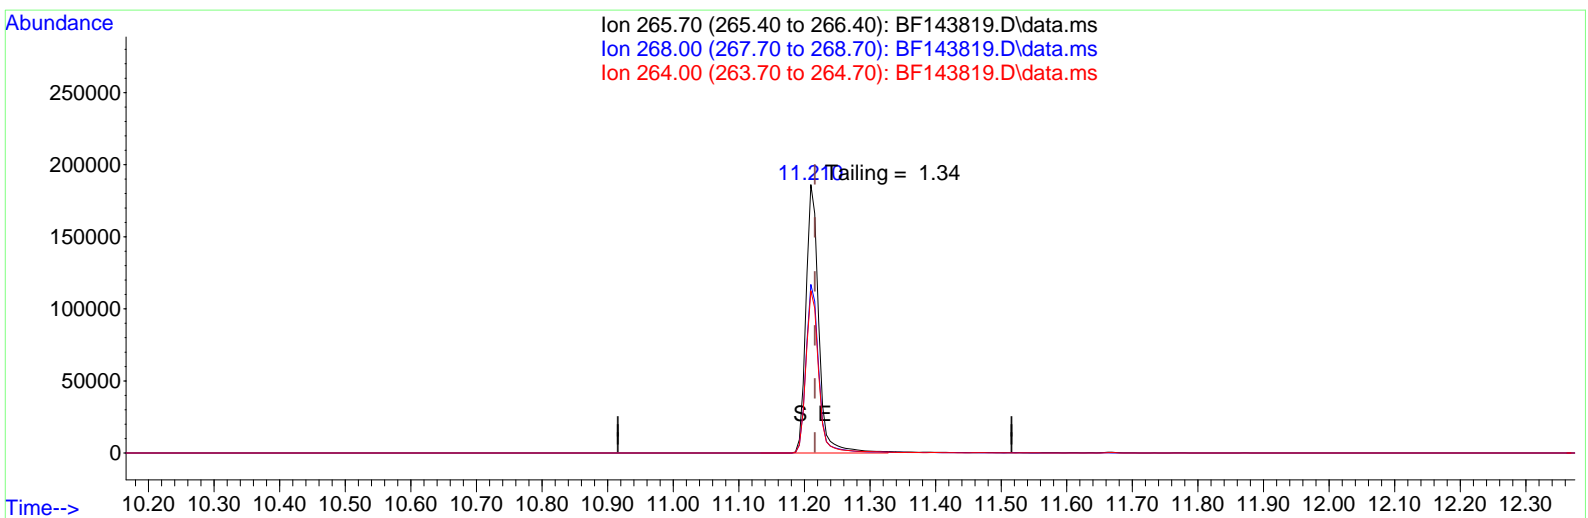

TIC: BF143819.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.006) 28093.51 ng

response 254856

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.78
264.00	61.00	60.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092925\
 Data File : BF143819.D
 Acq On : 29 Sep 2025 10:40
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 11:22:46 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF092325.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 24 05:00:00 2025
 Response via : Initial Calibration

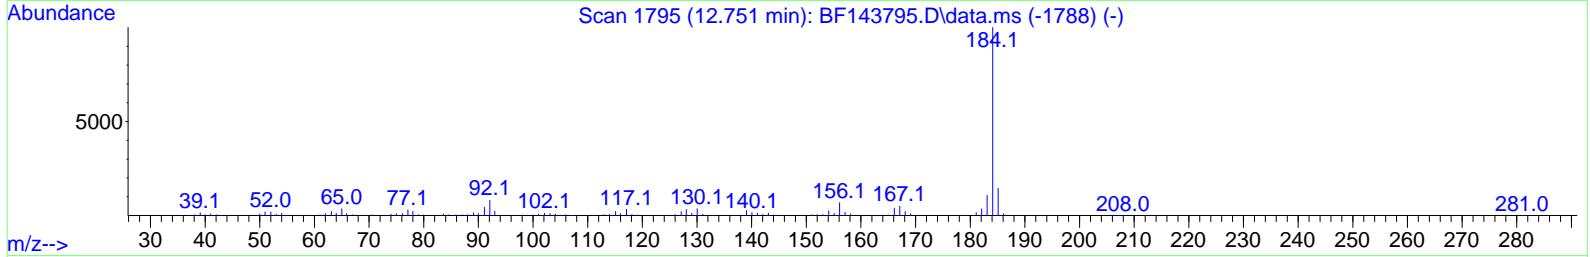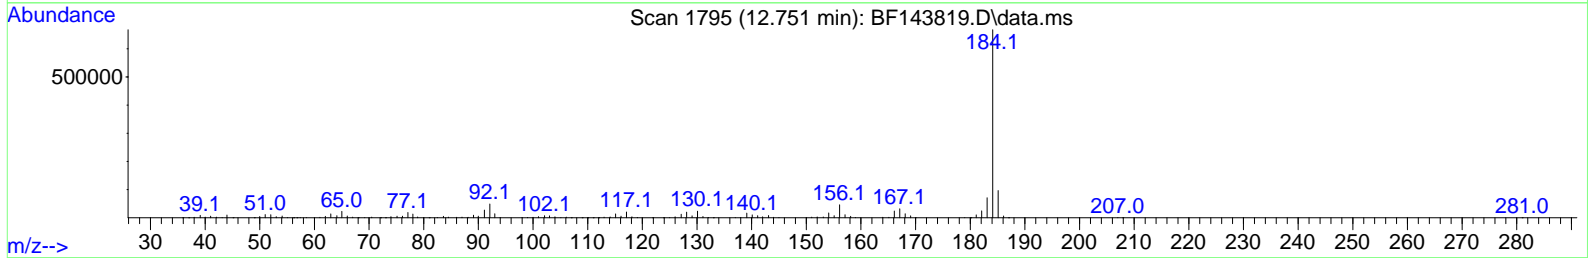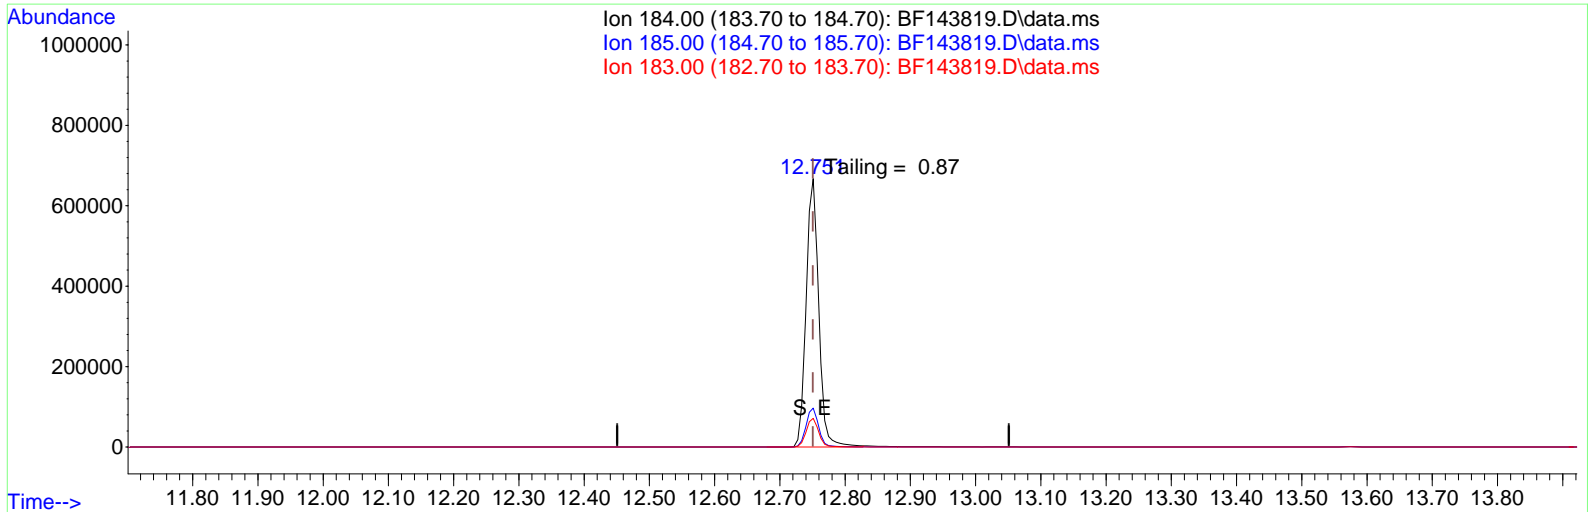

TIC: BF143819.D\data.ms

(77) Benzidine

12.751min (+ 0.000) 0.00 ng

response 903640

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.52
183.00	10.80	10.70
0.00	0.00	0.00