
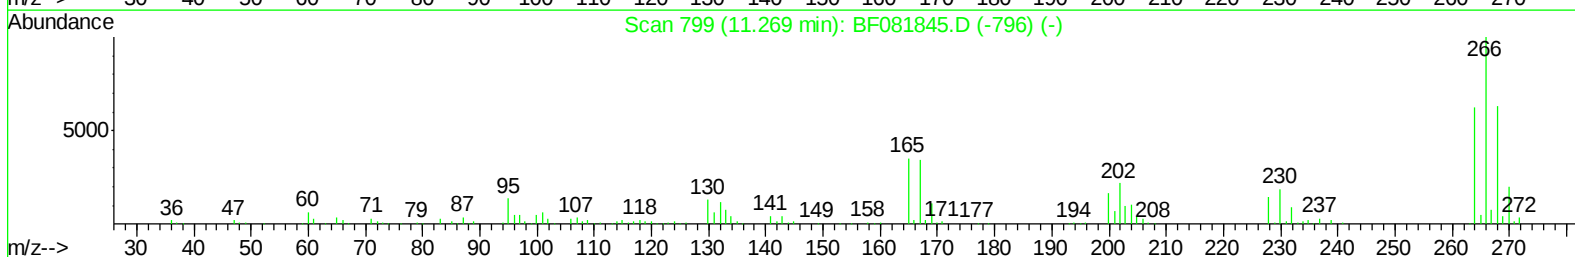
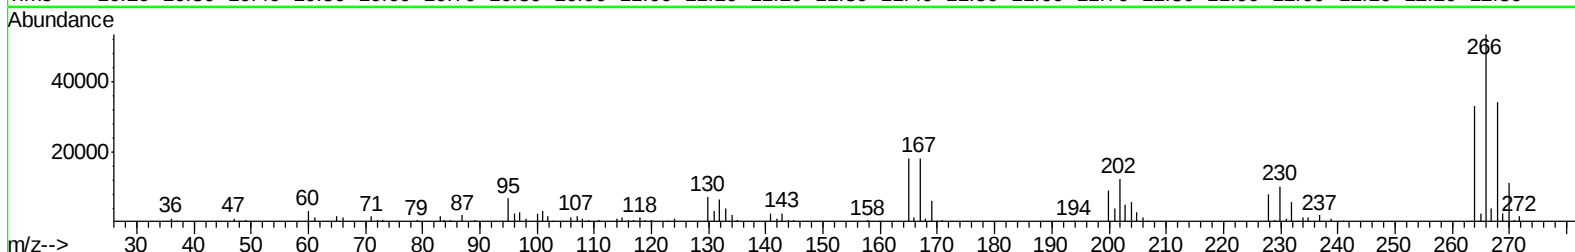


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF093015\
Data File : BF081910.D
Acq On : 30 Sep 2015 19:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 06:47:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 05:22:05 2015
Response via : Initial Calibration

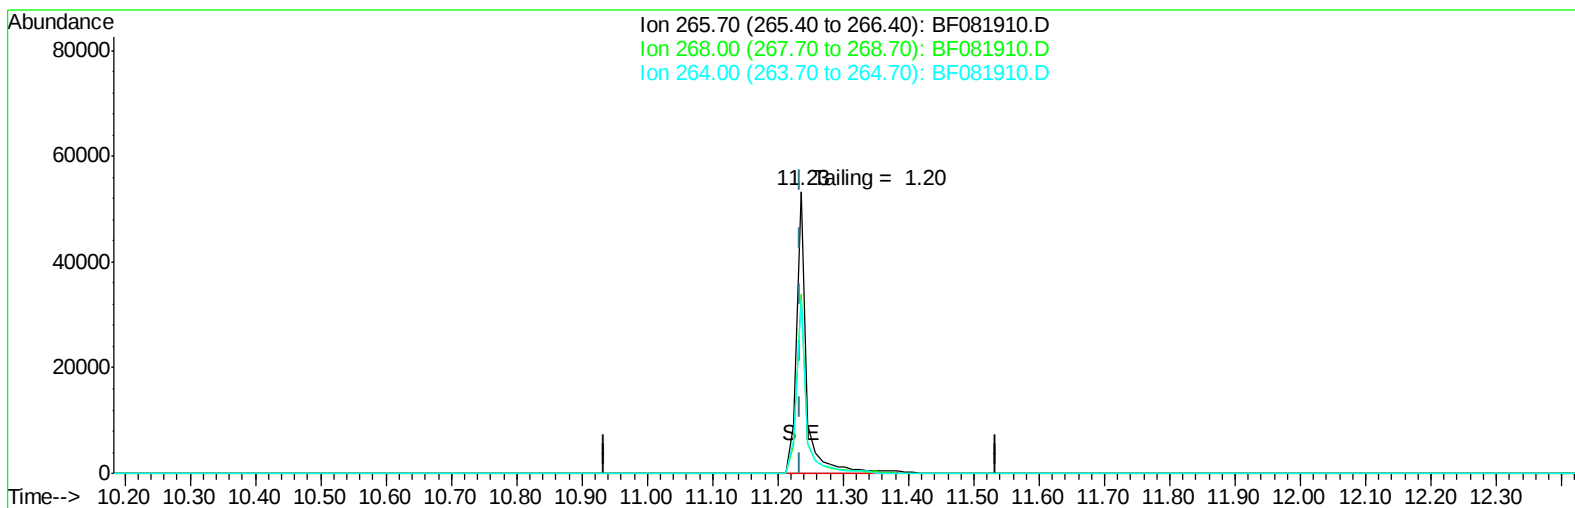

TIC: BF081910.D

(69) Pentachlorophenol (C)




11.235min (-0.000) 32998.60ng

response 59265

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.73
264.00	62.70	61.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF093015\
Data File : BF081910.D
Acq On : 30 Sep 2015 19:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 06:47:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 01 05:22:05 2015
Response via : Initial Calibration

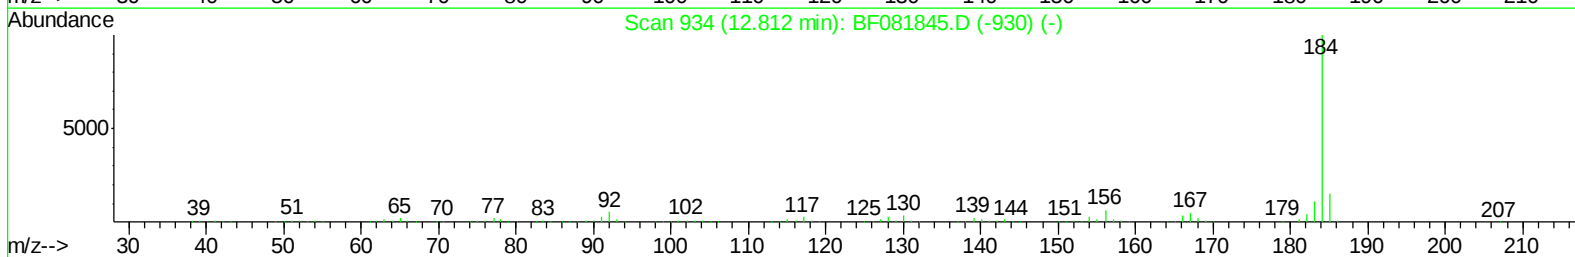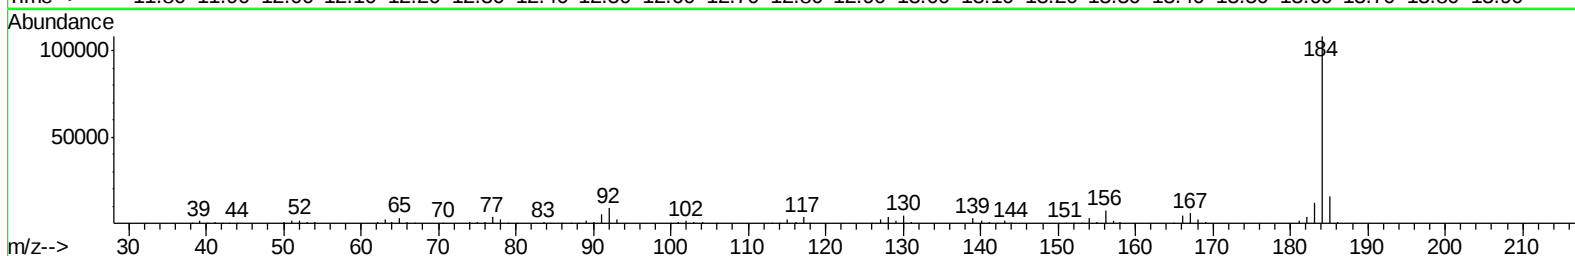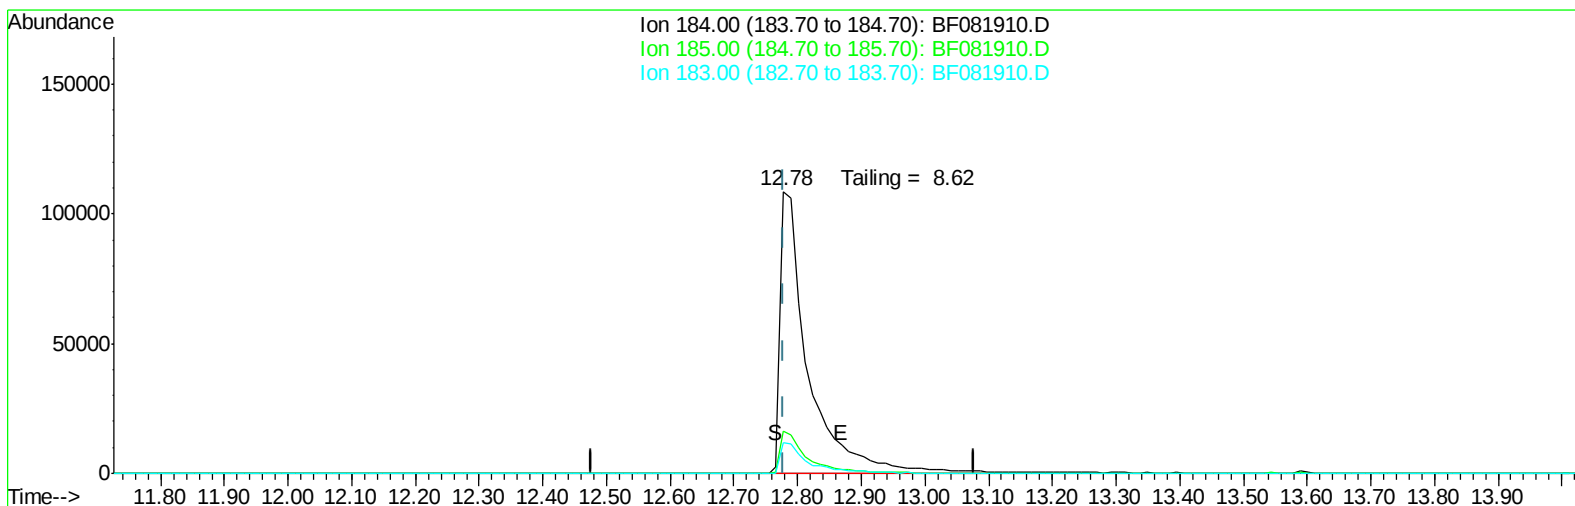

TIC: BF081910.D

(76) Benzidine

12.778min (-0.000) 0.00ng

response 324169

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.97
183.00	9.50	10.90
0.00	0.00	0.00