


Data Path : Z:\HPCHEM1\BNA F\DATA\BF093015\
 Data File : BF081910.D
 Acq On : 30 Sep 2015 19:17
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 28 18:10:42 2015

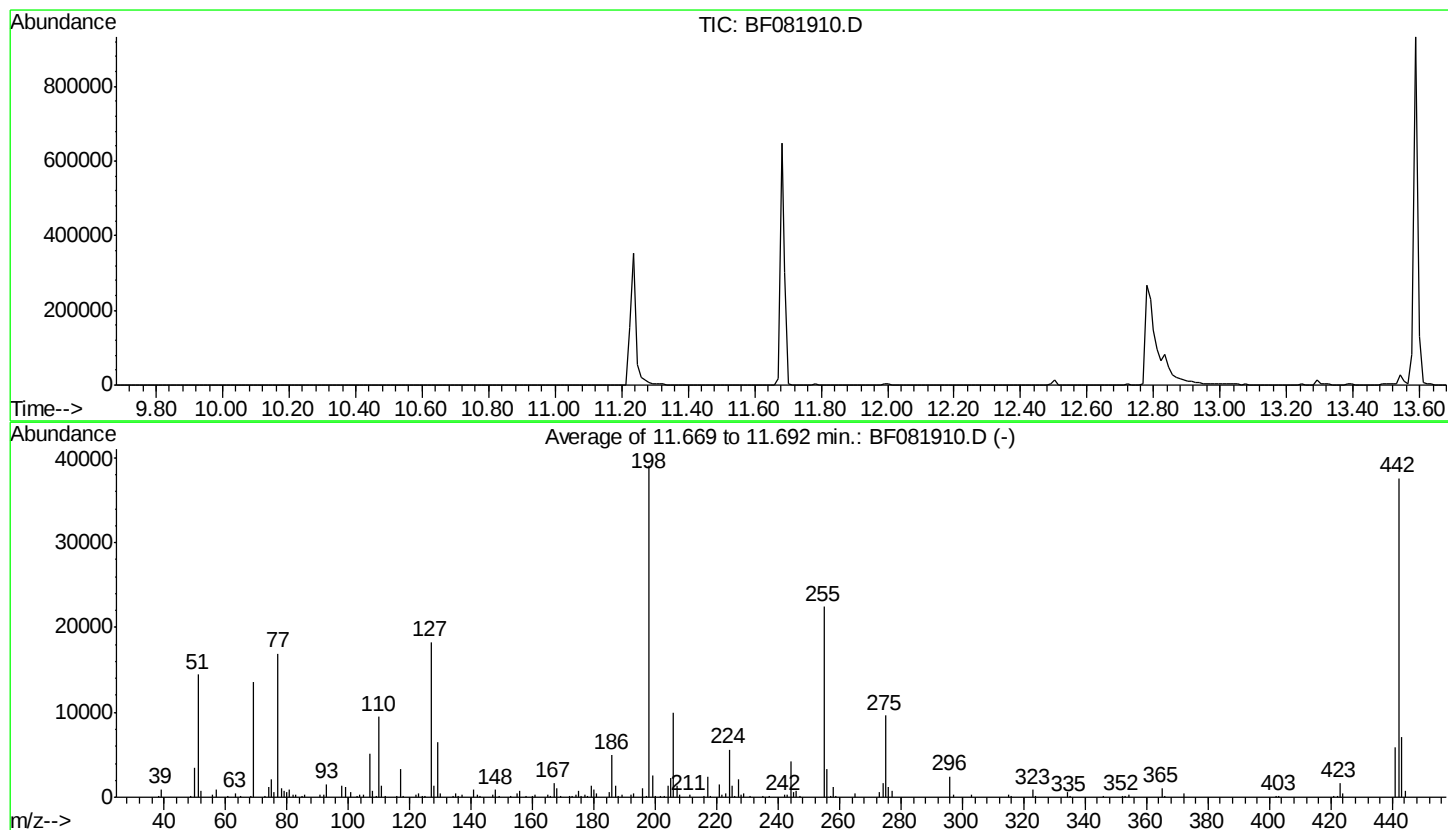

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	14436	PASS
68	69	0.00	2	1.5	200	PASS
69	198	0.00	100	34.9	13636	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.9	18321	PASS
197	198	0.00	2	0.4	156	PASS
198	198	100	100	100.0	39074	PASS
199	198	5	9	6.6	2560	PASS
275	198	10	60	24.6	9602	PASS
365	198	1	100	2.9	1120	PASS
441	442	0.01	24	15.6	5878	PASS
442	198	50	100	96.3	37632	PASS
443	442	15	24	18.9	7111	PASS