


Data Path : Z:\HPCHEM1\BNA F\DATA\BF093016\
 Data File : BF090310.D
 Acq On : 30 Sep 2016 11:16
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 26 15:58:38 2016

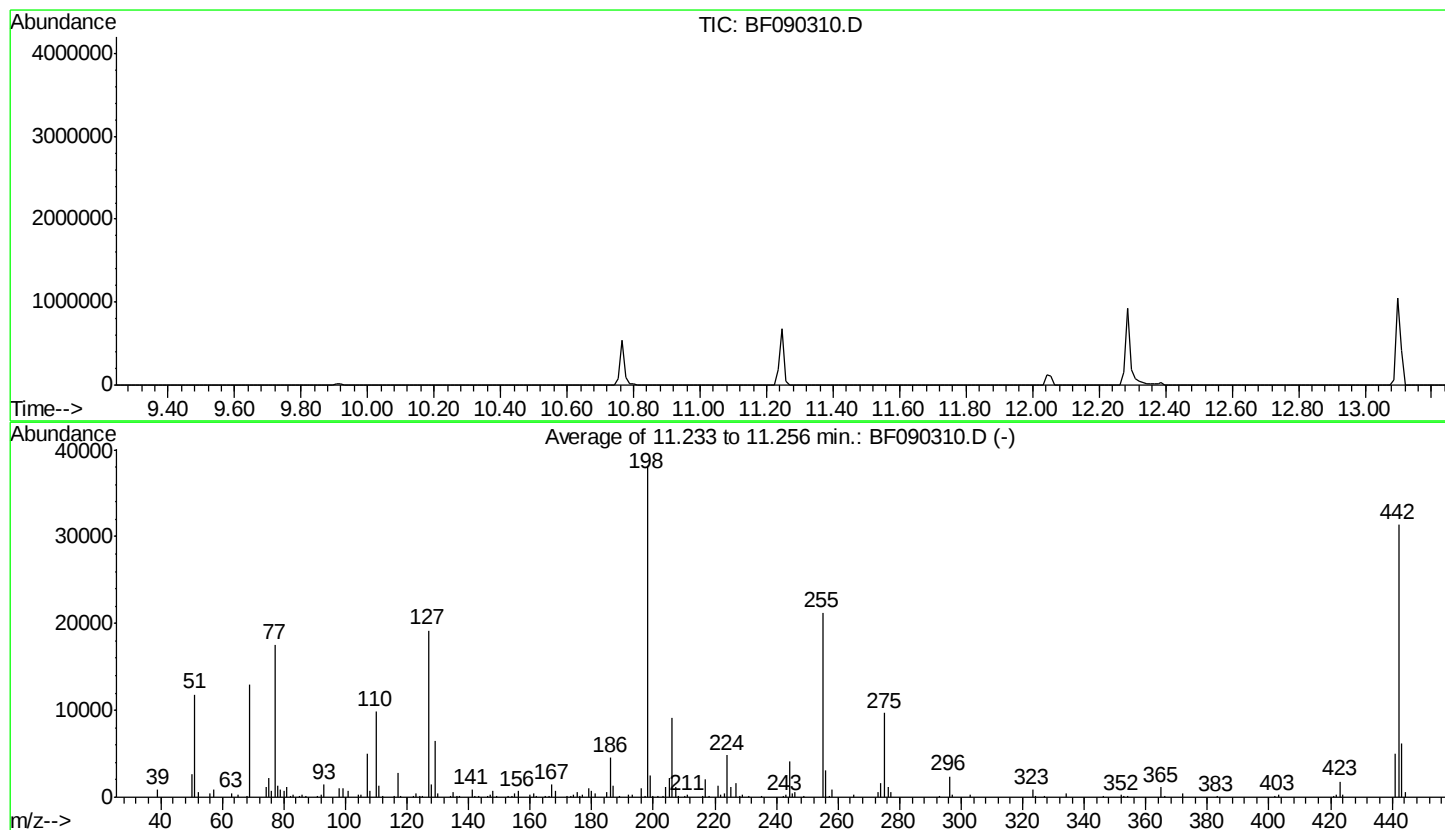

AutoFind: Scans 844, 845, 846; Background Corrected with Scan 841

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	11810	PASS
68	69	0.00	2	0.8	101	PASS
69	198	0.00	100	33.9	12949	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	19172	PASS
197	198	0.00	2	0.5	191	PASS
198	198	100	100	100.0	38177	PASS
199	198	5	9	6.7	2571	PASS
275	198	10	60	25.5	9717	PASS
365	198	1	100	3.1	1170	PASS
441	442	0.01	24	16.1	5056	PASS
442	198	50	100	82.2	31384	PASS
443	442	15	24	19.5	6122	PASS