

Data Path : Z:\HPCHEM1\BNA F\DATA\BF093017\
 Data File : BF098961.D
 Acq On : 30 Sep 2017 14:31
 Operator : SJ/JU
 Sample : I5530-01 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 30 23:25:02 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 23 13:50:58 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.92	152	144283	20.00	ng	0.00
21) Naphthalene-d8	8.20	136	597982	20.00	ng	0.00
38) Acenaphthene-d10	9.95	164	269269	20.00	ng	-0.01
63) Phenanthrene-d10	11.44	188	440381	20.00	ng	0.00
75) Chrysene-d12	14.07	240	249855	20.00	ng	-0.01
86) Perylene-d12	15.57	264	247678	20.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
5) 2-Fluorophenol	5.52	112	158165	17.45	ng	-0.02
7) Phenol-d6	6.53	99	194232	17.37	ng	-0.02
23) Nitrobenzene-d5	7.47	82	115154	12.35	ng	-0.02
41) 2,4,6-Tribromophenol	10.74	330	33209	15.07	ng	-0.01
44) 2-Fluorobiphenyl	9.27	172	234132	14.52	ng	-0.01
78) Terphenyl-d14	13.02	244	161934	14.74	ng	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
19) n-Nitroso-di-n-propylamine	7.47	70	15121	2.118	ng	# 79
25) Isophorone	7.47	82	114623	5.946	ng	# 64
50) 2,6-Dinitrotoluene	9.95	165	34405	7.776	ng	# 26
56) 2,4-Dinitrotoluene	9.95	165	34405	5.992	ng	# 23
70) Phenanthrene	11.46	178	87820	3.726	ng	95
74) Fluoranthene	12.65	202	126738	5.310	ng	97
77) Pyrene	12.88	202	114292	5.999	ng	99
80) Benzo(a)anthracene	14.07	228	46902	3.100	ng	92
82) Chrysene	14.10	228	44101	3.062	ng	98
85) Indeno(1,2,3-cd)pyrene	17.07	276	30358	2.635	ng	# 91
87) Benzo(b)fluoranthene	15.13	252	70855	4.653	ng	# 92
88) Benzo(k)fluoranthene	15.13	252	70855	4.711	ng	# 95
89) Benzo(a)pyrene	15.50	252	39097	2.797	ng	# 90
91) Benzo(a,h,i)perylene	17.53	276	31321	2.832	ng	# 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF093017\
Data File : BF098961.D
Acq On : 30 Sep 2017 14:31
Operator : SJ/JU
Sample : I5530-01 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 30 23:25:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

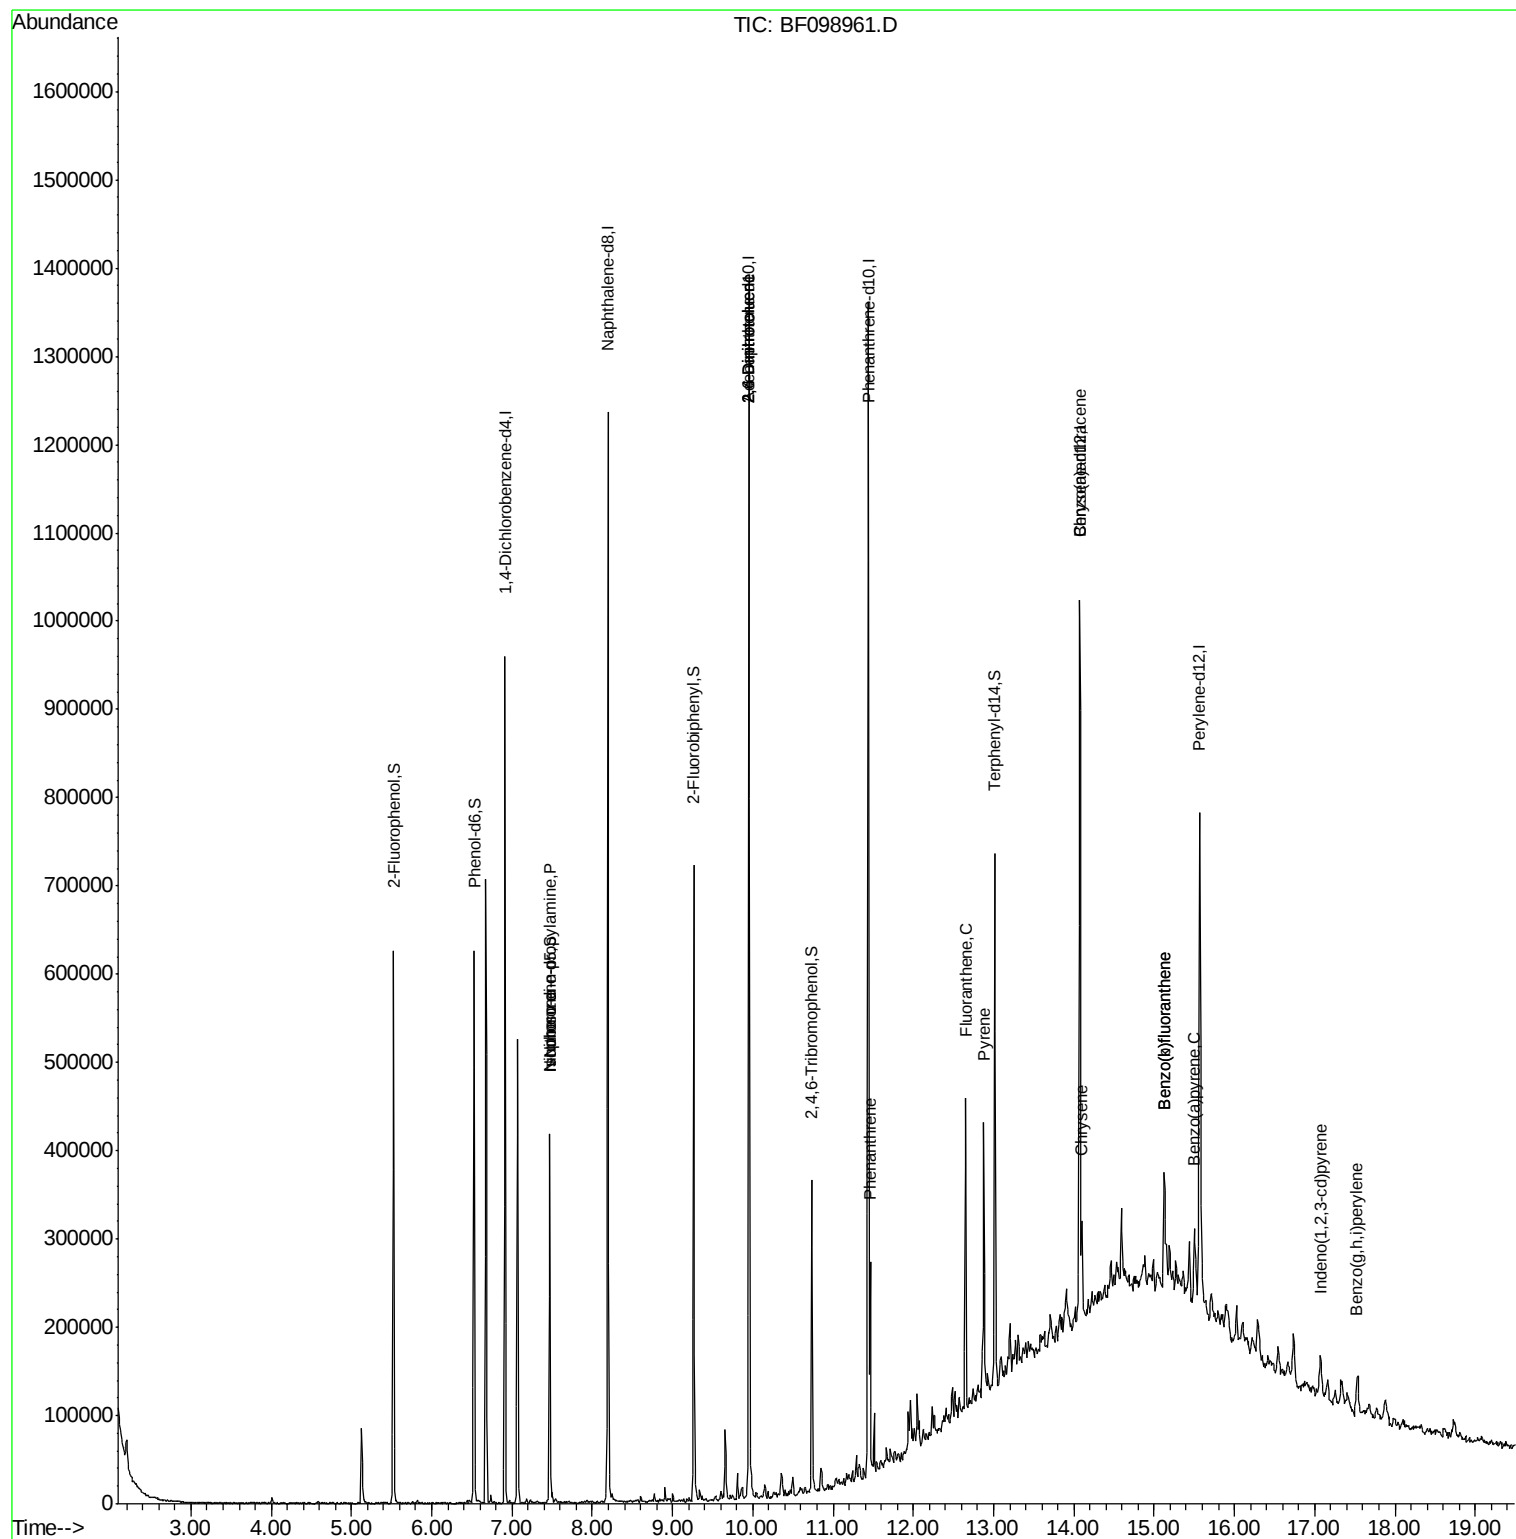

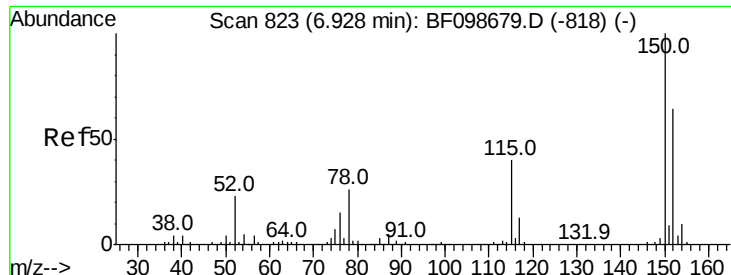


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.92 min Scan# 821
Delta R.T. -0.01 min
Lab File: BF098961.D
Acq: 30 Sep 2017 14:31

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 144283
Ion Ratio Lower Upper
152 100
150 152.6 124.6 186.8
115 58.7 50.1 75.1

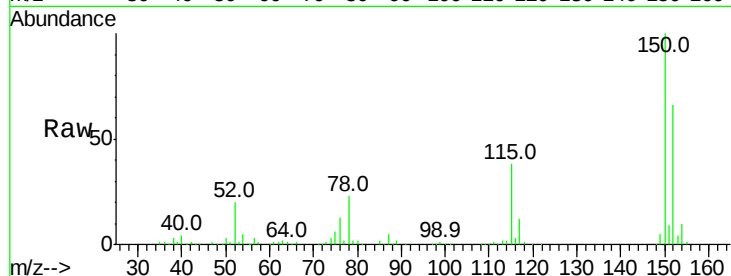


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

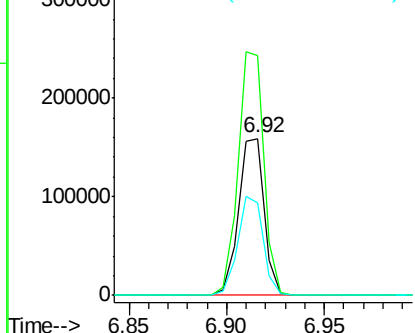



#5

2-Fluorophenol
Concen: 17.451 ng
RT: 5.52 min Scan# 584
Delta R.T. -0.02 min
Lab File: BF098961.D
Acq: 30 Sep 2017 14:31

Tgt Ion:112 Resp: 158165
Ion Ratio Lower Upper
112 100
64 58.0 47.9 71.9
63 28.5 23.7 35.5

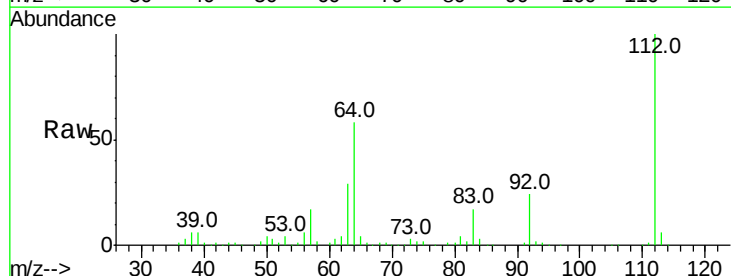

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

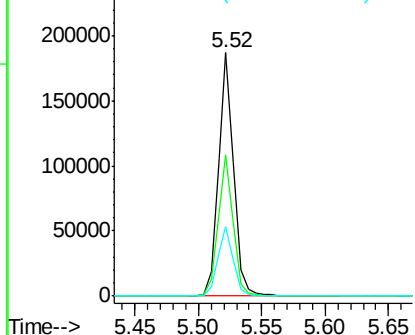



#7

Phenol-d6

Concen: 17.372 ng

RT: 6.53 min Scan# 755

Delta R.T. -0.02 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 194232

Ion Ratio Lower Upper

99 100

42 17.4 14.5 21.7

71 30.1 25.4 38.0

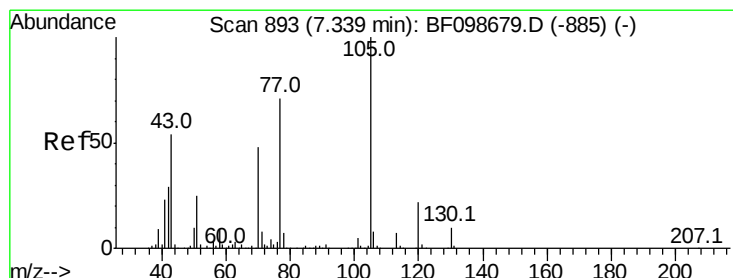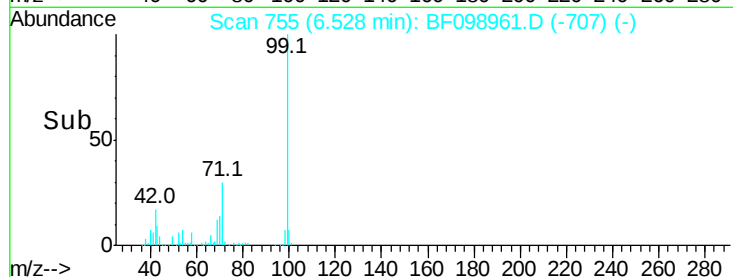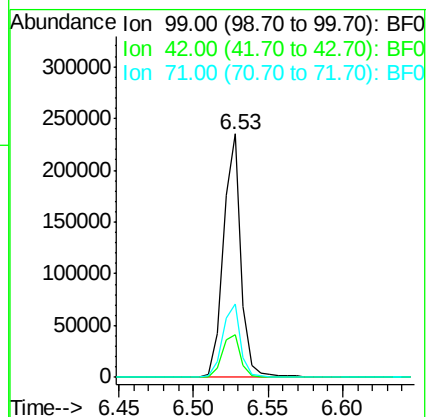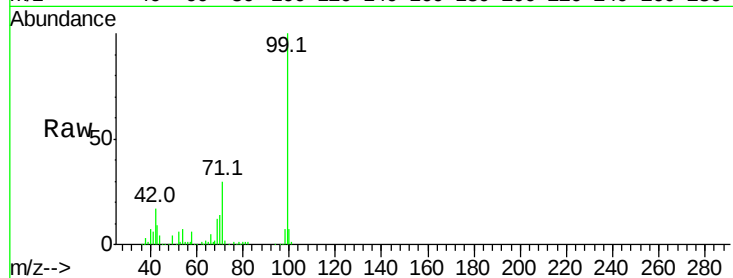

#19

n-Nitroso-di-n-propylamine

Concen: 2.118 ng

RT: 7.47 min Scan# 915

Delta R.T. 0.14 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31

Tgt Ion: 70 Resp: 15121




Ion Ratio Lower Upper


70 100

42 49.4 47.5 71.3

101 0.0 7.4 11.2#

130 2.0 16.6 25.0#

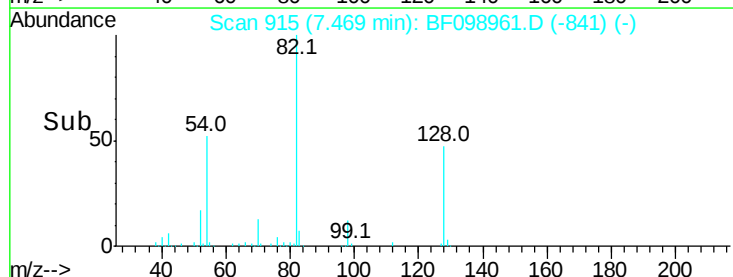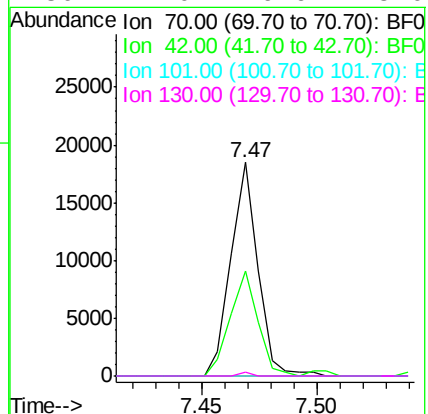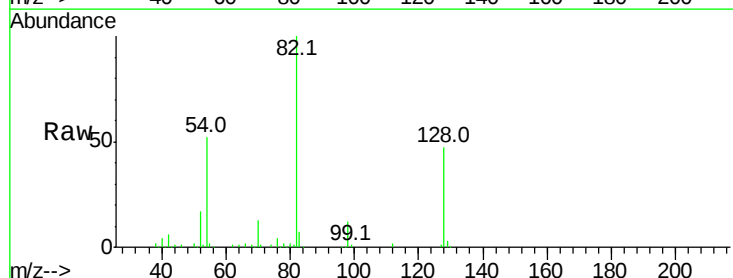

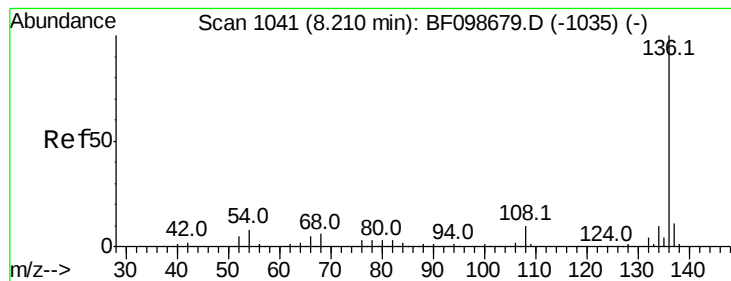

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.20 min Scan# 1039

Delta R.T. -0.01 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31

Instrument :

BNA_F

ClientSampled :

Tot Ion:136 Resp: 597982


Ion Ratio Lower Upper

136 100

137 10.7 8.9 13.3

54 6.9 6.6 9.8

68 5.5 5.0 7.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

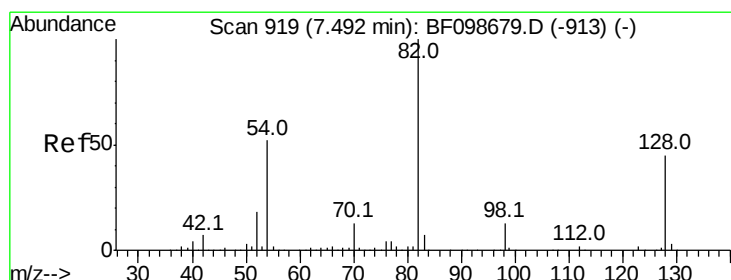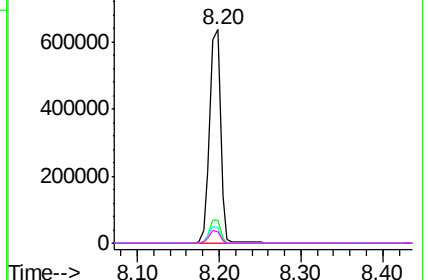

#23

Nitrobenzene-d5

Concen: 12.350 ng

RT: 7.47 min Scan# 915

Delta R.T. -0.02 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31


Tgt Ion: 82 Resp: 115154

Ion Ratio Lower Upper

82 100

128 46.7 36.1 54.1



54 52.2 41.4 62.2




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

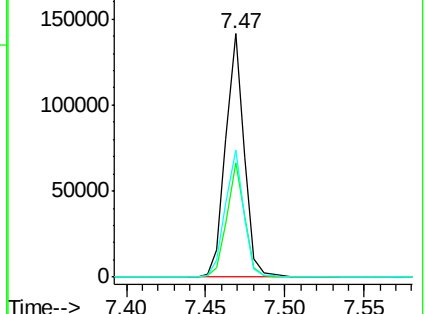

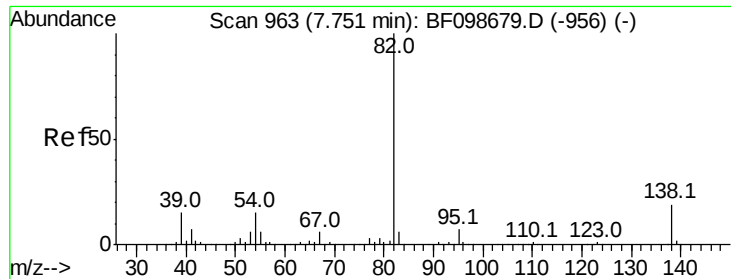

#25

Isophorone

Concen: 5.946 ng

RT: 7.47 min Scan# 915

Delta R.T. -0.28 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 114623

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

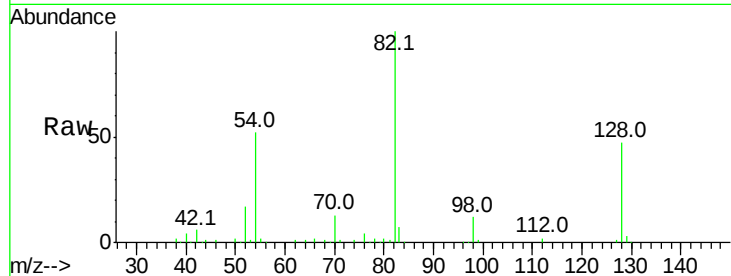

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): E

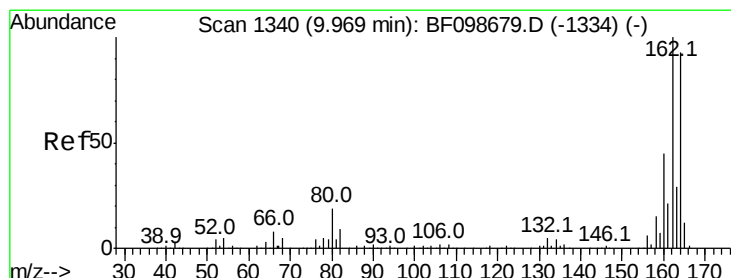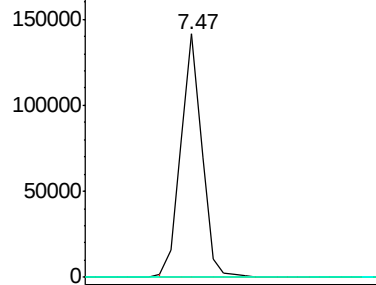

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.95 min Scan# 1337

Delta R.T. -0.01 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31


Tgt Ion:164 Resp: 269269

Ion Ratio Lower Upper



164 100


162 105.7 86.1 129.1

160 46.3 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

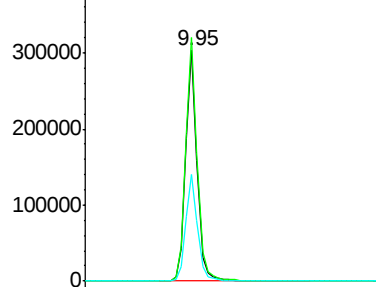


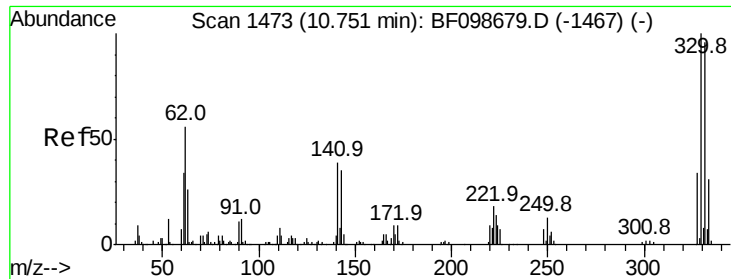




#41
 2,4,6-Tribromophenol
 Concen: 15.072 ng
 RT: 10.74 min Scan# 1471
 Delta R.T. -0.01 min
 Lab File: BF098961.D
 Acq: 30 Sep 2017 14:31

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 33209
 Ion Ratio Lower Upper
 330 100
 332 98.9 77.0 115.6
 141 53.4 29.9 44.9#

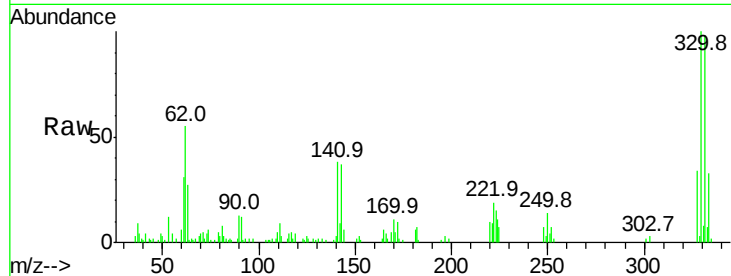


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


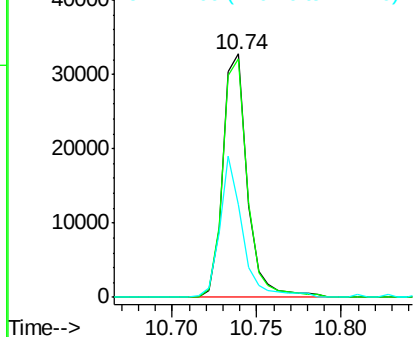



#44
 2-Fluorobiphenyl
 Concen: 14.516 ng
 RT: 9.27 min Scan# 1221
 Delta R.T. -0.01 min
 Lab File: BF098961.D
 Acq: 30 Sep 2017 14:31

Tgt Ion:172 Resp: 234132
 Ion Ratio Lower Upper
 172 100
 171 35.4 29.7 44.5
 170 22.9 19.6 29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

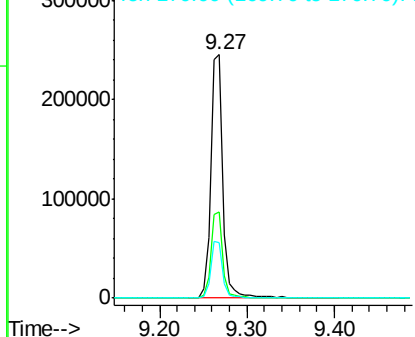

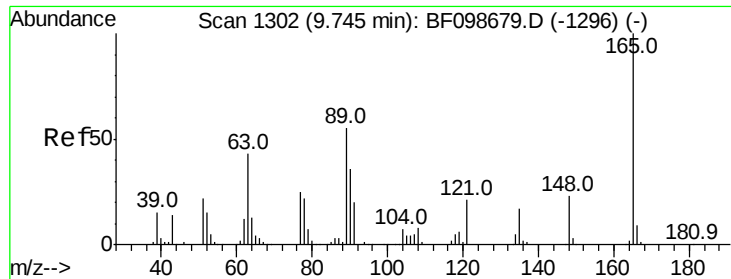

#50

2,6-Dinitrotoluene

Concen: 7.776 ng

RT: 9.95 min Scan# 1337





Delta R.T. 0.21 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	165	Resp:	34405
Ion	Ratio	Lower	Upper
165	100		
63	1.6	44.7	67.1#
89	1.2	44.0	66.0#

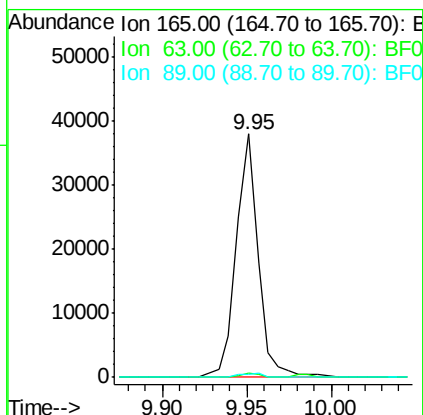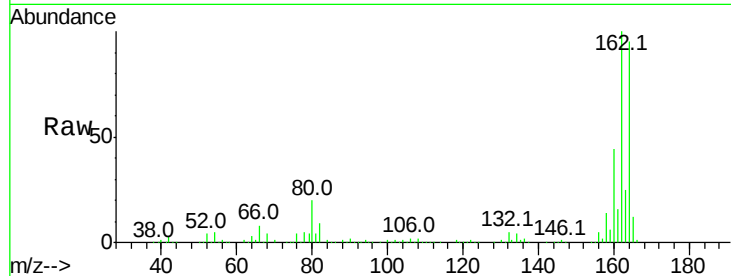

#56

2,4-Dinitrotoluene

Concen: 5.992 ng




RT: 9.95 min Scan# 1337


Delta R.T. -0.19 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31

Tgt Ion:	165	Resp:	34405
Ion	Ratio	Lower	Upper
165	100		
63	1.6	36.4	54.6#
89	1.2	57.8	86.6#
182	0.0	1.6	2.4#

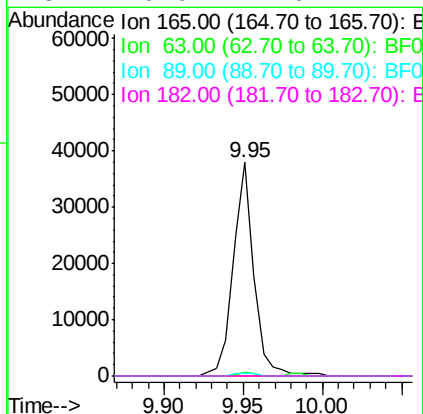



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.44 min Scan# 1590

Delta R.T. -0.01 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion:188 Resp: 440381

Ion Ratio Lower Upper

188 100

94 9.8 8.5 12.7




80 10.8 9.2 13.8



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

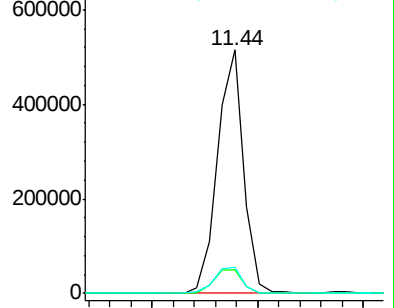

#70

Phenanthrene

Concen: 3.726 ng

RT: 11.46 min Scan# 1594

Delta R.T. -0.01 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31


Tgt Ion:178 Resp: 87820

Ion Ratio Lower Upper

178 100

176 18.0 15.8 23.8



179 13.8 13.0 19.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

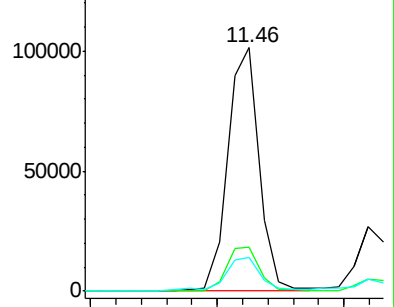



#74

Fluoranthene

Concen: 5.310 ng

RT: 12.65 min Scan# 1796

Delta R.T. -0.01 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion:202 Resp: 126738

Ion Ratio Lower Upper

202 100

101 11.9 0.0 34.1




203 17.4 0.0 38.1



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

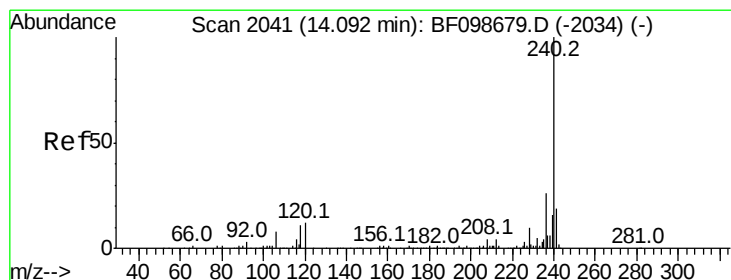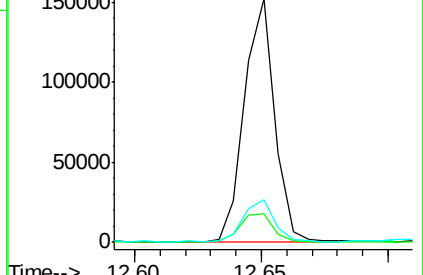

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.07 min Scan# 2038

Delta R.T. -0.01 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31


Tgt Ion:240 Resp: 249855

Ion Ratio Lower Upper

240 100

120 16.3 9.5 14.3#



236 26.4 20.7 31.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

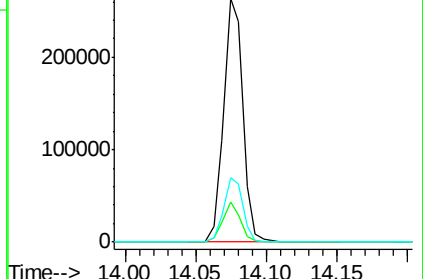

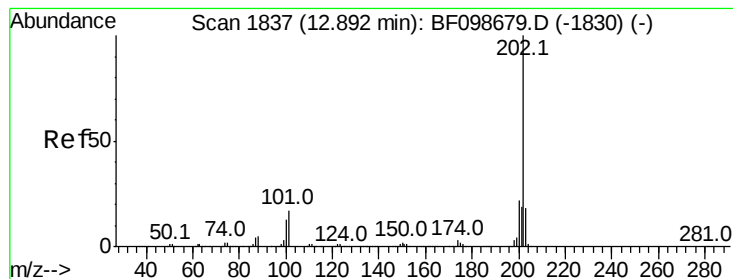

#77

Pvrene

Concen: 5.999 ng

RT: 12.88 min Scan# 1835

Delta R.T. -0.01 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31

Instrument :

BNA_F

ClientSampleId :


Tot Ion:202 Resp: 114292

Ion Ratio Lower Upper

202 100

200 20.7 17.4 26.2




203 17.7 14.3 21.5

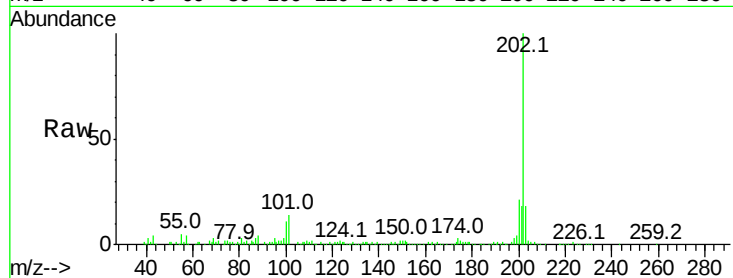

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

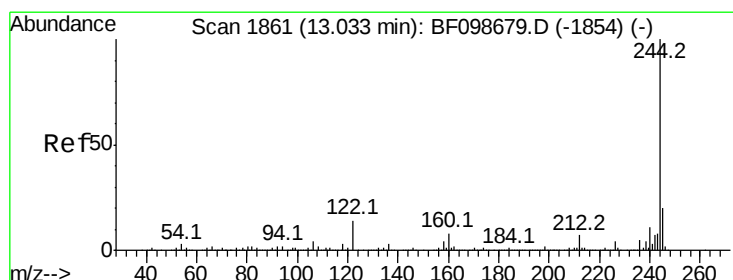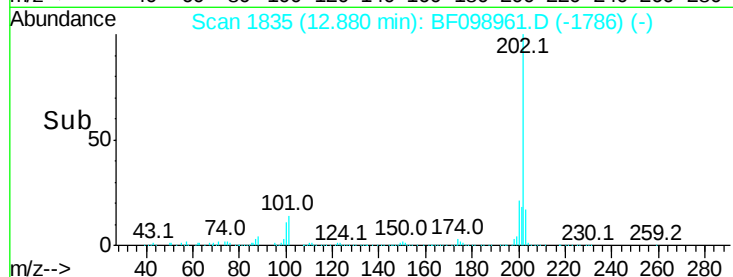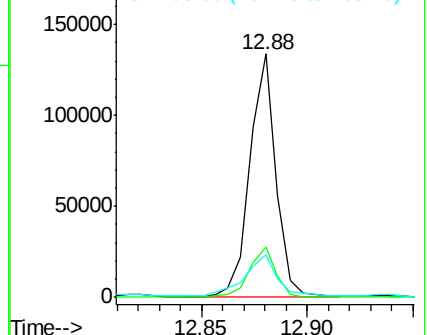

#78

Terphenyl-d14

Concen: 14.739 ng

RT: 13.02 min Scan# 1858

Delta R.T. -0.02 min

Lab File: BF098961.D

Acq: 30 Sep 2017 14:31


Tgt Ion:244 Resp: 161934

Ion Ratio Lower Upper

244 100

212 7.8 5.4 8.0



122 14.4 11.0 16.4

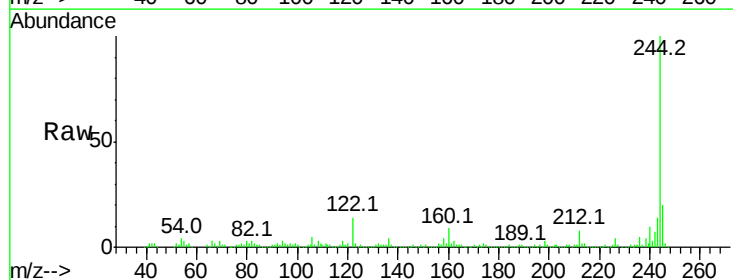


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

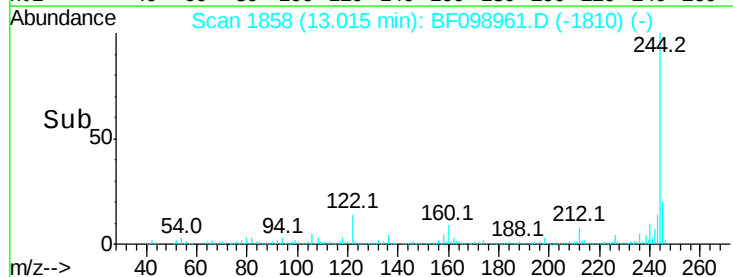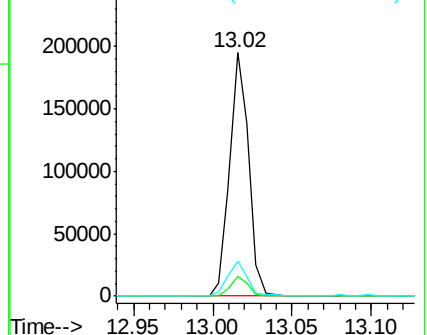







#80
Benzo(a)anthracene
Concen: 3.100 ng
RT: 14.07 min Scan# 2037
Delta R.T. -0.01 min
Lab File: BF098961.D
Acq: 30 Sep 2017 14:31

Instrument :
BNA_F
ClientSampleId :

Tot Ion:228 Resp: 46902
Ion Ratio Lower Upper
228 100
226 33.0 22.6 33.8
229 22.8 15.8 23.6




Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E


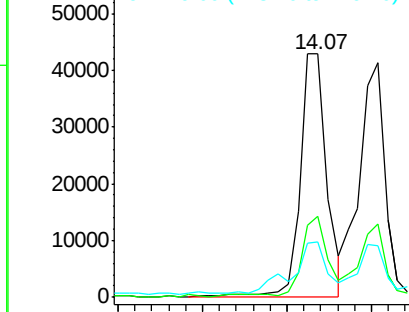



#82
Chrysene
Concen: 3.062 ng
RT: 14.10 min Scan# 2043
Delta R.T. -0.01 min
Lab File: BF098961.D
Acq: 30 Sep 2017 14:31

Tgt Ion:228 Resp: 44101
Ion Ratio Lower Upper
228 100
226 31.3 25.0 37.6
229 22.0 16.2 24.4



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E




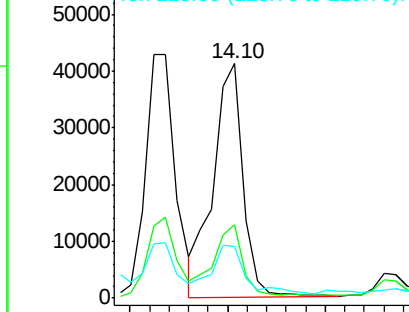




#85
 Indeno(1,2,3-cd)pyrene
 Concen: 2.635 ng
 RT: 17.07 min Scan# 2547
 Delta R.T. -0.02 min
 Lab File: BF098961.D
 Acq: 30 Sep 2017 14:31




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
276	100		
138	24.5	25.0	37.6#
277	27.1	20.1	30.1

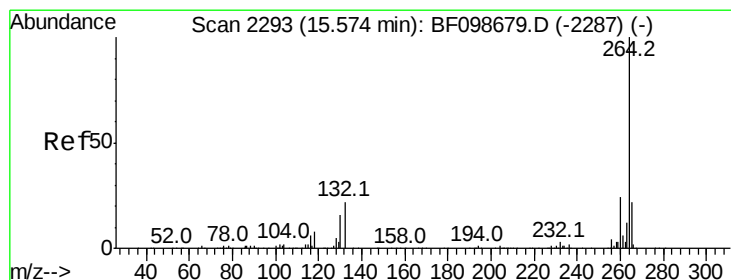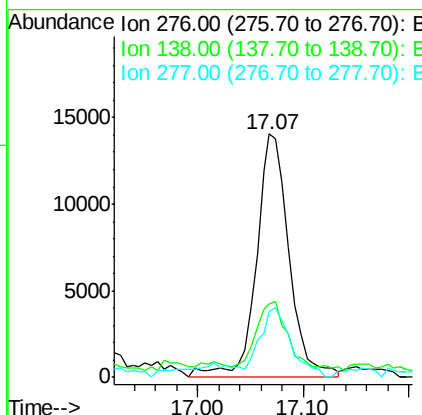

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.57 min Scan# 2292
 Delta R.T. -0.01 min
 Lab File: BF098961.D
 Acq: 30 Sep 2017 14:31

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.5	19.2	28.8
265	22.3	17.5	26.3



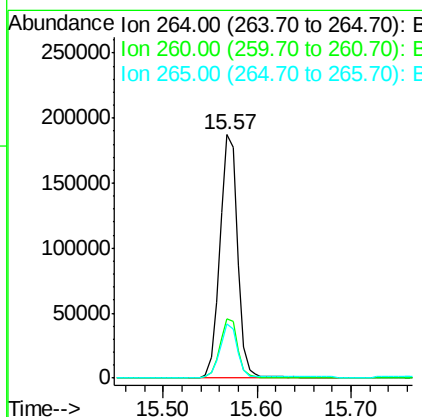
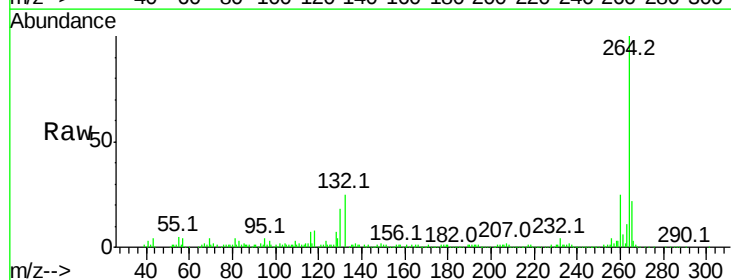


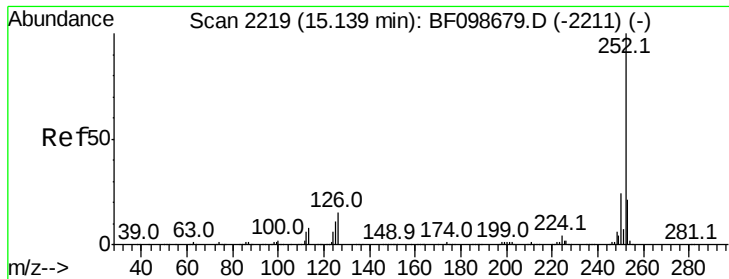

#87
Benzo(b)fluoranthene
Concen: 4.653 ng
RT: 15.13 min Scan# 2217
Delta R.T. -0.01 min
Lab File: BF098961.D
Acq: 30 Sep 2017 14:31




Instrument :
BNA_F
ClientSampleId :


Tot Ion	Ratio	Lower	Upper
252	100		
253	23.1	17.0	25.6
125	17.3	9.0	13.6

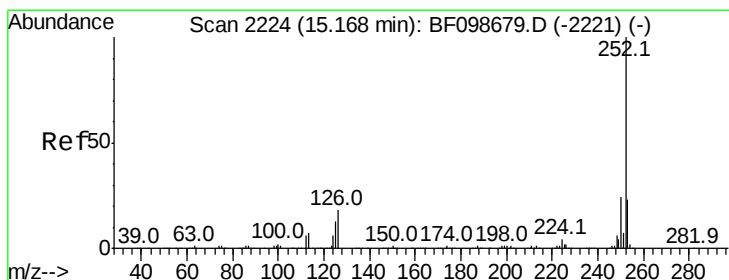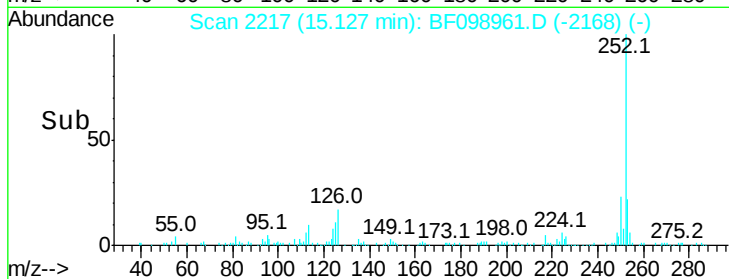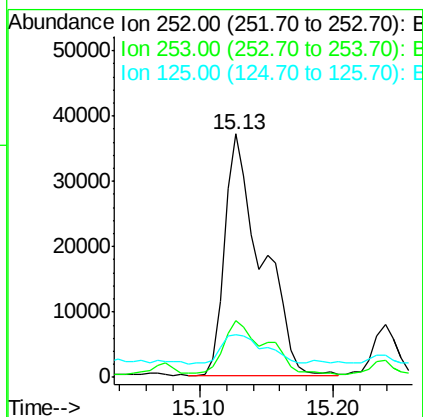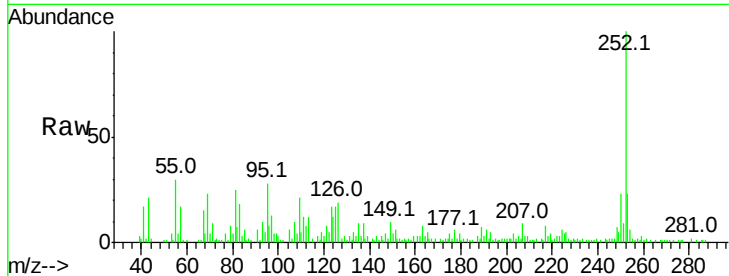

#88
Benzo(k)fluoranthene
Concen: 4.711 ng
RT: 15.13 min Scan# 2217
Delta R.T. -0.04 min
Lab File: BF098961.D
Acq: 30 Sep 2017 14:31

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.1	17.9	26.9
125	17.3	10.2	15.2


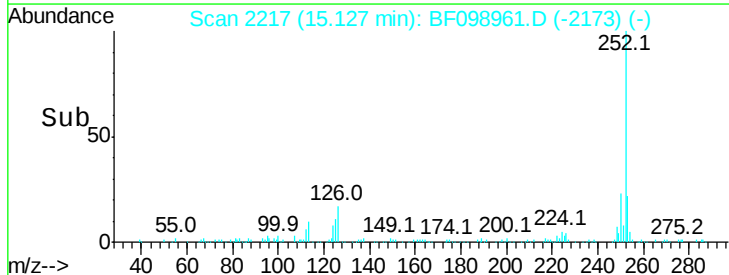
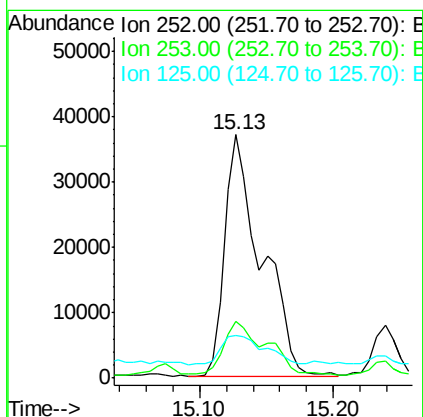
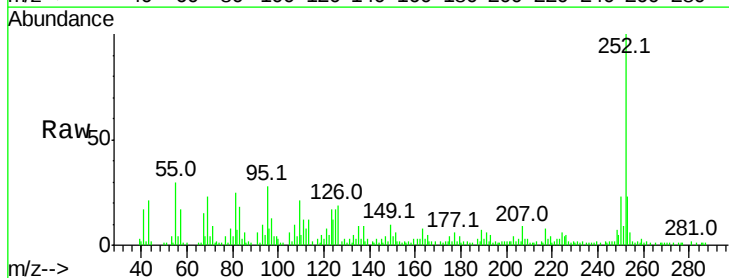




#89
Benzo(a)pyrene
Concen: 2.797 ng
RT: 15.50 min Scan# 2281
Delta R.T. -0.01 min
Lab File: BF098961.D
Acq: 30 Sep 2017 14:31

Instrument :
BNA_F
ClientSampleId :

Tot Ion:252 Resp: 39097
Ion Ratio Lower Upper
252 100
253 24.4 17.1 25.7
125 18.5 9.8 14.6#

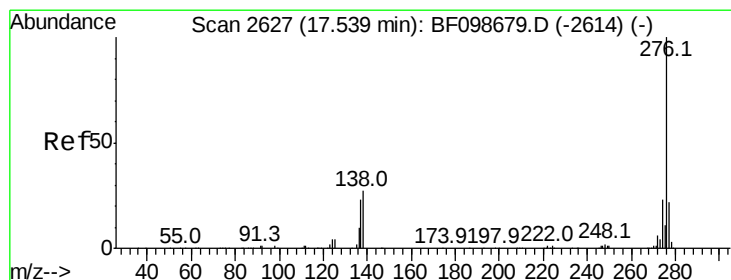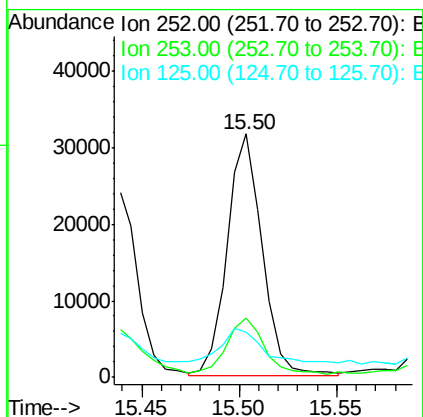

#91
Benzo(g,h,i)perylene
Concen: 2.832 ng
RT: 17.53 min Scan# 2625
Delta R.T. -0.02 min
Lab File: BF098961.D
Acq: 30 Sep 2017 14:31

Tgt Ion:276 Resp: 31321
Ion Ratio Lower Upper
276 100
277 26.5 17.9 26.9
138 33.0 21.8 32.8#

