

Data Path : Z:\HPCHEM1\BNA F\DATA\BF093017\
 Data File : BF098965.D
 Acq On : 30 Sep 2017 16:23
 Operator : SJ/JU
 Sample : I5519-01 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 30 23:26:01 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 23 13:50:58 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.92	152	129425	20.00	ng	0.00
21) Naphthalene-d8	8.19	136	520825	20.00	ng	-0.01
38) Acenaphthene-d10	9.95	164	216323	20.00	ng	-0.01
63) Phenanthrene-d10	11.44	188	296537	20.00	ng	0.00
75) Chrysene-d12	14.07	240	223426	20.00	ng	-0.01
86) Perylene-d12	15.57	264	232655	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	178140	21.91	ng	-0.02
7) Phenol-d6	6.53	99	213259	21.26	ng	-0.02
23) Nitrobenzene-d5	7.47	82	124962	15.39	ng	-0.02
41) 2,4,6-Tribromophenol	10.74	330	27065	15.29	ng	-0.01
44) 2-Fluorobiphenyl	9.27	172	245393	18.94	ng	-0.01
78) Terphenyl-d14	13.02	244	134324	13.67	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.47	70	15440	2.411	ng	# 81
25) Isophorone	7.47	82	124960	7.442	ng	# 64
50) 2,6-Dinitrotoluene	9.95	165	26764	7.530	ng	# 26
56) 2,4-Dinitrotoluene	9.95	165	26764	5.802	ng	# 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF093017\
Data File : BF098965.D
Acq On : 30 Sep 2017 16:23
Operator : SJ/JU
Sample : I5519-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Sep 30 23:26:01 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF092317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 23 13:50:58 2017
Response via : Initial Calibration

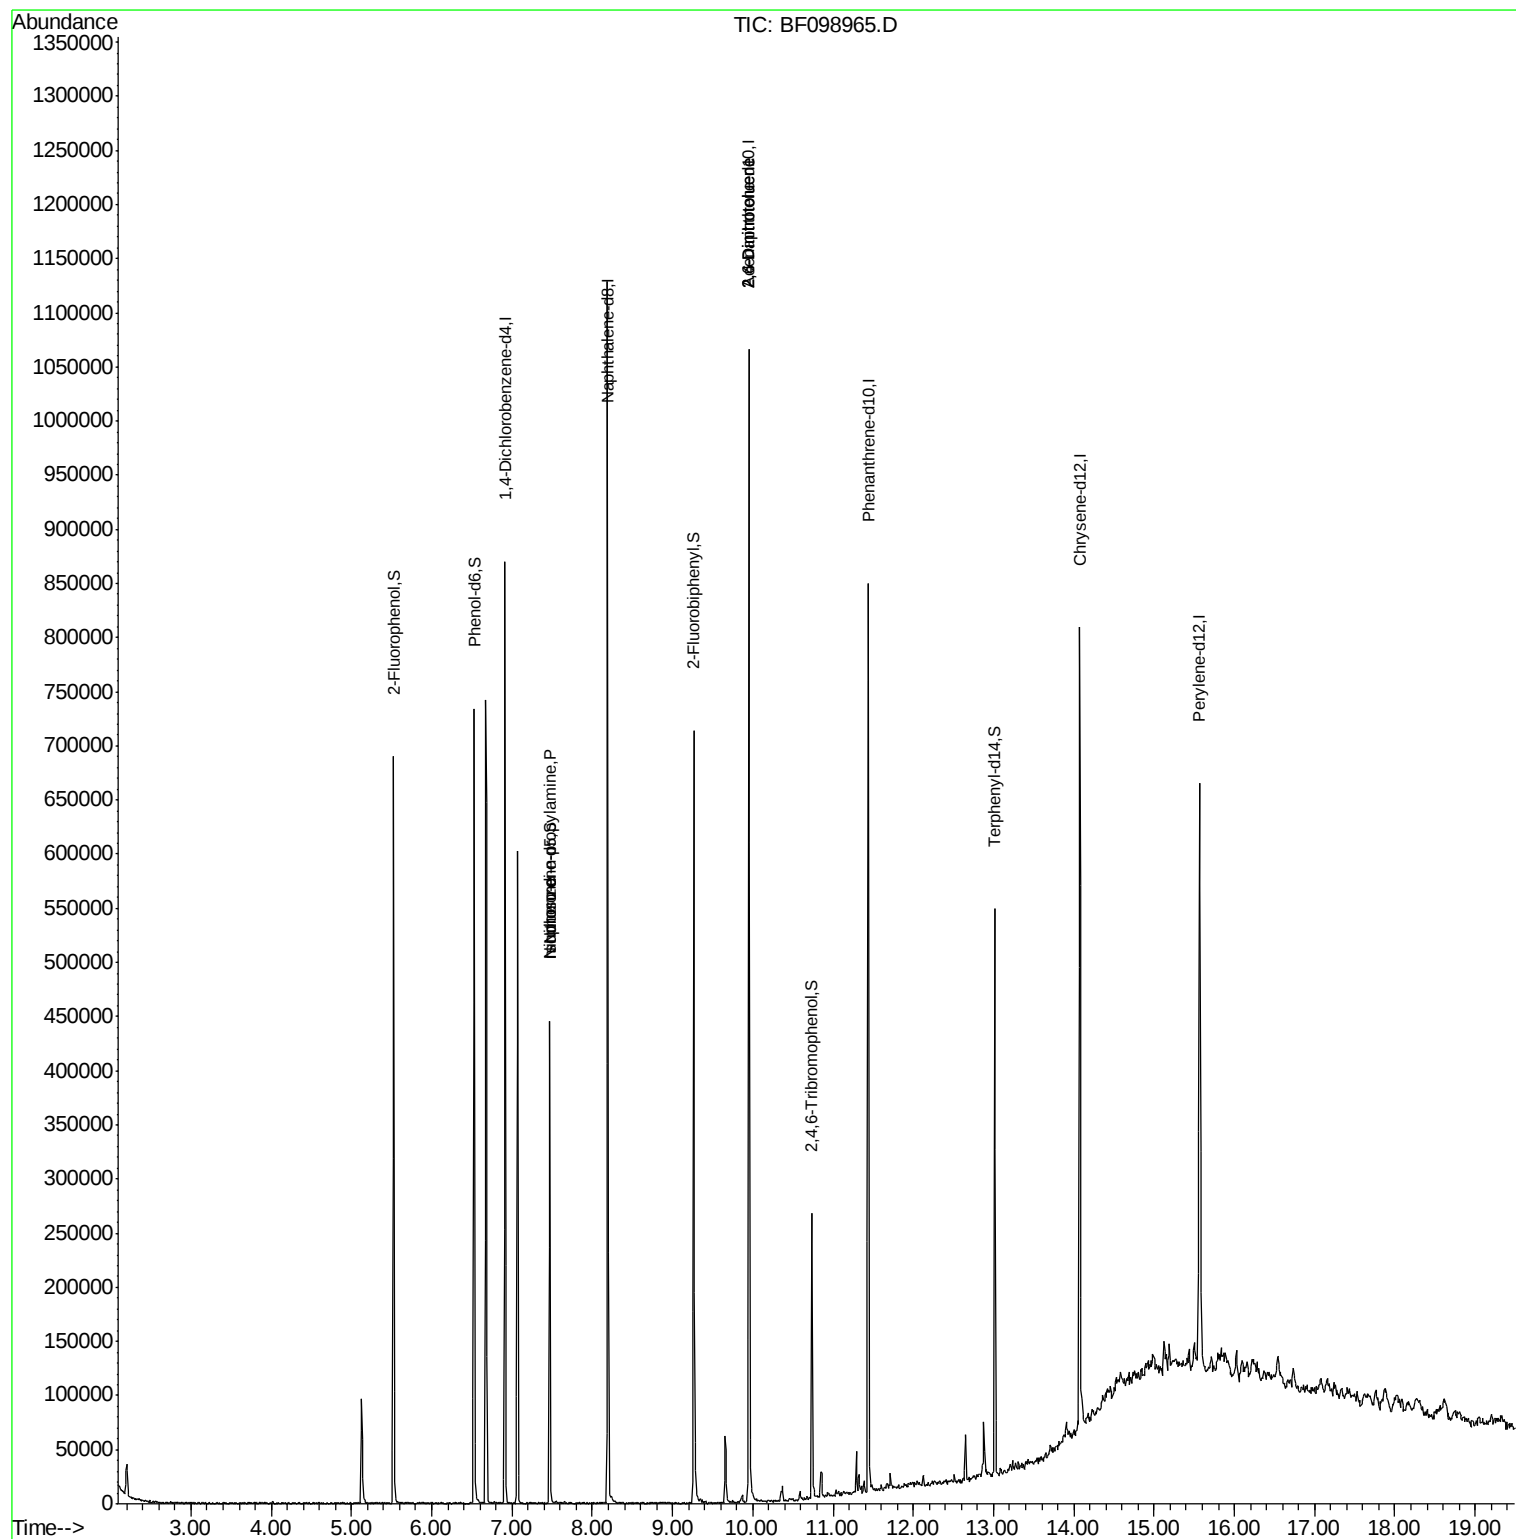

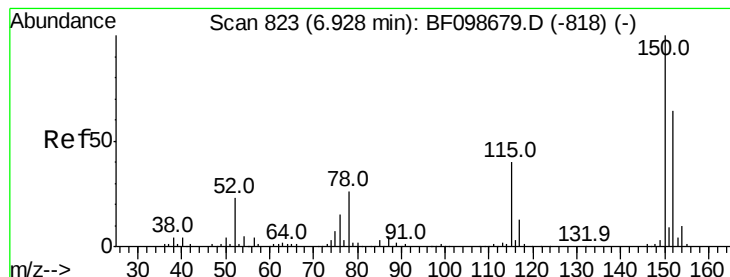


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.92 min Scan# 821
Delta R.T. -0.01 min
Lab File: BF098965.D
Acq: 30 Sep 2017 16:23

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 129425
Ion Ratio Lower Upper
152 100
150 158.4 124.6 186.8
115 59.9 50.1 75.1

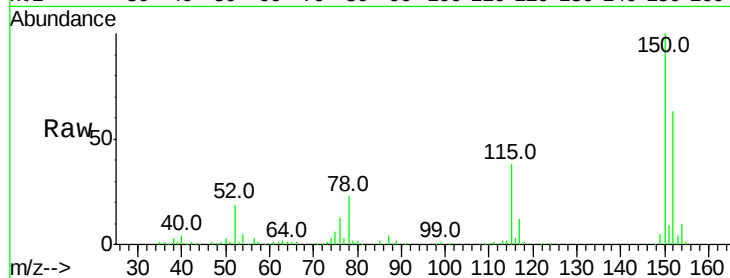


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

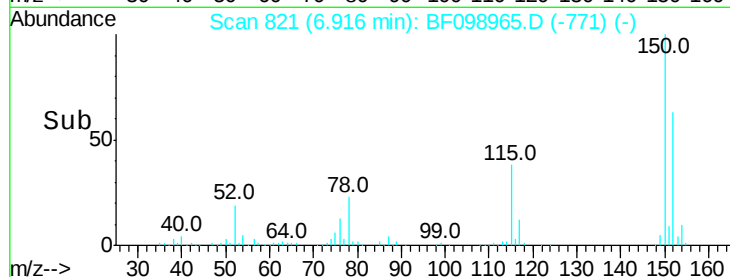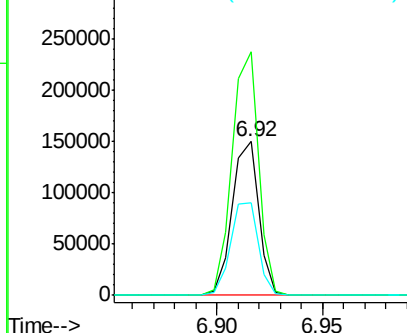



#5

2-Fluorophenol
Concen: 21.911 ng
RT: 5.52 min Scan# 584
Delta R.T. -0.02 min
Lab File: BF098965.D
Acq: 30 Sep 2017 16:23

Tgt Ion:112 Resp: 178140
Ion Ratio Lower Upper
112 100
64 59.1 47.9 71.9
63 30.0 23.7 35.5

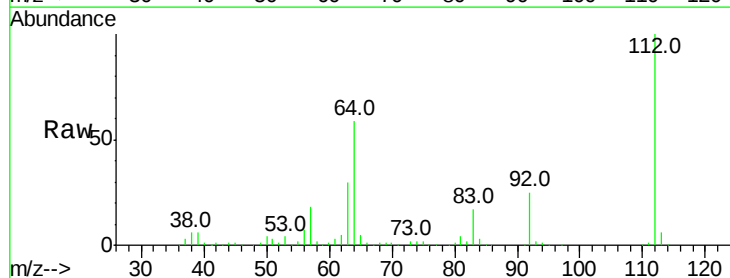

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

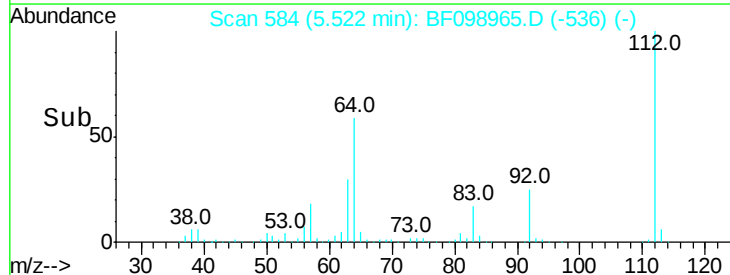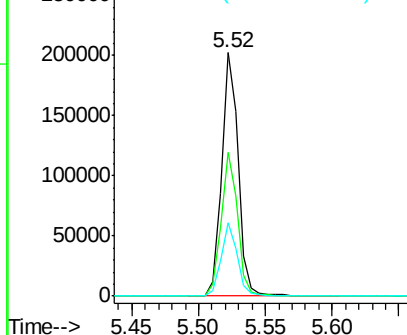



#7

Phenol-d6

Concen: 21.263 ng

RT: 6.53 min Scan# 755

Delta R.T. -0.02 min

Lab File: BF098965.D

Acq: 30 Sep 2017 16:23

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 213259

Ion Ratio Lower Upper

99 100

42 17.8 14.5 21.7

71 32.0 25.4 38.0

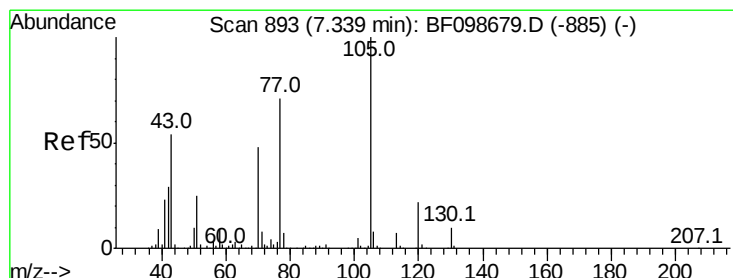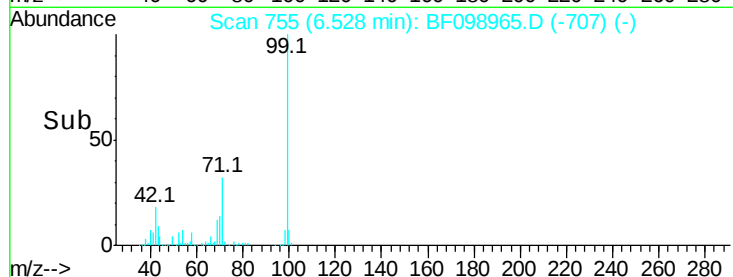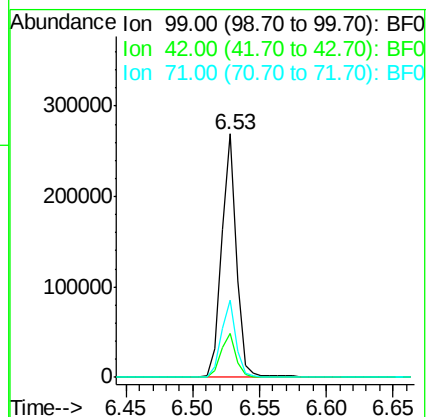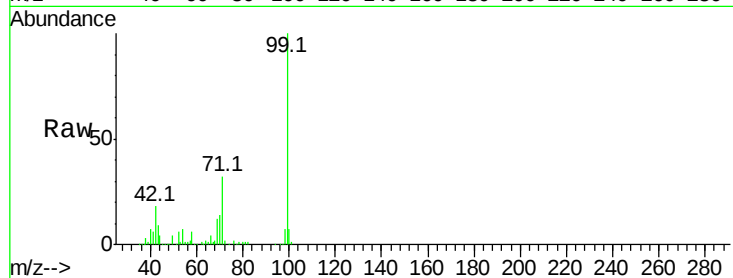

#19

n-Nitroso-di-n-propylamine

Concen: 2.411 ng

RT: 7.47 min Scan# 915

Delta R.T. 0.14 min

Lab File: BF098965.D

Acq: 30 Sep 2017 16:23

Tgt Ion: 70 Resp: 15440




Ion Ratio Lower Upper


70 100

42 51.4 47.5 71.3

101 0.0 7.4 11.2#

130 2.4 16.6 25.0#


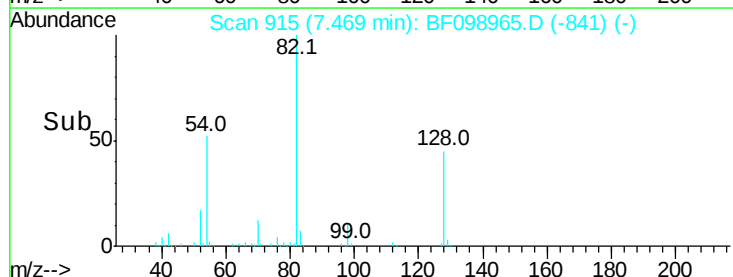
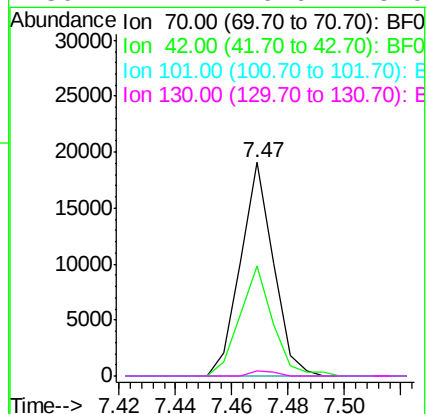
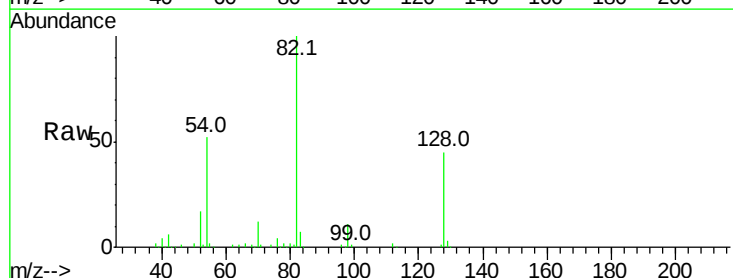


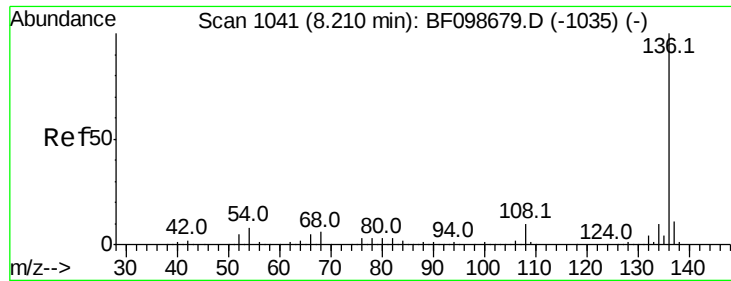

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.19 min Scan# 1038
Delta R.T. -0.01 min
Lab File: BF098965.D
Acq: 30 Sep 2017 16:23




Instrument :
BNA_F
ClientSampleId :


Tot Ion:136	Resp:	520825
Ion Ratio	Lower	Upper
136	100	
137	10.9	8.9 13.3
54	8.6	6.6 9.8
68	6.2	5.0 7.4

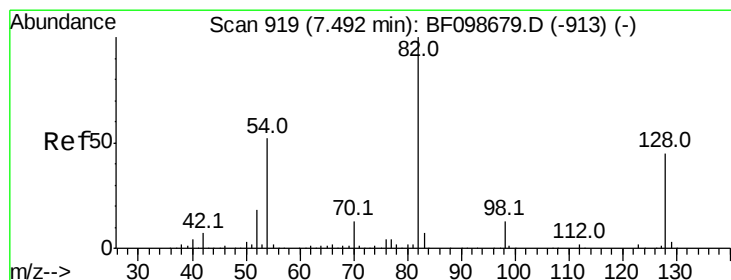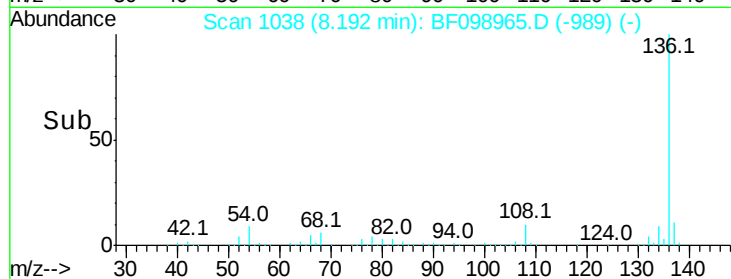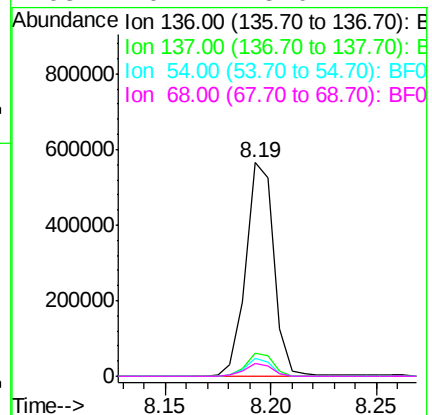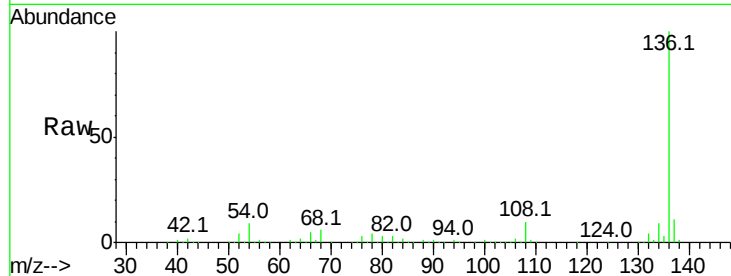

#23
Nitrobenzene-d5
Concen: 15.387 ng
RT: 7.47 min Scan# 915
Delta R.T. -0.02 min
Lab File: BF098965.D
Acq: 30 Sep 2017 16:23

Tgt Ion: 82	Resp:	124962
Ion Ratio	Lower	Upper
82	100	
128	44.6	36.1 54.1
54	51.8	41.4 62.2

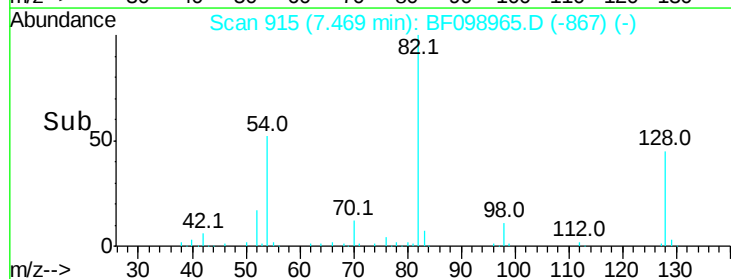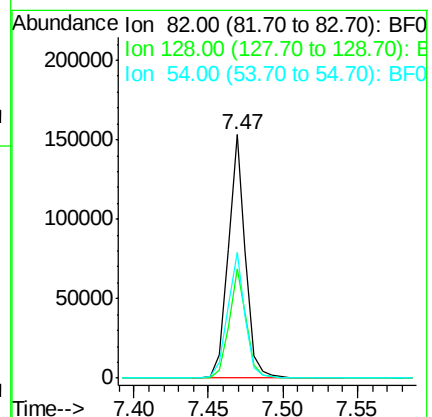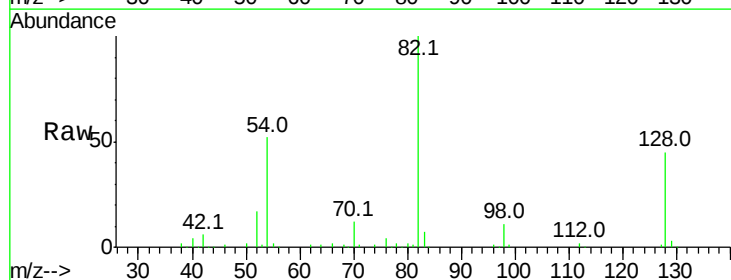

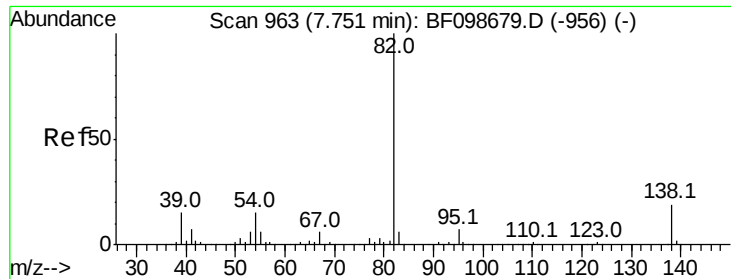

#25

Isophorone

Concen: 7.442 ng

RT: 7.47 min Scan# 915

Delta R.T. -0.28 min

Lab File: BF098965.D

Acq: 30 Sep 2017 16:23

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 124960

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

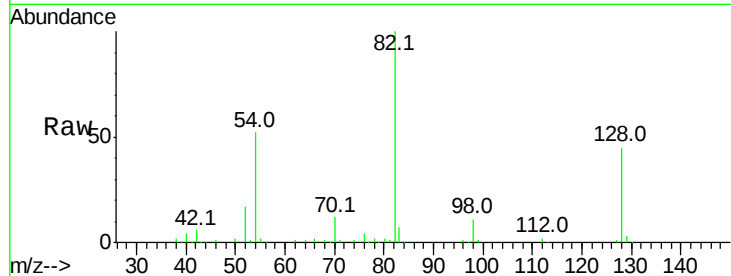

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): BF0

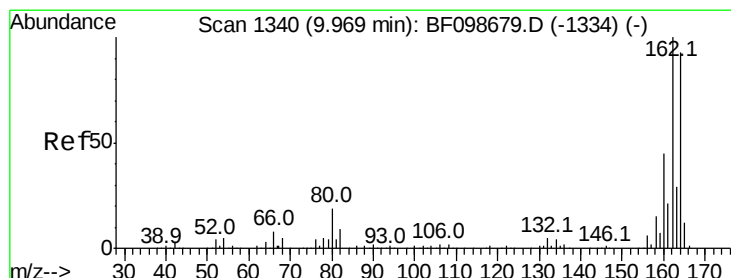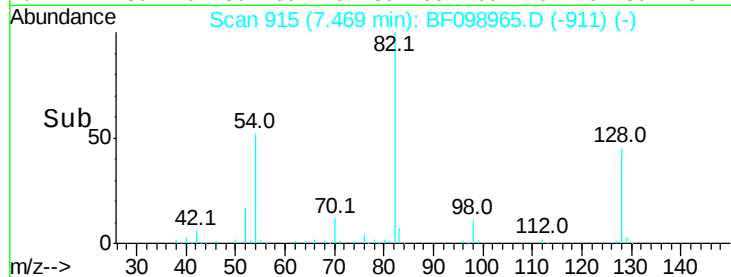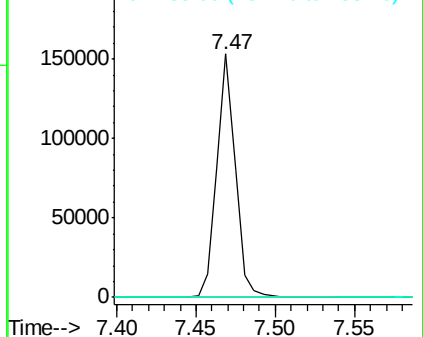

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.95 min Scan# 1337

Delta R.T. -0.01 min

Lab File: BF098965.D

Acq: 30 Sep 2017 16:23


Tgt Ion:164 Resp: 216323

Ion Ratio Lower Upper



164 100


162 105.4 86.1 129.1

160 47.2 38.3 57.5

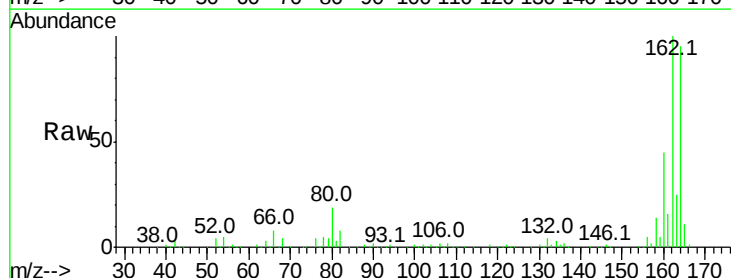

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

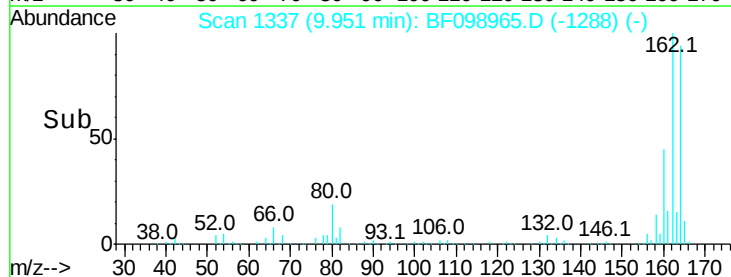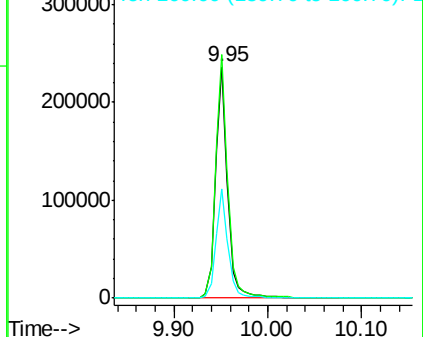


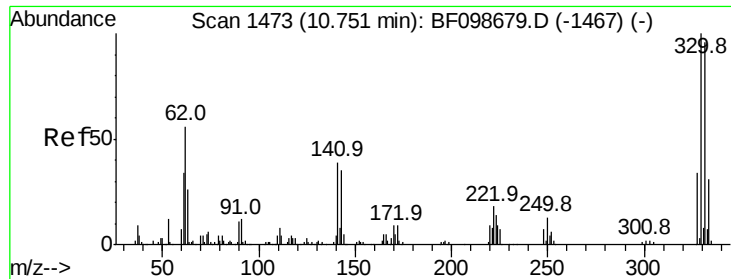




#41
 2,4,6-Tribromophenol
 Concen: 15.290 ng
 RT: 10.74 min Scan# 1471
 Delta R.T. -0.01 min
 Lab File: BF098965.D
 Acq: 30 Sep 2017 16:23

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.5	77.0	115.6
141	49.9	29.9	44.9#

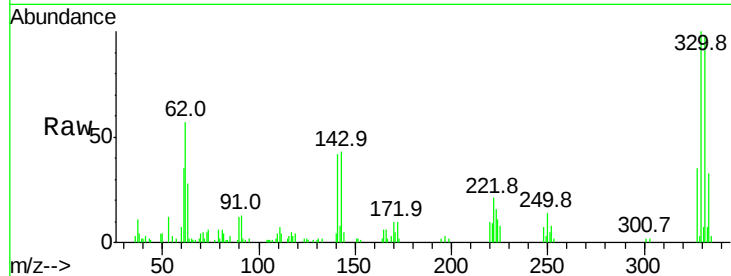


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

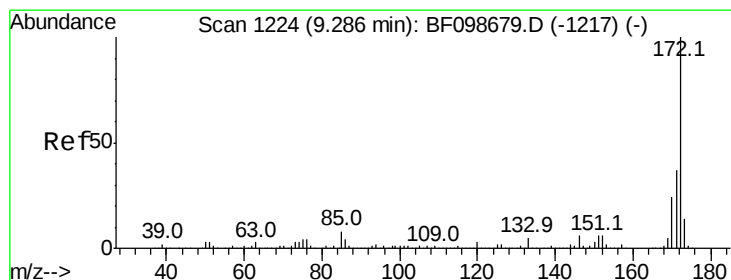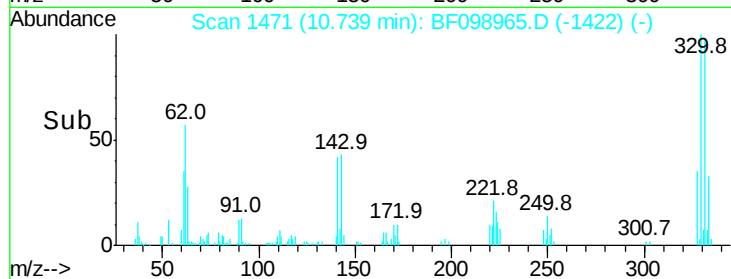
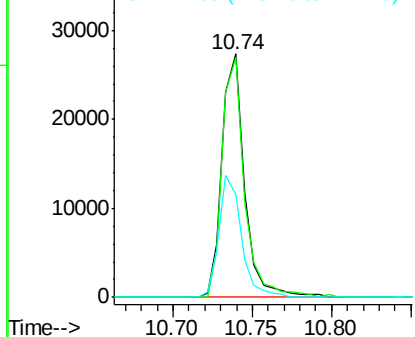



#44
 2-Fluorobiphenyl
 Concen: 18.938 ng
 RT: 9.27 min Scan# 1221
 Delta R.T. -0.01 min
 Lab File: BF098965.D
 Acq: 30 Sep 2017 16:23

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.3	29.7	44.5
170	23.2	19.6	29.4

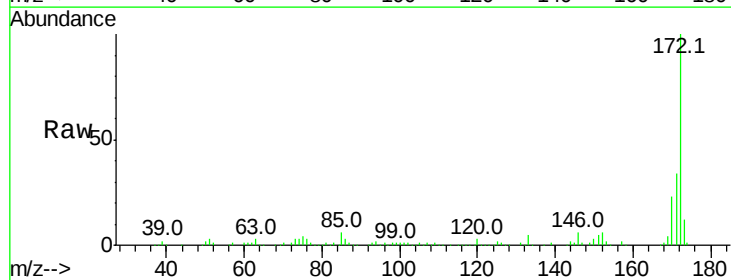

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

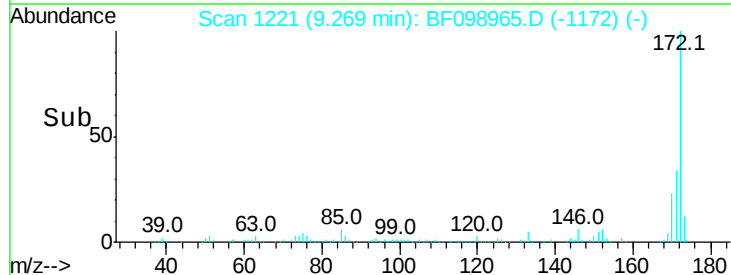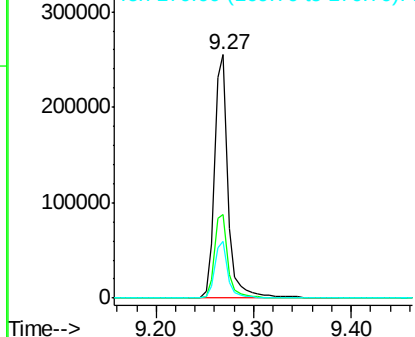


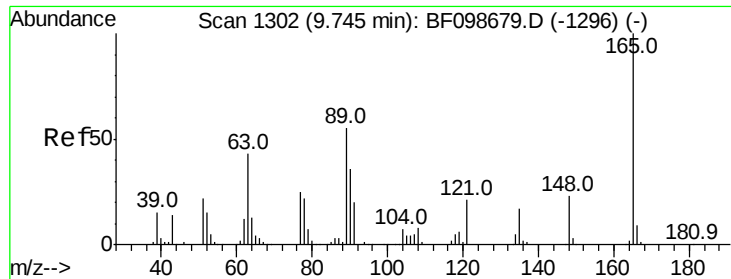




#50
 2,6-Dinitrotoluene
 Concen: 7.530 ng
 RT: 9.95 min Scan# 1337
 Delta R.T. 0.21 min
 Lab File: BF098965.D
 Acq: 30 Sep 2017 16:23

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.2	44.7	67.1#
89	1.6	44.0	66.0#

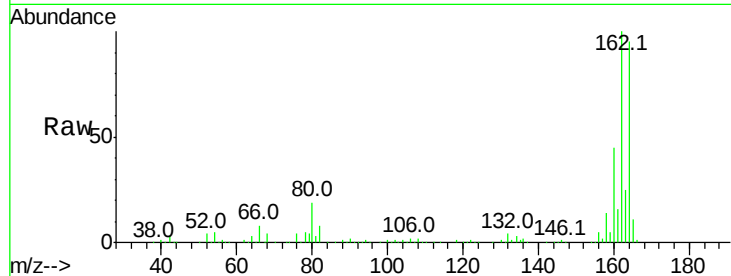




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0

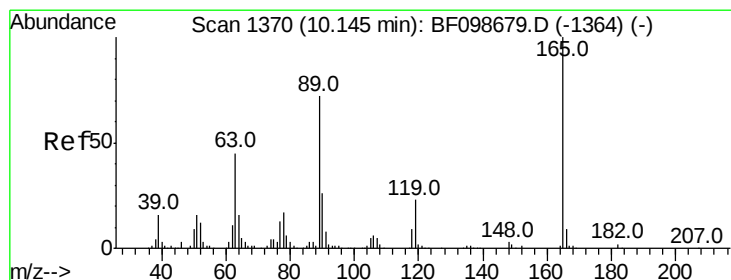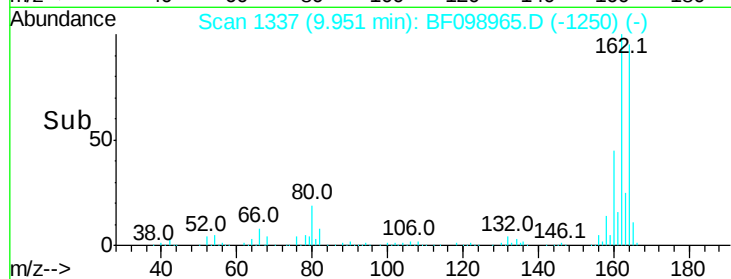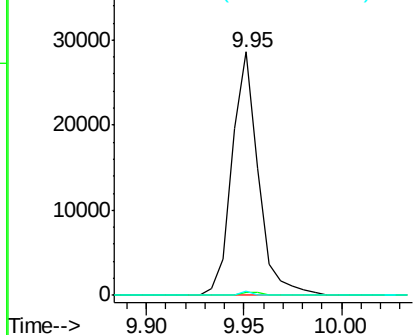


#56
 2,4-Dinitrotoluene
 Concen: 5.802 ng
 RT: 9.95 min Scan# 1337
 Delta R.T. -0.19 min
 Lab File: BF098965.D
 Acq: 30 Sep 2017 16:23

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.2	36.4	54.6#
89	1.6	57.8	86.6#
182	0.0	1.6	2.4#

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0
 Ion 182.00 (181.70 to 182.70): E

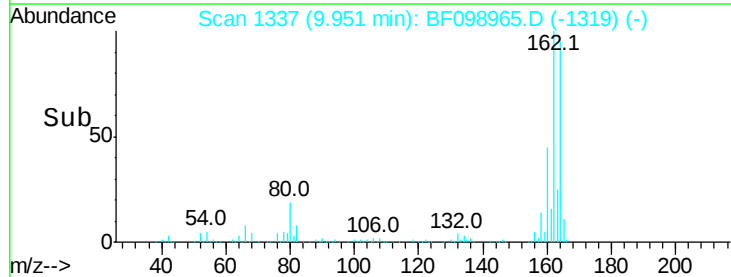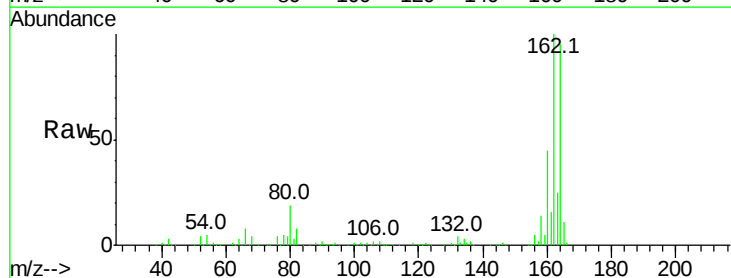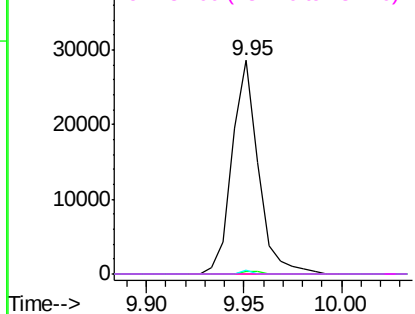

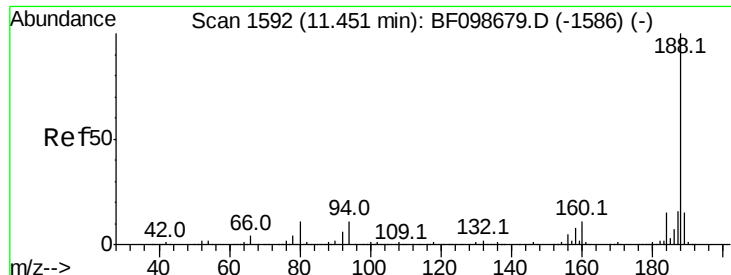

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.44 min Scan# 1590

Delta R.T. -0.01 min

Lab File: BF098965.D

Acq: 30 Sep 2017 16:23

Instrument :

BNA_F

ClientSampleId :


Tot Ion:188 Resp: 296537

Ion Ratio Lower Upper

188 100

94 9.8 8.5 12.7




80 10.4 9.2 13.8

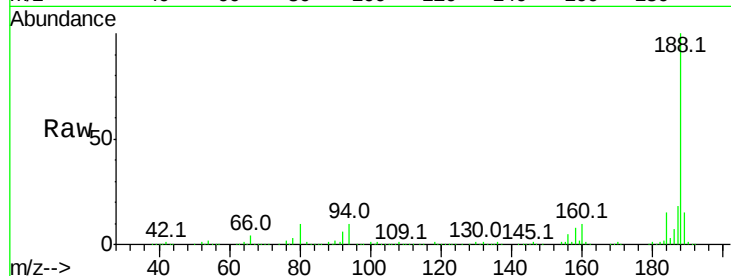

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

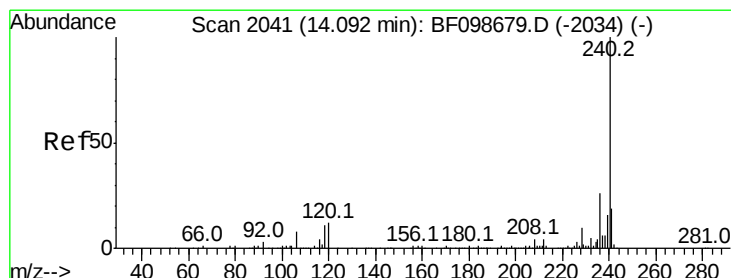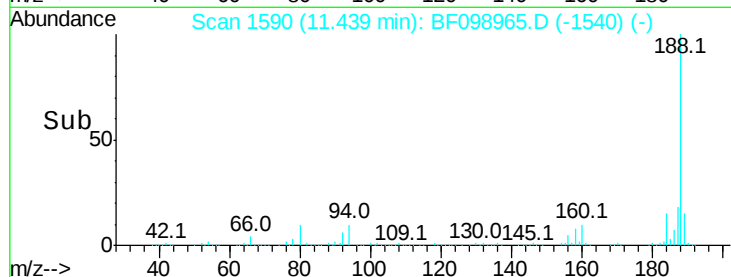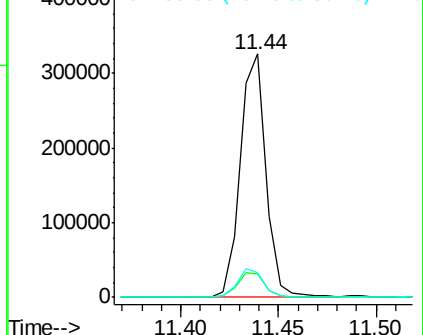

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.07 min Scan# 2038

Delta R.T. -0.01 min

Lab File: BF098965.D

Acq: 30 Sep 2017 16:23


Tgt Ion:240 Resp: 223426

Ion Ratio Lower Upper

240 100

120 14.4 9.5 14.3#



236 25.7 20.7 31.1

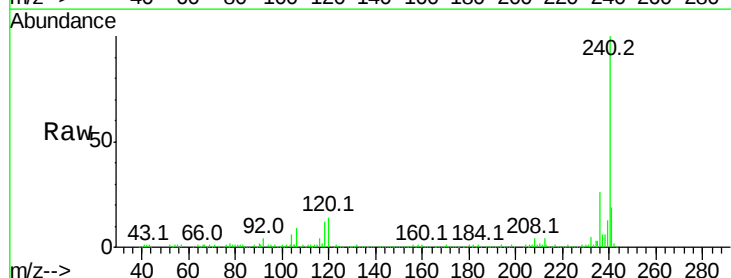


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

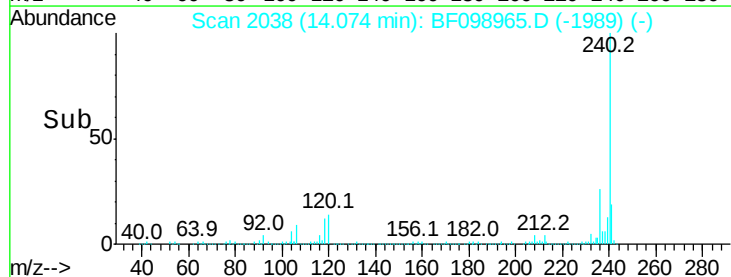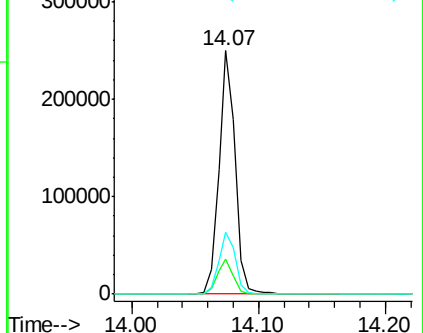

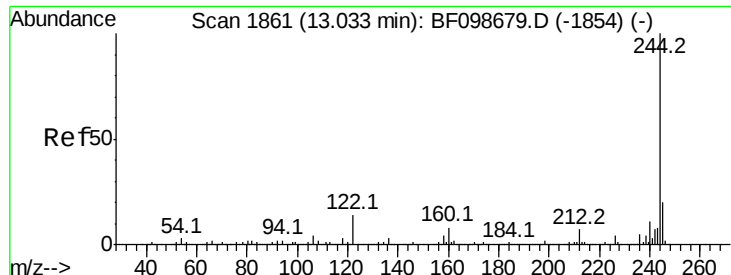

#78

Terphenyl-d14

Concen: 13.673 ng

RT: 13.02 min Scan# 1858

Delta R.T. -0.02 min

Lab File: BF098965.D

Acq: 30 Sep 2017 16:23

Instrument :

BNA_F

ClientSampled :


Tot Ion:244 Resp: 134324

Ion Ratio Lower Upper

244 100

212 7.3 5.4 8.0




122 14.6 11.0 16.4

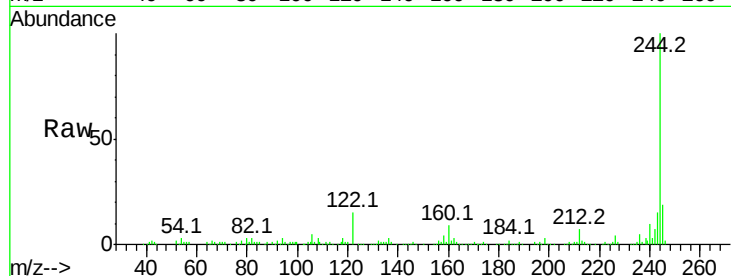

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

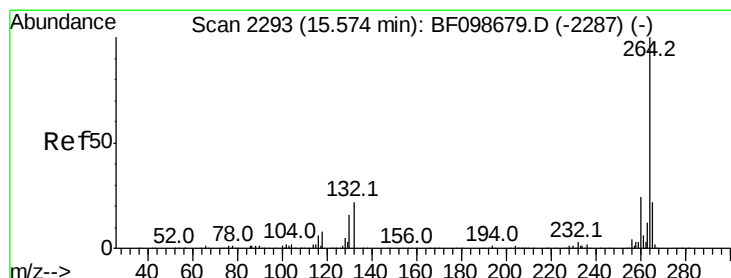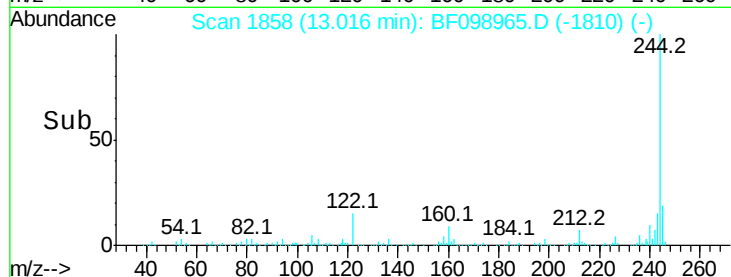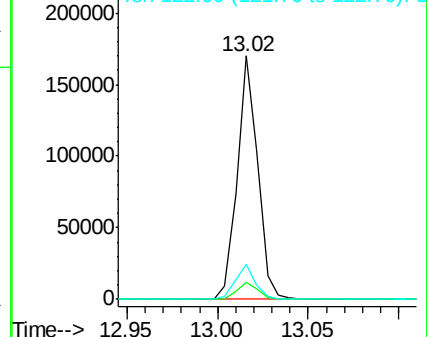

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.57 min Scan# 2292

Delta R.T. -0.01 min

Lab File: BF098965.D

Acq: 30 Sep 2017 16:23


Tgt Ion:264 Resp: 232655

Ion Ratio Lower Upper

264 100

260 23.3 19.2 28.8

265 22.3 17.5 26.3

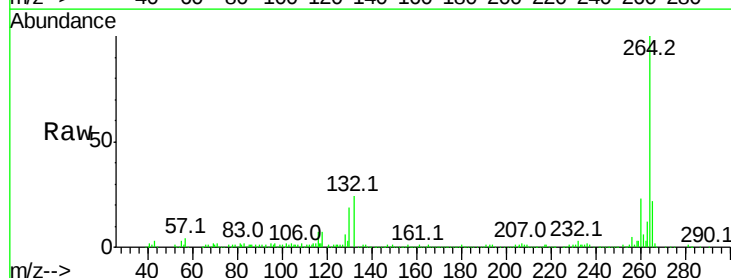

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

