


Data Path : Z:\HPCHEM1\BNA F\Data\BF093017\
 Data File : BF098957.D
 Acq On : 30 Sep 2017 12:31
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF092317.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 23 13:50:58 2017

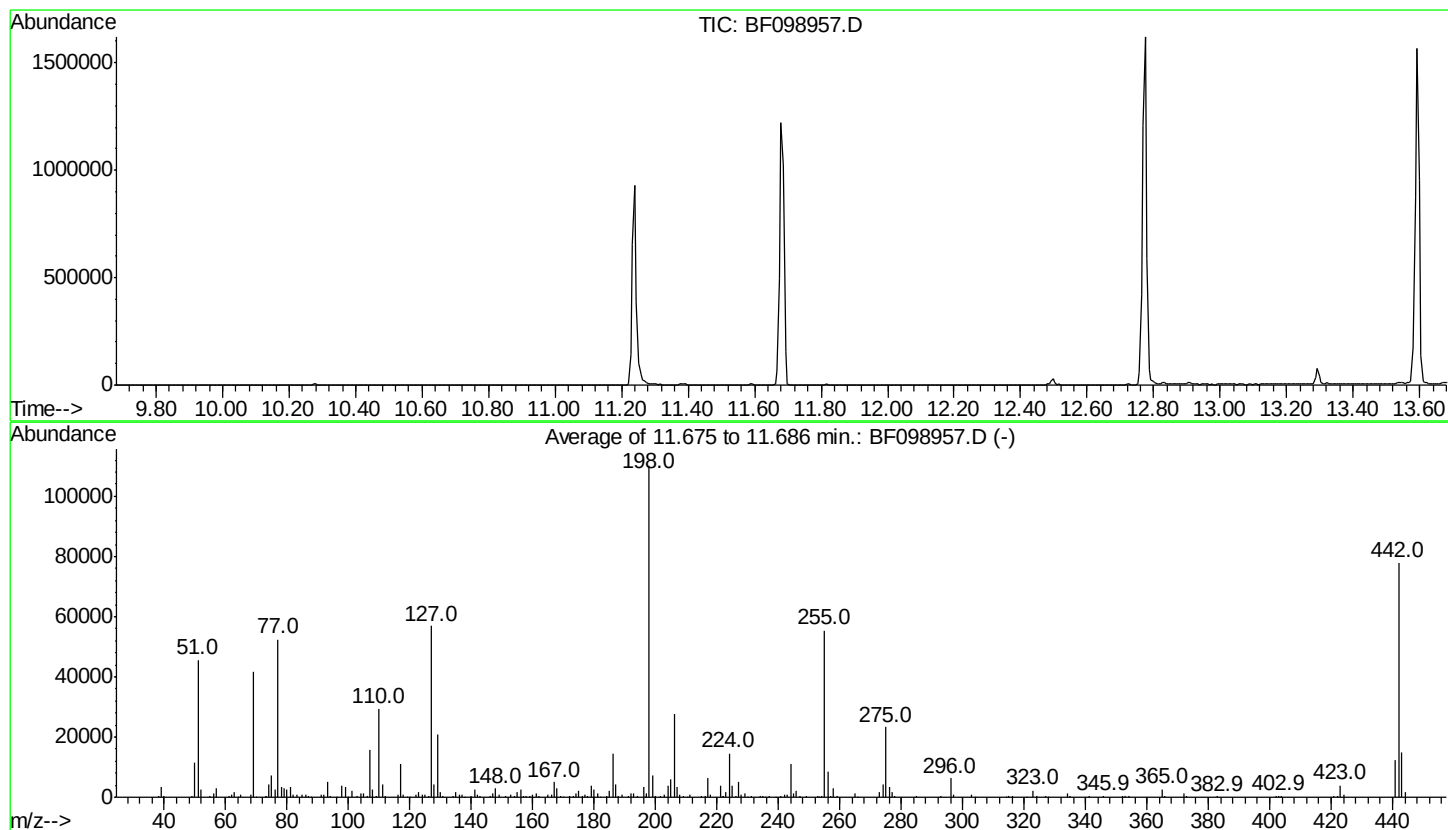

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	45517	PASS
68	69	0.00	2	2.0	818	PASS
69	198	0.00	100	37.9	41722	PASS
70	69	0.00	2	0.3	126	PASS
127	198	10	80	51.6	56853	PASS
197	198	0.00	2	1.0	1105	PASS
198	198	100	100	100.0	110165	PASS
199	198	5	9	6.7	7385	PASS
275	198	10	60	21.1	23271	PASS
365	198	1	100	2.4	2681	PASS
441	442	0.01	24	15.6	12177	PASS
442	198	50	100	70.8	78026	PASS
443	442	15	24	19.1	14931	PASS