
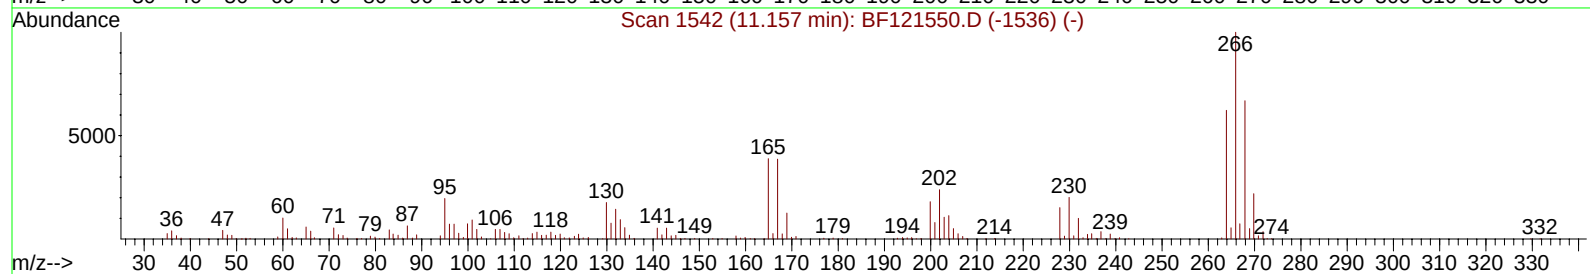
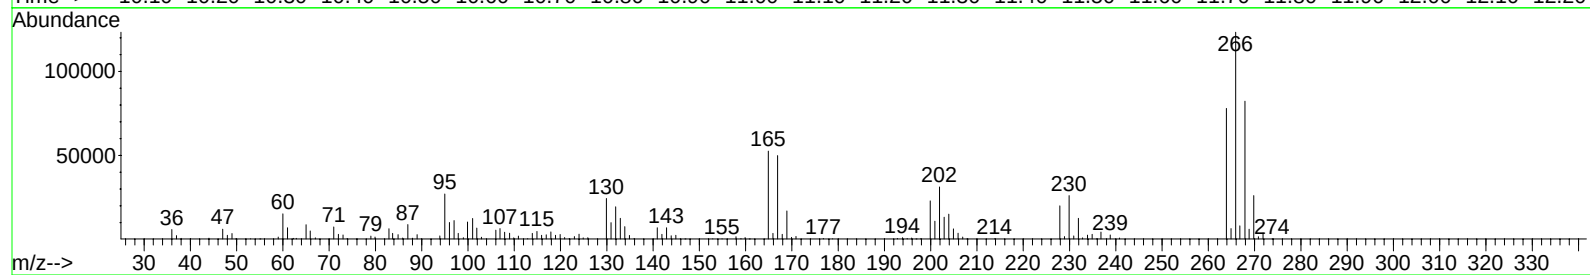


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF093020\  
 Data File : BF121740.D  
 Acq On : 30 Sep 2020 15:59  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 18:34:01 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Sep 29 11:12:14 2020  
 Response via : Initial Calibration

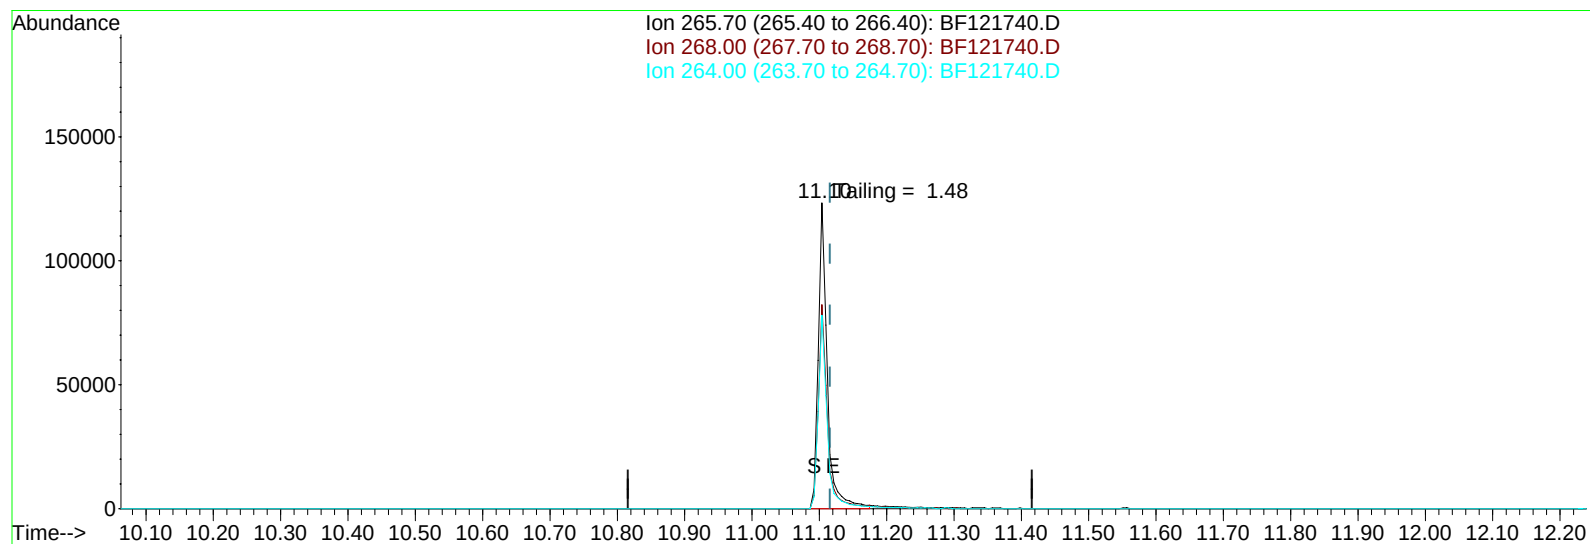

TIC: BF121740.D

(70) Pentachlorophenol (C)




11.104min (-0.012) 48370.40ng

response 118097

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 66.50 | 66.71 |
| 264.00 | 62.60 | 63.29 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF093020\  
 Data File : BF121740.D  
 Acq On : 30 Sep 2020 15:59  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 18:34:01 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Sep 29 11:12:14 2020  
 Response via : Initial Calibration

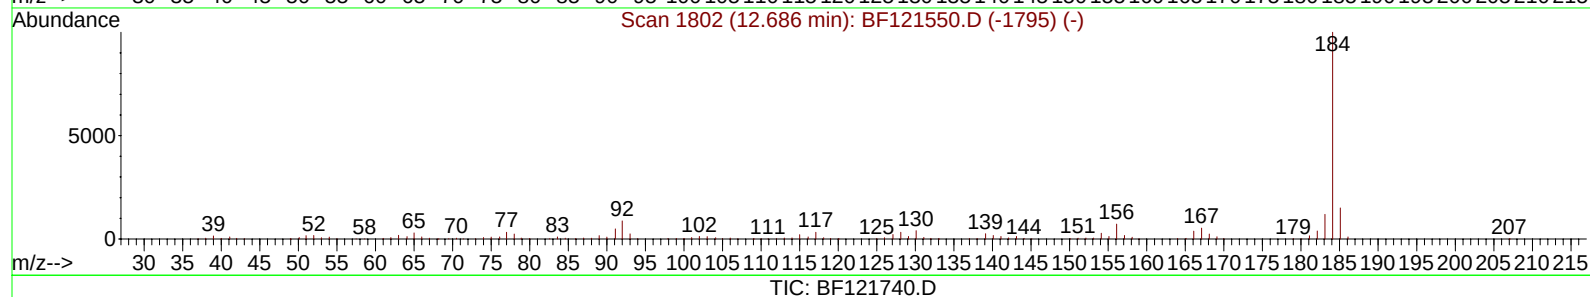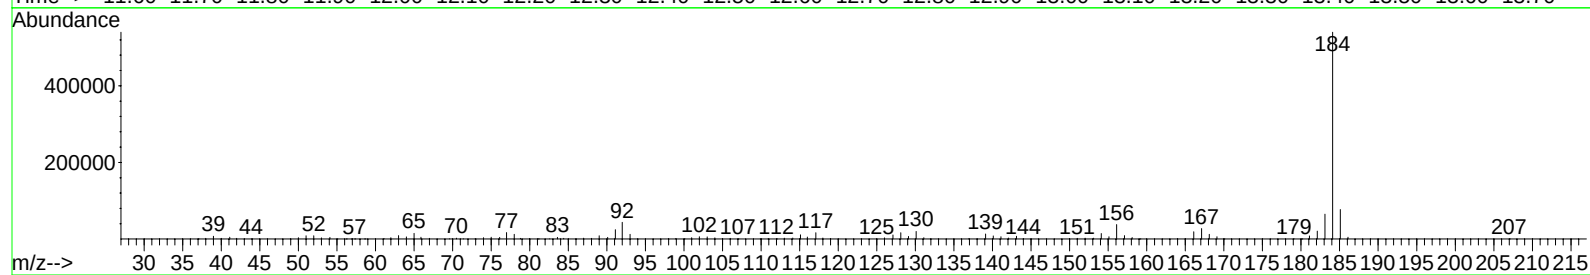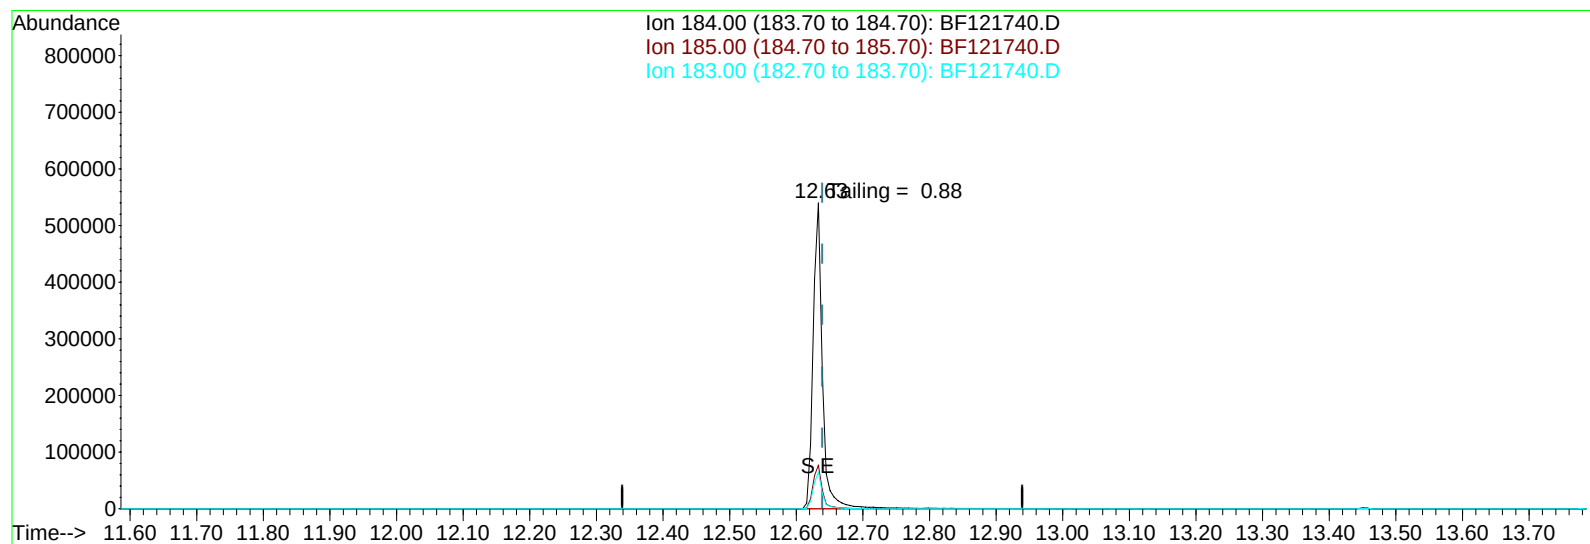

(77) Benzidine

12.633min (-0.006) 0.00ng

response 525923

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 14.70 | 14.29 |
| 183.00 | 11.60 | 12.03 |
| 0.00   | 0.00  | 0.00  |