

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF093020\
 Data File : BF121748.D
 Acq On : 30 Sep 2020 20:04
 Operator : JU/CG
 Sample : PB132010BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB132010BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.204	16	20	30	rVB	72767	102608	1.76%	0.263%
2	5.016	492	498	509	rBV	70833	108525	1.86%	0.279%
3	5.410	559	565	568	rBV	3569331	3973095	68.21%	10.197%
4	6.416	730	736	739	rBV	3645102	3955796	67.91%	10.153%
5	6.775	793	797	800	rBV	2033142	1665199	28.59%	4.274%
6	7.339	887	893	896	rBV	2570009	2895293	49.70%	7.431%
7	8.057	1010	1015	1019	rBV	2137884	2217789	38.07%	5.692%
8	9.133	1192	1198	1202	rBV	4075936	5173621	88.82%	13.278%
9	9.810	1307	1313	1317	rBV	2251452	2606725	44.75%	6.690%
10	10.604	1441	1448	1451	rBV	2887972	3217129	55.23%	8.257%
11	11.298	1559	1566	1569	rBV	2760160	2730190	46.87%	7.007%
12	12.886	1829	1836	1839	rBV	5204615	5825139	100.00%	14.950%
13	13.933	2010	2014	2018	rBV	2481241	2444773	41.97%	6.275%
14	15.374	2253	2259	2272	rBV	1612961	2047018	35.14%	5.254%


Sum of corrected areas: 38962900

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF093020\
Data File : BF121748.D
Acq On : 30 Sep 2020 20:04
Operator : JU/CG
Sample : PB132010BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132010BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

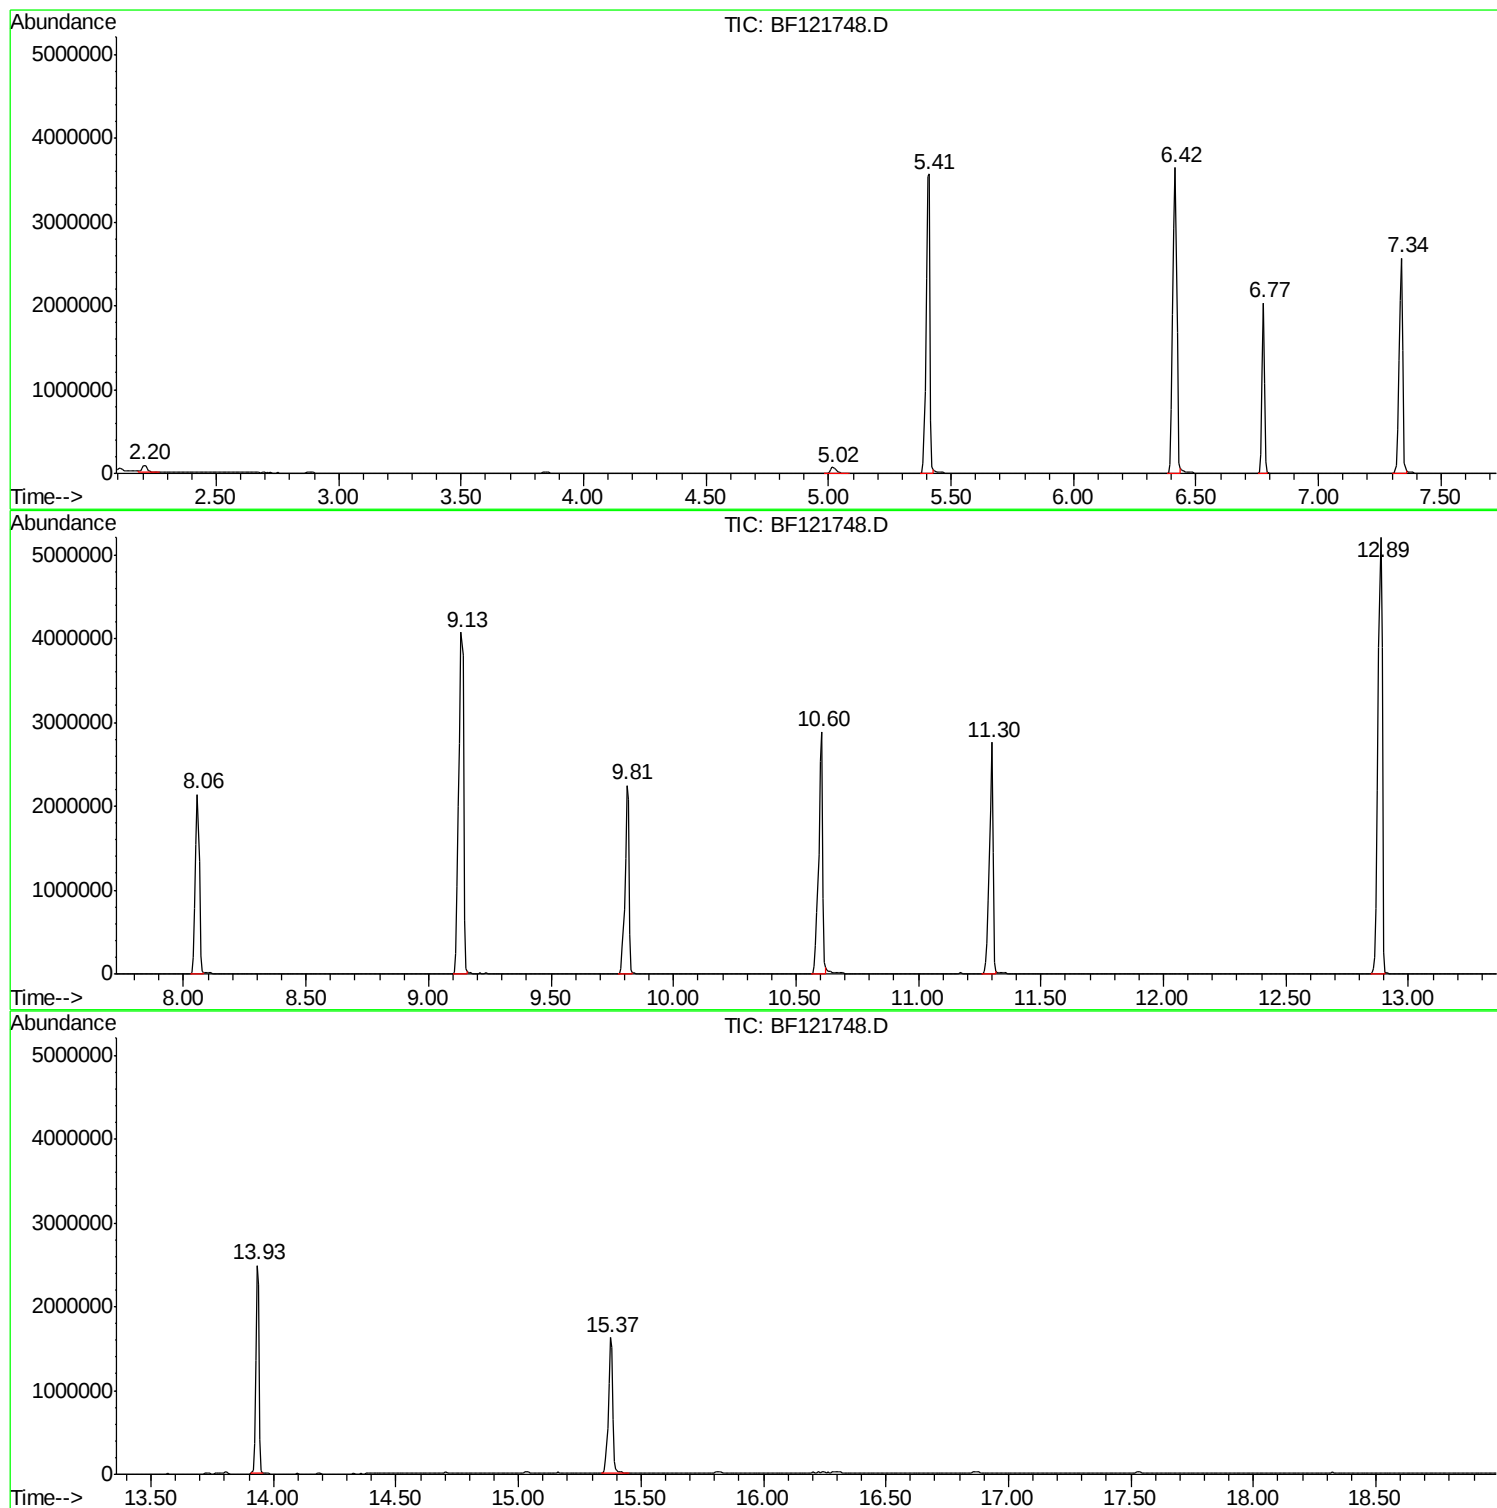

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF093020\
Data File : BF121748.D
Acq On : 30 Sep 2020 20:04
Operator : JU/CG
Sample : PB132010BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132010BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF093020\
Data File : BF121748.D
Acq On : 30 Sep 2020 20:04
Operator : JU/CG
Sample : PB132010BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB132010BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc